

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
 Data File : BP024221.D
 Acq On : 08 Apr 2025 20:31
 Operator : RC/JU
 Sample : Q1730-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OU4-PCS-TC-23-040325

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP024221.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.899	302	308	317	rBV	454869	655013	4.95%	0.972%
2	5.358	379	386	398	rBV	3761965	5415842	40.89%	8.038%
3	6.922	644	652	671	rBV	3622927	5691323	42.97%	8.447%
4	7.740	783	791	798	rBV	1291705	2007932	15.16%	2.980%
5	8.887	978	986	1002	rBV	2173869	3419148	25.82%	5.075%
6	9.452	1073	1082	1092	rBV2	73363	137037	1.03%	0.203%
7	10.516	1255	1263	1275	rBV	1591741	2695109	20.35%	4.000%
8	12.993	1676	1684	1694	rBV	5311796	7866922	59.40%	11.676%
9	14.381	1912	1920	1933	rBV	2349731	3438372	25.96%	5.103%
10	15.769	2150	2156	2165	rBV	516530	700981	5.29%	1.040%
11	15.892	2171	2177	2197	rBV	4390463	6090268	45.98%	9.039%
12	17.192	2390	2398	2410	rBV2	2511992	4025060	30.39%	5.974%
13	18.139	2553	2559	2568	rBV	637777	1044841	7.89%	1.551%
14	19.457	2779	2783	2790	rBV	235373	321035	2.42%	0.476%
15	19.910	2855	2860	2865	rBV	11449084	13244567	100.00%	19.658%
16	21.310	3094	3098	3116	rBV3	257321	707570	5.34%	1.050%
17	21.639	3148	3154	3161	rBV2	3072551	4910122	37.07%	7.288%
18	25.004	3718	3726	3740	rVB	2071751	5005017	37.79%	7.428%




Sum of corrected areas: 67376159

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
Data File : BP024221.D
Acq On : 08 Apr 2025 20:31
Operator : RC/JU
Sample : Q1730-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-PCS-TC-23-040325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

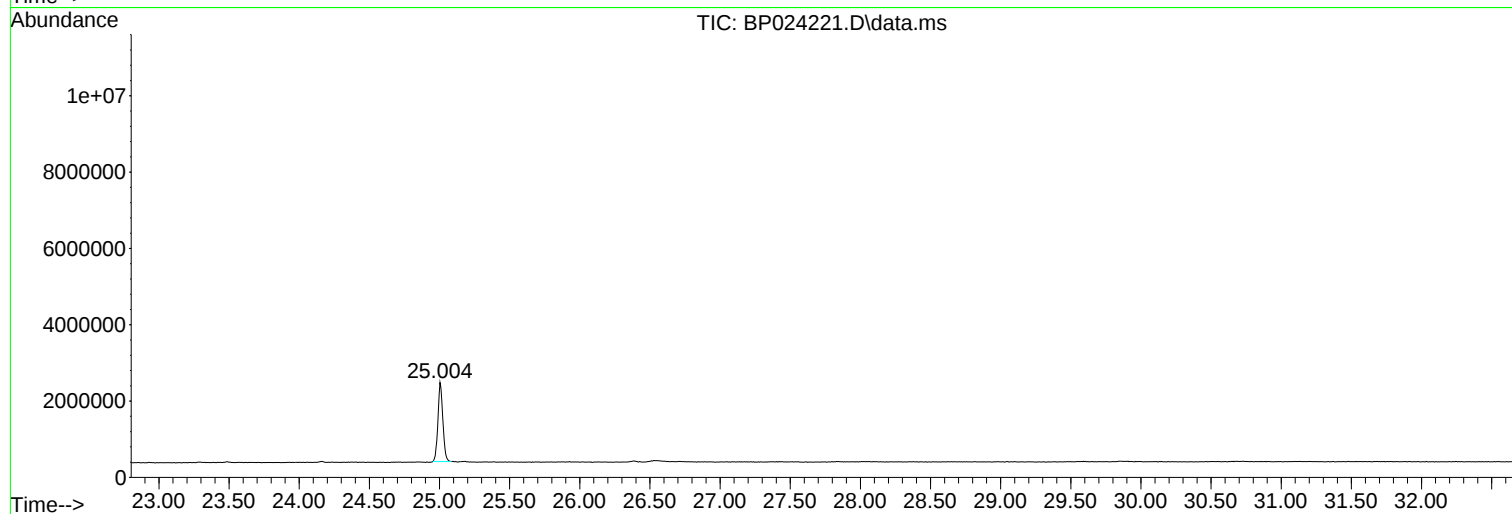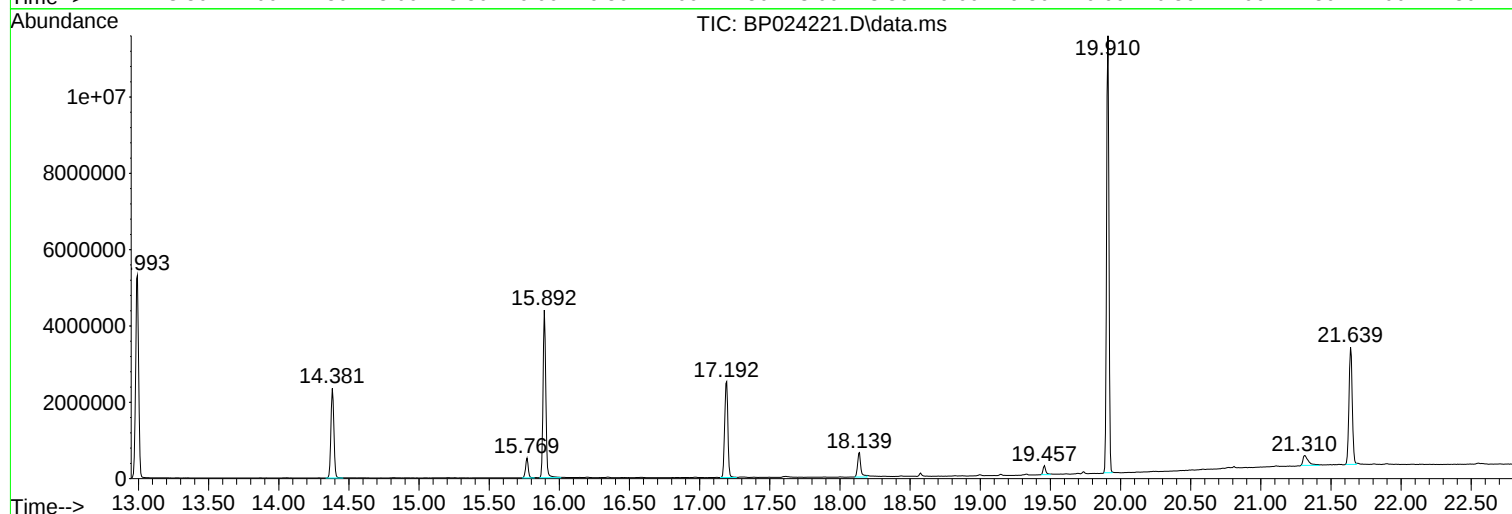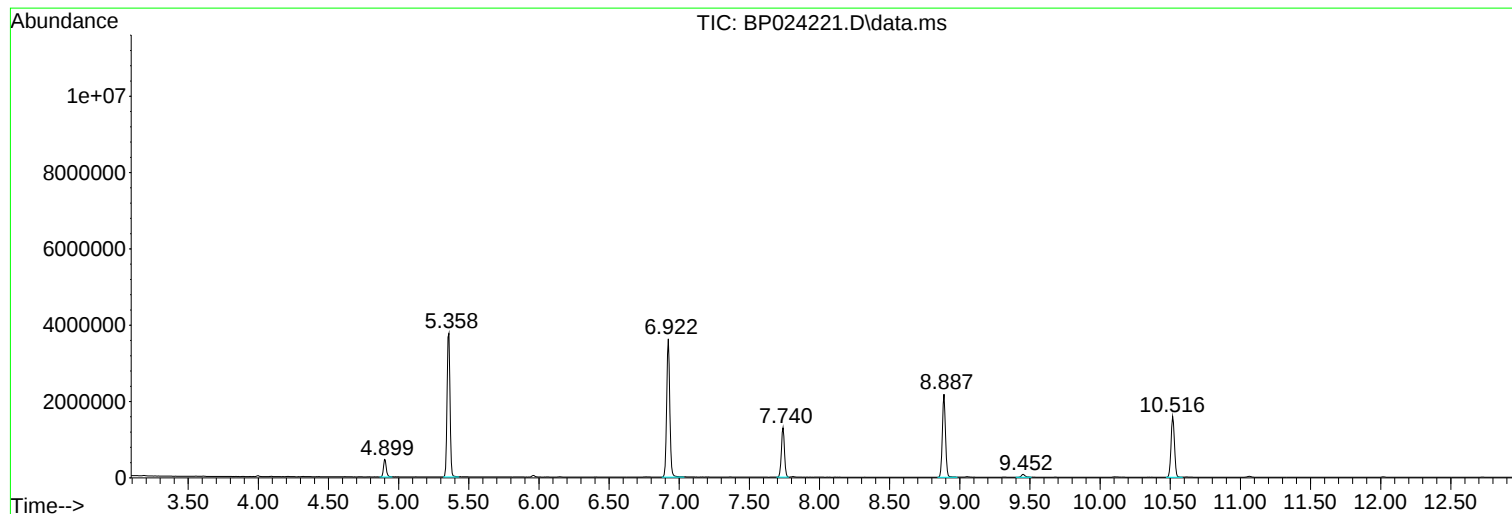

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
Data File : BP024221.D
Acq On : 08 Apr 2025 20:31
Operator : RC/JU
Sample : Q1730-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-PCS-TC-23-040325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
Data File : BP024221.D
Acq On : 08 Apr 2025 20:31
Operator : RC/JU
Sample : Q1730-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-PCS-TC-23-040325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc