

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
 Data File : BP024223.D
 Acq On : 08 Apr 2025 21:52
 Operator : RC/JU
 Sample : Q1730-15
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OU4-PCS-TC-25-040325

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP024223.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.899	302	308	317	rBV	348911	520822	2.69%	0.673%
2	5.358	379	386	404	rBV	3085560	4574099	23.62%	5.911%
3	6.922	643	652	666	rBV	3340689	5206625	26.88%	6.729%
4	7.740	784	791	799	rBV	820824	1276523	6.59%	1.650%
5	8.893	978	987	1005	rBV	1934637	3181482	16.43%	4.112%
6	10.522	1254	1264	1276	rBV	1244710	2018389	10.42%	2.609%
7	12.987	1675	1683	1696	rBV	5680247	8400719	43.37%	10.857%
8	14.381	1909	1920	1935	rBV	2110422	3215101	16.60%	4.155%
9	15.769	2149	2156	2165	rBV	791335	995577	5.14%	1.287%
10	15.892	2171	2177	2192	rBV	5703590	7994805	41.28%	10.332%
11	17.181	2389	2396	2409	rBV	3079039	4483640	23.15%	5.795%
12	18.122	2549	2556	2565	rBV	799202	1275542	6.59%	1.648%
13	19.445	2776	2781	2788	rBV2	193917	306259	1.58%	0.396%
14	19.904	2853	2859	2868	rBV	14627948	19368669	100.00%	25.032%
15	21.310	3092	3098	3117	rBV2	465997	1181239	6.10%	1.527%
16	21.627	3146	3152	3160	rBV2	4320455	6374758	32.91%	8.239%
17	25.004	3717	3726	3744	rVB	2707090	7002820	36.16%	9.050%




Sum of corrected areas: 77377069

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
Data File : BP024223.D
Acq On : 08 Apr 2025 21:52
Operator : RC/JU
Sample : Q1730-15
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-PCS-TC-25-040325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

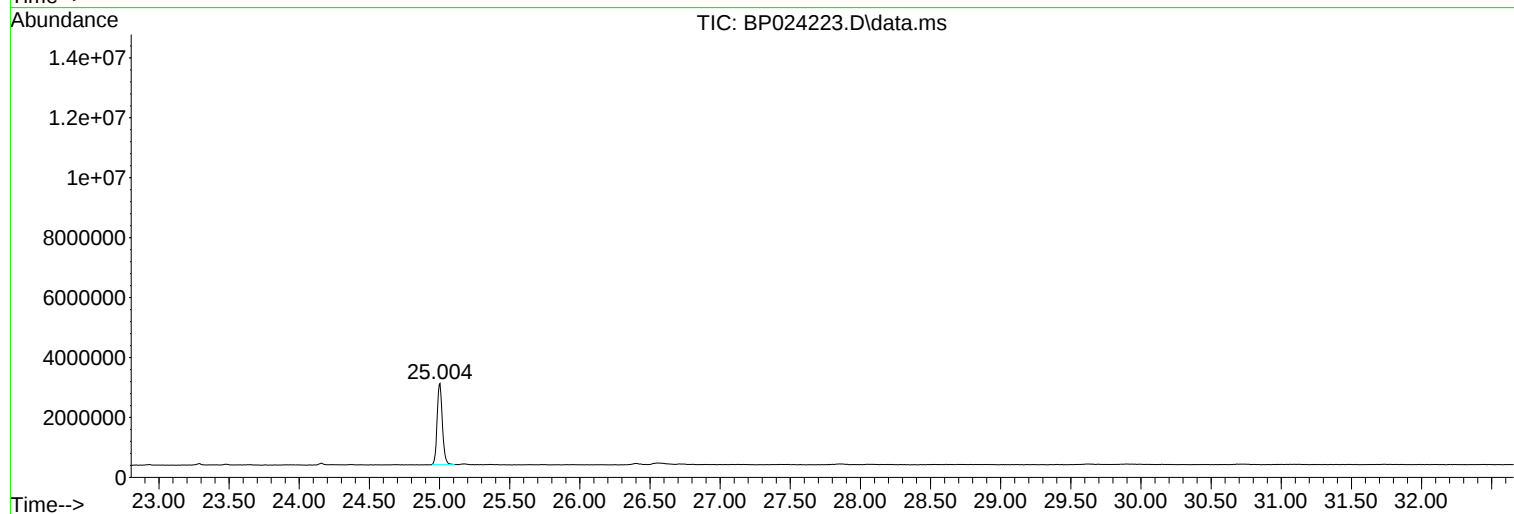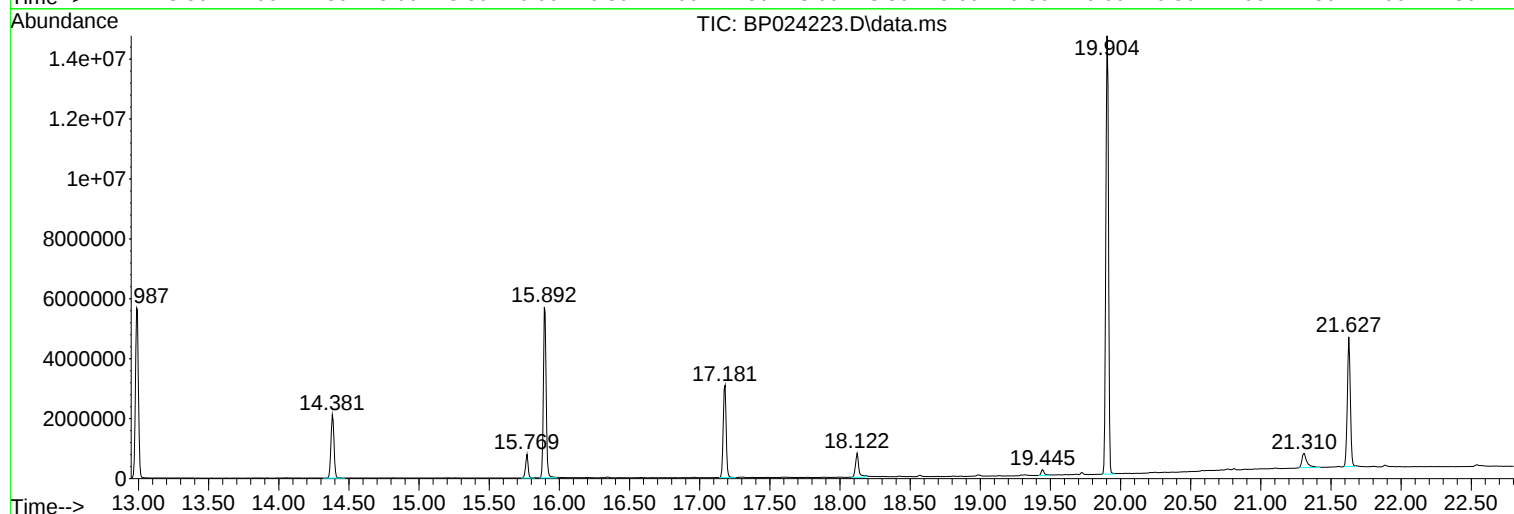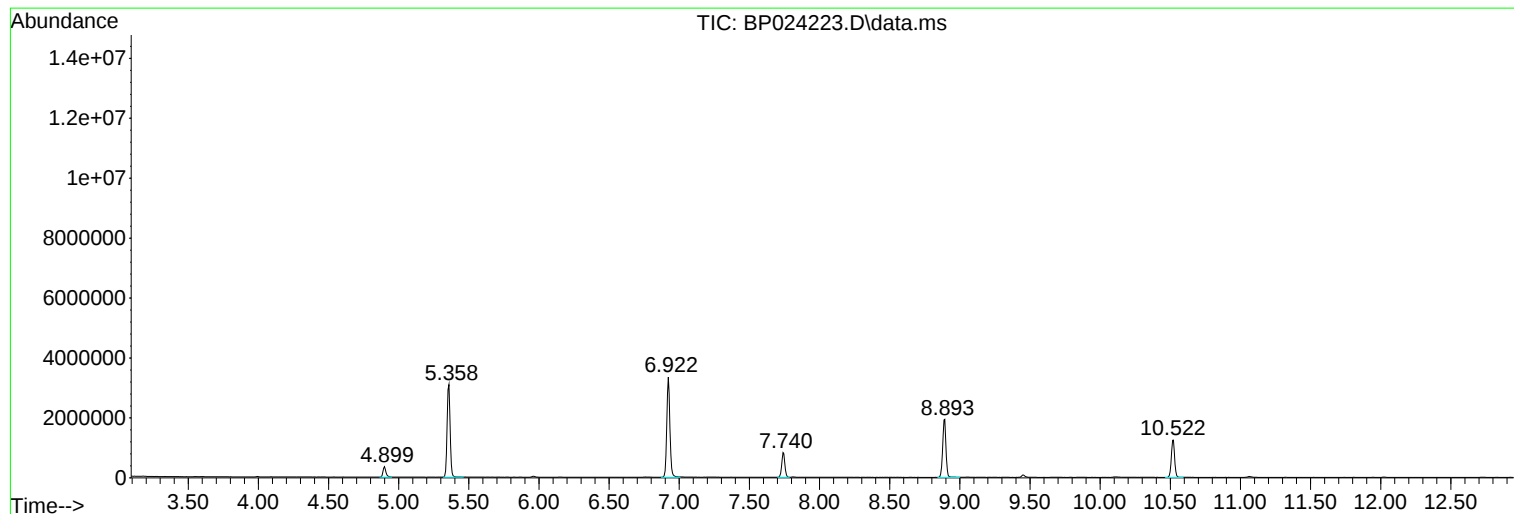

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
Data File : BP024223.D
Acq On : 08 Apr 2025 21:52
Operator : RC/JU
Sample : Q1730-15
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-PCS-TC-25-040325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
Data File : BP024223.D
Acq On : 08 Apr 2025 21:52
Operator : RC/JU
Sample : Q1730-15
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-PCS-TC-25-040325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc