

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
 Data File : BP024224.D
 Acq On : 08 Apr 2025 22:33
 Operator : RC/JU
 Sample : Q1730-17
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OU4-PCS-TC-26-040325

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP024224.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.899	302	308	317	rBV	726070	982065	5.86%	1.147%
2	5.358	379	386	403	rBV	5880957	8289357	49.47%	9.679%
3	6.922	643	652	675	rBV	5476376	8478227	50.60%	9.900%
4	7.740	784	791	799	rBV	1345323	2130656	12.72%	2.488%
5	8.887	978	986	1004	rBV	3202586	5329693	31.81%	6.223%
6	10.522	1256	1264	1275	rBV	1665506	2922615	17.44%	3.413%
7	12.987	1676	1683	1695	rBV	8100128	11964842	71.40%	13.971%
8	14.375	1909	1919	1933	rBV	2412659	3674231	21.93%	4.290%
9	15.763	2148	2155	2162	rBV	618145	803491	4.80%	0.938%
10	15.893	2171	2177	2196	rBV	6388574	8898807	53.11%	10.391%
11	17.187	2389	2397	2408	rBV2	2683866	4094246	24.43%	4.781%
12	18.128	2551	2557	2567	rBV	536970	924801	5.52%	1.080%
13	19.457	2779	2783	2792	rBV	133283	195556	1.17%	0.228%
14	19.922	2855	2862	2871	rBV	11875420	16756604	100.00%	19.566%
15	21.316	3095	3099	3115	rBV3	238404	610062	3.64%	0.712%
16	21.633	3147	3153	3163	rBV2	3257474	4768657	28.46%	5.568%
17	25.010	3719	3727	3743	rVB	1717884	4817068	28.75%	5.625%




Sum of corrected areas: 85640978

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
Data File : BP024224.D
Acq On : 08 Apr 2025 22:33
Operator : RC/JU
Sample : Q1730-17
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-PCS-TC-26-040325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

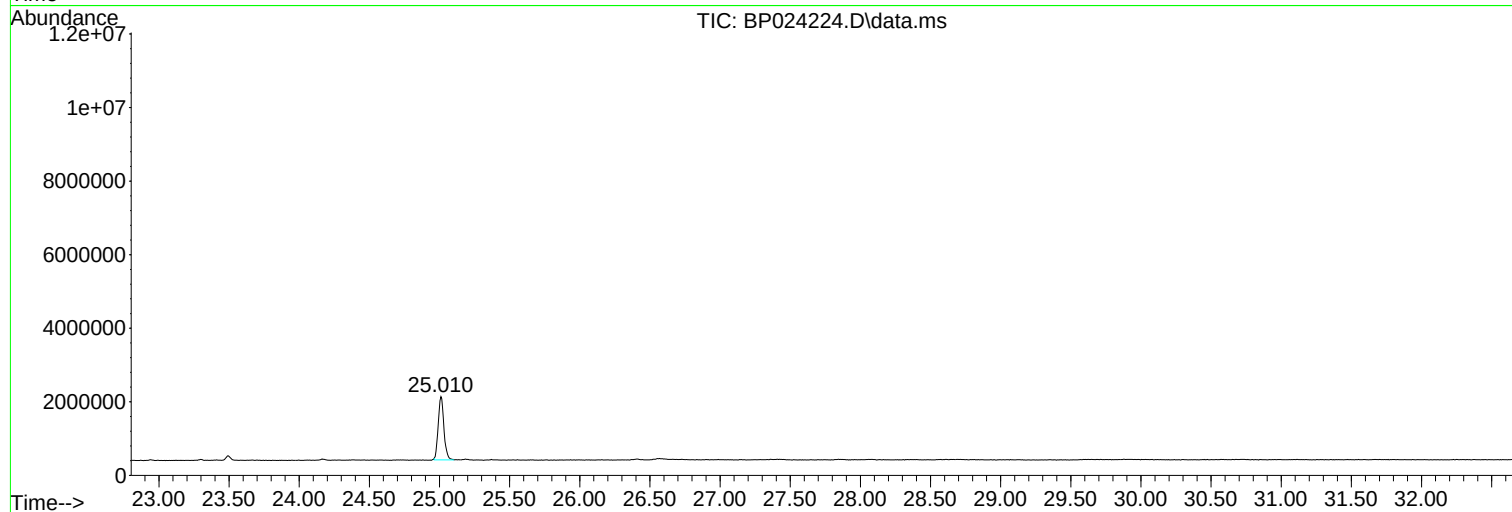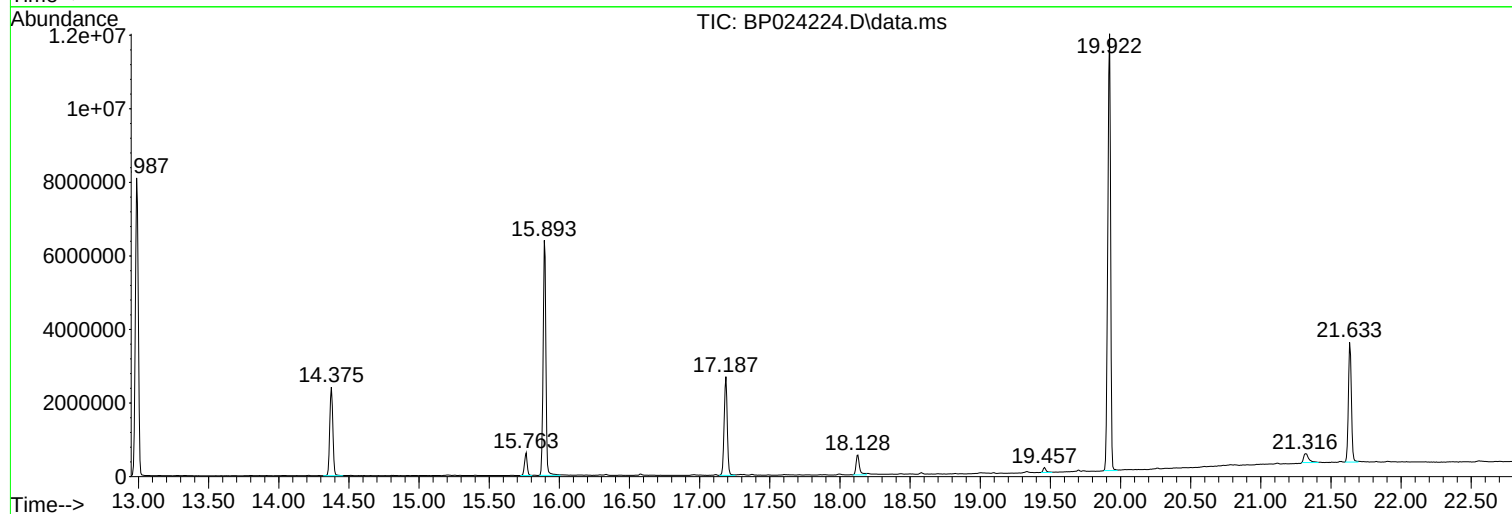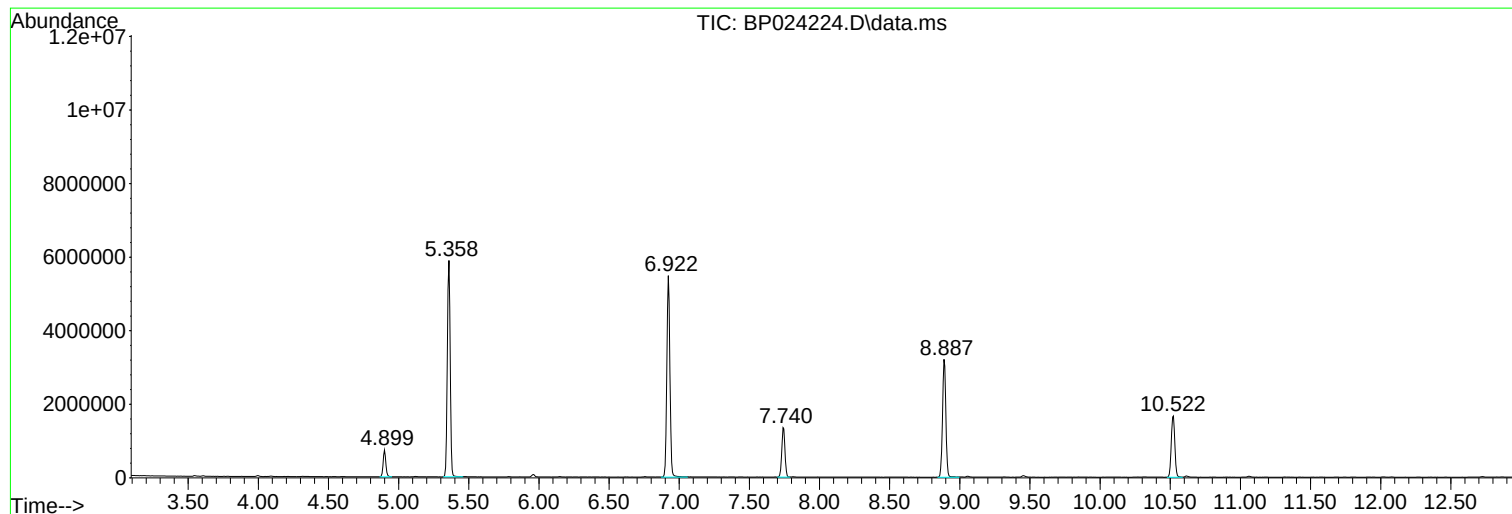

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
Data File : BP024224.D
Acq On : 08 Apr 2025 22:33
Operator : RC/JU
Sample : Q1730-17
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-PCS-TC-26-040325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
Data File : BP024224.D
Acq On : 08 Apr 2025 22:33
Operator : RC/JU
Sample : Q1730-17
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-PCS-TC-26-040325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------