
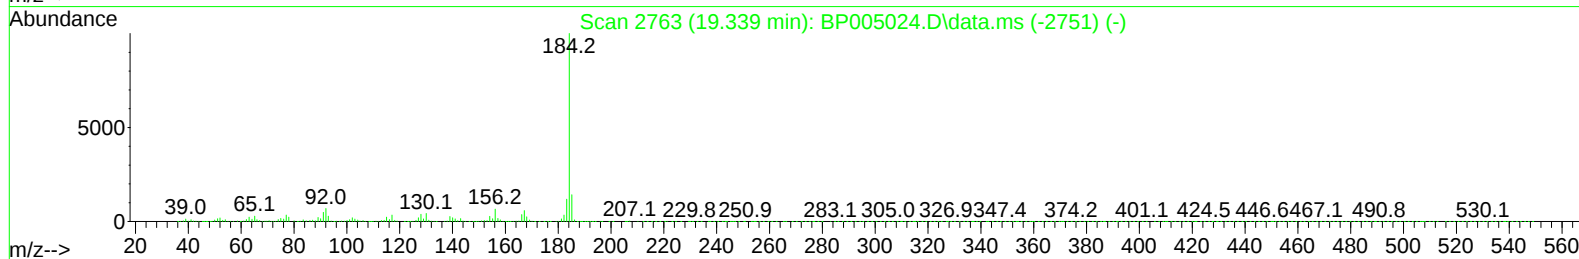
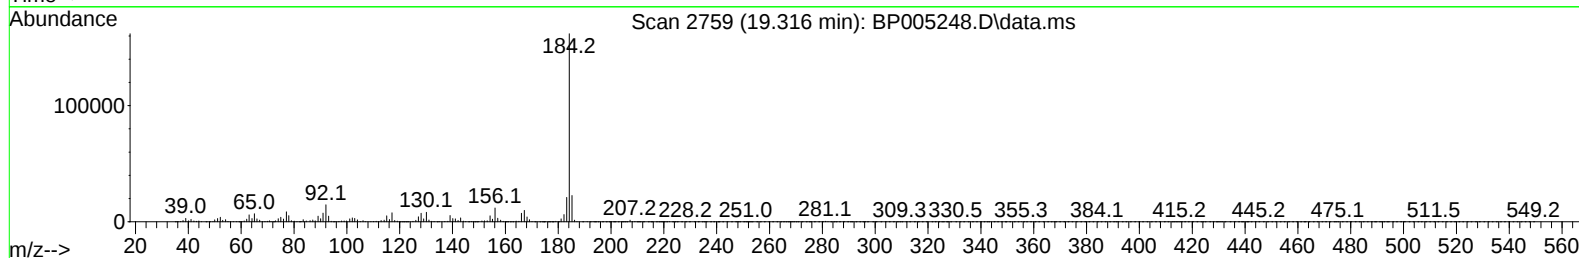


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040921\
 Data File : BP005248.D
 Acq On : 09 Apr 2021 13:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 09 13:44:04 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 06 12:33:08 2021
 Response via : Initial Calibration

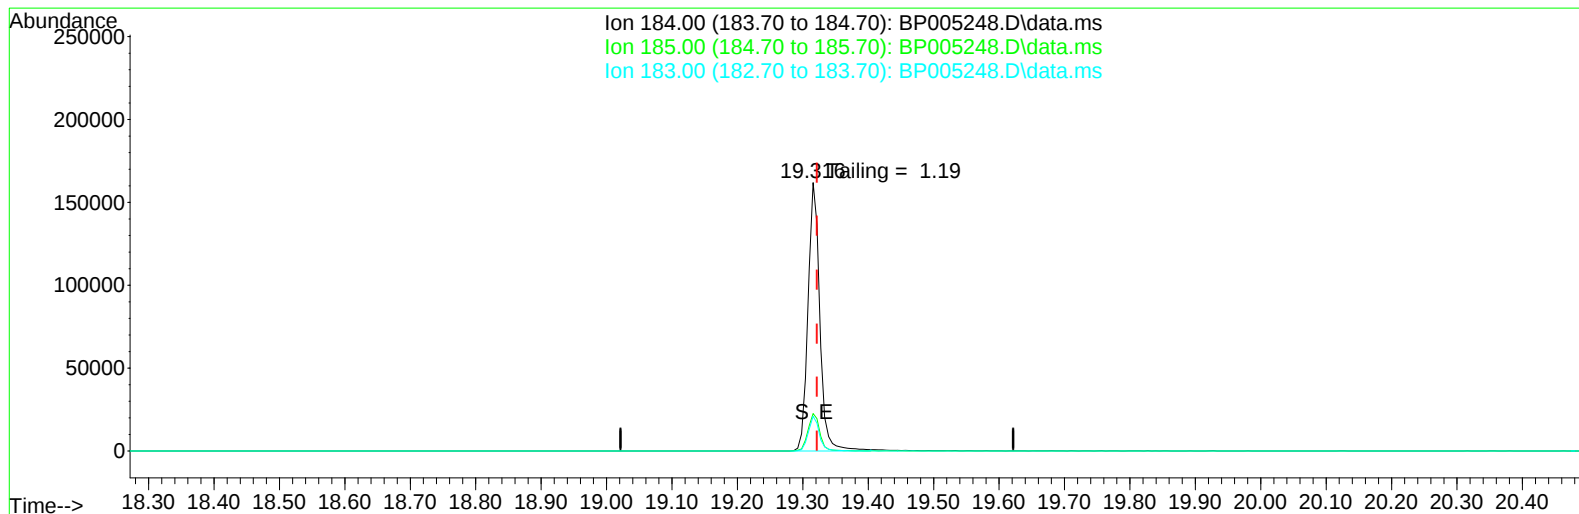

TIC: BP005248.D\data.ms

(77) Benzidine




19.316min (-0.006) 494321.25 ng

response 206065

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.99
183.00	12.00	12.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040921\
Data File : BP005248.D
Acq On : 09 Apr 2021 13:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 09 13:44:04 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 06 12:33:08 2021
Response via : Initial Calibration

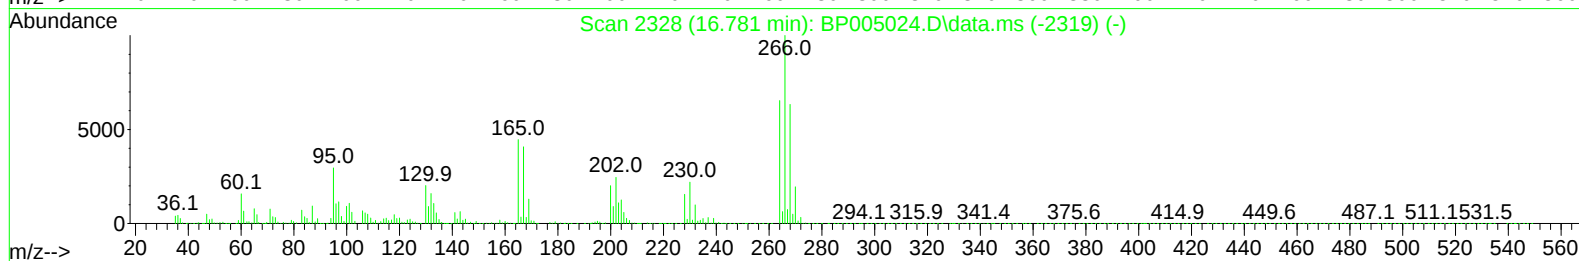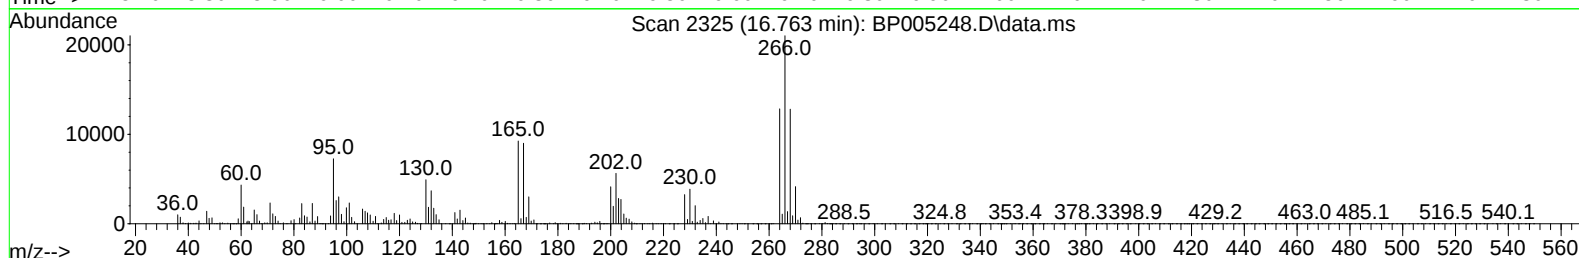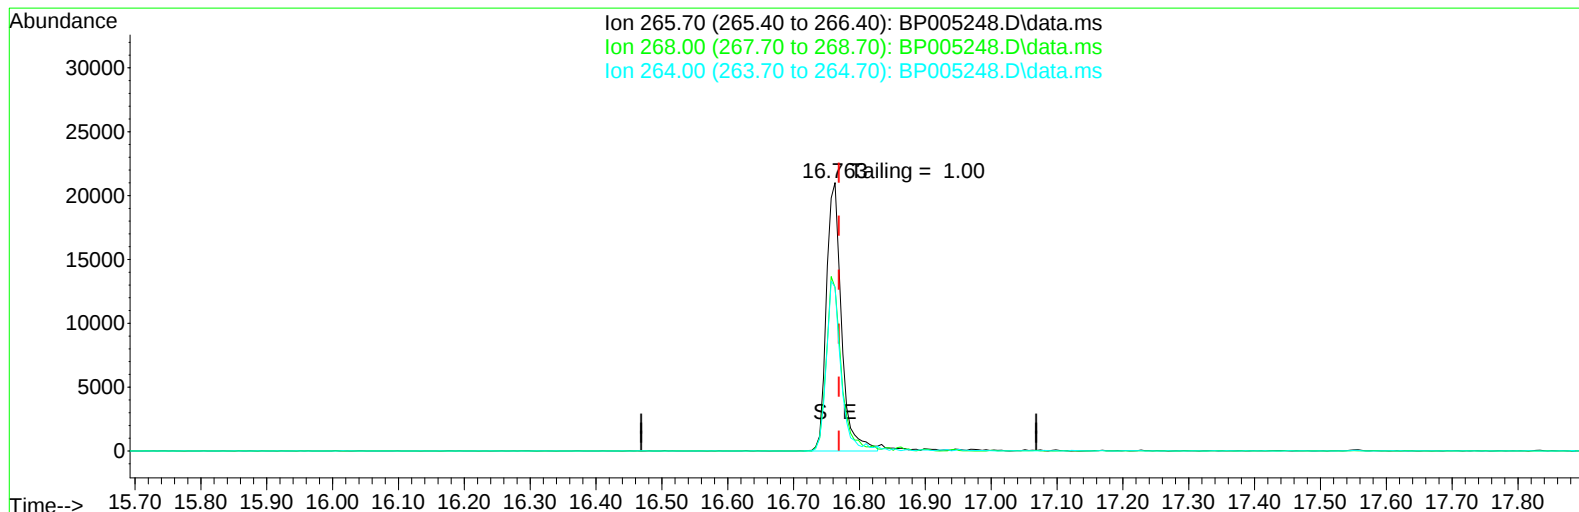

TIC: BP005248.D\data.ms

(70) Pentachlorophenol (C)

16.763min (-0.006) 362288.77 ng

response 34284

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	60.93
264.00	63.30	61.07
0.00	0.00	0.00