




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
 Data File : BP014626.D
 Acq On : 10 Apr 2023 10:58
 Operator : CG/JU
 Sample : PB151978BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK978

Manual IntegrationsAPPROVED

Quant Time: Apr 11 00:55:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 11 00:52:14 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/11/2023
 Supervised By :Jagrut Upadhyay 04/11/2023

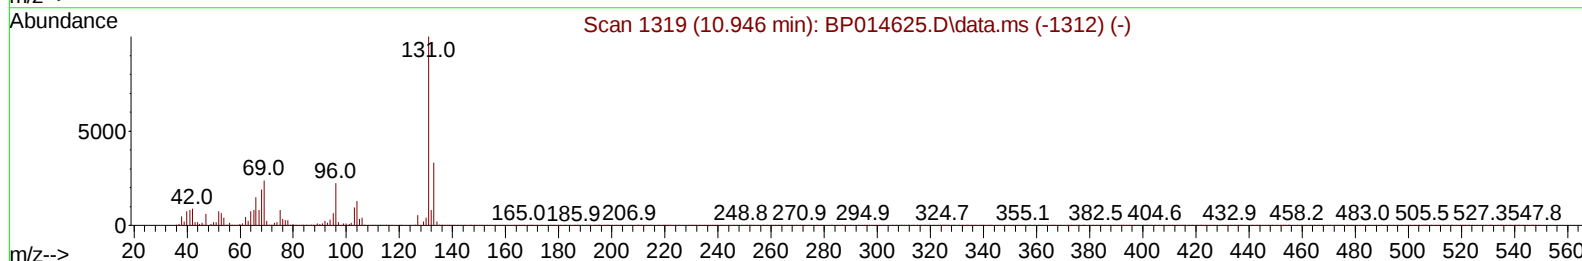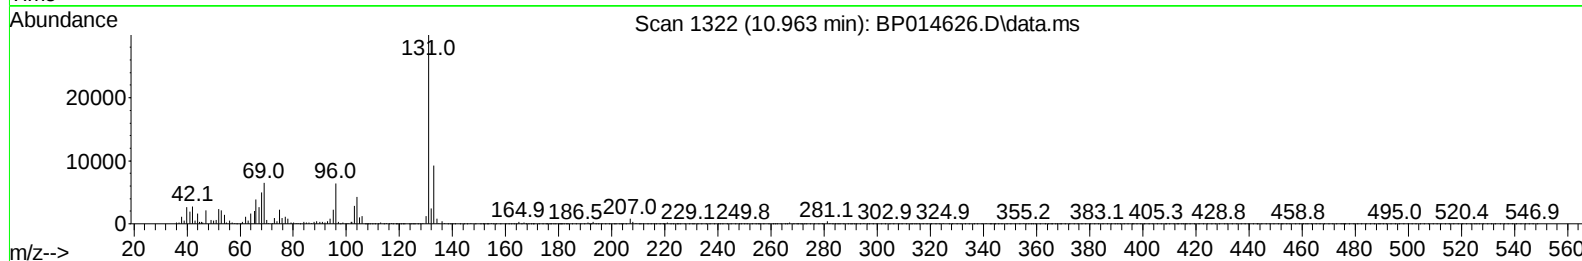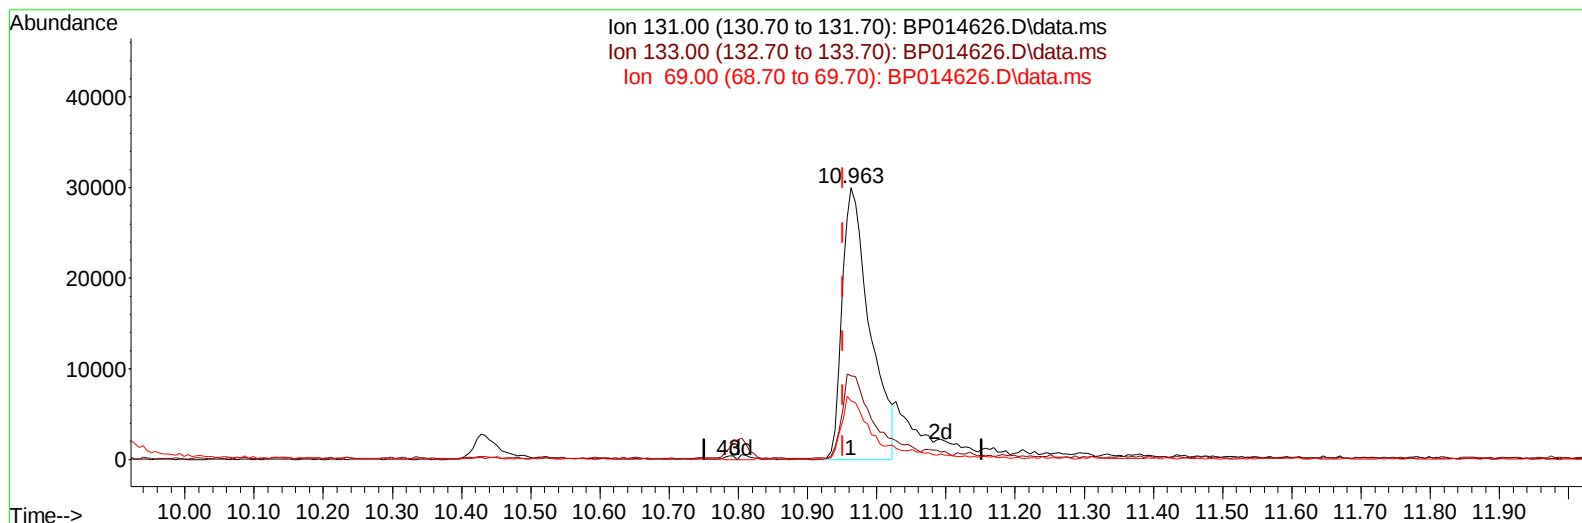

TIC: BP014626.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.963min (+ 0.012) 7.76 ng/u1

response 82761

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	30.79
69.00	21.30	21.62
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
 Data File : BP014626.D
 Acq On : 10 Apr 2023 10:58
 Operator : CG/JU
 Sample : PB151978BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK978

Manual IntegrationsAPPROVED

Quant Time: Apr 11 00:55:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 11 00:52:14 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/11/2023
 Supervised By :Jagrut Upadhyay 04/11/2023

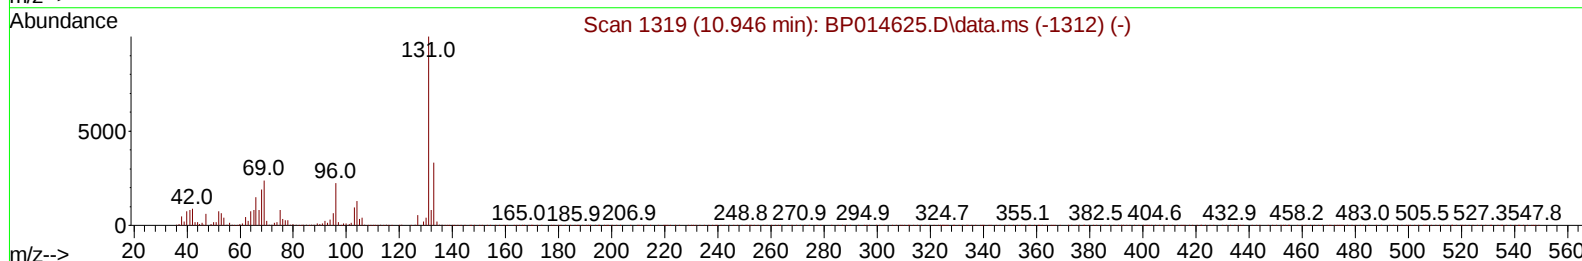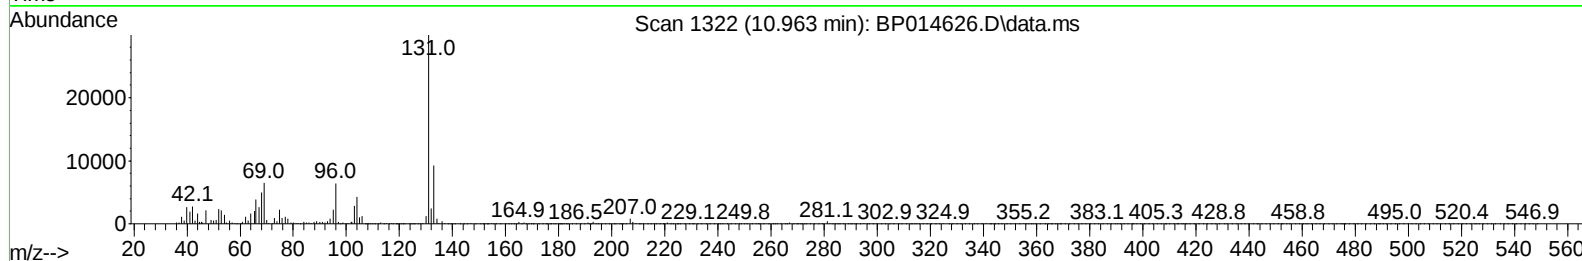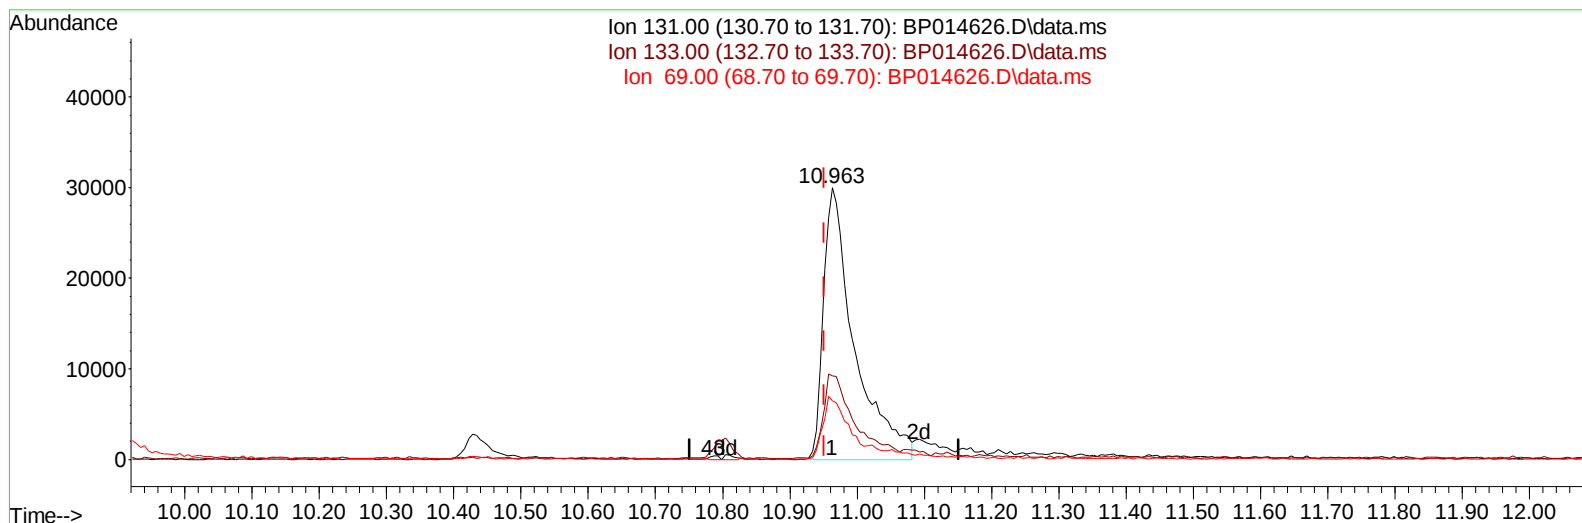

TIC: BP014626.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.963min (+ 0.012) 8.98 ng/ul m

response 95754

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	30.79
69.00	21.30	21.62
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
 Data File : BP014626.D
 Acq On : 10 Apr 2023 10:58
 Operator : CG/JU
 Sample : PB151978BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK978

Manual IntegrationsAPPROVED

Quant Time: Apr 11 00:55:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 11 00:52:14 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/11/2023
 Supervised By :Jagrut Upadhyay 04/11/2023

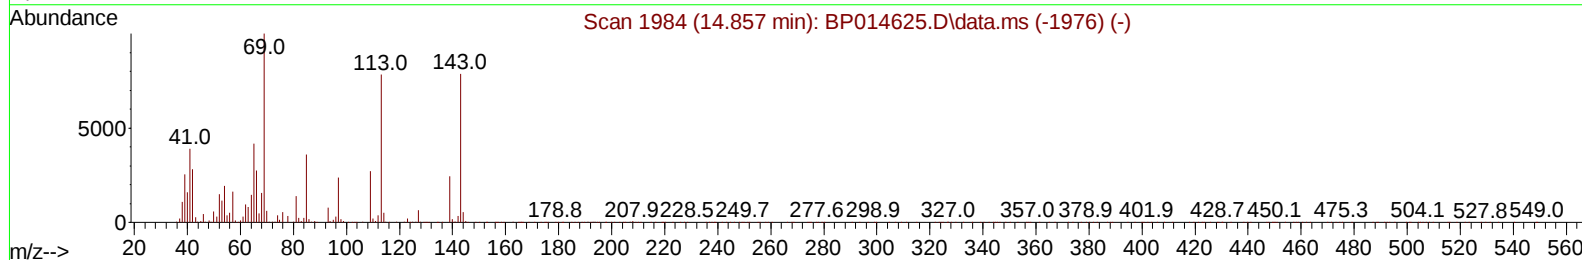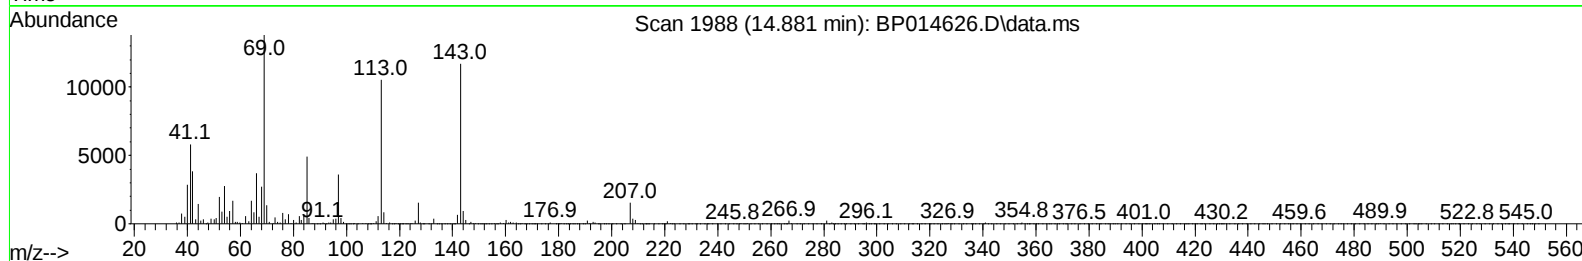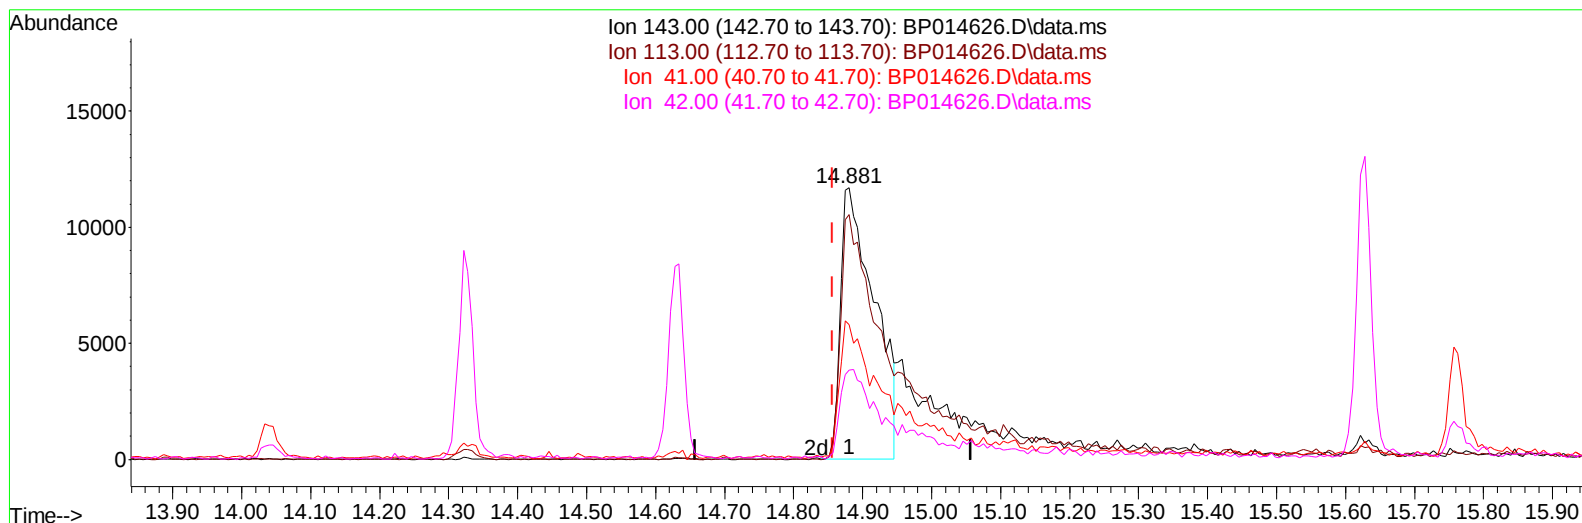

TIC: BP014626.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.881min (+ 0.023) 11.00 ng/u1

response 39875

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	90.17
41.00	44.20	49.76
42.00	31.50	32.91




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
 Data File : BP014626.D
 Acq On : 10 Apr 2023 10:58
 Operator : CG/JU
 Sample : PB151978BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK978

Manual IntegrationsAPPROVED

Quant Time: Apr 11 00:55:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 11 00:52:14 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/11/2023
 Supervised By :Jagrut Upadhyay 04/11/2023

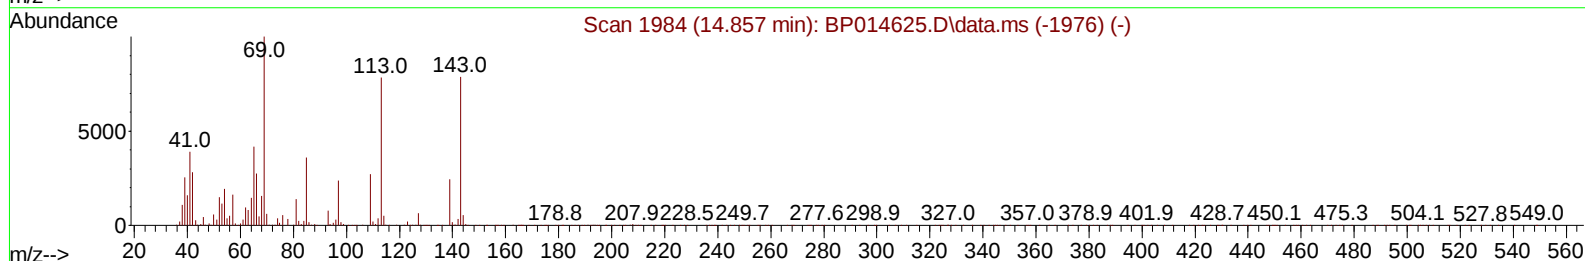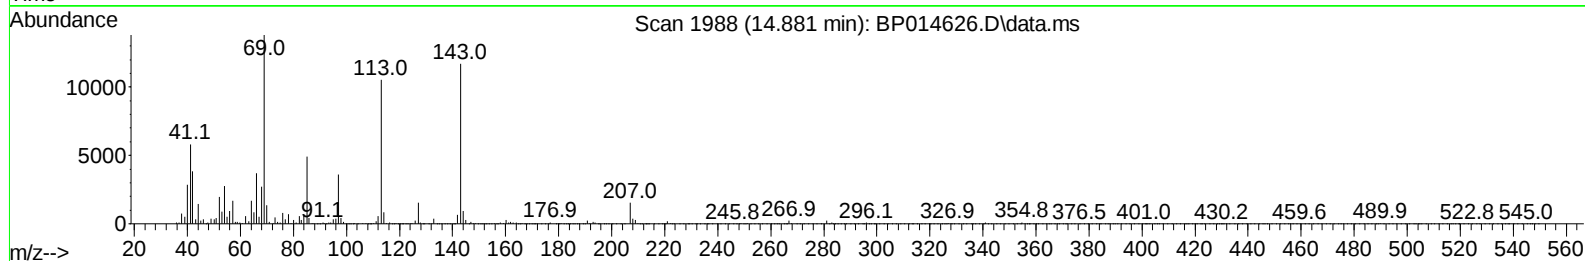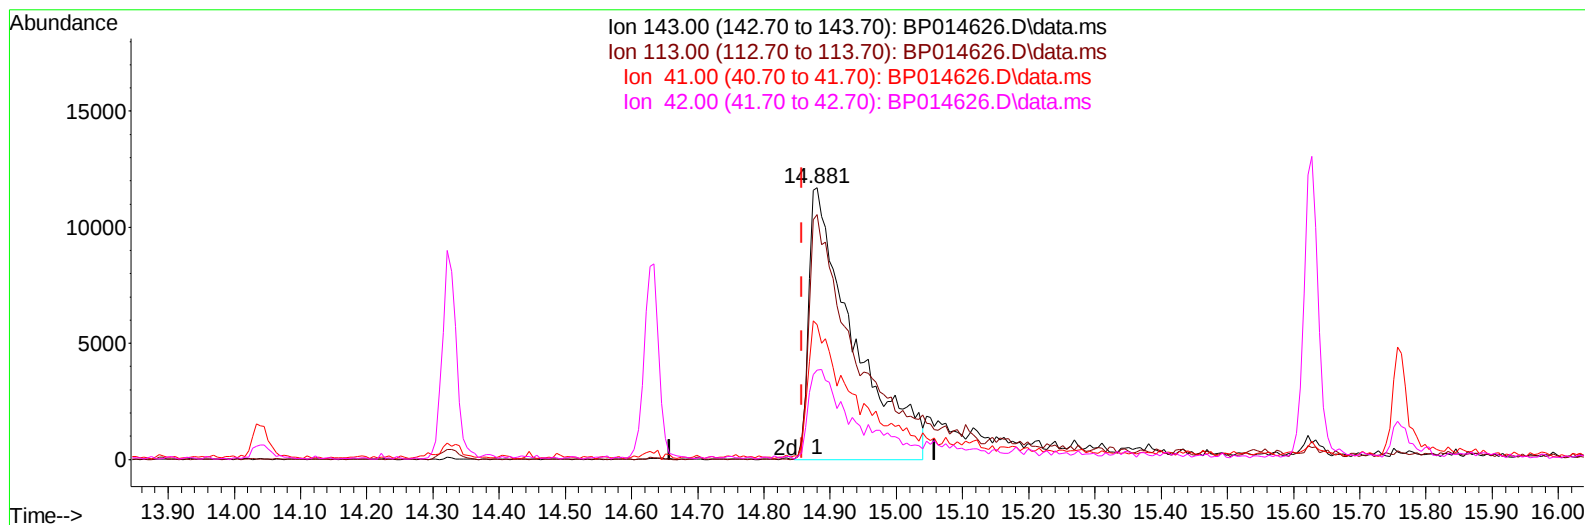

TIC: BP014626.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.881min (+ 0.023) 15.09 ng/ul m

response 54663

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	90.17
41.00	44.20	49.76
42.00	31.50	32.91




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014626.D
Acq On : 10 Apr 2023 10:58
Operator : CG/JU
Sample : PB151978BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK978

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/11/2023
Supervised By :Jagrut Upadhyay 04/11/2023

Quant Time: Apr 11 00:55:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 00:52:14 2023
Response via : Initial Calibration

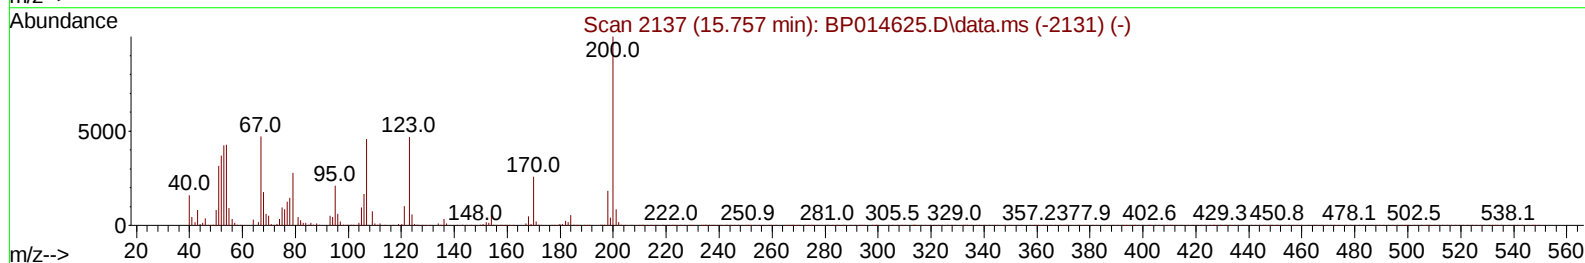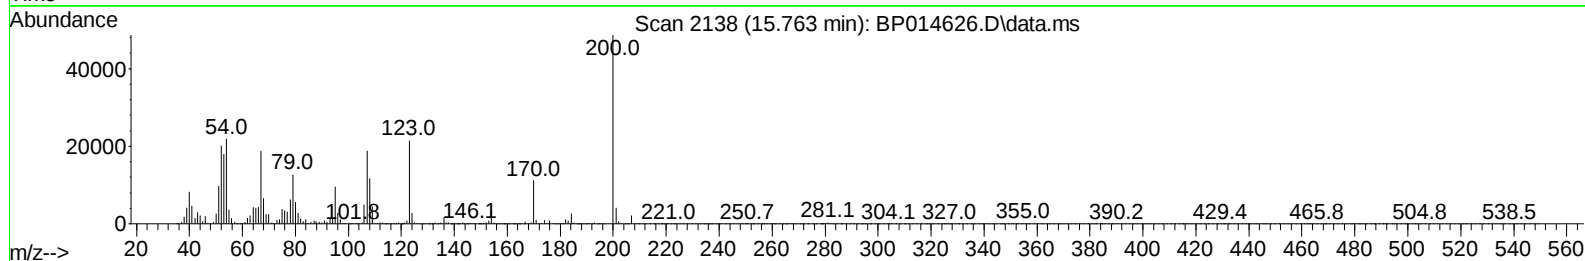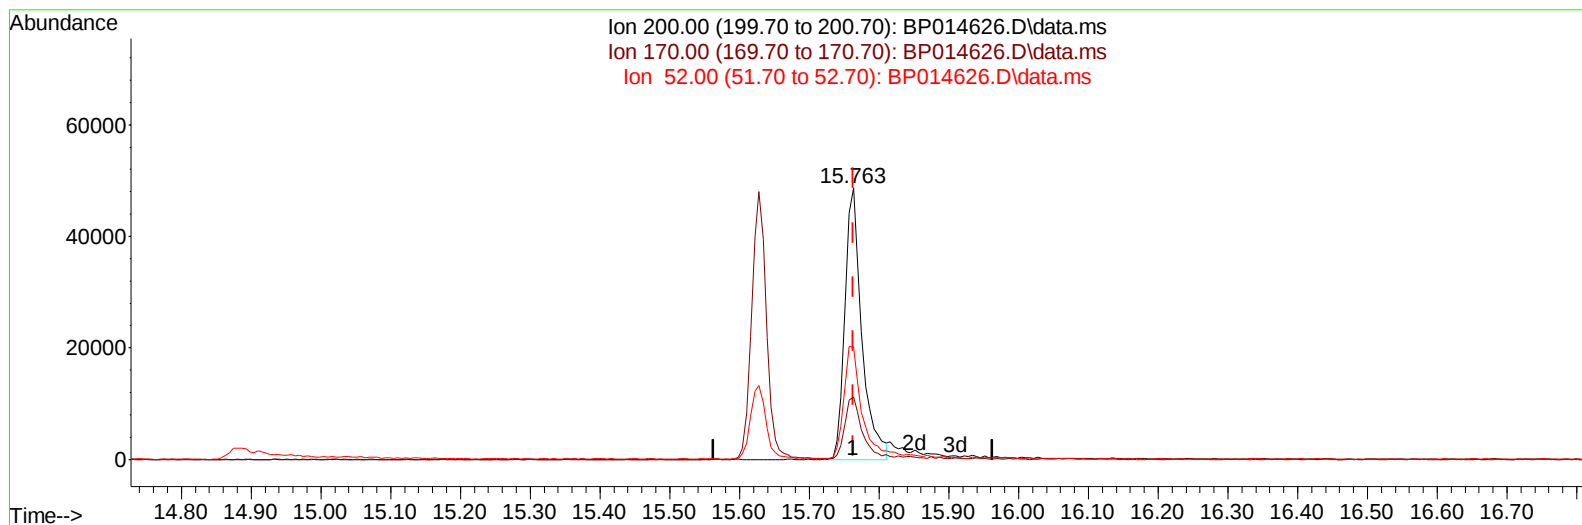

TIC: BP014626.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.763min (-0.000) 18.57 ng/u1

response 82106

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	22.10	23.01
52.00	45.50	41.36
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
 Data File : BP014626.D
 Acq On : 10 Apr 2023 10:58
 Operator : CG/JU
 Sample : PB151978BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK978

Manual IntegrationsAPPROVED

Quant Time: Apr 11 00:55:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 11 00:52:14 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/11/2023
 Supervised By :Jagrut Upadhyay 04/11/2023

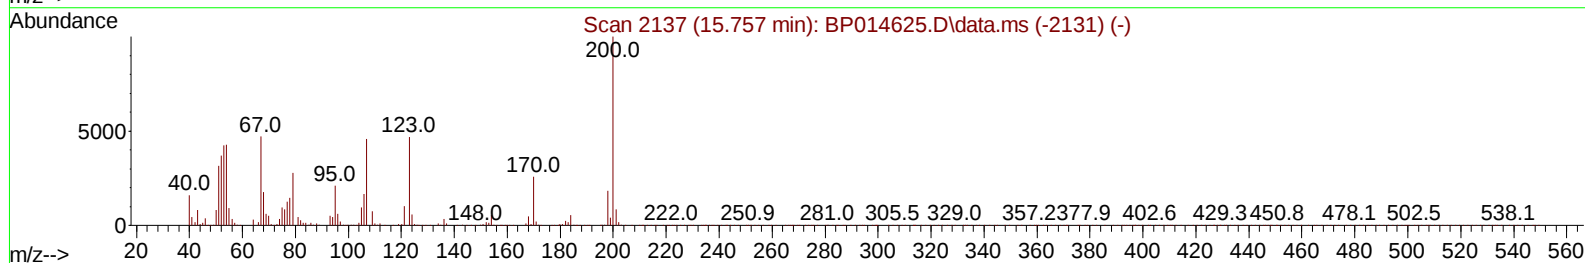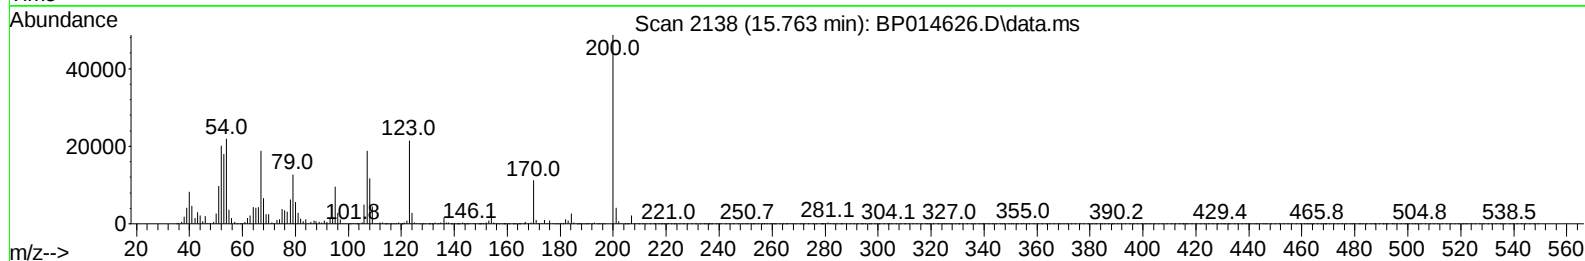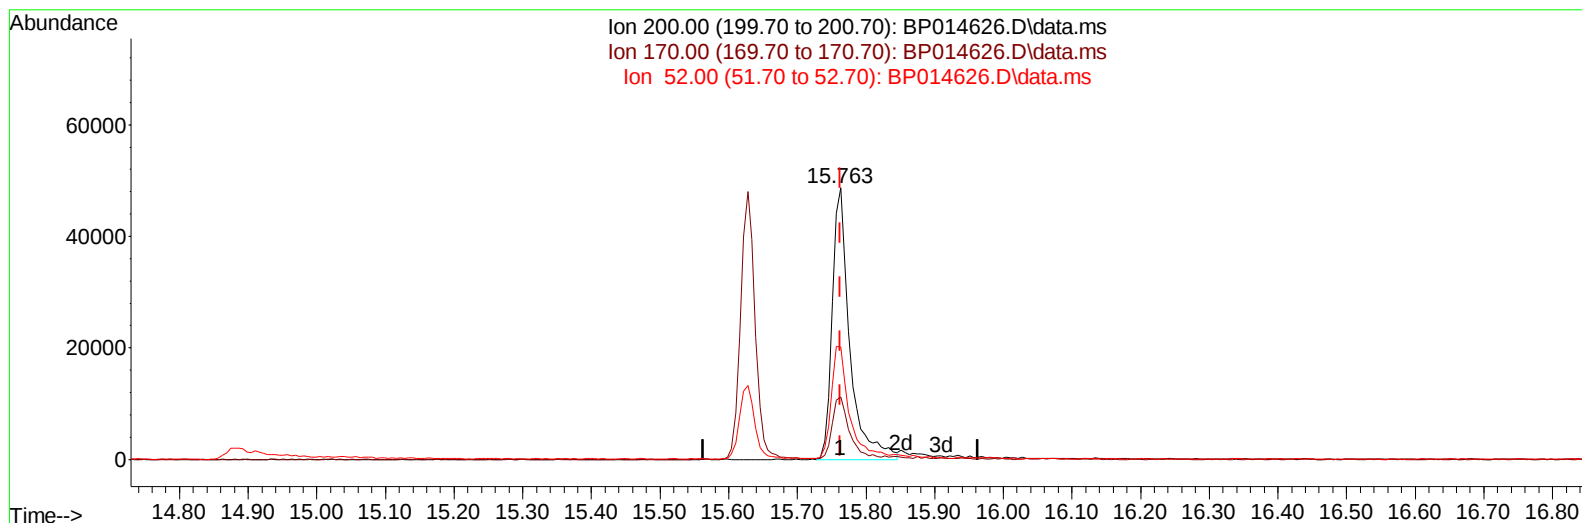

TIC: BP014626.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.763min (-0.000) 19.54 ng/ul m

response 86359

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	22.10	23.01
52.00	45.50	41.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
 Data File : BP014626.D
 Acq On : 10 Apr 2023 10:58
 Operator : CG/JU
 Sample : PB151978BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK978

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/11/2023
 Supervised By :Jagrut Upadhyay 04/11/2023

Quant Time: Apr 11 00:55:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 11 00:52:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.981	152	113880	20.000	ng/ul	0.00
20) Naphthalene-d8	10.799	136	480946	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.634	164	295811	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.392	188	600777	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	518645	20.000	ng/ul	0.00
88) Perylene-d12	23.980	264	590854	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	18501	6.300	ng/uL	0.00
4) Pyridine-d5	3.799	84	102671	13.643	ng/ul	0.00
7) Phenol-d5	7.146	99	278746	26.541	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.305	67	203379	30.182	ng/ul	0.00
11) 2-Chlorophenol-d4	7.510	132	220344	29.027	ng/ul	0.00
15) 4-Methylphenol-d8	8.699	113	221405	26.135	ng/ul	0.00
21) Nitrobenzene-d5	9.157	128	103877	26.755	ng/ul	0.00
24) 2-Nitrophenol-d4	9.881	143	119191	26.809	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.428	165	196199	24.232	ng/ul	0.00
31) 4-Chloroaniline-d4	10.963	131	95754m	8.978	ng/ul	0.01
46) Dimethylphthalate-d6	14.040	166	673691	28.088	ng/ul	0.00
49) Acenaphthylene-d8	14.328	160	764680	28.733	ng/ul	0.00
54) 4-Nitrophenol-d4	14.881	143	54663m	15.086	ng/ul	0.02
60) Fluorene-d10	15.628	176	569565	28.476	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.763	200	86359m	19.536	ng/ul	0.00
73) Anthracene-d10	17.492	188	859689	29.568	ng/ul	0.00
81) Pyrene-d10	19.722	212	950904	27.296	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.815	264	955872	30.450	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014626.D
Acq On : 10 Apr 2023 10:58
Operator : CG/JU
Sample : PB151978BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK978

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/11/2023
Supervised By :Jagrut Upadhyay 04/11/2023

Quant Time: Apr 11 00:55:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 00:52:14 2023
Response via : Initial Calibration

