




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014630.D
Acq On : 10 Apr 2023 17:06
Operator : CG/JU
Sample : PB152000BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK000

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/11/2023
Supervised By :Jagrut Upadhyay 04/11/2023

Quant Time: Apr 11 01:23:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

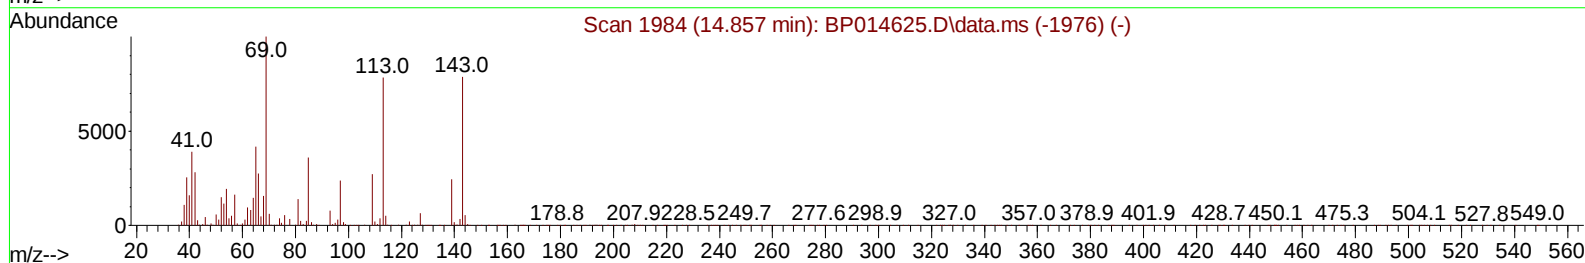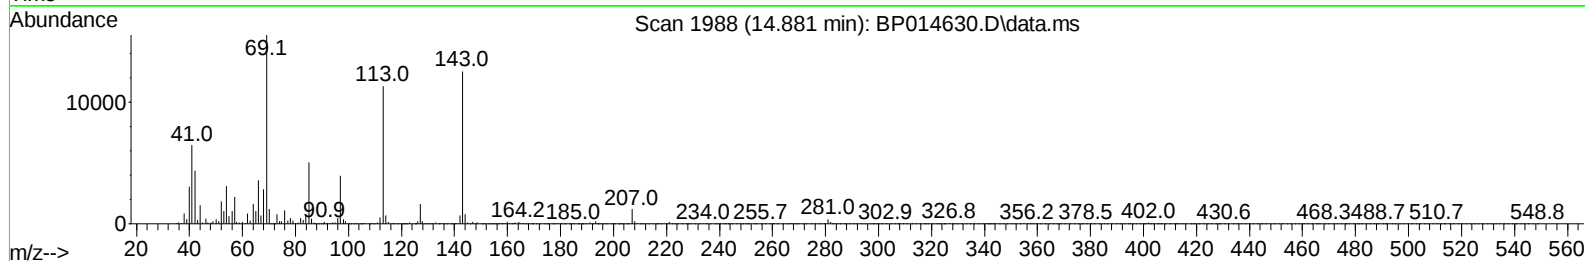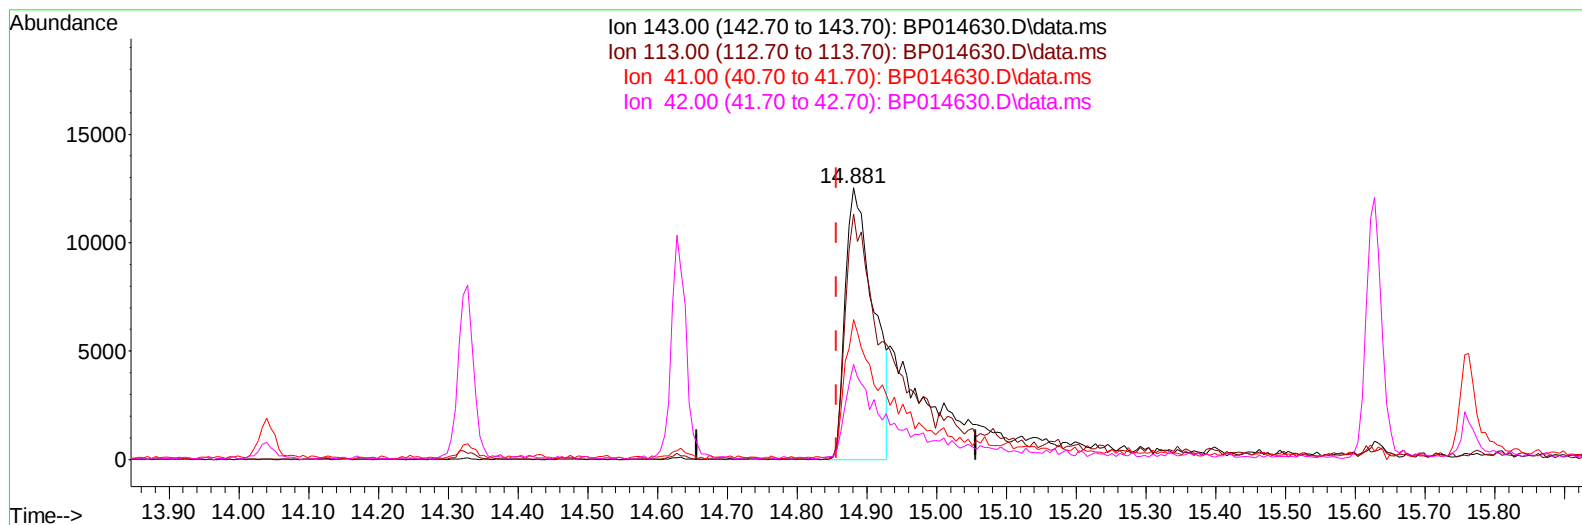

TIC: BP014630.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.881min (+ 0.024) 8.22 ng/u1

response 35053

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	90.35
41.00	44.20	51.51
42.00	31.50	35.04




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014630.D
Acq On : 10 Apr 2023 17:06
Operator : CG/JU
Sample : PB152000BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK000

Manual IntegrationsAPPROVED

Quant Time: Apr 11 01:23:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/11/2023
Supervised By :Jagrut Upadhyay 04/11/2023

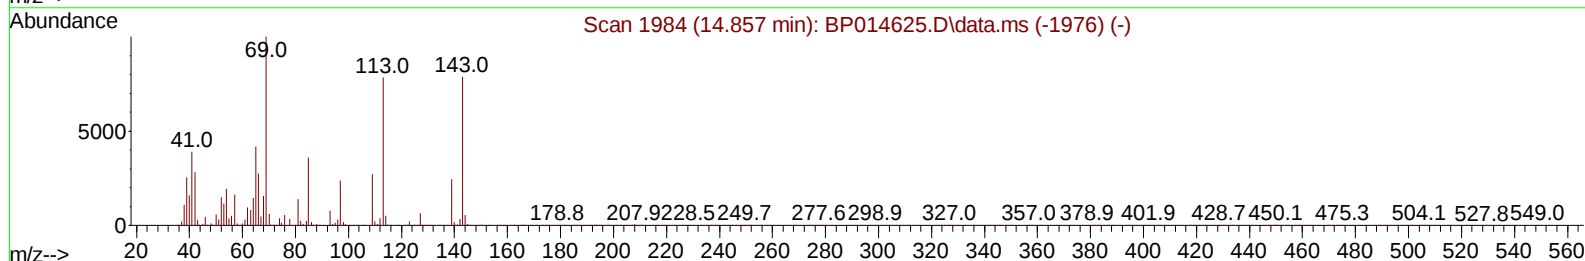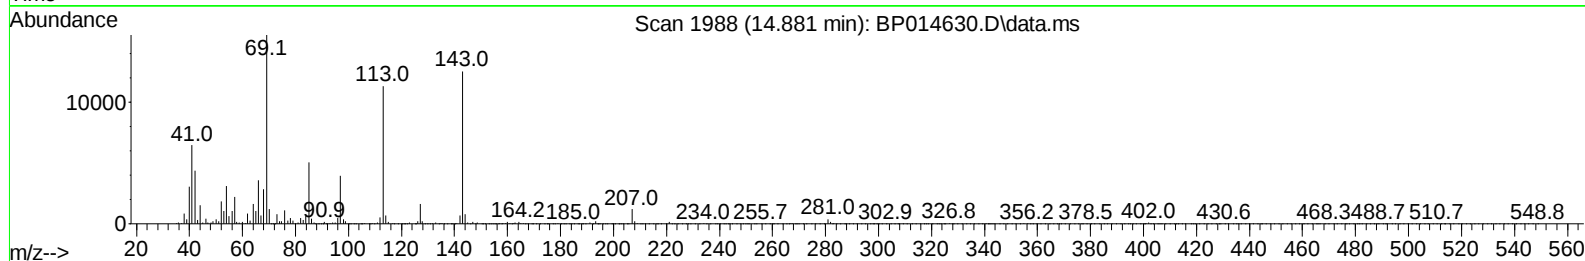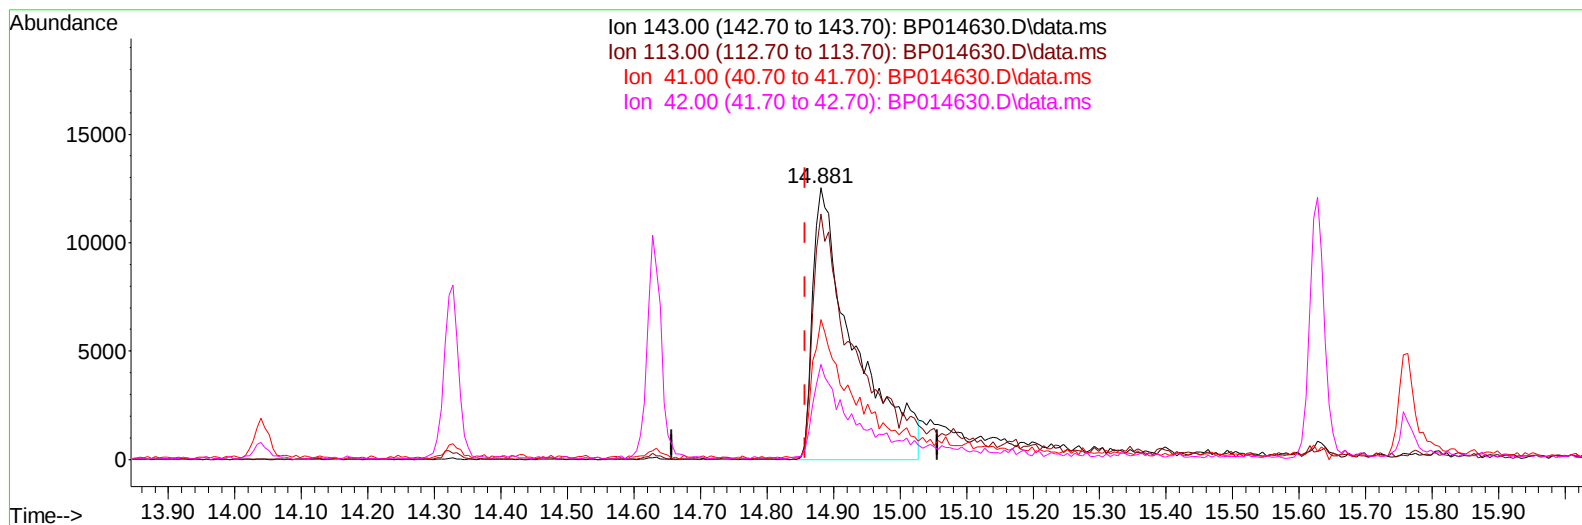

TIC: BP014630.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.881min (+ 0.024) 12.56 ng/ul m

response 53509

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	90.35
41.00	44.20	51.51
42.00	31.50	35.04

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
 Data File : BP014630.D
 Acq On : 10 Apr 2023 17:06
 Operator : CG/JU
 Sample : PB152000BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK000

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/11/2023
 Supervised By :Jagrut Upadhyay 04/11/2023

Quant Time: Apr 11 01:23:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 11 01:21:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.975	152	137039	20.000	ng/ul	0.00
20) Naphthalene-d8	10.798	136	589868	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.634	164	347923	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.392	188	655463	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.486	240	591334	20.000	ng/ul	0.00
88) Perylene-d12	23.992	264	711636	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	19432	5.499	ng/uL	0.00
4) Pyridine-d5	3.793	84	224897	24.834	ng/ul	0.00
7) Phenol-d5	7.146	99	295666	23.394	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.305	67	219358	27.052	ng/ul	0.00
11) 2-Chlorophenol-d4	7.510	132	228894	25.058	ng/ul	0.00
15) 4-Methylphenol-d8	8.699	113	235947	23.144	ng/ul	0.00
21) Nitrobenzene-d5	9.157	128	111134	23.338	ng/ul	0.00
24) 2-Nitrophenol-d4	9.881	143	128158	23.503	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.428	165	211557	21.304	ng/ul	0.00
31) 4-Chloroaniline-d4	10.951	131	277209	21.193	ng/ul	0.00
46) Dimethylphthalate-d6	14.039	166	673109	23.860	ng/ul	0.00
49) Acenaphthylene-d8	14.328	160	763576	24.394	ng/ul	0.00
54) 4-Nitrophenol-d4	14.881	143	53509m	12.555	ng/ul	0.02
60) Fluorene-d10	15.628	176	544872	23.161	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.763	200	85031	17.630	ng/ul	0.00
73) Anthracene-d10	17.492	188	787361	24.821	ng/ul	0.00
81) Pyrene-d10	19.727	212	872920	21.977	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.821	264	958804	25.359	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014630.D
Acq On : 10 Apr 2023 17:06
Operator : CG/JU
Sample : PB152000BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK000

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/11/2023
Supervised By :Jagrut Upadhyay 04/11/2023

Quant Time: Apr 11 01:23:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

