




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014649.D
Acq On : 11 Apr 2023 11:10
Operator : CG/JU
Sample : PB152026BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK026

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/12/2023
Supervised By :Jagrut Upadhyay 04/12/2023

Quant Time: Apr 11 23:00:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

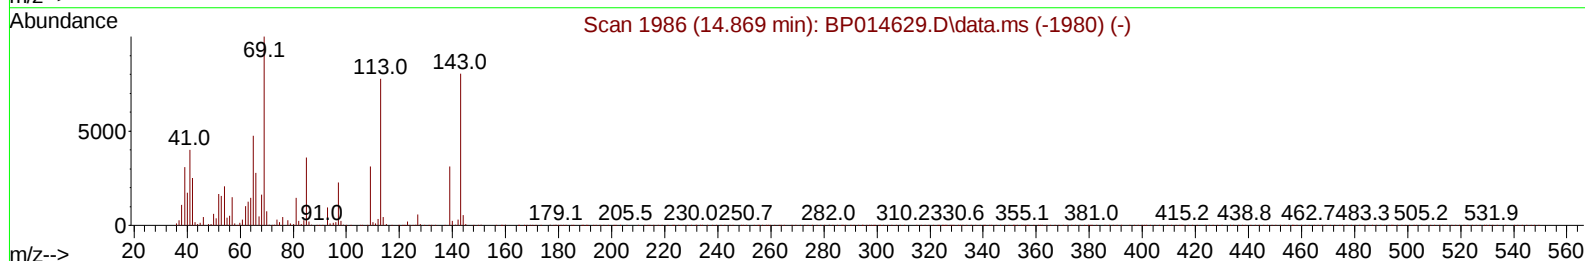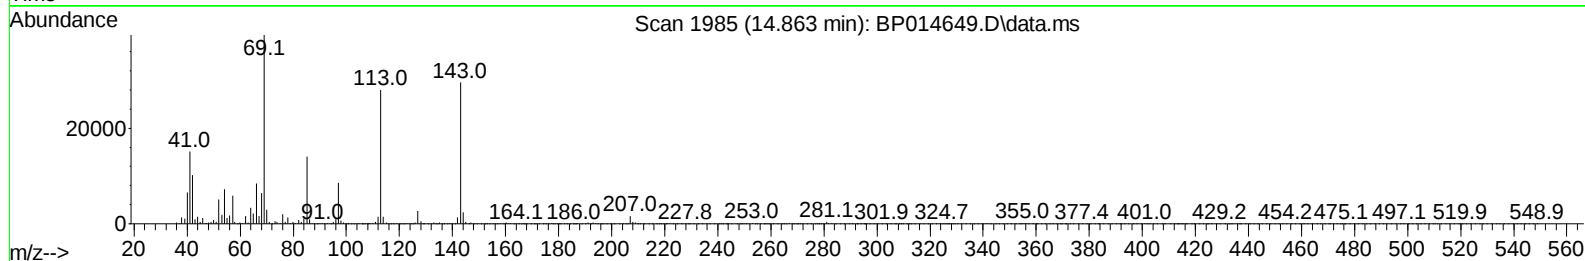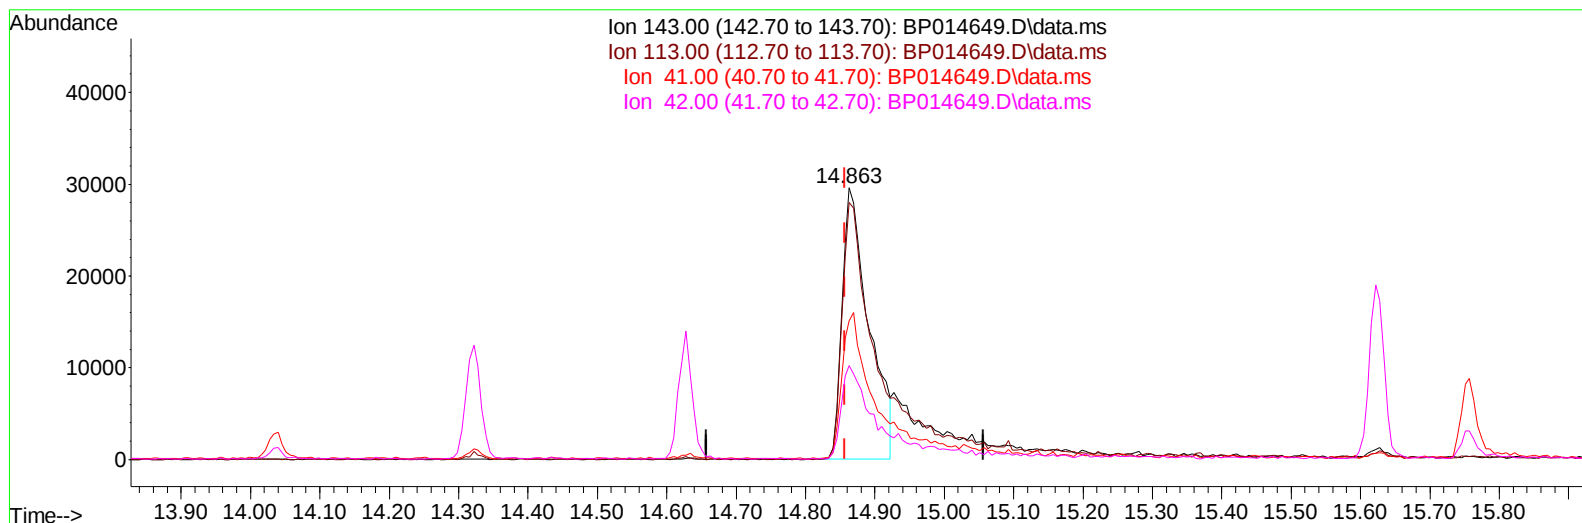

TIC: BP014649.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.863min (+ 0.006) 14.80 ng/u1

response 78854

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	94.70
41.00	44.20	51.08
42.00	31.50	34.60




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
 Data File : BP014649.D
 Acq On : 11 Apr 2023 11:10
 Operator : CG/JU
 Sample : PB152026BL
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK026

Manual IntegrationsAPPROVED

Quant Time: Apr 11 23:00:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 11 01:21:43 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/12/2023
 Supervised By :Jagrut Upadhyay 04/12/2023

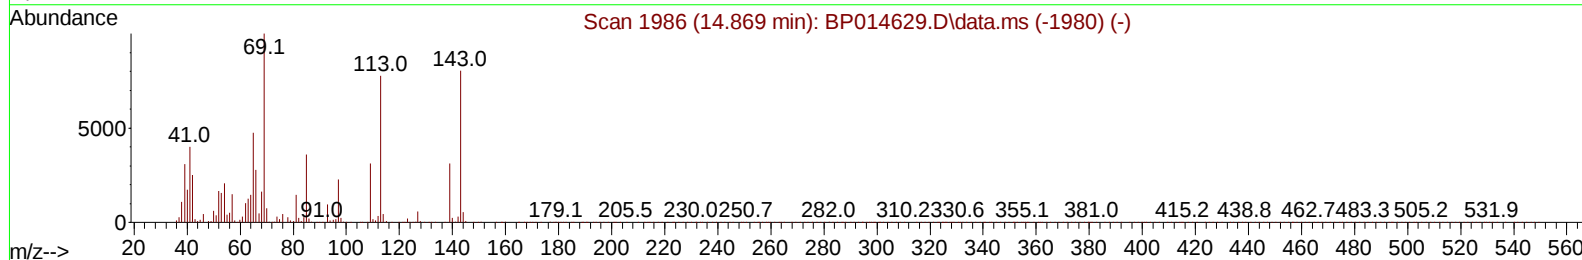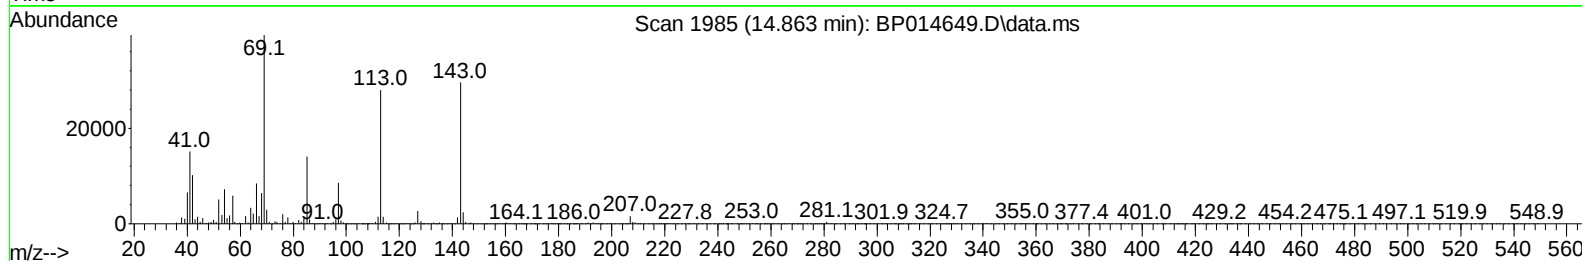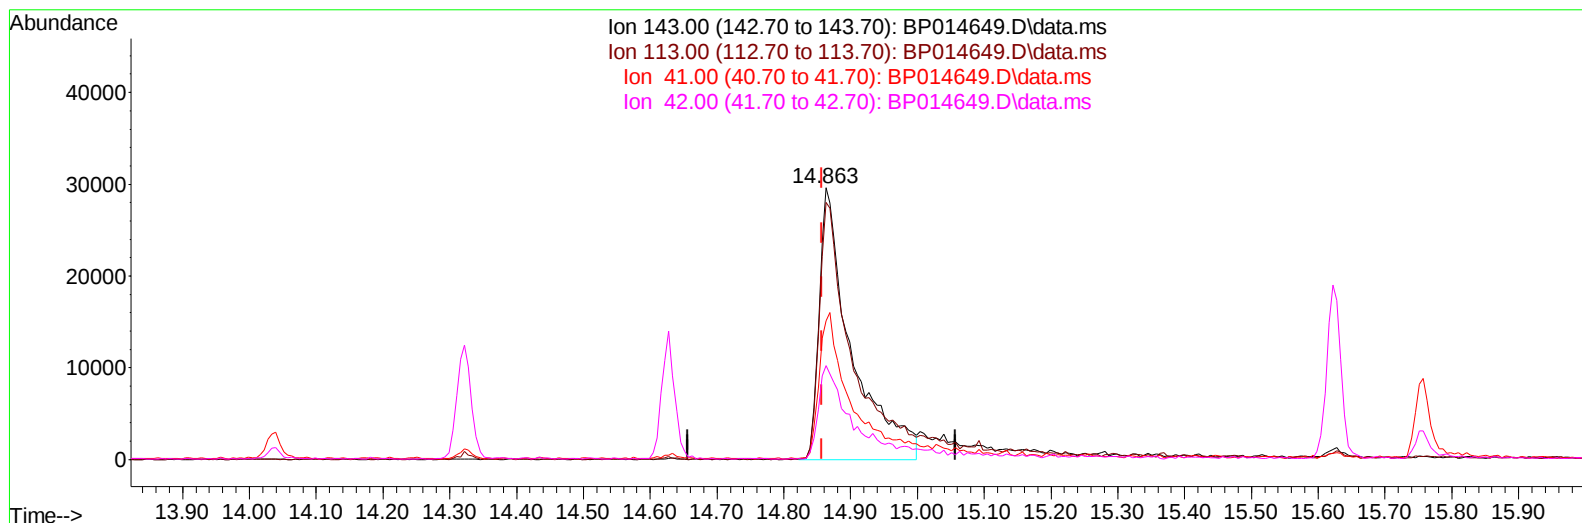

TIC: BP014649.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.863min (+ 0.006) 18.63 ng/ul m

response 99241

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	94.70
41.00	44.20	51.08
42.00	31.50	34.60

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
 Data File : BP014649.D
 Acq On : 11 Apr 2023 11:10
 Operator : CG/JU
 Sample : PB152026BL
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK026

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/12/2023
 Supervised By :Jagrut Upadhyay 04/12/2023

Quant Time: Apr 11 23:00:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 11 01:21:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.975	152	148343	20.000	ng/ul	0.00
20) Naphthalene-d8	10.793	136	673191	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.628	164	434960	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.392	188	921299	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	614808	20.000	ng/ul	0.00
88) Perylene-d12	23.986	264	702201	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	22497	5.881	ng/uL	0.00
4) Pyridine-d5	3.793	84	276258	28.181	ng/ul	0.00
7) Phenol-d5	7.140	99	375182	27.424	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.305	67	273520	31.161	ng/ul	0.00
11) 2-Chlorophenol-d4	7.505	132	291402	29.470	ng/ul	0.00
15) 4-Methylphenol-d8	8.693	113	310798	28.164	ng/ul	0.00
21) Nitrobenzene-d5	9.152	128	147851	27.206	ng/ul	0.00
24) 2-Nitrophenol-d4	9.881	143	168940	27.148	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.422	165	278472	24.571	ng/ul	0.00
31) 4-Chloroaniline-d4	10.946	131	433561	29.043	ng/ul	0.00
46) Dimethylphthalate-d6	14.040	166	1027036	29.121	ng/ul	0.00
49) Acenaphthylene-d8	14.322	160	1112192	28.421	ng/ul	0.00
54) 4-Nitrophenol-d4	14.863	143	99241m	18.627	ng/ul	0.00
60) Fluorene-d10	15.622	176	852194	28.976	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	146836	21.660	ng/ul	0.00
73) Anthracene-d10	17.492	188	1329692	29.823	ng/ul	0.00
81) Pyrene-d10	19.722	212	1344728	32.563	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.816	264	1154910	30.956	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014649.D
Acq On : 11 Apr 2023 11:10
Operator : CG/JU
Sample : PB152026BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK026

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/12/2023
Supervised By :Jagrut Upadhyay 04/12/2023

Quant Time: Apr 11 23:00:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

