




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014653.D
Acq On : 11 Apr 2023 13:26
Operator : CG/JU
Sample : 02251-02
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMC0

Manual IntegrationsAPPROVED

Quant Time: Apr 11 23:01:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/12/2023
Supervised By :Jagrut Upadhyay 04/12/2023

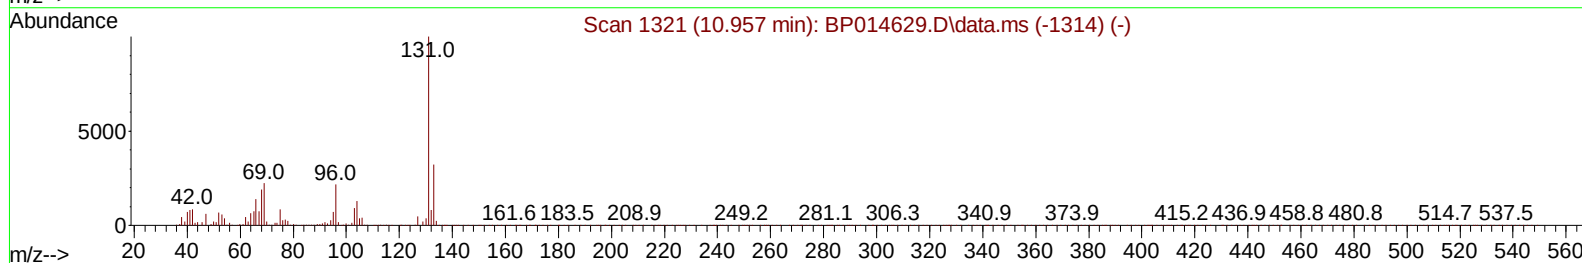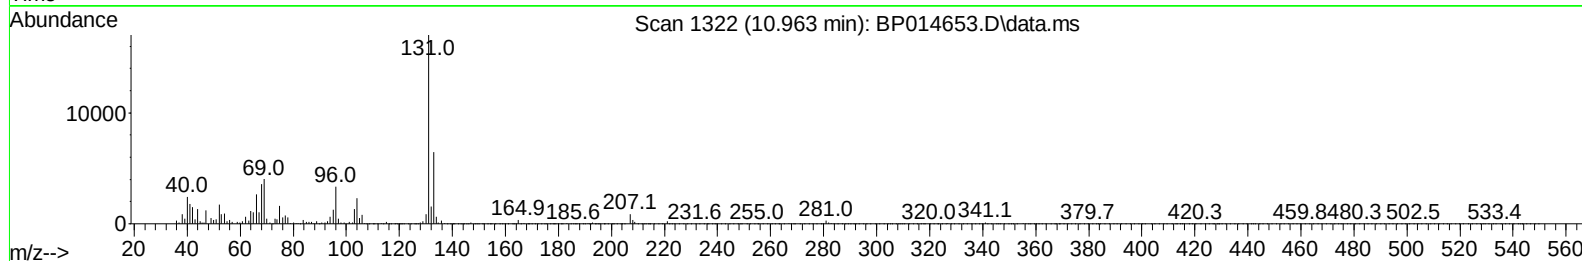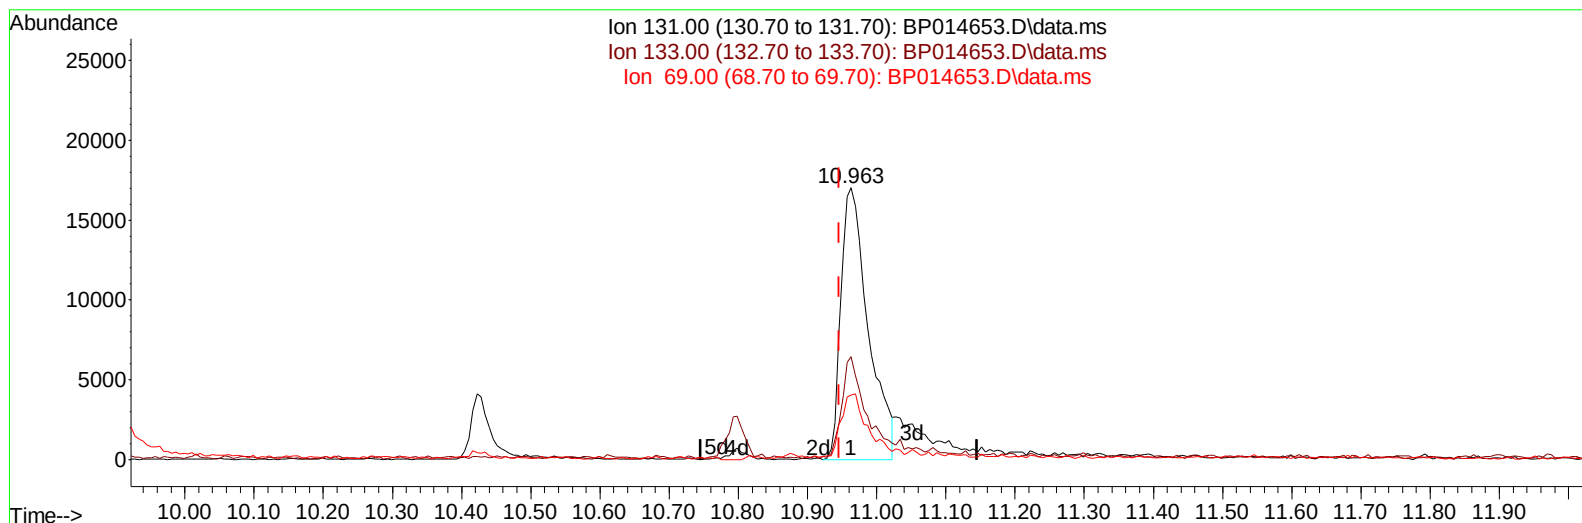

TIC: BP014653.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.963min (+ 0.018) 3.87 ng/u1

response 46608

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	37.83
69.00	21.30	23.65
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
 Data File : BP014653.D
 Acq On : 11 Apr 2023 13:26
 Operator : CG/JU
 Sample : 02251-02
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COMC0

Manual IntegrationsAPPROVED

Quant Time: Apr 11 23:01:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 11 01:21:43 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/12/2023
 Supervised By :Jagrut Upadhyay 04/12/2023

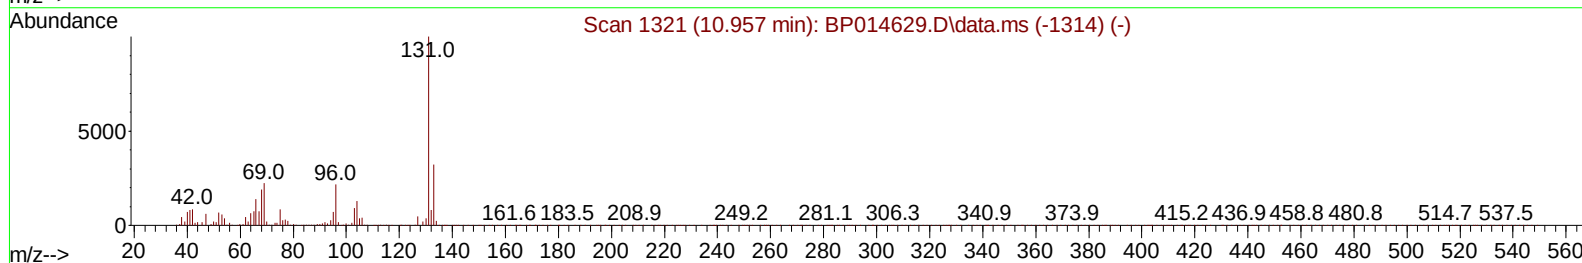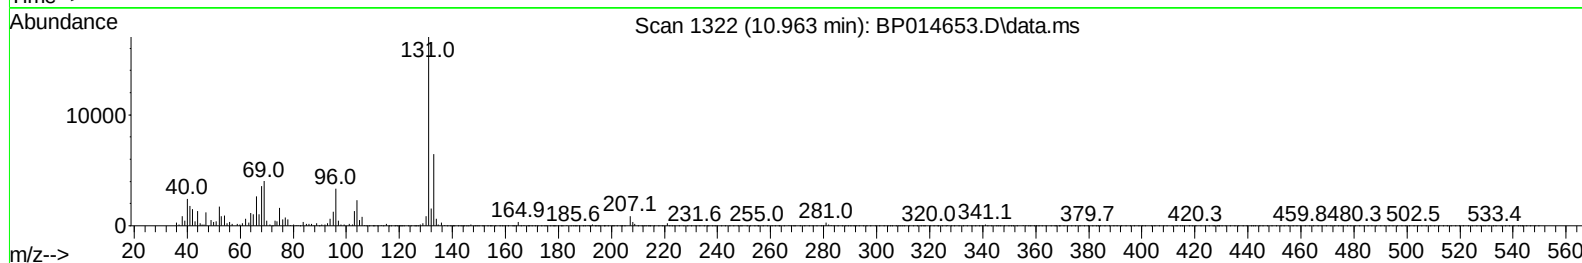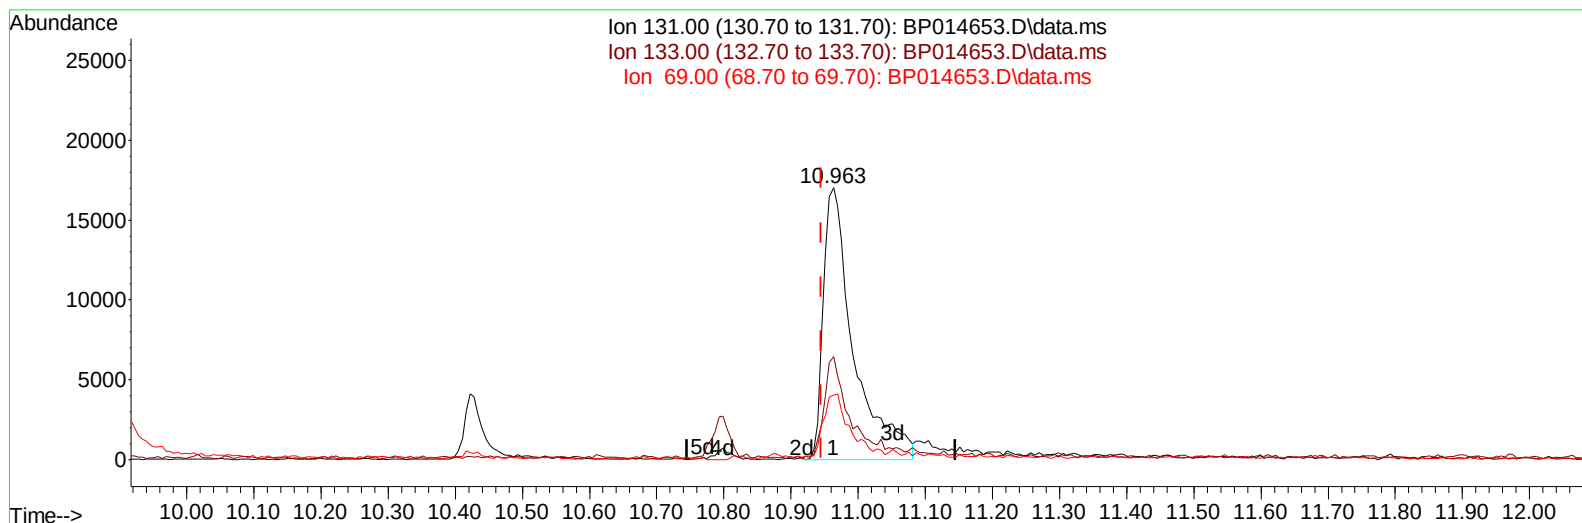

TIC: BP014653.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.963min (+ 0.018) 4.42 ng/ul m

response 53290

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	37.83
69.00	21.30	23.65
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014653.D
Acq On : 11 Apr 2023 13:26
Operator : CG/JU
Sample : 02251-02
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMCO

Manual IntegrationsAPPROVED

Quant Time: Apr 11 23:01:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/12/2023
Supervised By :Jagrut Upadhyay 04/12/2023

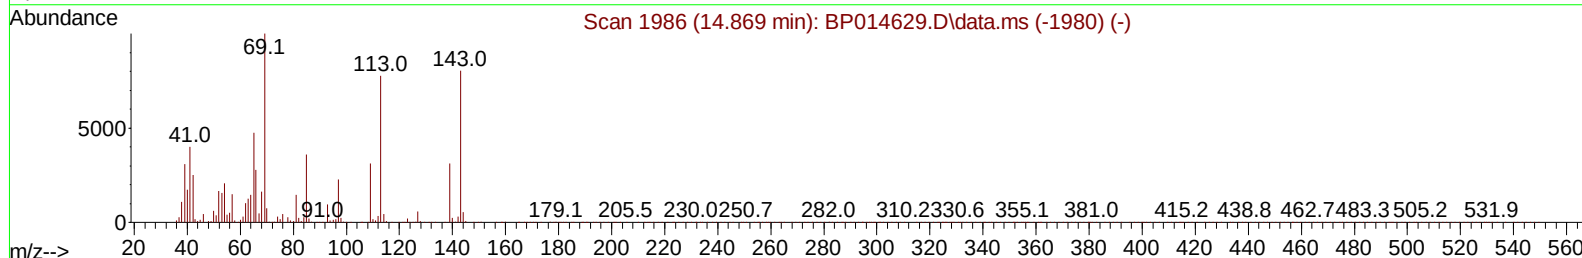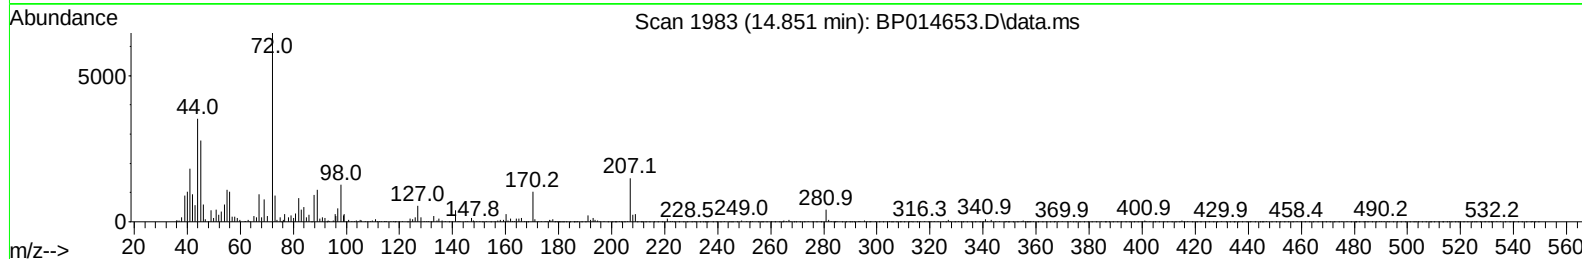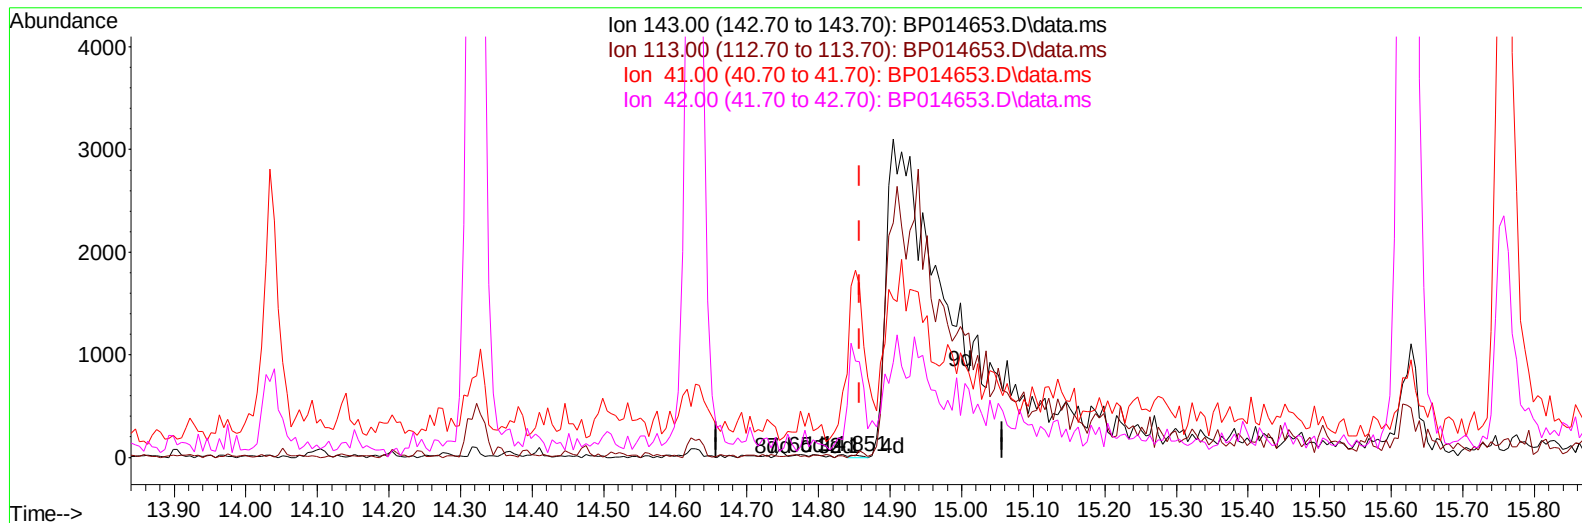

TIC: BP014653.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.851min (-0.006) 0.00 ng/u1

response 20

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	89.47
41.00	44.20	9615.79#
42.00	31.50	4936.84#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014653.D
Acq On : 11 Apr 2023 13:26
Operator : CG/JU
Sample : 02251-02
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMCO

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/12/2023
Supervised By :Jagrut Upadhyay 04/12/2023

Quant Time: Apr 11 23:01:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

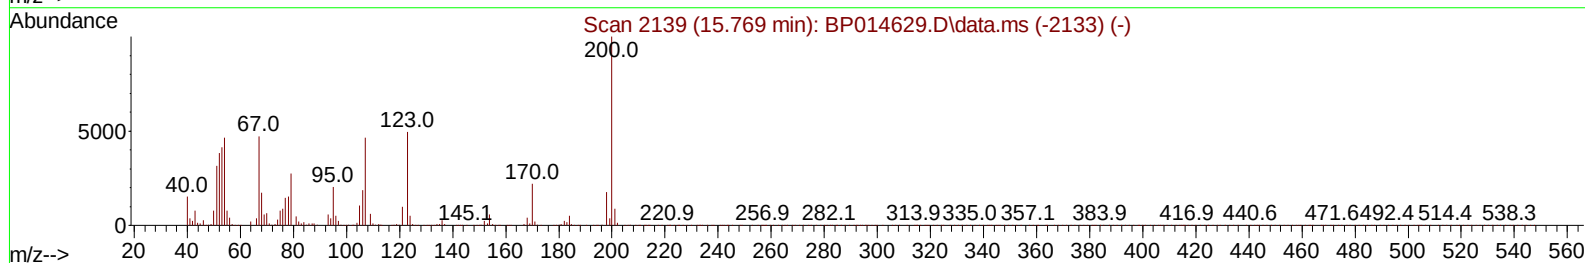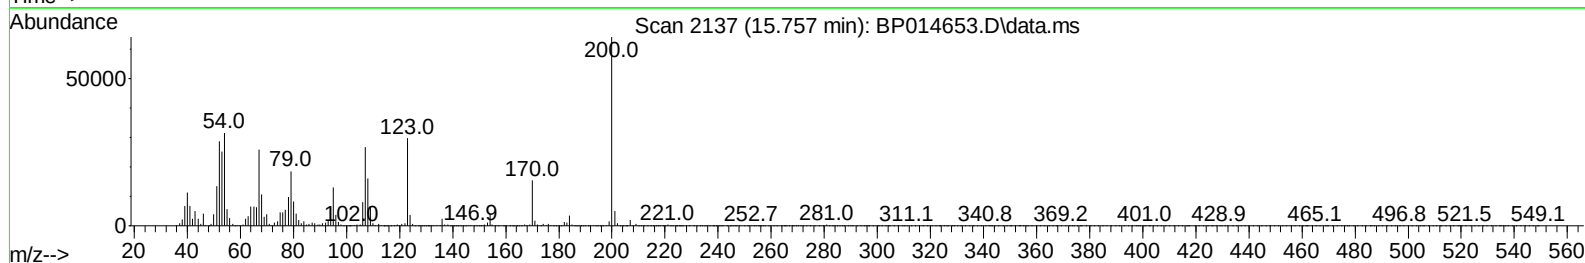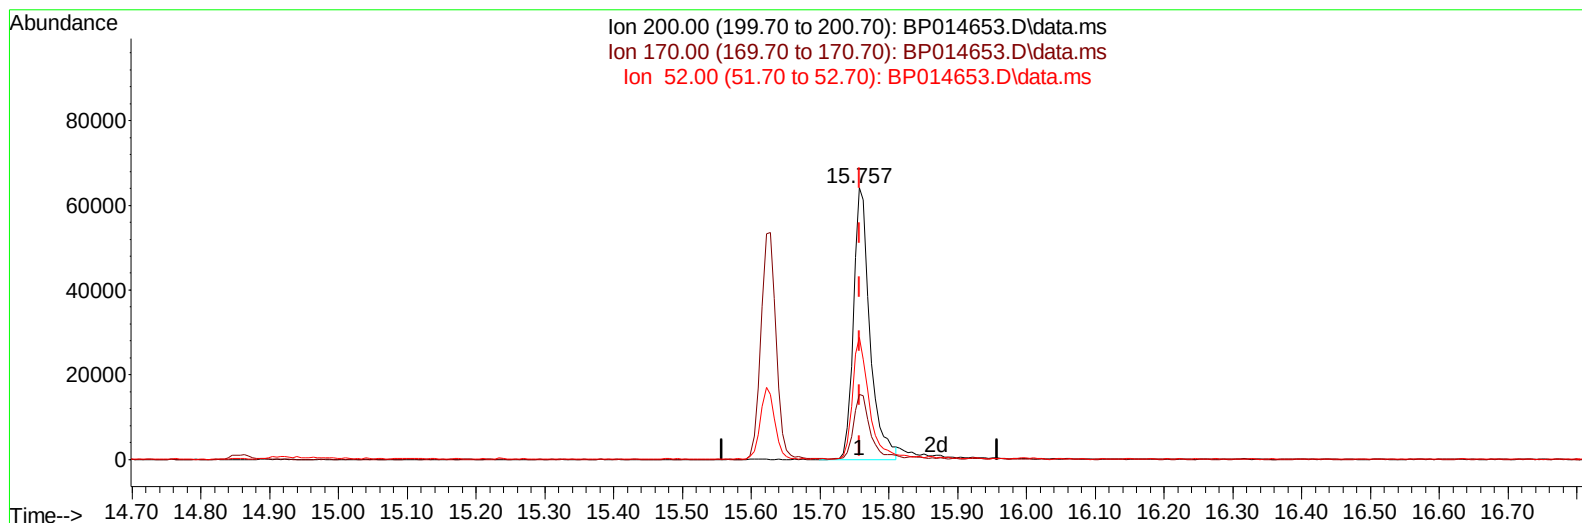

TIC: BP014653.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.757min (+ 0.000) 22.85 ng/ul

response 107162

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	22.10	23.97
52.00	45.50	44.87
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014653.D
Acq On : 11 Apr 2023 13:26
Operator : CG/JU
Sample : 02251-02
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMC0

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/12/2023
Supervised By :Jagrut Upadhyay 04/12/2023

Quant Time: Apr 11 23:01:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

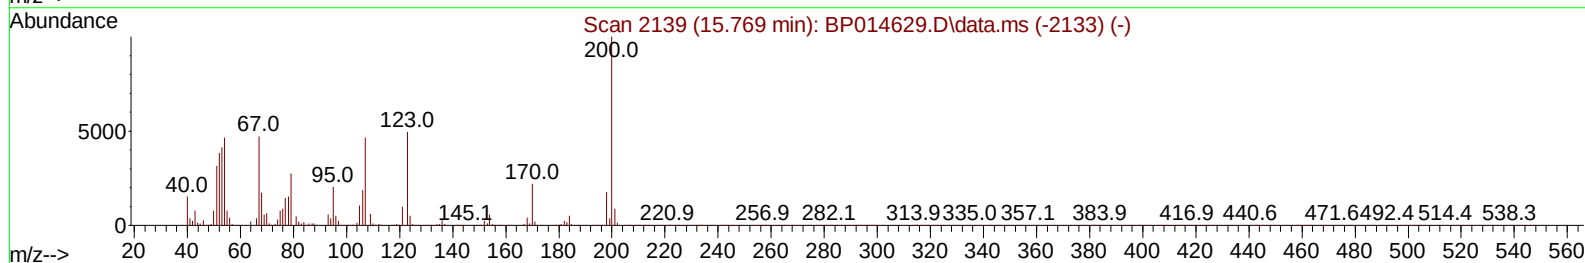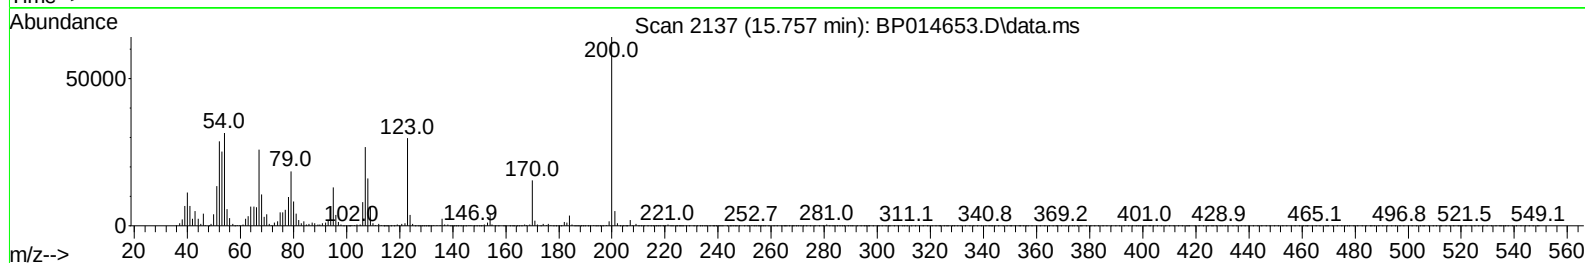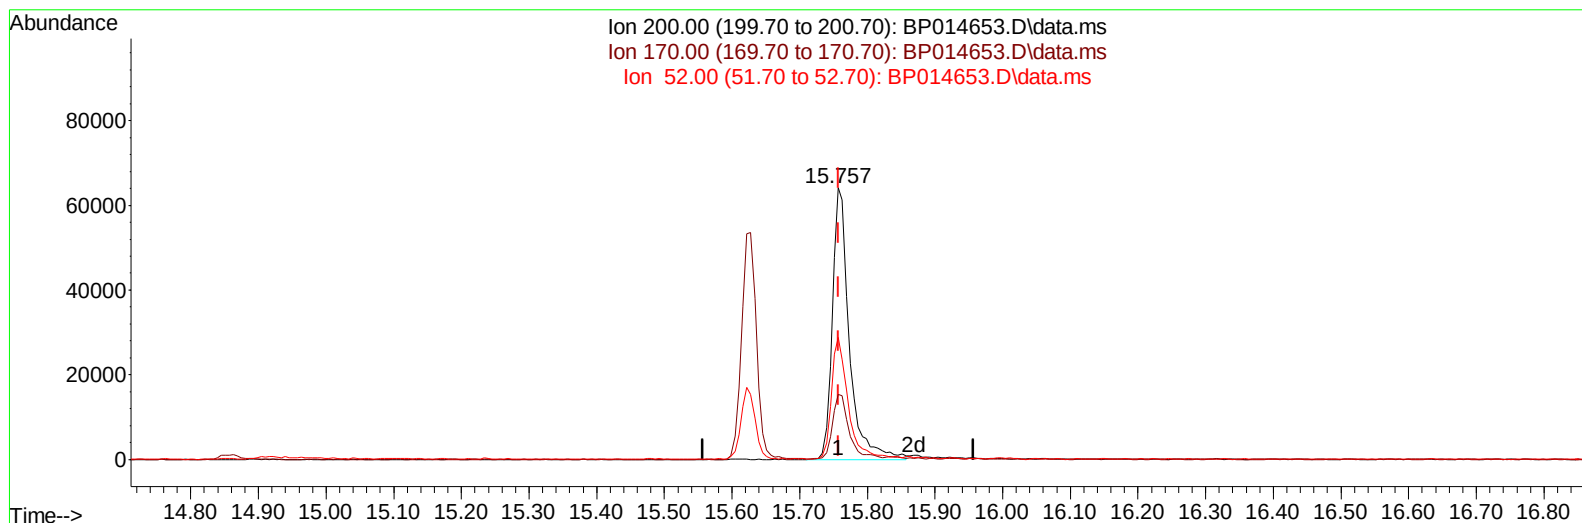

TIC: BP014653.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.757min (+ 0.000) 23.79 ng/ul m

response 111560

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	22.10	23.97
52.00	45.50	44.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
 Data File : BP014653.D
 Acq On : 11 Apr 2023 13:26
 Operator : CG/JU
 Sample : 02251-02
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COMCO

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/12/2023
 Supervised By :Jagrut Upadhyay 04/12/2023

Quant Time: Apr 11 23:01:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 11 01:21:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.975	152	125920	20.000	ng/ul	0.00
20) Naphthalene-d8	10.793	136	543732	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.628	164	329639	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.392	188	637345	20.000	ng/ul	0.00
79) Chrysene-d12	21.486	240	531053	20.000	ng/ul	0.00
88) Perylene-d12	23.986	264	654603	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	16035	4.938	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.152	99	85128	7.330	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.305	67	233447	31.331	ng/ul	0.00
11) 2-Chlorophenol-d4	7.505	132	206995	24.661	ng/ul	0.00
15) 4-Methylphenol-d8	8.699	113	151398	16.162	ng/ul	0.00
21) Nitrobenzene-d5	9.152	128	120368	27.422	ng/ul	0.00
24) 2-Nitrophenol-d4	9.881	143	139696	27.793	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.428	165	215181	23.507	ng/ul	0.00
31) 4-Chloroaniline-d4	10.963	131	53290m	4.420	ng/ul	0.02
46) Dimethylphthalate-d6	14.040	166	806535	30.176	ng/ul	0.00
49) Acenaphthylene-d8	14.322	160	883948	29.806	ng/ul	0.00
54) 4-Nitrophenol-d4	14.904	143	19671m	4.872	ng/ul	0.05
60) Fluorene-d10	15.622	176	664362	29.807	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	111560m	23.788	ng/ul	0.00
73) Anthracene-d10	17.492	188	1054889	34.200	ng/ul	0.00
81) Pyrene-d10	19.722	212	1133929	31.789	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.821	264	1211504	34.835	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014653.D
Acq On : 11 Apr 2023 13:26
Operator : CG/JU
Sample : 02251-02
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMC0

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/12/2023
Supervised By :Jagrut Upadhyay 04/12/2023

Quant Time: Apr 11 23:01:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

