




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014655.D
Acq On : 11 Apr 2023 14:35
Operator : CG/JU
Sample : 02251-04
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMC2

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/12/2023
Supervised By :Jagrut Upadhyay 04/12/2023

Quant Time: Apr 11 23:01:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

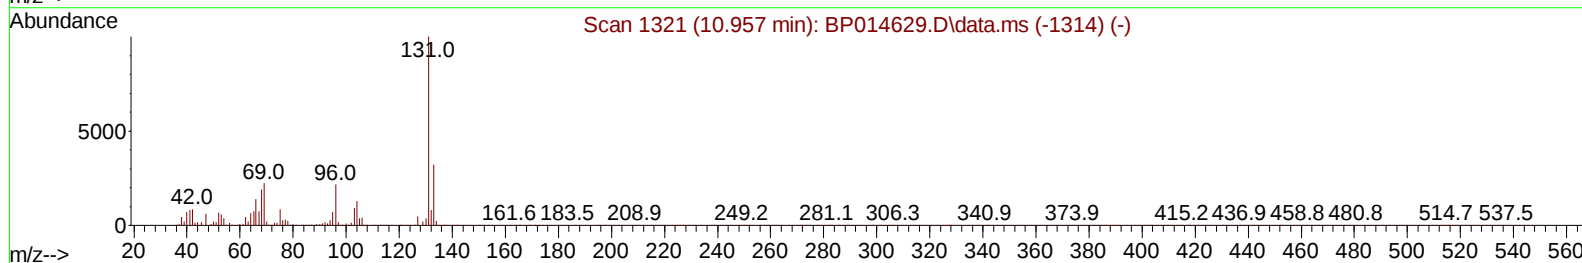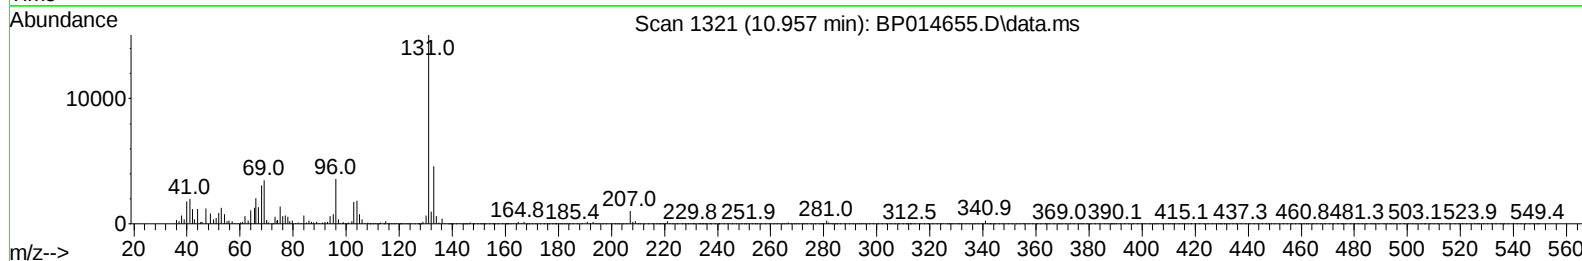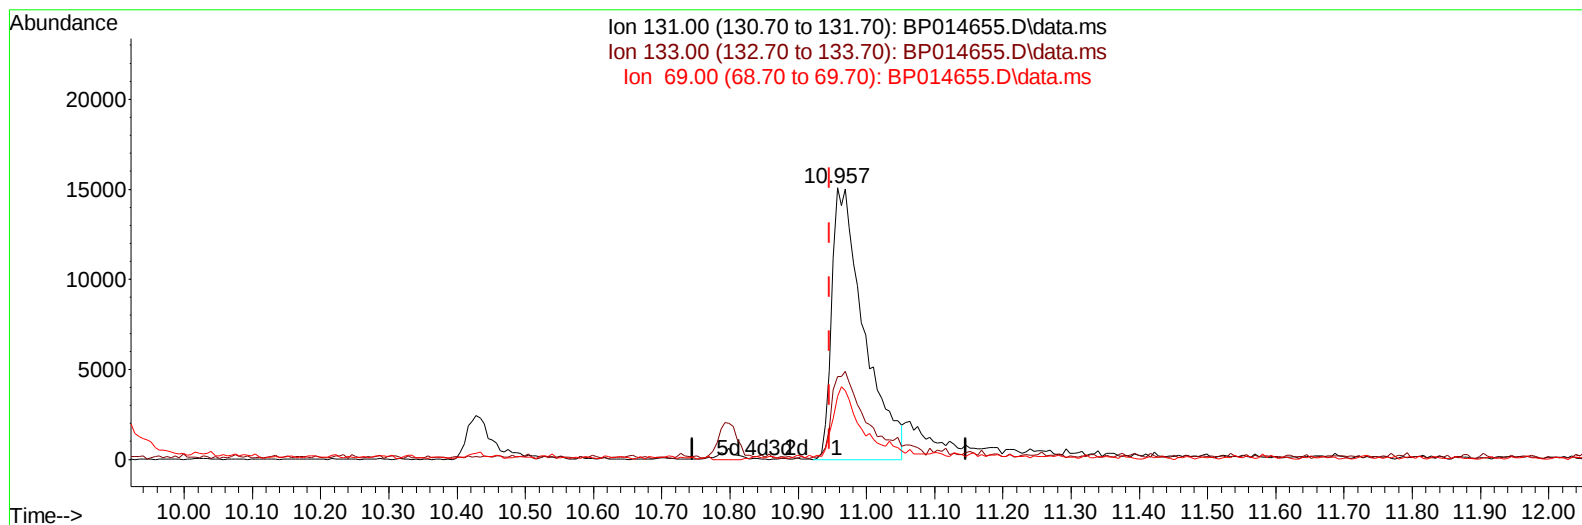

TIC: BP014655.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.957min (+ 0.012) 4.69 ng/u1

response 49268

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	30.64
69.00	21.30	23.19
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014655.D
Acq On : 11 Apr 2023 14:35
Operator : CG/JU
Sample : 02251-04
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMC2

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/12/2023
Supervised By :Jagrut Upadhyay 04/12/2023

Quant Time: Apr 11 23:01:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

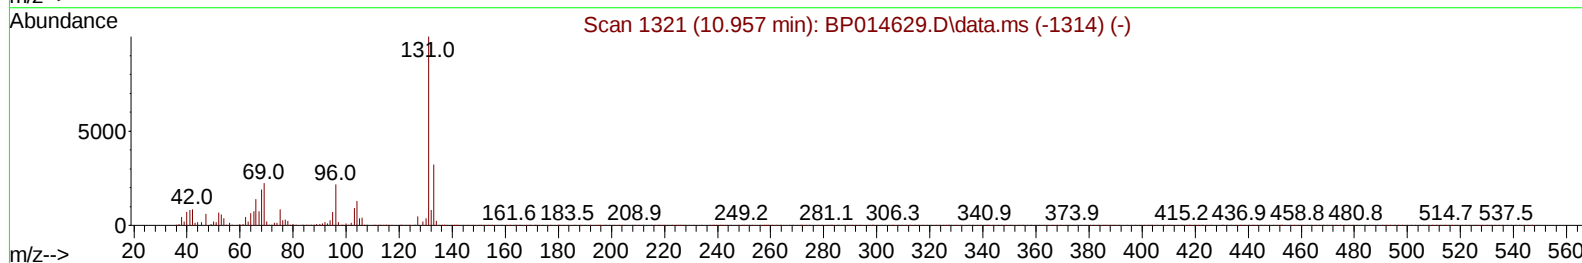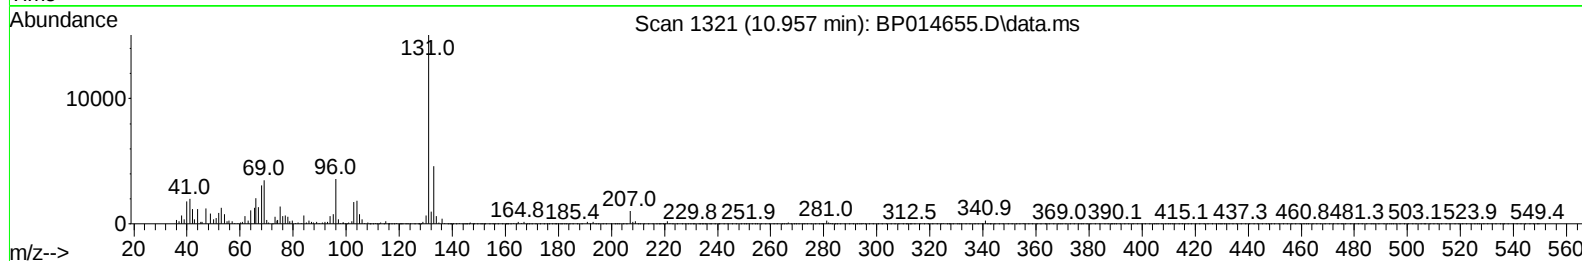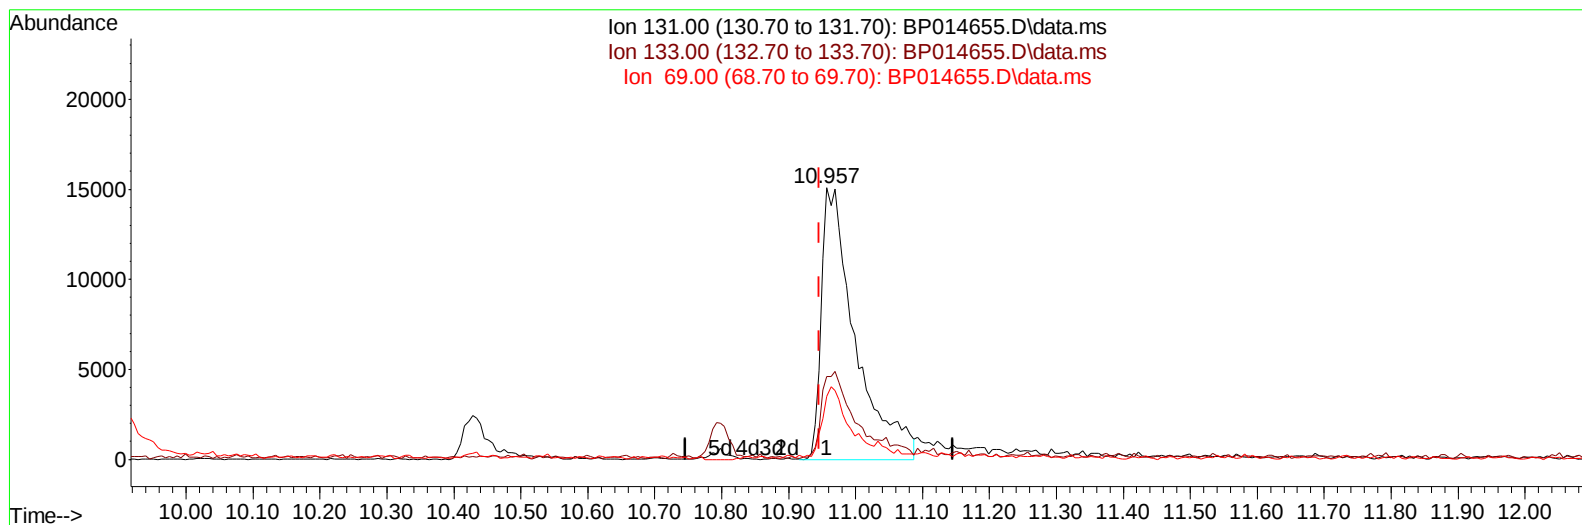

TIC: BP014655.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.957min (+ 0.012) 5.04 ng/ul m

response 52852

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	30.64
69.00	21.30	23.19
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
 Data File : BP014655.D
 Acq On : 11 Apr 2023 14:35
 Operator : CG/JU
 Sample : 02251-04
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COMC2

Manual IntegrationsAPPROVED

Quant Time: Apr 11 23:01:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 11 01:21:43 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/12/2023
 Supervised By :Jagrut Upadhyay 04/12/2023

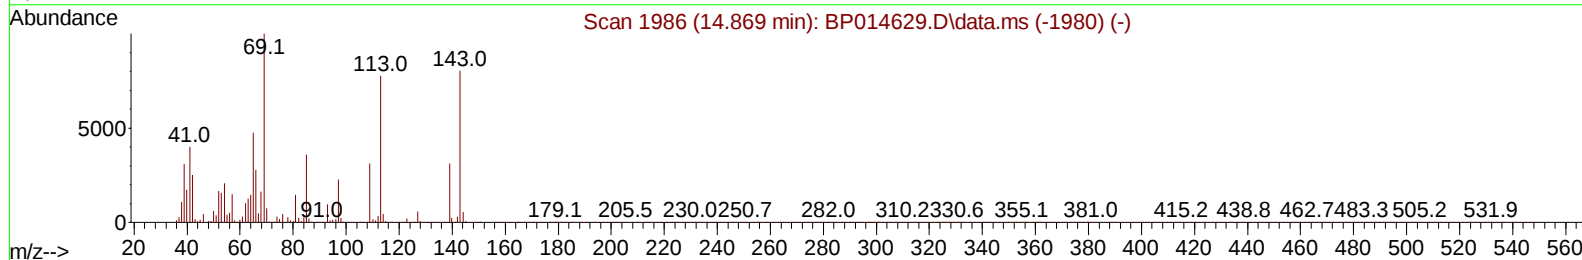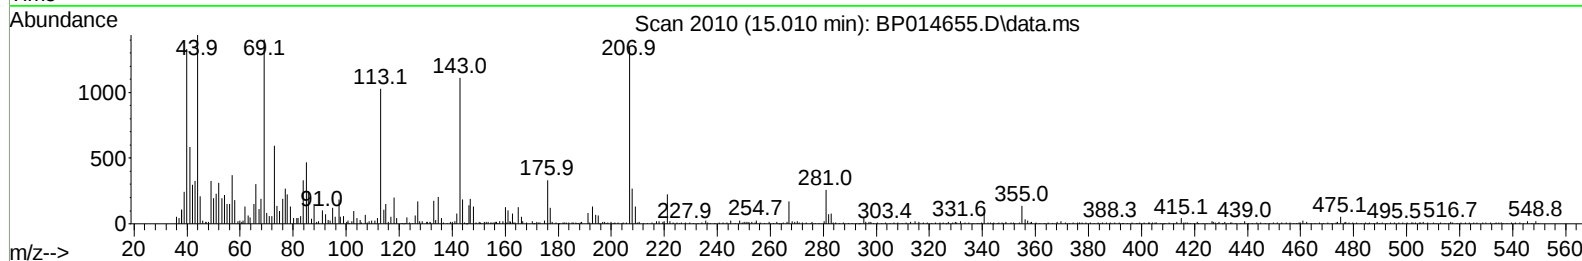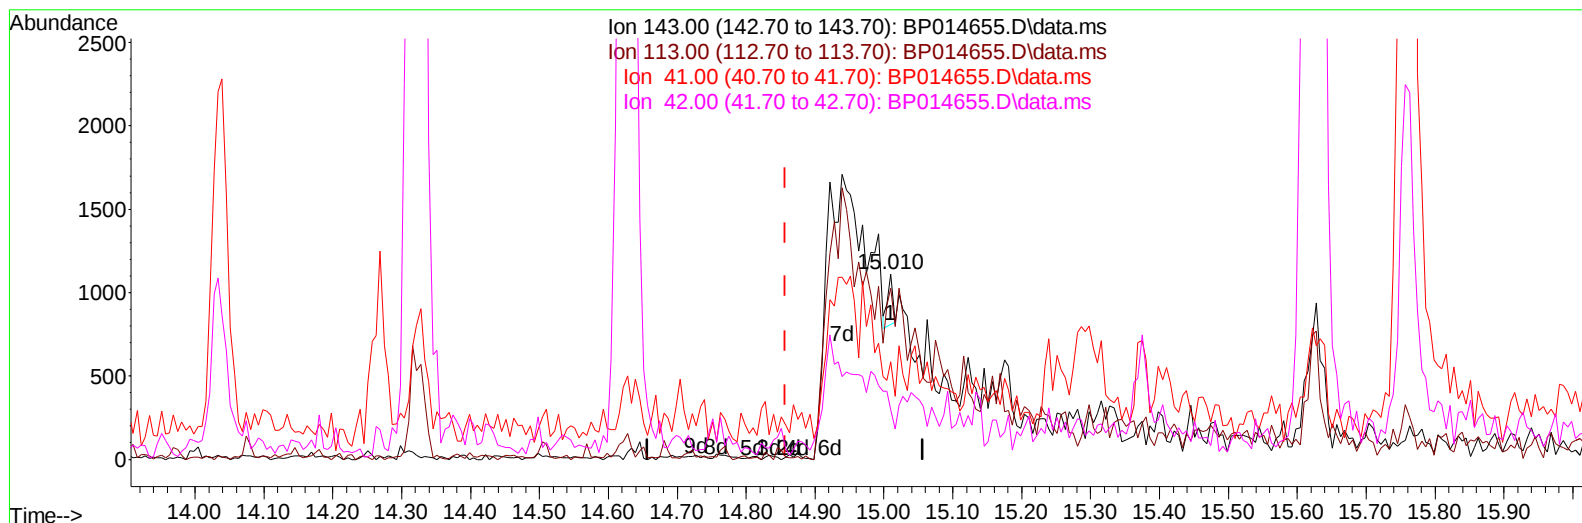

TIC: BP014655.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.010min (+ 0.153) 0.04 ng/u1

response 160

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	92.53
41.00	44.20	52.75
42.00	31.50	26.91




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014655.D
Acq On : 11 Apr 2023 14:35
Operator : CG/JU
Sample : 02251-04
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMC2

Manual IntegrationsAPPROVED

Quant Time: Apr 11 23:01:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/12/2023
Supervised By :Jagrut Upadhyay 04/12/2023

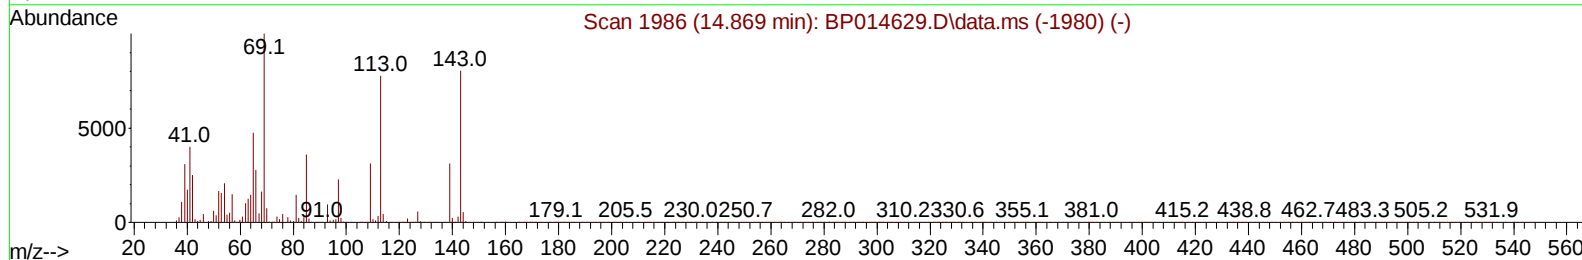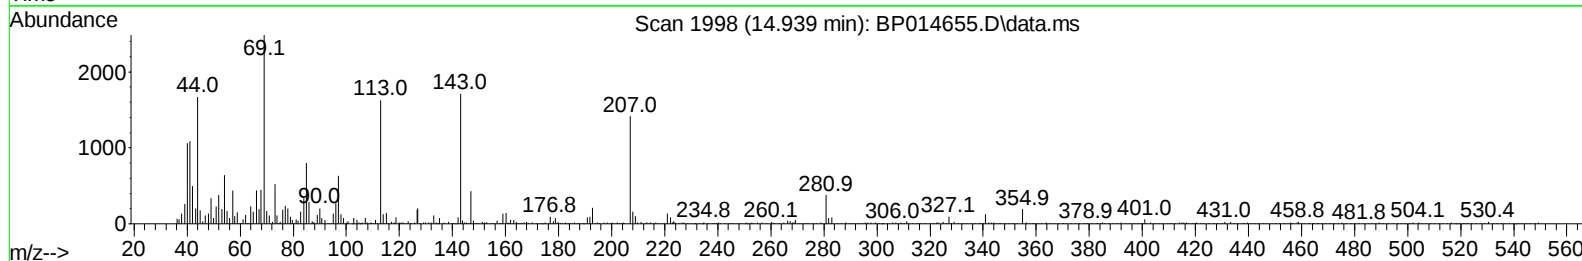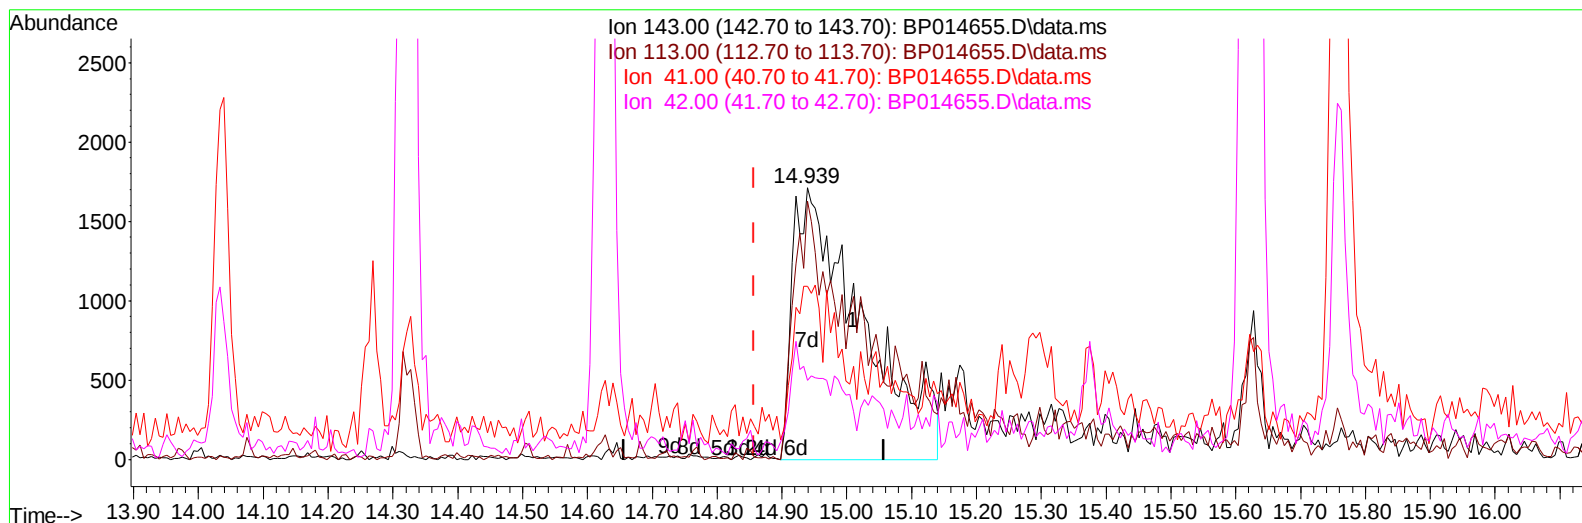

TIC: BP014655.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.939min (+ 0.082) 3.44 ng/ul m

response 12601

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	95.15
41.00	44.20	63.76#
42.00	31.50	29.11

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
 Data File : BP014655.D
 Acq On : 11 Apr 2023 14:35
 Operator : CG/JU
 Sample : 02251-04
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COMC2

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/12/2023
 Supervised By :Jagrut Upadhyay 04/12/2023

Quant Time: Apr 11 23:01:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 11 01:21:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.975	152	113752	20.000	ng/ul	0.00
20) Naphthalene-d8	10.793	136	473327	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.628	164	298634	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.392	188	677549	20.000	ng/ul	0.00
79) Chrysene-d12	21.486	240	694961	20.000	ng/ul	0.00
88) Perylene-d12	23.986	264	785002	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	14503	4.944	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.152	99	51751	4.933	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.305	67	226584	33.663	ng/ul	0.00
11) 2-Chlorophenol-d4	7.505	132	158470	20.900	ng/ul	0.00
15) 4-Methylphenol-d8	8.699	113	99718	11.784	ng/ul	0.00
21) Nitrobenzene-d5	9.157	128	115708	30.281	ng/ul	0.00
24) 2-Nitrophenol-d4	9.881	143	109427	25.009	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.428	165	172536	21.652	ng/ul	0.00
31) 4-Chloroaniline-d4	10.957	131	52852m	5.035	ng/ul	0.01
46) Dimethylphthalate-d6	14.039	166	846901	34.976	ng/ul	0.00
49) Acenaphthylene-d8	14.322	160	919948	34.240	ng/ul	0.00
54) 4-Nitrophenol-d4	14.939	143	12601m	3.445	ng/ul	0.08
60) Fluorene-d10	15.622	176	731386	36.221	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	108513	21.766	ng/ul	0.00
73) Anthracene-d10	17.492	188	1237504	37.740	ng/ul	0.00
81) Pyrene-d10	19.722	212	1577778	33.800	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.821	264	1608176	38.559	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014655.D
Acq On : 11 Apr 2023 14:35
Operator : CG/JU
Sample : 02251-04
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0MC2

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/12/2023
Supervised By :Jagrut Upadhyay 04/12/2023

Quant Time: Apr 11 23:01:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

