




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014656.D
Acq On : 11 Apr 2023 15:09
Operator : CG/JU
Sample : 02251-05
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMC3

Manual IntegrationsAPPROVED

Quant Time: Apr 11 23:01:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/12/2023
Supervised By :Jagrut Upadhyay 04/12/2023

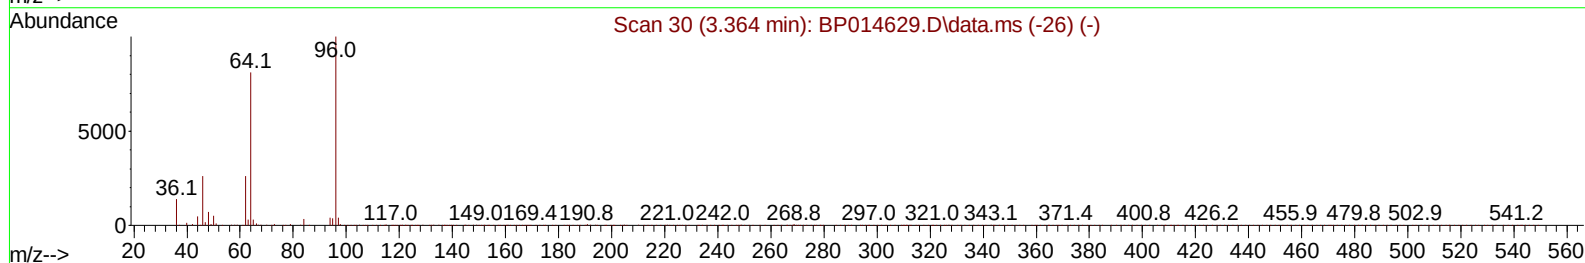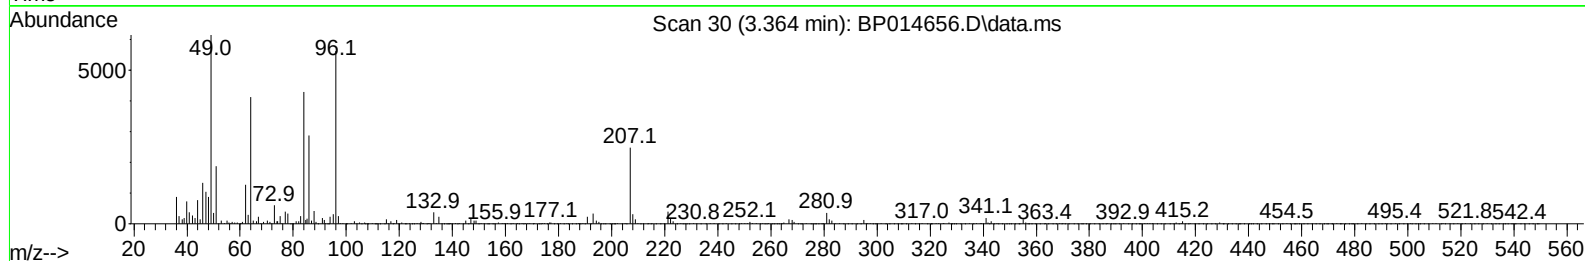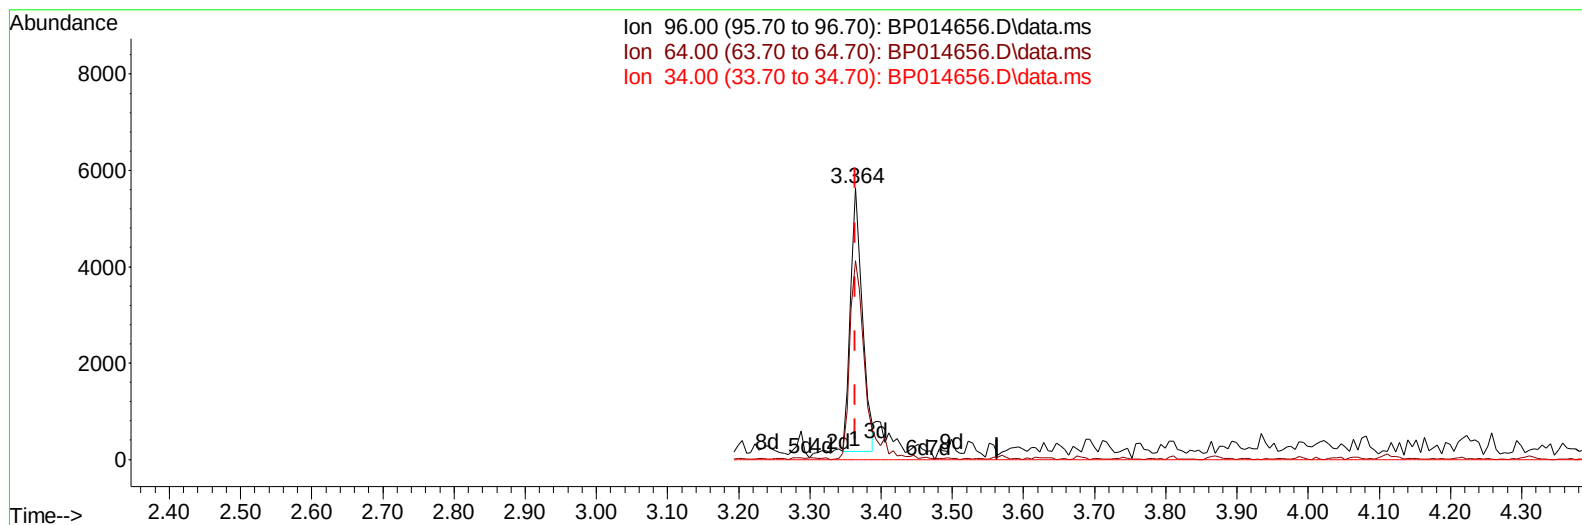

TIC: BP014656.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.364min (+ 0.000) 1.85 ng/uL

response 6419

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	75.70	73.16
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014656.D
Acq On : 11 Apr 2023 15:09
Operator : CG/JU
Sample : 02251-05
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMC3

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/12/2023
Supervised By :Jagrut Upadhyay 04/12/2023

Quant Time: Apr 11 23:01:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

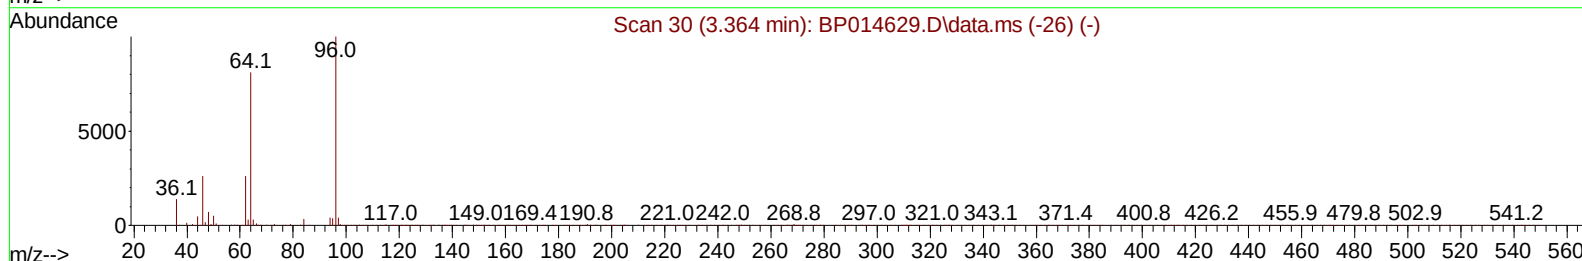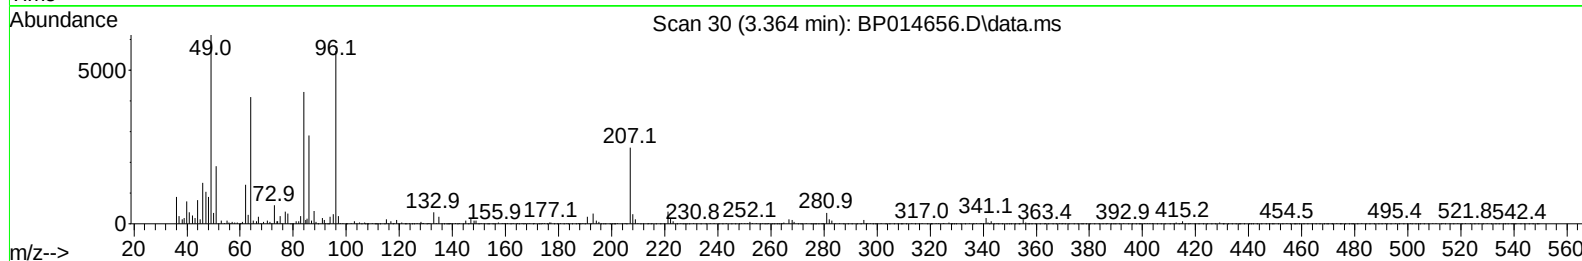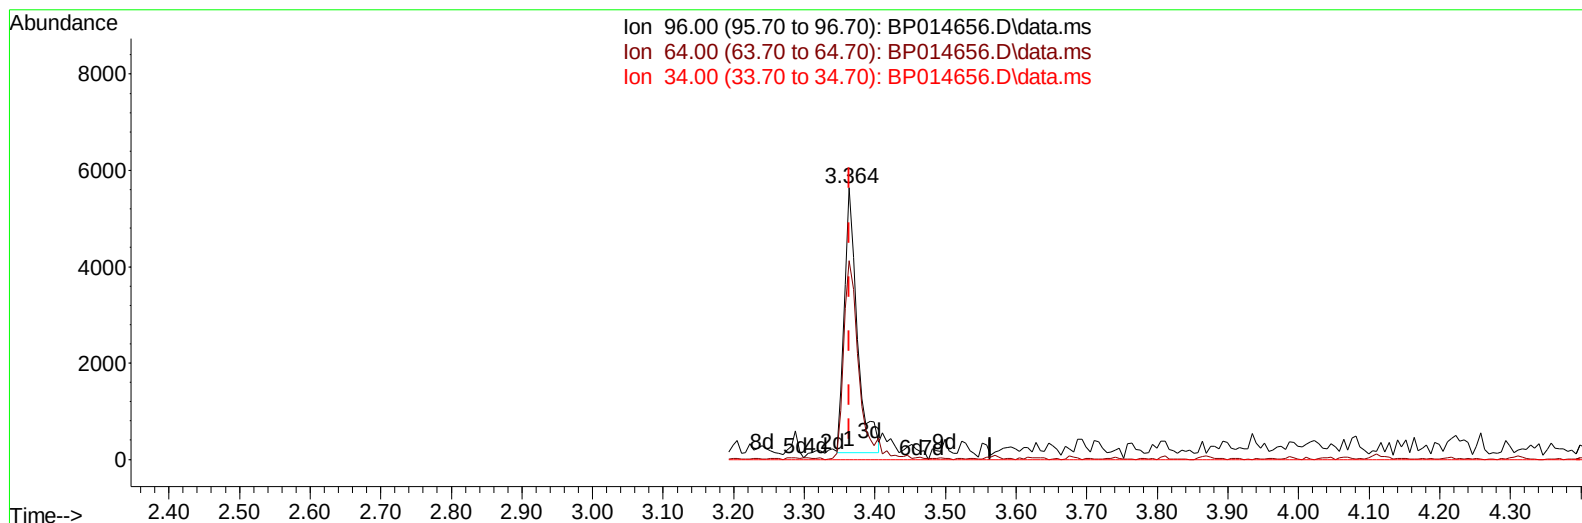

TIC: BP014656.D\data.ms

(3) 1,4-Dioxane-d8 (S)**3.364min (+ 0.000) 2.02 ng/uL m****response 7004**

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	75.70	73.16
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014656.D
Acq On : 11 Apr 2023 15:09
Operator : CG/JU
Sample : 02251-05
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMC3

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/12/2023
Supervised By :Jagrut Upadhyay 04/12/2023

Quant Time: Apr 11 23:01:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

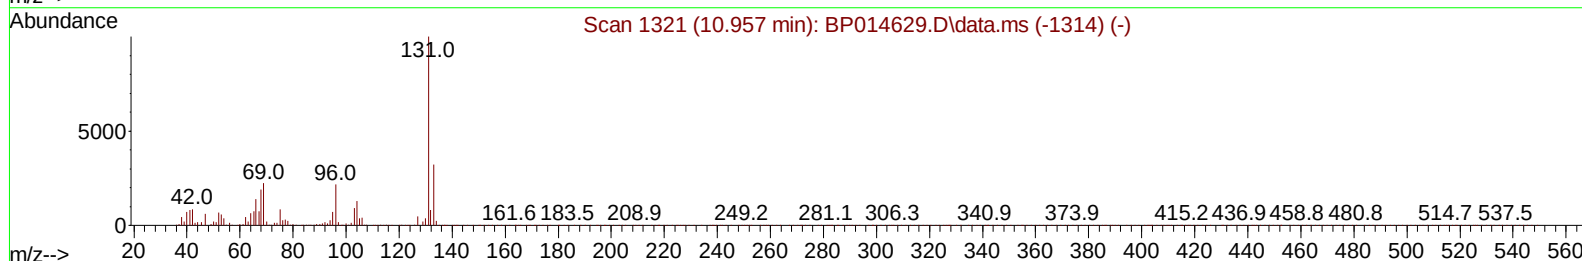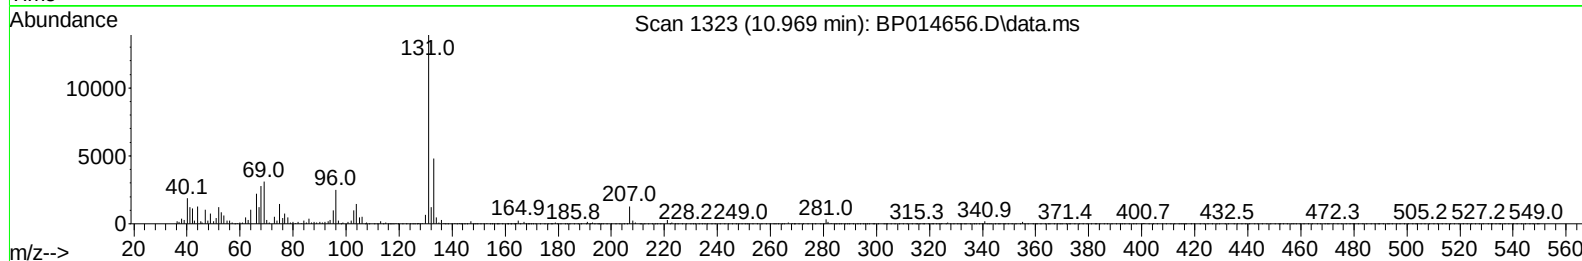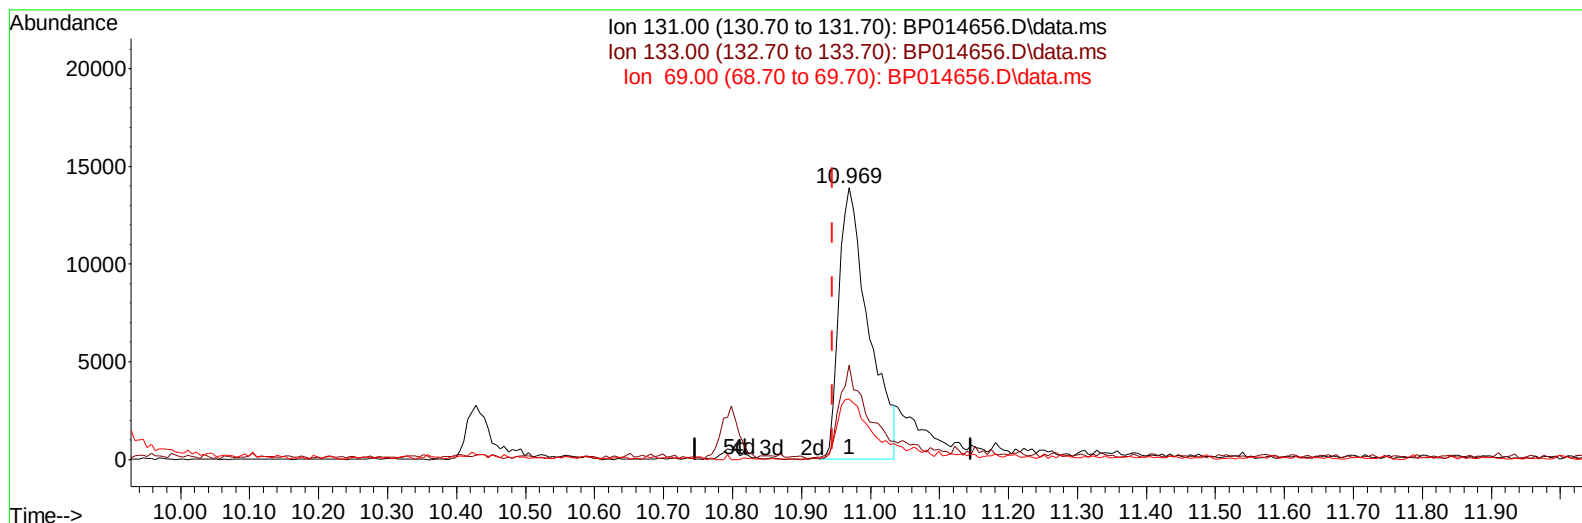

TIC: BP014656.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.969min (+ 0.024) 3.25 ng/u1

response 41195

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	34.75
69.00	21.30	22.26
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014656.D
Acq On : 11 Apr 2023 15:09
Operator : CG/JU
Sample : 02251-05
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMC3

Manual IntegrationsAPPROVED

Quant Time: Apr 11 23:01:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/12/2023
Supervised By :Jagrut Upadhyay 04/12/2023

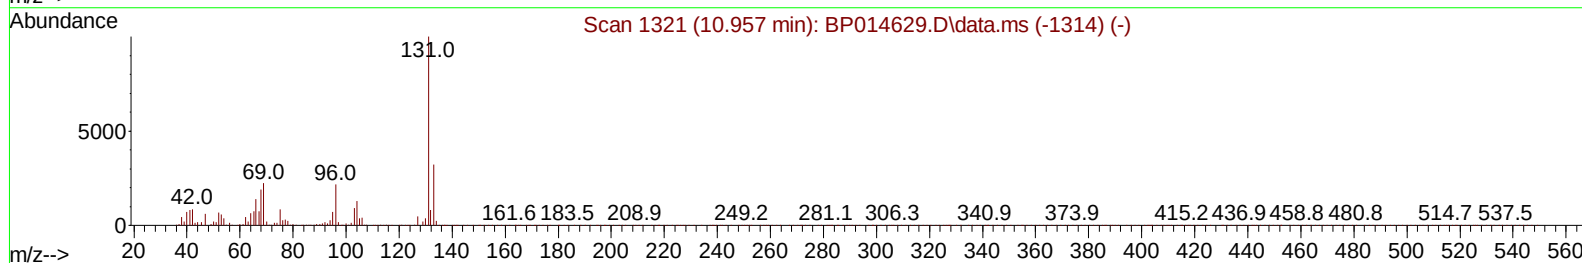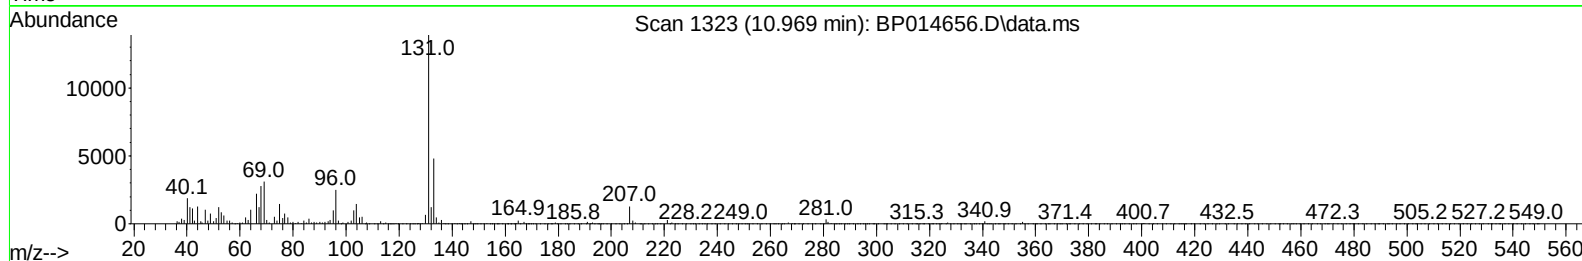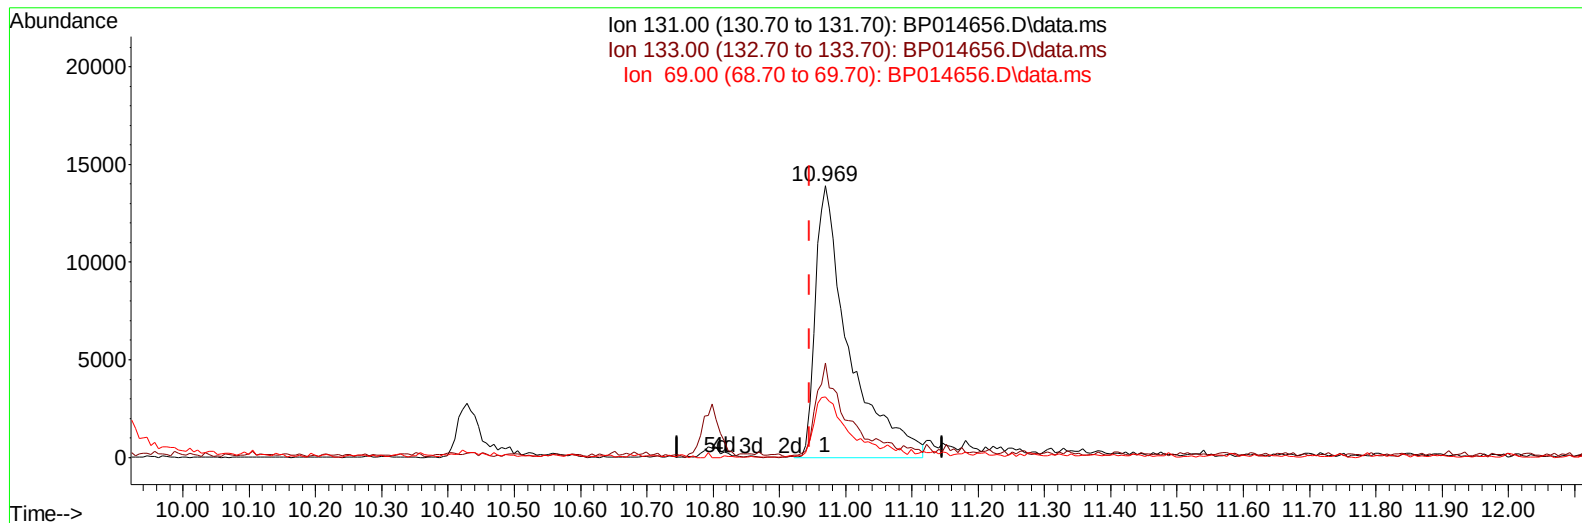

TIC: BP014656.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.969min (+ 0.024) 3.87 ng/ul m

response 49056

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	34.75
69.00	21.30	22.26
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014656.D
Acq On : 11 Apr 2023 15:09
Operator : CG/JU
Sample : 02251-05
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMC3

Manual IntegrationsAPPROVED

Quant Time: Apr 11 23:01:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/12/2023
Supervised By :Jagrut Upadhyay 04/12/2023

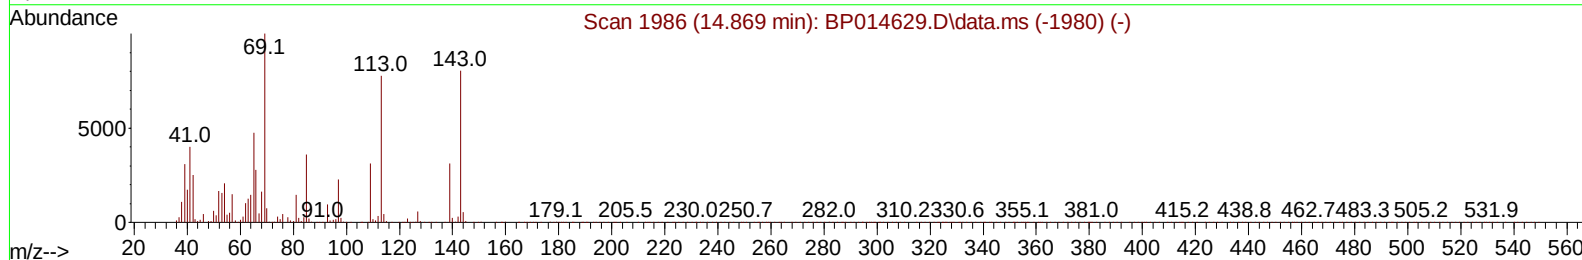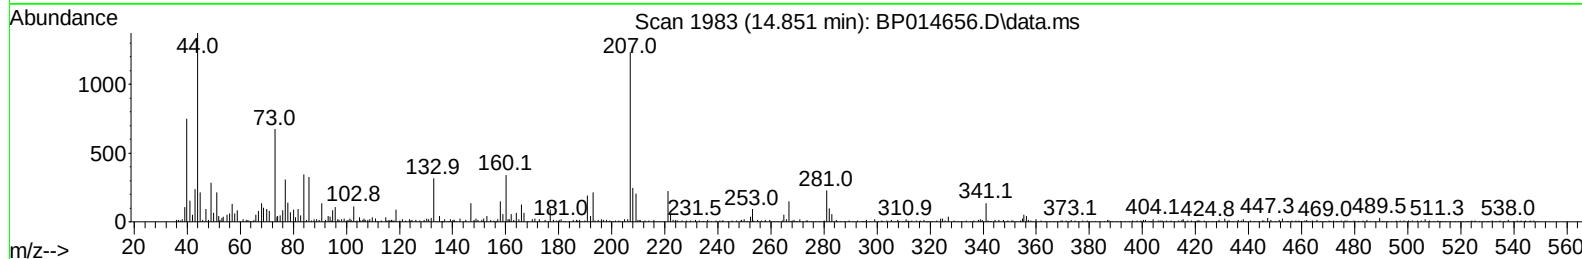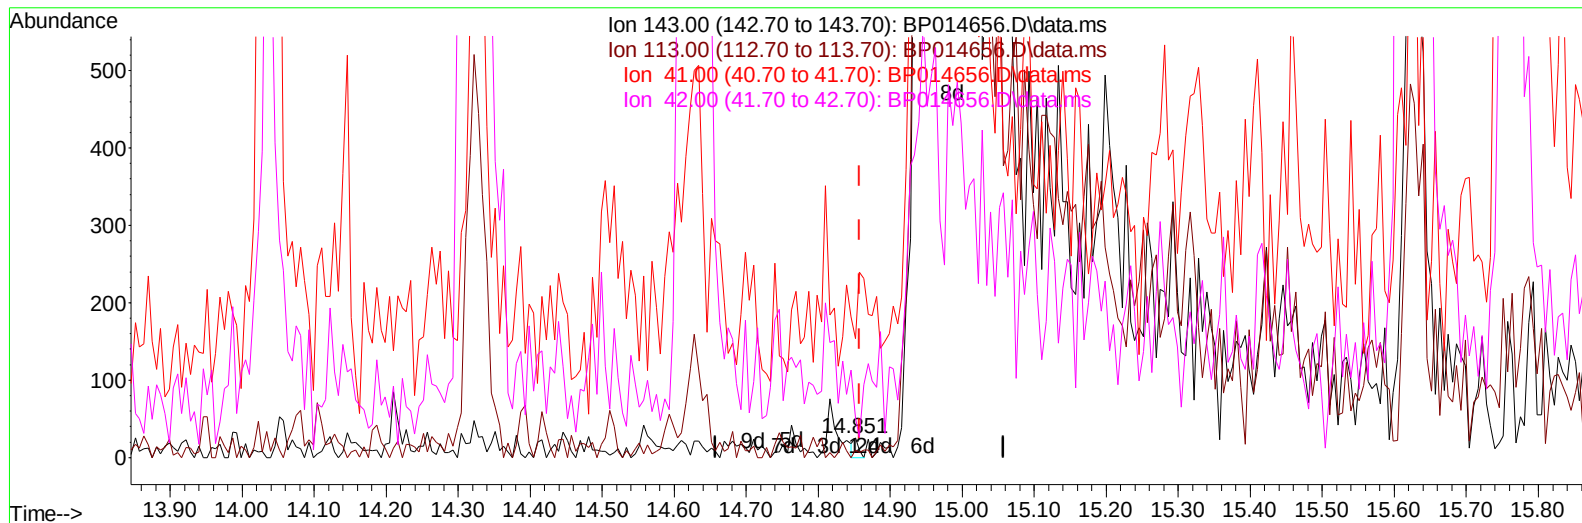

TIC: BP014656.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.851min (-0.006) 0.00 ng/ul

response 12

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	40.00#
41.00	44.20	616.00#
42.00	31.50	204.00#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014656.D
Acq On : 11 Apr 2023 15:09
Operator : CG/JU
Sample : 02251-05
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMC3

Manual IntegrationsAPPROVED

Quant Time: Apr 11 23:01:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/12/2023
Supervised By :Jagrut Upadhyay 04/12/2023

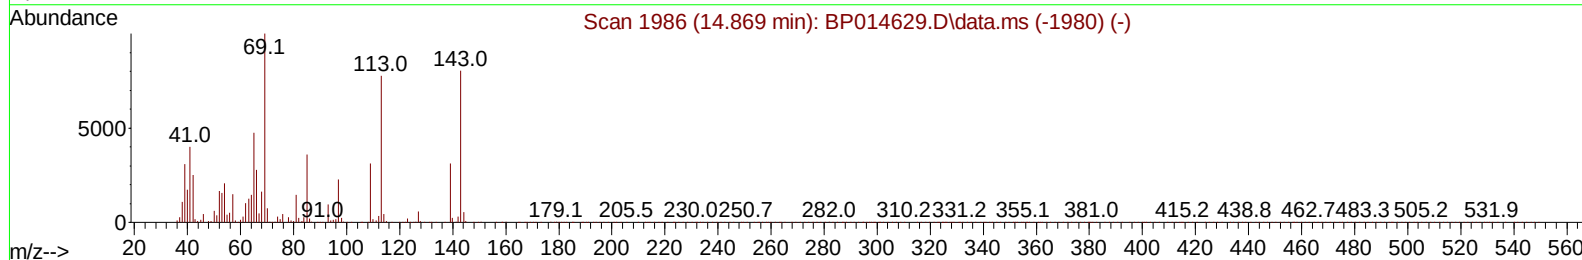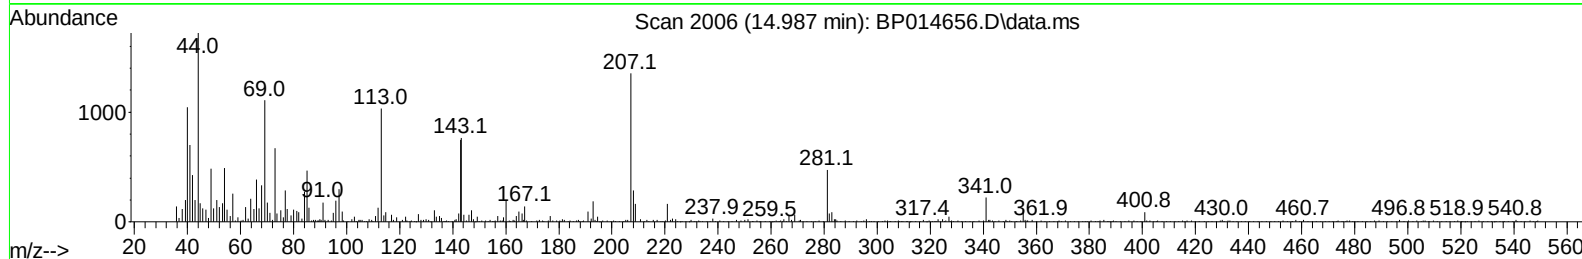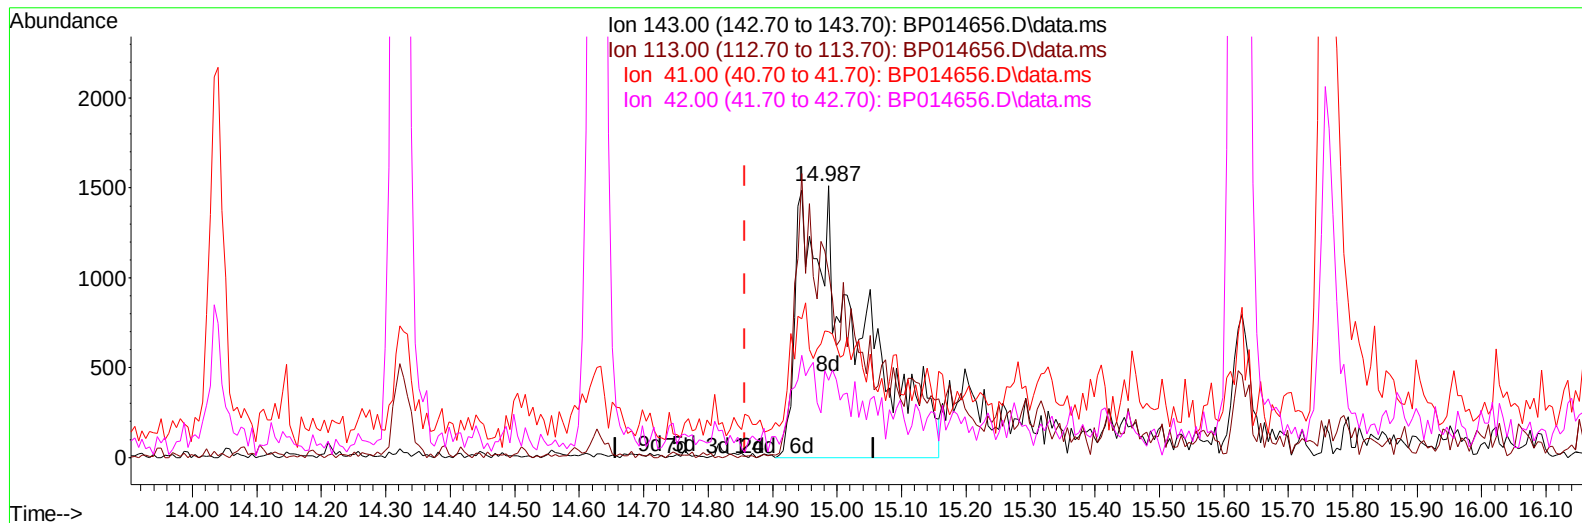

TIC: BP014656.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.987min (+ 0.130) 2.30 ng/ul m

response 9802

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	135.26#
41.00	44.20	91.87#
42.00	31.50	56.23#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
 Data File : BP014656.D
 Acq On : 11 Apr 2023 15:09
 Operator : CG/JU
 Sample : 02251-05
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COMC3

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/12/2023
 Supervised By :Jagrut Upadhyay 04/12/2023

Quant Time: Apr 11 23:01:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 11 01:21:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.975	152	134721	20.000	ng/ul	0.00
20) Naphthalene-d8	10.793	136	571657	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.628	164	347234	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.392	188	685948	20.000	ng/ul	0.00
79) Chrysene-d12	21.486	240	622165	20.000	ng/ul	0.00
88) Perylene-d12	23.986	264	752905	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	7004m	2.016	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.152	99	55641	4.478	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.305	67	218011	27.348	ng/ul	0.00
11) 2-Chlorophenol-d4	7.505	132	174484	19.430	ng/ul	0.00
15) 4-Methylphenol-d8	8.699	113	108287	10.805	ng/ul	0.00
21) Nitrobenzene-d5	9.152	128	109358	23.697	ng/ul	0.00
24) 2-Nitrophenol-d4	9.881	143	119162	22.550	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.428	165	183910	19.110	ng/ul	0.00
31) 4-Chloroaniline-d4	10.969	131	49056m	3.870	ng/ul	0.02
46) Dimethylphthalate-d6	14.040	166	712463	25.306	ng/ul	0.00
49) Acenaphthylene-d8	14.322	160	789416	25.269	ng/ul	0.00
54) 4-Nitrophenol-d4	14.987	143	9802m	2.305	ng/ul	0.13
60) Fluorene-d10	15.622	176	604287	25.738	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.763	200	93895	18.603	ng/ul	0.00
73) Anthracene-d10	17.492	188	945749	28.489	ng/ul	0.00
81) Pyrene-d10	19.722	212	1060250	25.371	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.822	264	1146042	28.650	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014656.D
Acq On : 11 Apr 2023 15:09
Operator : CG/JU
Sample : 02251-05
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMC3

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/12/2023
Supervised By :Jagrut Upadhyay 04/12/2023

Quant Time: Apr 11 23:01:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

