

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
 Data File : BP014626.D
 Acq On : 10 Apr 2023 10:58
 Operator : CG/JU
 Sample : PB151978BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK978

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014626.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	27	30	43	rVB	45710	63708	2.37%	0.216%
2	3.799	102	104	119	rBV	175289	323804	12.04%	1.098%
3	4.122	154	159	161	rBV4	7988	11559	0.43%	0.039%
4	4.746	263	265	268	rVV3	2440	2952	0.11%	0.010%
5	6.369	538	541	544	rBV5	2391	3248	0.12%	0.011%
6	7.146	666	673	694	rBV	449540	888961	33.05%	3.013%
7	7.305	694	700	713	rVV	426033	702872	26.13%	2.383%
8	7.510	728	735	749	rBV	516216	925438	34.41%	3.137%
9	7.975	806	814	829	rBV	449918	761007	28.29%	2.580%
10	8.699	930	937	953	rBV	550084	1075158	39.97%	3.644%
11	9.157	1008	1015	1029	rBV	518787	911608	33.89%	3.090%
12	9.881	1131	1138	1155	rBV	418831	773082	28.74%	2.621%
13	10.428	1223	1231	1253	rBV	409479	1042536	38.76%	3.534%
14	10.799	1286	1294	1305	rBV	637244	1095324	40.72%	3.713%
15	10.963	1315	1322	1339	rBV2	112704	352274	13.10%	1.194%
16	12.416	1564	1569	1570	rBV5	6115	8031	0.30%	0.027%
17	12.628	1601	1605	1610	rBV8	1686	3361	0.12%	0.011%
18	13.610	1769	1772	1778	rVB7	2693	3981	0.15%	0.013%
19	14.040	1837	1845	1862	rBV	1035382	1608374	59.79%	5.452%
20	14.328	1885	1894	1910	rBV	1239815	1903529	70.77%	6.452%
21	14.445	1912	1914	1920	rVB7	3367	4843	0.18%	0.016%
22	14.628	1938	1945	1961	rBV	893599	1414577	52.59%	4.795%
23	14.881	1980	1988	2006	rBV2	89915	383154	14.24%	1.299%
24	15.628	2108	2115	2130	rBV	1501249	2291226	85.18%	7.767%
25	15.763	2132	2138	2152	rVV	359522	679091	25.25%	2.302%
26	15.869	2154	2156	2161	rVV5	13029	21059	0.78%	0.071%
27	16.469	2255	2258	2263	rBV7	2156	3028	0.11%	0.010%
28	17.075	2357	2361	2364	rVB5	3514	5173	0.19%	0.018%
29	17.186	2377	2380	2382	rVV4	3387	3751	0.14%	0.013%
30	17.292	2395	2398	2399	rBV3	3037	2764	0.10%	0.009%
31	17.392	2409	2415	2426	rBV	1086398	1557287	57.90%	5.279%
32	17.492	2426	2432	2453	rVV	1519512	2340564	87.02%	7.934%
33	18.386	2582	2584	2587	rBV3	4218	4044	0.15%	0.014%
34	19.304	2737	2740	2745	rVB5	19578	24376	0.91%	0.083%
35	19.375	2749	2752	2758	rVV2	13937	22364	0.83%	0.076%
36	19.722	2806	2811	2821	rBV	1776550	2526167	93.92%	8.563%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014626.D
Acq On : 10 Apr 2023 10:58
Operator : CG/JU
Sample : PB151978BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK978

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Title : SVOA CALIBRATION

37	21.480	3106	3110	3127	rBV	885331	1536107	57.11%	5.207%
38	23.815	3500	3507	3519	rBV2	1244768	2689820	100.00%	9.118%
39	23.980	3529	3535	3547	rVB2	694698	1530769	56.91%	5.189%




Sum of corrected areas: 29500971

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014626.D
Acq On : 10 Apr 2023 10:58
Operator : CG/JU
Sample : PB151978BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK978

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

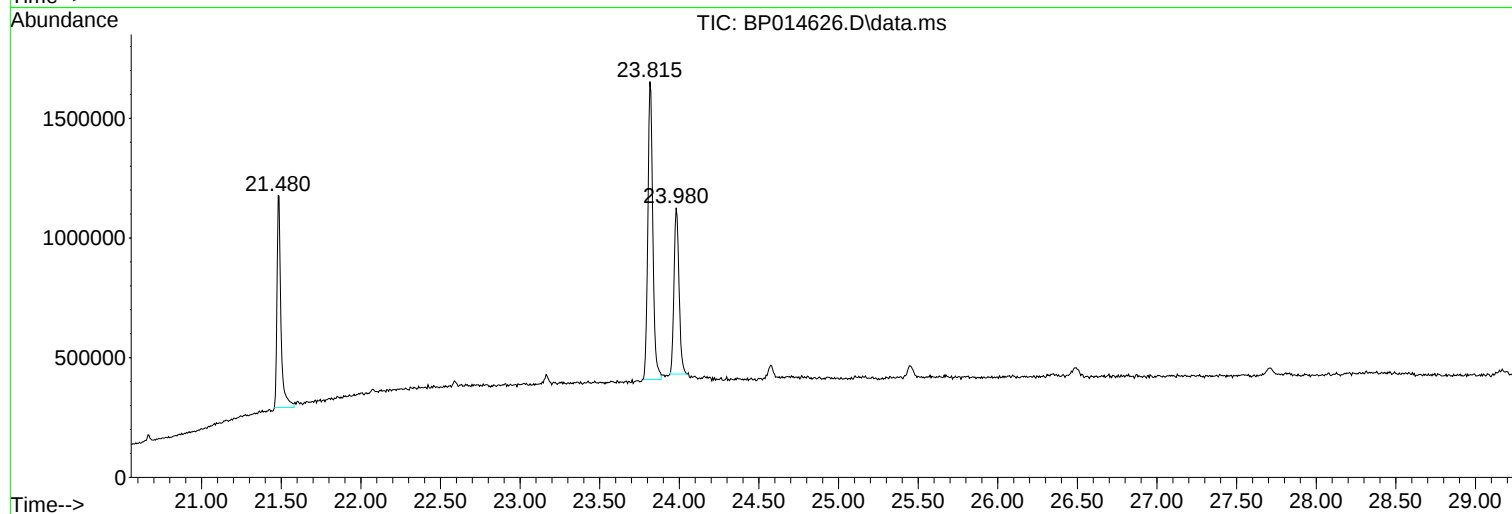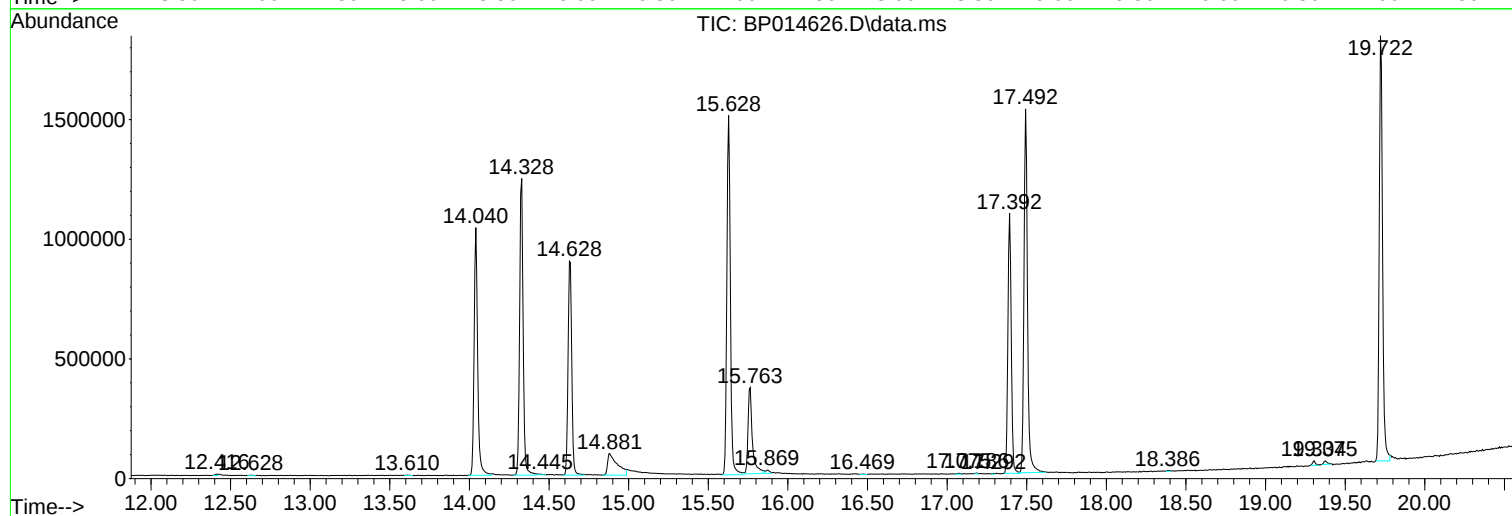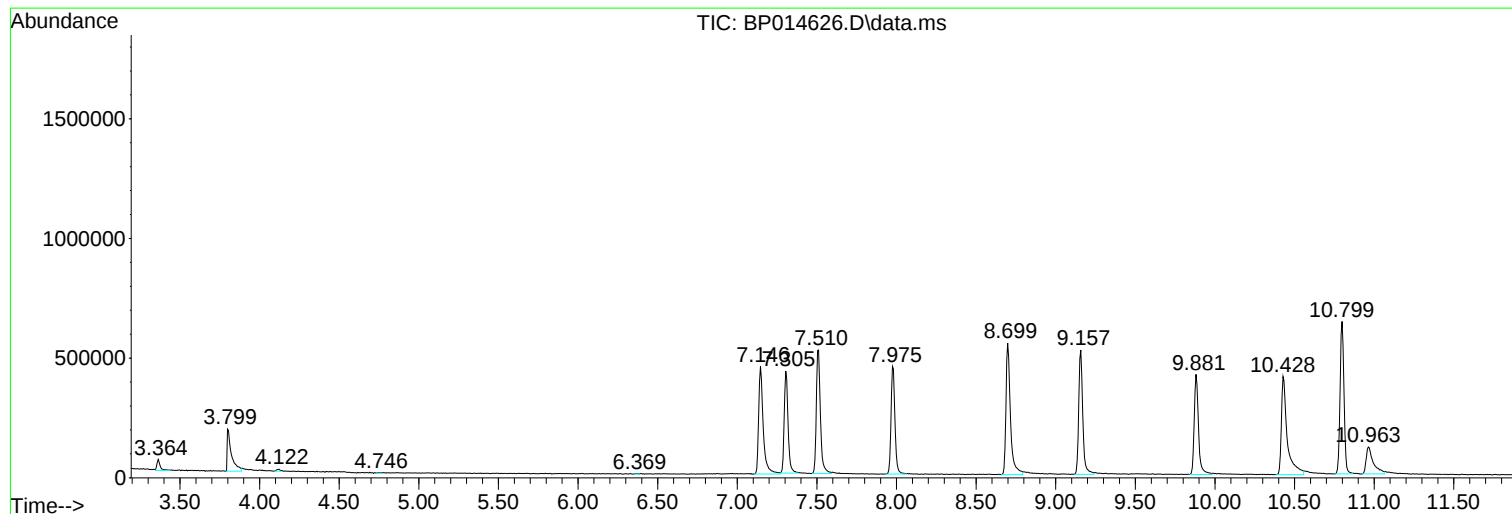

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014626.D
Acq On : 10 Apr 2023 10:58
Operator : CG/JU
Sample : PB151978BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK978

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014626.D
Acq On : 10 Apr 2023 10:58
Operator : CG/JU
Sample : PB151978BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK978

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc