

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
 Data File : BP014630.D
 Acq On : 10 Apr 2023 17:06
 Operator : CG/JU
 Sample : PB152000BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK000

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014630.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	27	30	40	rVB	41604	53997	2.00%	0.170%
2	3.793	100	103	128	rBV	403453	712713	26.41%	2.240%
3	4.116	155	158	163	rVB2	9979	14861	0.55%	0.047%
4	4.722	257	261	264	rBV6	2867	5090	0.19%	0.016%
5	5.781	440	441	446	rBV5	1981	3092	0.11%	0.010%
6	7.146	666	673	690	rVV	495371	936824	34.71%	2.944%
7	7.305	694	700	720	rVB	462648	765111	28.35%	2.405%
8	7.505	728	734	748	rBV	549613	962364	35.66%	3.025%
9	7.975	806	814	829	rBV	553335	927315	34.36%	2.915%
10	8.699	930	937	961	rBV	606595	1154518	42.78%	3.629%
11	9.157	1007	1015	1028	rBV	529826	962100	35.65%	3.024%
12	9.881	1130	1138	1157	rBV	469779	847408	31.40%	2.663%
13	10.428	1224	1231	1259	rBV	518343	1143448	42.37%	3.594%
14	10.798	1284	1294	1306	rBV	800514	1355089	50.21%	4.259%
15	10.951	1313	1320	1344	rBV	467539	1126212	41.73%	3.540%
16	11.204	1361	1363	1367	rVB5	2361	2779	0.10%	0.009%
17	12.398	1562	1566	1572	rBV5	6219	14290	0.53%	0.045%
18	14.039	1837	1845	1859	rBV	1095499	1598967	59.25%	5.026%
19	14.328	1886	1894	1907	rBV	1233033	1885780	69.88%	5.927%
20	14.634	1938	1946	1961	rBV	1081105	1658848	61.47%	5.214%
21	14.881	1982	1988	2008	rBV	95599	389305	14.43%	1.224%
22	15.628	2108	2115	2127	rBV	1428703	2176332	80.64%	6.840%
23	15.763	2132	2138	2154	rBV	363979	643173	23.83%	2.022%
24	16.422	2247	2250	2256	rVB7	2745	4337	0.16%	0.014%
25	17.181	2376	2379	2384	rVB8	2663	4521	0.17%	0.014%
26	17.392	2409	2415	2426	rBV	1157001	1707955	63.29%	5.368%
27	17.492	2426	2432	2446	rVV	1386169	2132726	79.03%	6.703%
28	18.575	2614	2616	2619	rBV4	3930	5040	0.19%	0.016%
29	19.310	2737	2741	2746	rVB6	19943	32690	1.21%	0.103%
30	19.727	2806	2812	2825	rBV	1629779	2348642	87.03%	7.382%
31	21.486	3106	3111	3124	rBV2	1038227	1735379	64.30%	5.454%
32	23.821	3501	3508	3527	rBV2	1234437	2698706	100.00%	8.482%
33	23.992	3530	3537	3545	rVB2	821393	1806967	66.96%	5.679%




Sum of corrected areas: 31816579

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014630.D
Acq On : 10 Apr 2023 17:06
Operator : CG/JU
Sample : PB152000BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK000

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

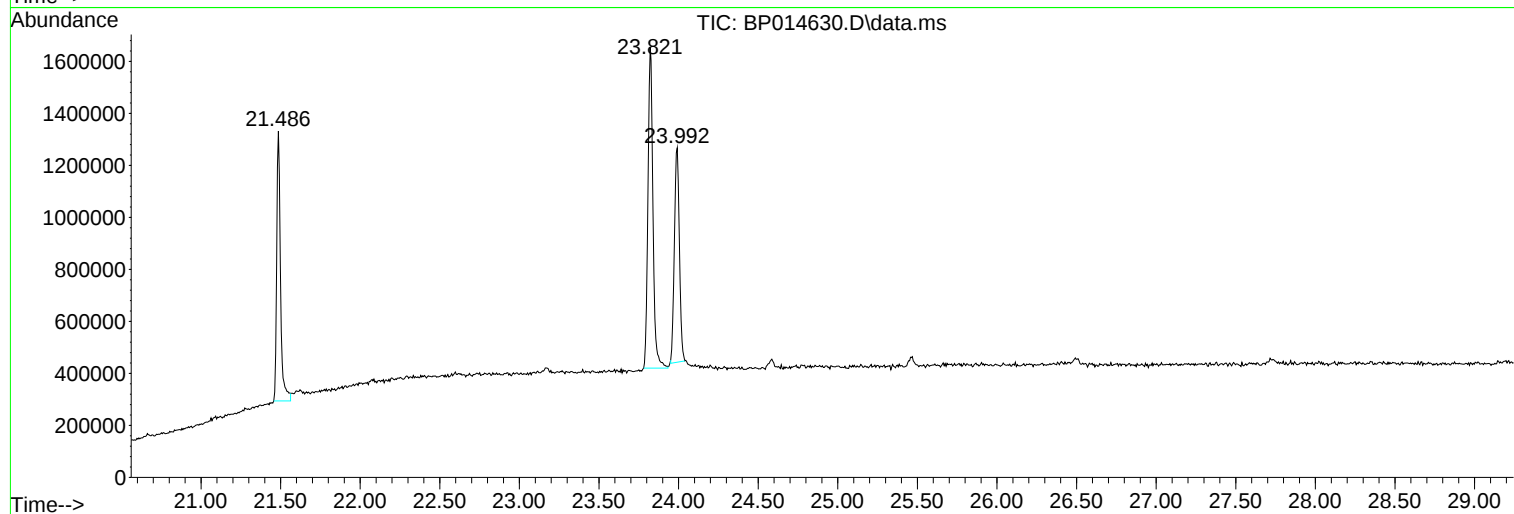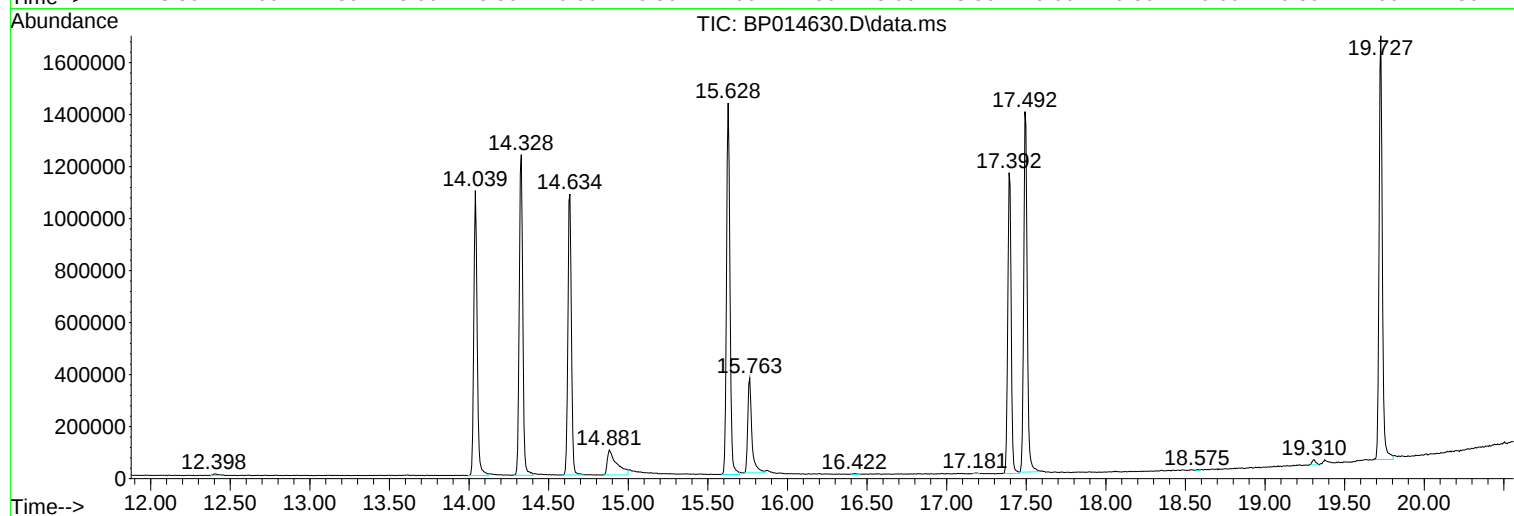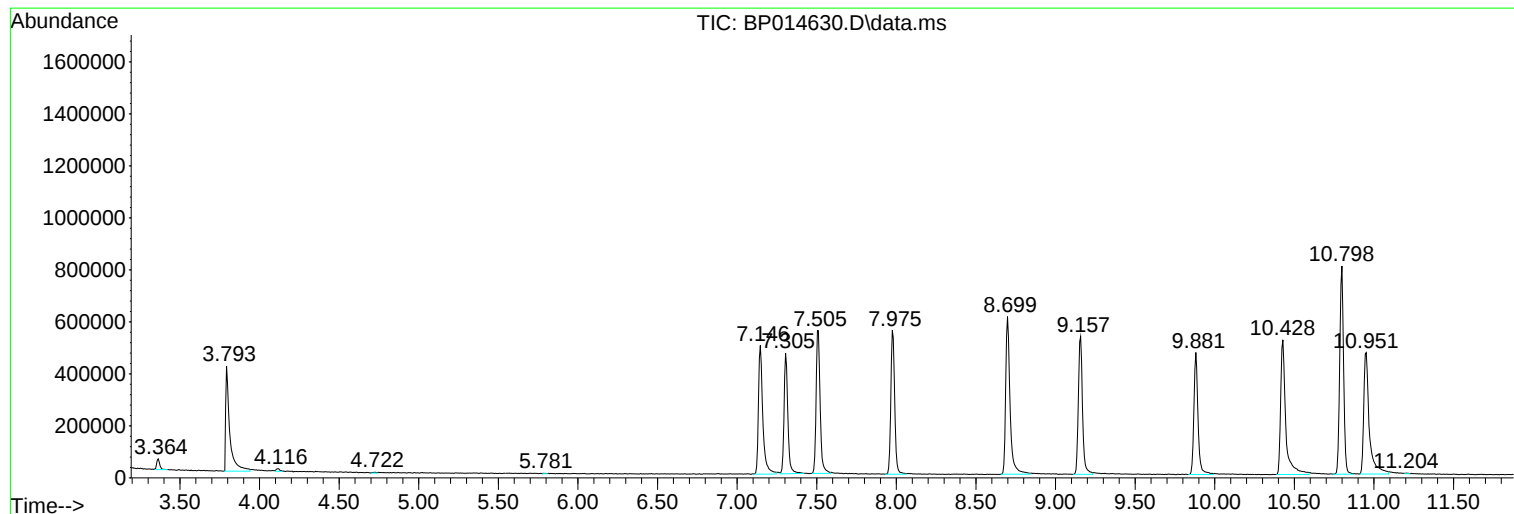

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014630.D
Acq On : 10 Apr 2023 17:06
Operator : CG/JU
Sample : PB152000BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK000

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014630.D
Acq On : 10 Apr 2023 17:06
Operator : CG/JU
Sample : PB152000BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK000

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------