

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
 Data File : BP014631.D
 Acq On : 10 Apr 2023 17:40
 Operator : CG/JU
 Sample : PB152002BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014631.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.363	26	30	37	rBV	38850	50212	1.73%	0.170%
2	3.793	100	103	125	rBV	338521	605272	20.90%	2.046%
3	4.122	155	159	162	rVB6	8258	12362	0.43%	0.042%
4	7.145	665	673	687	rBV	418383	797056	27.53%	2.695%
5	7.304	694	700	714	rBV	383590	632804	21.86%	2.139%
6	7.510	727	735	752	rBV	482475	848976	29.32%	2.870%
7	7.975	808	814	828	rBV	430765	720103	24.87%	2.434%
8	8.698	927	937	959	rBV	508030	983934	33.98%	3.326%
9	9.157	1008	1015	1032	rBV	456849	818399	28.27%	2.767%
10	9.881	1131	1138	1154	rBV	383158	706380	24.40%	2.388%
11	10.428	1223	1231	1252	rBV	426102	948423	32.76%	3.206%
12	10.798	1286	1294	1303	rBV	603015	1015821	35.08%	3.434%
13	10.951	1313	1320	1351	rBV	384923	961508	33.21%	3.251%
14	12.410	1561	1568	1577	rBV	5759	16168	0.56%	0.055%
15	14.039	1839	1845	1862	rBV	965008	1435270	49.57%	4.852%
16	14.327	1887	1894	1909	rBV	1081089	1667994	57.61%	5.639%
17	14.633	1938	1946	1958	rBV	870342	1309922	45.24%	4.428%
18	14.880	1981	1988	2015	rBV2	94178	452823	15.64%	1.531%
19	15.627	2109	2115	2132	rBV	1351186	2026438	69.99%	6.851%
20	15.763	2132	2138	2153	rBV	371560	655440	22.64%	2.216%
21	17.068	2356	2360	2362	rBV4	3560	4302	0.15%	0.015%
22	17.186	2377	2380	2384	rVB6	2626	3583	0.12%	0.012%
23	17.392	2408	2415	2425	rBV	1047515	1525985	52.70%	5.159%
24	17.492	2426	2432	2456	rVV2	1470130	2234555	77.18%	7.554%
25	17.639	2456	2457	2462	rVB4	3190	3211	0.11%	0.011%
26	18.586	2616	2618	2621	rBV3	4226	4035	0.14%	0.014%
27	19.304	2737	2740	2745	rBV5	16466	20213	0.70%	0.068%
28	19.380	2749	2753	2763	rVV3	12844	28274	0.98%	0.096%
29	19.727	2806	2812	2828	rBV	1868871	2683621	92.69%	9.072%
30	21.486	3106	3111	3123	rBV	1073048	1726905	59.64%	5.838%
31	23.821	3501	3508	3527	rVB2	1340016	2895385	100.00%	9.788%
32	23.986	3530	3536	3549	rVB2	789373	1784601	61.64%	6.033%




Sum of corrected areas: 29579975

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014631.D
Acq On : 10 Apr 2023 17:40
Operator : CG/JU
Sample : PB152002BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

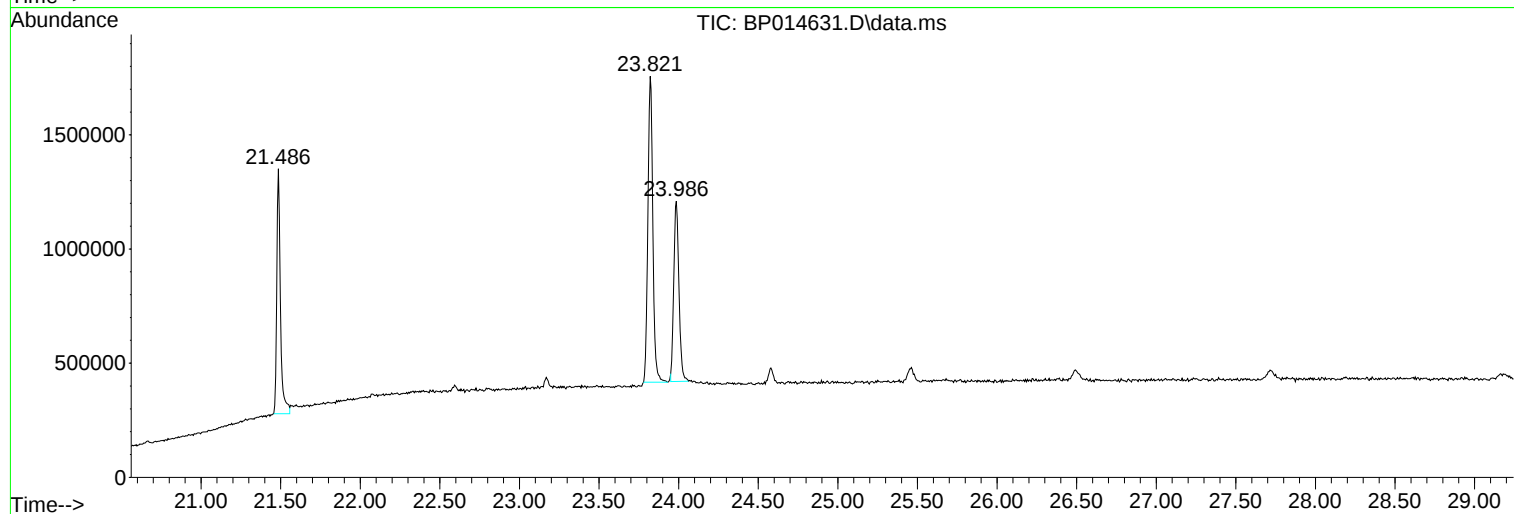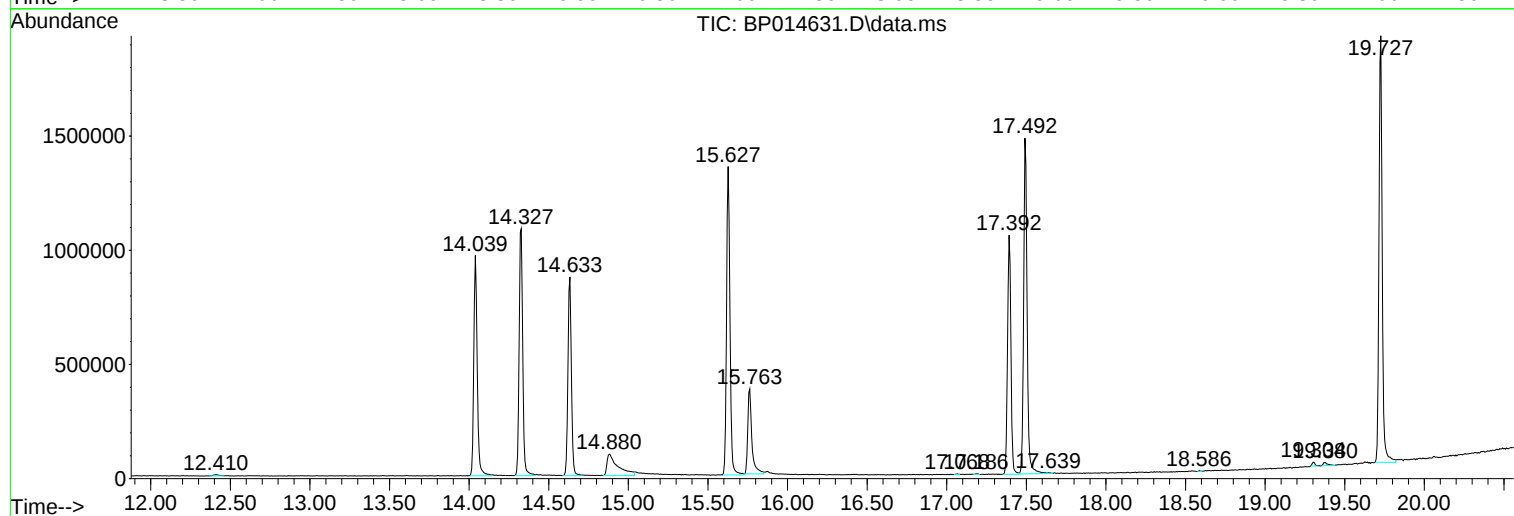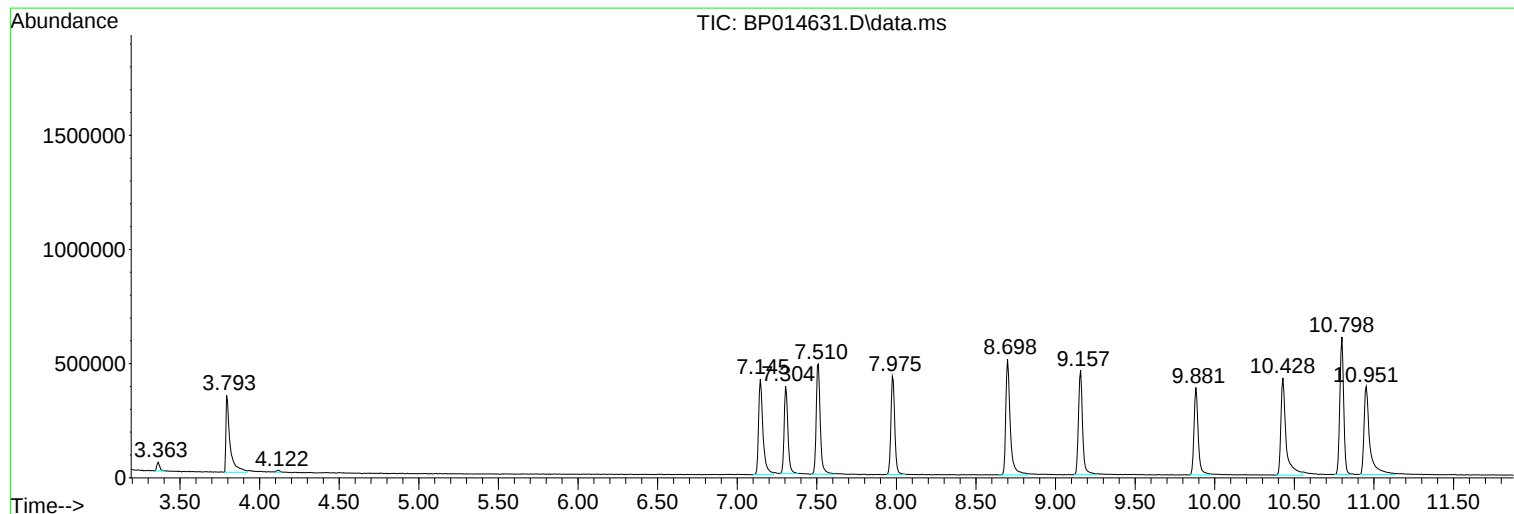

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014631.D
Acq On : 10 Apr 2023 17:40
Operator : CG/JU
Sample : PB152002BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014631.D
Acq On : 10 Apr 2023 17:40
Operator : CG/JU
Sample : PB152002BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc