

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
 Data File : BP014634.D
 Acq On : 10 Apr 2023 19:22
 Operator : CG/JU
 Sample : 02250-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHD33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014634.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	20	24	27	rBV2	43877	53865	1.74%	0.193%
2	3.364	27	30	34	rVB	26868	34160	1.10%	0.122%
3	3.817	105	107	125	rBV	47593	105676	3.41%	0.379%
4	4.117	155	158	164	rVB3	11252	16556	0.53%	0.059%
5	4.652	244	249	256	rVB2	25561	37516	1.21%	0.134%
6	6.787	608	612	615	rBV6	2050	3173	0.10%	0.011%
7	7.152	666	674	685	rBV	75296	178187	5.76%	0.639%
8	7.305	694	700	713	rBV	368082	601111	19.42%	2.155%
9	7.510	728	735	750	rBV	363138	651215	21.04%	2.334%
10	7.669	760	762	766	rVB5	2927	3688	0.12%	0.013%
11	7.975	806	814	826	rBV	470926	795494	25.70%	2.851%
12	8.705	932	938	958	rBV	244240	514910	16.64%	1.846%
13	9.157	1008	1015	1033	rBV	432958	791159	25.56%	2.836%
14	9.469	1064	1068	1072	rVV7	2209	3121	0.10%	0.011%
15	9.510	1072	1075	1082	rVB8	2759	4989	0.16%	0.018%
16	9.881	1130	1138	1156	rBV	365393	673113	21.75%	2.413%
17	10.428	1222	1231	1253	rBV	369489	858327	27.73%	3.077%
18	10.799	1286	1294	1308	rBV	645236	1116713	36.08%	4.003%
19	10.951	1314	1320	1346	rBV	269447	657113	21.23%	2.355%
20	12.404	1559	1567	1574	rBV	6443	15746	0.51%	0.056%
21	12.763	1624	1628	1631	rVB6	2540	4072	0.13%	0.015%
22	14.040	1835	1845	1859	rBV	986830	1426109	46.08%	5.112%
23	14.151	1862	1864	1869	rVB5	4001	5143	0.17%	0.018%
24	14.328	1884	1894	1910	rBV	1010518	1570878	50.75%	5.631%
25	14.628	1938	1945	1959	rBV	936726	1389365	44.89%	4.980%
26	14.940	1992	1998	2001	rBV6	10846	26460	0.85%	0.095%
27	15.410	2075	2078	2082	rBV3	7062	8446	0.27%	0.030%
28	15.451	2082	2085	2094	rVB8	4982	9501	0.31%	0.034%
29	15.628	2108	2115	2132	rBV	1375327	2047188	66.14%	7.338%
30	15.763	2132	2138	2154	rBV	370365	685664	22.15%	2.458%
31	17.063	2357	2359	2360	rBV2	4297	3125	0.10%	0.011%
32	17.392	2408	2415	2425	rBV	1113304	1575689	50.91%	5.648%
33	17.492	2426	2432	2445	rVV	1655902	2394603	77.37%	8.584%
34	17.810	2483	2486	2488	rBV4	4005	5238	0.17%	0.019%
35	18.275	2563	2565	2567	rBV3	5609	5300	0.17%	0.019%
36	19.298	2736	2739	2743	rBV4	20401	28214	0.91%	0.101%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014634.D
Acq On : 10 Apr 2023 19:22
Operator : CG/JU
Sample : 02250-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHD3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Title : SVOA CALIBRATION

37	19.375	2749	2752	2759	rVB6	20787	35713	1.15%	0.128%
38	19.722	2806	2811	2825	rBV	2099210	2810501	90.81%	10.074%
39	21.480	3105	3110	3124	rBV	1112827	1868789	60.38%	6.699%
40	23.821	3501	3508	3518	rVB	1525355	3095050	100.00%	11.094%
41	23.986	3530	3536	3545	rVB2	842926	1786733	57.73%	6.405%




Sum of corrected areas: 27897613

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014634.D
Acq On : 10 Apr 2023 19:22
Operator : CG/JU
Sample : 02250-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

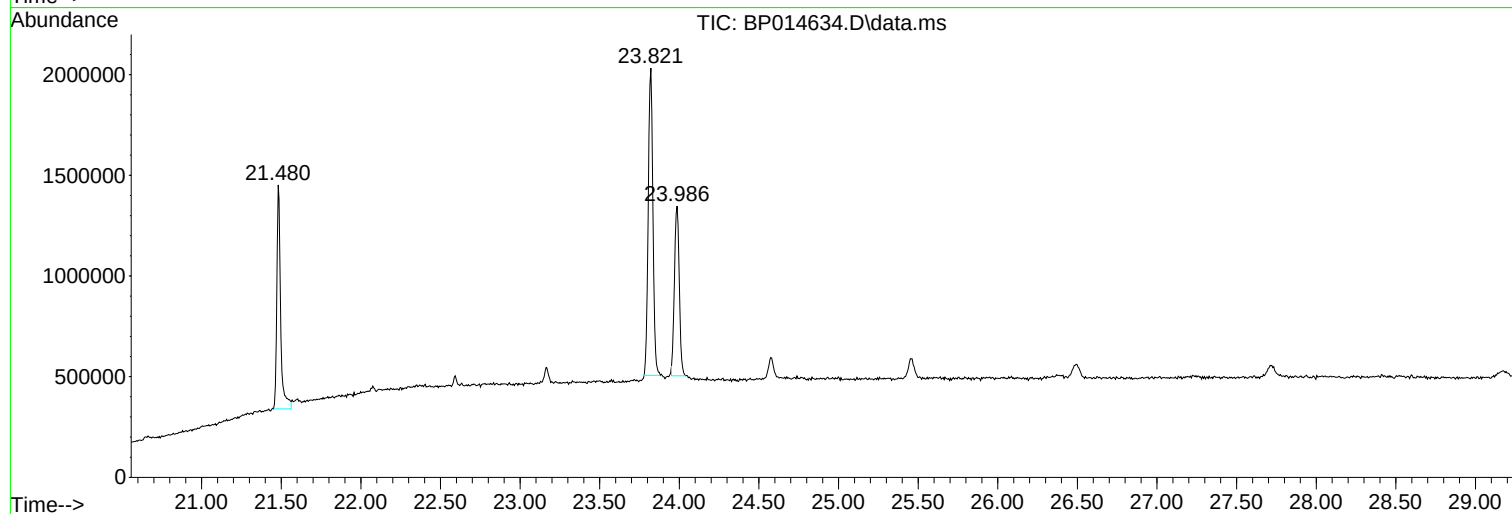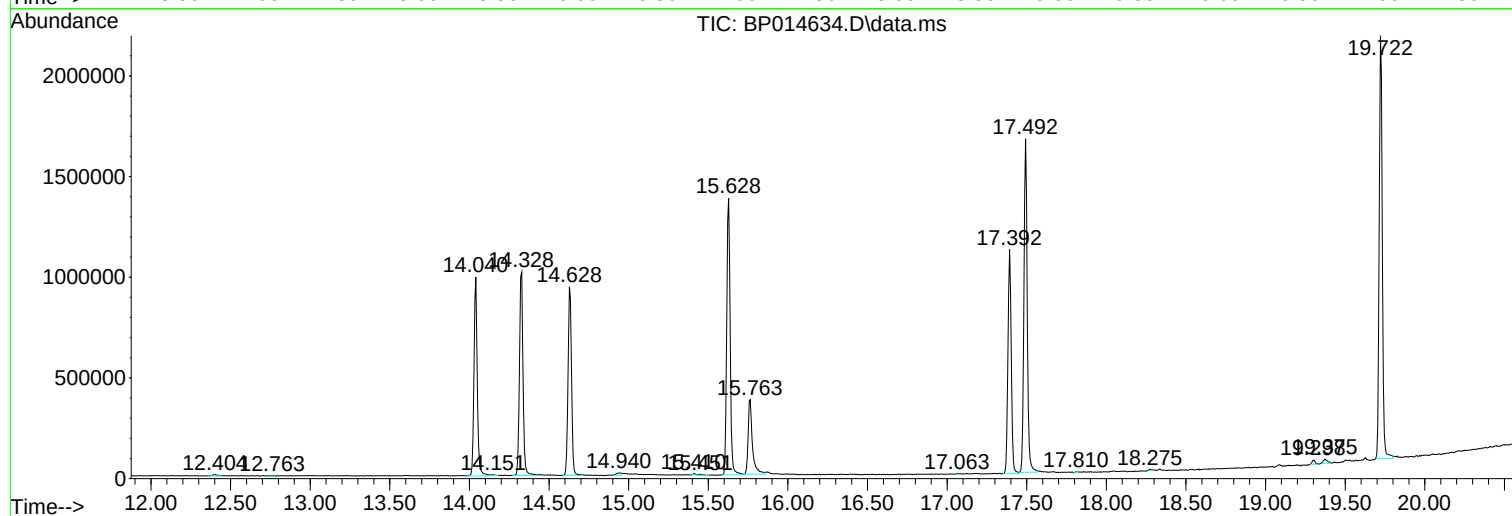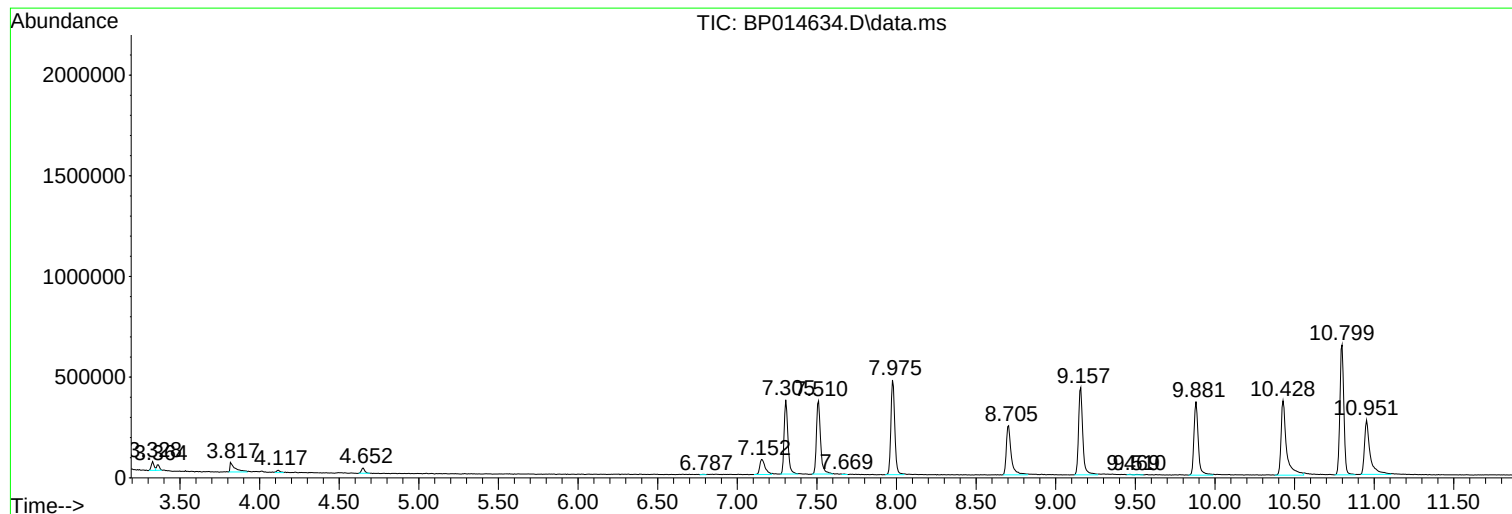

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014634.D
Acq On : 10 Apr 2023 19:22
Operator : CG/JU
Sample : 02250-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014634.D
Acq On : 10 Apr 2023 19:22
Operator : CG/JU
Sample : 02250-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------