

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
 Data File : BP014645.D
 Acq On : 11 Apr 2023 08:54
 Operator : CG/JU
 Sample : PB152002BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014645.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	27	30	40	rVB	41440	56965	1.91%	0.189%
2	3.799	102	104	125	rBV	301339	554917	18.60%	1.842%
3	4.123	155	159	162	rVB3	8811	9920	0.33%	0.033%
4	6.317	527	532	535	rBV7	1584	3192	0.11%	0.011%
5	7.158	668	675	691	rBV	412721	767656	25.74%	2.548%
6	7.317	695	702	713	rBV	374017	592178	19.85%	1.965%
7	7.517	730	736	753	rBV	479970	791530	26.54%	2.627%
8	7.987	808	816	826	rBV	422683	674126	22.60%	2.237%
9	8.711	930	939	953	rBV	502229	932999	31.28%	3.096%
10	9.163	1009	1016	1031	rBV	423296	771857	25.88%	2.562%
11	9.893	1130	1140	1152	rBV	370066	671265	22.51%	2.228%
12	10.440	1225	1233	1251	rBV	423737	920272	30.85%	3.054%
13	10.810	1288	1296	1307	rBV	561571	944835	31.68%	3.136%
14	10.963	1314	1322	1343	rBV	400649	912540	30.60%	3.028%
15	12.404	1563	1567	1574	rBV4	7272	15222	0.51%	0.051%
16	13.628	1767	1775	1780	rBV4	5592	17908	0.60%	0.059%
17	14.051	1841	1847	1861	rBV	976711	1424881	47.77%	4.729%
18	14.334	1888	1895	1910	rBV2	1072174	1658384	55.60%	5.504%
19	14.640	1941	1947	1957	rBV	848643	1272635	42.67%	4.223%
20	14.887	1983	1989	2008	rBV	161161	540674	18.13%	1.794%
21	15.516	2089	2096	2097	rBV7	8729	16422	0.55%	0.054%
22	15.640	2110	2117	2131	rBV	1438437	2063468	69.18%	6.848%
23	15.769	2133	2139	2151	rVV	446327	718078	24.08%	2.383%
24	15.887	2154	2159	2162	rVB7	7478	14658	0.49%	0.049%
25	16.187	2205	2210	2211	rBV5	3367	4345	0.15%	0.014%
26	16.216	2213	2215	2218	rVB4	3470	3665	0.12%	0.012%
27	16.434	2248	2252	2258	rVB9	3160	5606	0.19%	0.019%
28	16.657	2284	2290	2293	rBV8	3885	6133	0.21%	0.020%
29	16.822	2314	2318	2325	rVB2	15328	26922	0.90%	0.089%
30	16.881	2325	2328	2332	rBV5	2365	3399	0.11%	0.011%
31	17.145	2368	2373	2376	rBV7	2436	5613	0.19%	0.019%
32	17.204	2379	2383	2388	rVB8	5406	9906	0.33%	0.033%
33	17.404	2410	2417	2427	rBV	1123171	1611078	54.02%	5.347%
34	17.504	2428	2434	2453	rVB	1591465	2332775	78.21%	7.742%
35	17.763	2474	2478	2482	rBV7	4562	7366	0.25%	0.024%
36	17.904	2498	2502	2508	rVB2	13502	18061	0.61%	0.060%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
 Data File : BP014645.D
 Acq On : 11 Apr 2023 08:54
 Operator : CG/JU
 Sample : PB152002BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	18.198	2549	2552	2554	rBV4	3432	4457	0.15%	0.015%
38	18.234	2556	2558	2561	rVV4	4374	4649	0.16%	0.015%
39	18.304	2565	2570	2572	rBV6	6205	10710	0.36%	0.036%
40	18.810	2653	2656	2662	rVB2	18012	24448	0.82%	0.081%
41	19.310	2739	2741	2747	rVB5	18841	24112	0.81%	0.080%
42	19.386	2751	2754	2757	rVV	13294	15661	0.53%	0.052%
43	19.581	2785	2787	2792	rBV3	16580	17679	0.59%	0.059%
44	19.734	2807	2813	2820	rBV	2109764	2860116	95.89%	9.492%
45	20.675	2971	2973	2977	rBV3	32776	31918	1.07%	0.106%
46	21.492	3107	3112	3124	rBV	1184572	1921189	64.41%	6.376%
47	23.839	3504	3511	3523	rVB	1459517	2982628	100.00%	9.898%
48	24.004	3532	3539	3550	rVB2	869268	1853538	62.14%	6.151%




Sum of corrected areas: 30132556

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014645.D
Acq On : 11 Apr 2023 08:54
Operator : CG/JU
Sample : PB152002BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

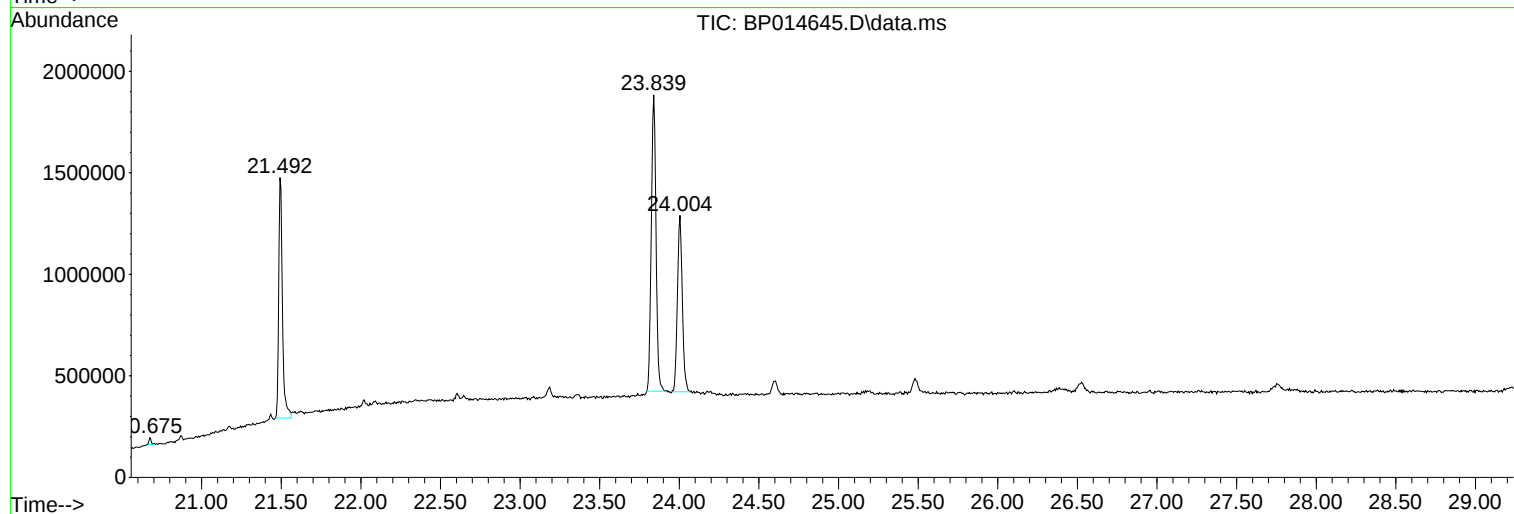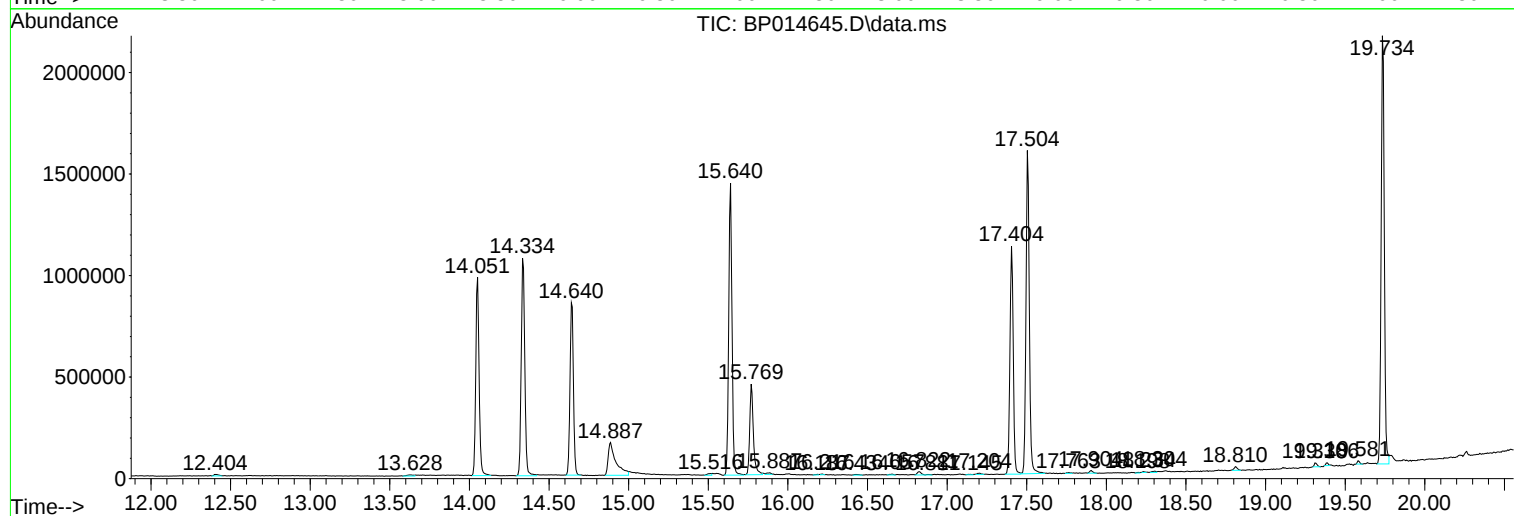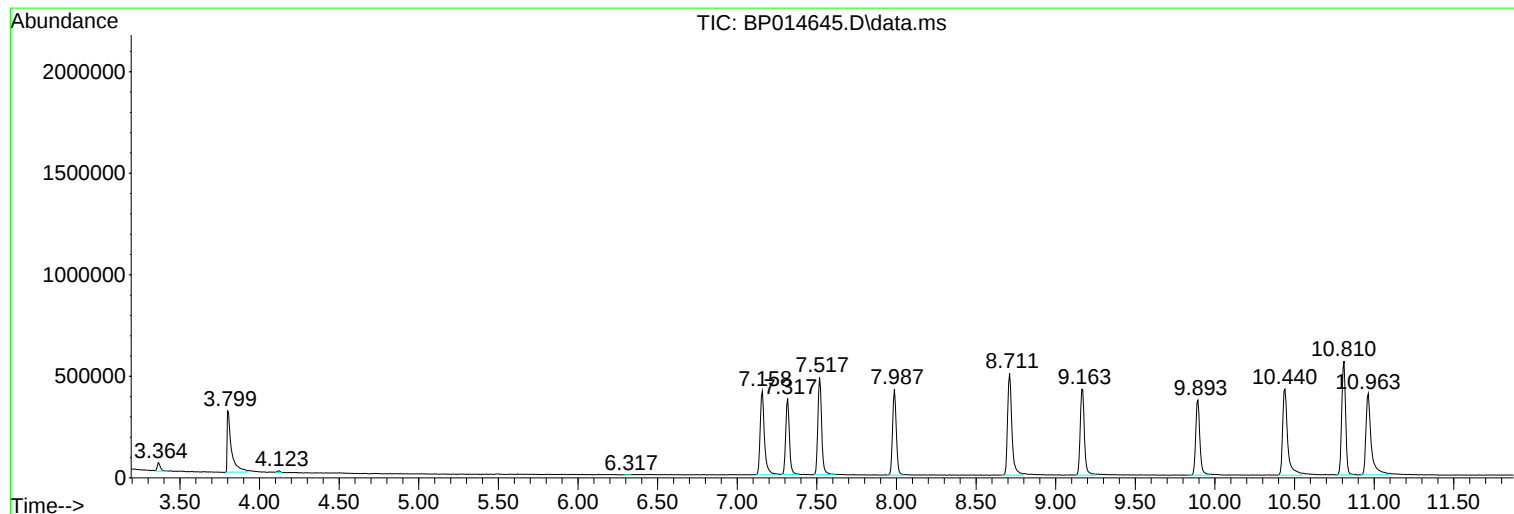

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014645.D
Acq On : 11 Apr 2023 08:54
Operator : CG/JU
Sample : PB152002BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014645.D
Acq On : 11 Apr 2023 08:54
Operator : CG/JU
Sample : PB152002BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc