

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
 Data File : BP014647.D
 Acq On : 11 Apr 2023 10:02
 Operator : CG/JU
 Sample : 02250-05DL 2X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHDx6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014647.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	19	24	32	rBV	869080	1196878	59.87%	5.179%
2	3.393	32	35	48	rVB	211837	286577	14.34%	1.240%
3	3.822	106	108	119	rBV2	28655	62945	3.15%	0.272%
4	4.111	154	157	166	rVB	14650	22870	1.14%	0.099%
5	4.222	174	176	180	rVB5	5542	6534	0.33%	0.028%
6	4.646	242	248	260	rBV	385569	570416	28.54%	2.468%
7	5.234	343	348	359	rVB2	33834	59294	2.97%	0.257%
8	5.958	469	471	475	rVB5	1778	2021	0.10%	0.009%
9	5.993	475	477	480	rBV4	2090	2412	0.12%	0.010%
10	6.110	494	497	500	rVV5	2024	2804	0.14%	0.012%
11	6.163	502	506	507	rVV3	2359	2428	0.12%	0.011%
12	6.193	507	511	514	rVB6	3161	4121	0.21%	0.018%
13	6.469	555	558	564	rBV8	3423	7543	0.38%	0.033%
14	6.646	586	588	591	rVB4	2276	2146	0.11%	0.009%
15	7.157	669	675	688	rBV	39846	110535	5.53%	0.478%
16	7.305	693	700	714	rBV	232604	391347	19.58%	1.694%
17	7.510	729	735	749	rBV	204701	398586	19.94%	1.725%
18	7.652	757	759	764	rVB6	4587	6042	0.30%	0.026%
19	7.857	791	794	796	rBV4	2280	2323	0.12%	0.010%
20	7.899	799	801	804	rVB3	1915	2071	0.10%	0.009%
21	7.975	804	814	823	rBV	508325	846534	42.35%	3.663%
22	8.334	871	875	880	rBV7	3602	6930	0.35%	0.030%
23	8.704	932	938	955	rBV	136248	303848	15.20%	1.315%
24	8.828	957	959	964	rVB6	2916	4525	0.23%	0.020%
25	8.910	971	973	978	rVB5	2040	2980	0.15%	0.013%
26	9.022	988	992	995	rVB6	2173	2979	0.15%	0.013%
27	9.157	1006	1015	1028	rBV	250400	477763	23.90%	2.068%
28	9.369	1050	1051	1055	rVB4	2484	2087	0.10%	0.009%
29	9.522	1074	1077	1080	rBV5	2408	2769	0.14%	0.012%
30	9.881	1130	1138	1152	rBV	204930	402045	20.11%	1.740%
31	10.357	1216	1219	1222	rVB4	1909	2367	0.12%	0.010%
32	10.434	1224	1232	1252	rBV	205033	544839	27.26%	2.358%
33	10.581	1252	1257	1275	rVV2	50026	178049	8.91%	0.771%
34	10.793	1286	1293	1307	rBV	683932	1196824	59.87%	5.179%
35	10.957	1315	1321	1331	rBV	69904	183548	9.18%	0.794%
36	11.145	1352	1353	1357	rVB4	2896	2245	0.11%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
 Data File : BP014647.D
 Acq On : 11 Apr 2023 10:02
 Operator : CG/JU
 Sample : 02250-05DL 2X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHDx6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	11.293	1373	1378	1380	rVB6	1469	2160	0.11%	0.009%
38	11.504	1410	1414	1415	rBV4	2375	2257	0.11%	0.010%
39	12.122	1516	1519	1521	rBV4	1974	2314	0.12%	0.010%
40	12.204	1526	1533	1537	rVB10	2373	5672	0.28%	0.025%
41	12.316	1549	1552	1554	rBV4	2104	2424	0.12%	0.010%
42	12.392	1562	1565	1569	rBV5	3365	4870	0.24%	0.021%
43	12.710	1615	1619	1621	rBV5	2168	2299	0.12%	0.010%
44	12.763	1624	1628	1632	rVV7	1650	2859	0.14%	0.012%
45	12.840	1638	1641	1643	rBV4	2081	2555	0.13%	0.011%
46	12.963	1658	1662	1663	rBV4	1958	2170	0.11%	0.009%
47	13.157	1689	1695	1697	rBV7	5710	10506	0.53%	0.045%
48	13.228	1704	1707	1713	rVB8	3208	6016	0.30%	0.026%
49	13.375	1727	1732	1735	rBV6	1582	3438	0.17%	0.015%
50	13.434	1740	1742	1744	rVB3	2924	2135	0.11%	0.009%
51	13.504	1752	1754	1757	rBV4	2470	2481	0.12%	0.011%
52	13.634	1772	1776	1784	rVB	14133	19483	0.97%	0.084%
53	13.939	1823	1828	1830	rBV5	3099	4881	0.24%	0.021%
54	13.957	1830	1831	1836	rVV5	2586	2690	0.13%	0.012%
55	14.039	1838	1845	1856	rVV	626668	940704	47.06%	4.071%
56	14.145	1859	1863	1871	rVB	6808	13957	0.70%	0.060%
57	14.234	1875	1878	1879	rBV3	1858	2000	0.10%	0.009%
58	14.322	1887	1893	1912	rBV	655783	988076	49.43%	4.276%
59	14.498	1920	1923	1927	rVB6	3147	4530	0.23%	0.020%
60	14.628	1938	1945	1957	rBV	1021256	1526713	76.37%	6.607%
61	14.775	1969	1970	1974	rVB4	2297	2143	0.11%	0.009%
62	14.869	1982	1986	1988	rBV5	2593	3437	0.17%	0.015%
63	14.951	1992	2000	2002	rBV9	7837	15853	0.79%	0.069%
64	15.081	2018	2022	2026	rBV7	2752	5165	0.26%	0.022%
65	15.128	2026	2030	2032	rVV5	2551	4090	0.20%	0.018%
66	15.404	2075	2077	2081	rVB5	2503	2854	0.14%	0.012%
67	15.457	2081	2086	2090	rBV8	9562	13060	0.65%	0.057%
68	15.557	2099	2103	2105	rVV5	2241	2536	0.13%	0.011%
69	15.628	2108	2115	2132	rBV	799240	1282389	64.15%	5.550%
70	15.763	2132	2138	2149	rBV2	148373	298357	14.93%	1.291%
71	16.004	2174	2179	2186	rVB4	15187	28504	1.43%	0.123%
72	16.086	2191	2193	2196	rVB4	4637	4333	0.22%	0.019%
73	16.110	2196	2197	2199	rBV2	2663	2418	0.12%	0.010%
74	16.322	2229	2233	2241	rBV2	17903	29798	1.49%	0.129%
75	16.410	2246	2248	2252	rVB5	1794	2291	0.11%	0.010%
76	16.510	2261	2265	2267	rBV4	3019	4084	0.20%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
 Data File : BP014647.D
 Acq On : 11 Apr 2023 10:02
 Operator : CG/JU
 Sample : 02250-05DL 2X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHDx6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

77	16.622	2281	2284	2286	rBV4	2100	2367	0.12%	0.010%
78	16.663	2289	2291	2294	rVV4	2046	2696	0.13%	0.012%
79	16.728	2300	2302	2304	rVB3	2014	2032	0.10%	0.009%
80	16.910	2331	2333	2335	rVB3	3919	3114	0.16%	0.013%
81	16.933	2335	2337	2340	rBV4	3281	4249	0.21%	0.018%
82	17.122	2366	2369	2373	rVB	18419	20156	1.01%	0.087%
83	17.180	2375	2379	2384	rVB8	7546	14560	0.73%	0.063%
84	17.216	2384	2385	2387	rBV2	2263	2201	0.11%	0.010%
85	17.275	2393	2395	2400	rVB6	2572	2766	0.14%	0.012%
86	17.392	2409	2415	2426	rBV	1197012	1670933	83.59%	7.231%
87	17.492	2426	2432	2445	rVV	905625	1350821	67.58%	5.846%
88	17.669	2458	2462	2467	rBV8	4431	6565	0.33%	0.028%
89	17.863	2491	2495	2498	rBV4	11412	15517	0.78%	0.067%
90	18.269	2560	2564	2568	rBV6	16005	29112	1.46%	0.126%
91	18.527	2606	2608	2613	rVB6	5970	6787	0.34%	0.029%
92	19.492	2770	2772	2779	rBV8	12705	19284	0.96%	0.083%
93	19.721	2806	2811	2820	rBV	1174279	1620386	81.06%	7.012%
94	21.480	3105	3110	3119	rBV	1310520	1926434	96.37%	8.337%
95	23.815	3501	3507	3519	rBV2	904845	1850379	92.57%	8.007%
96	23.980	3529	3535	3545	rVB2	963631	1998988	100.00%	8.651%




Sum of corrected areas: 23108074

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014647.D
Acq On : 11 Apr 2023 10:02
Operator : CG/JU
Sample : 02250-05DL 2X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHD6DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

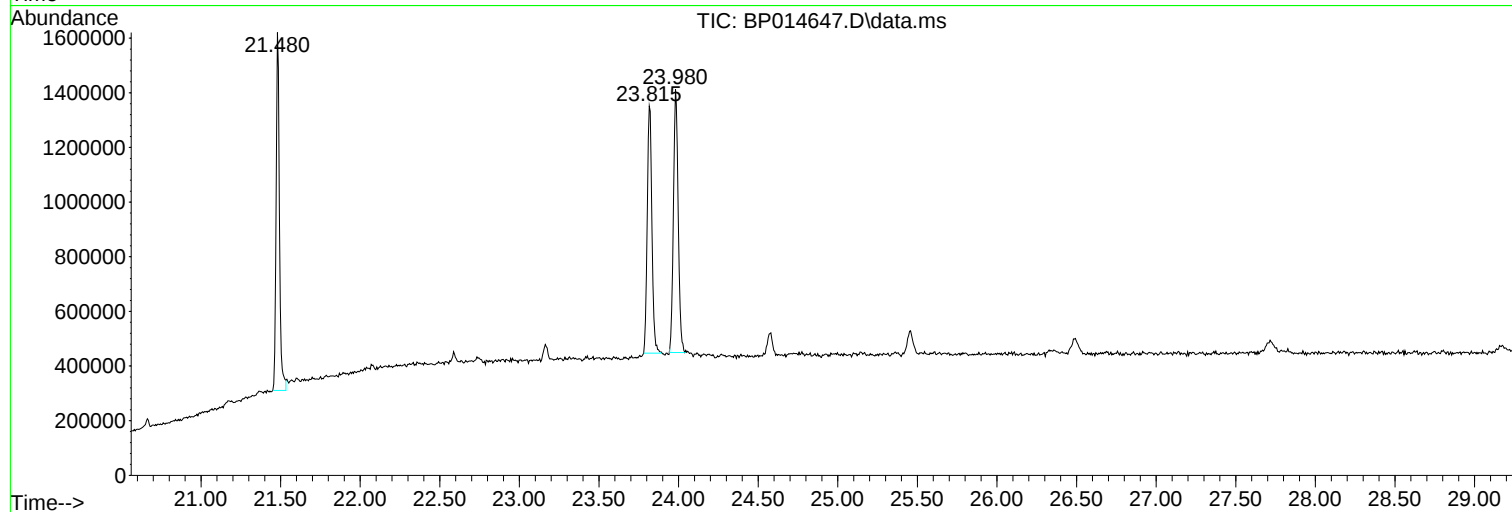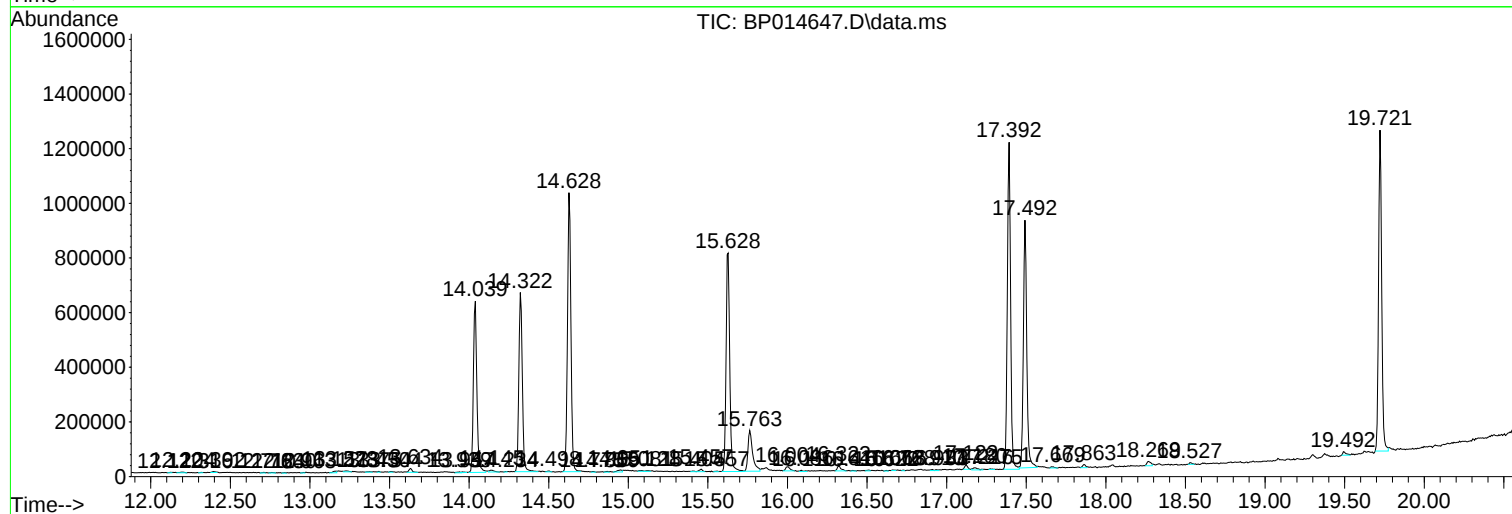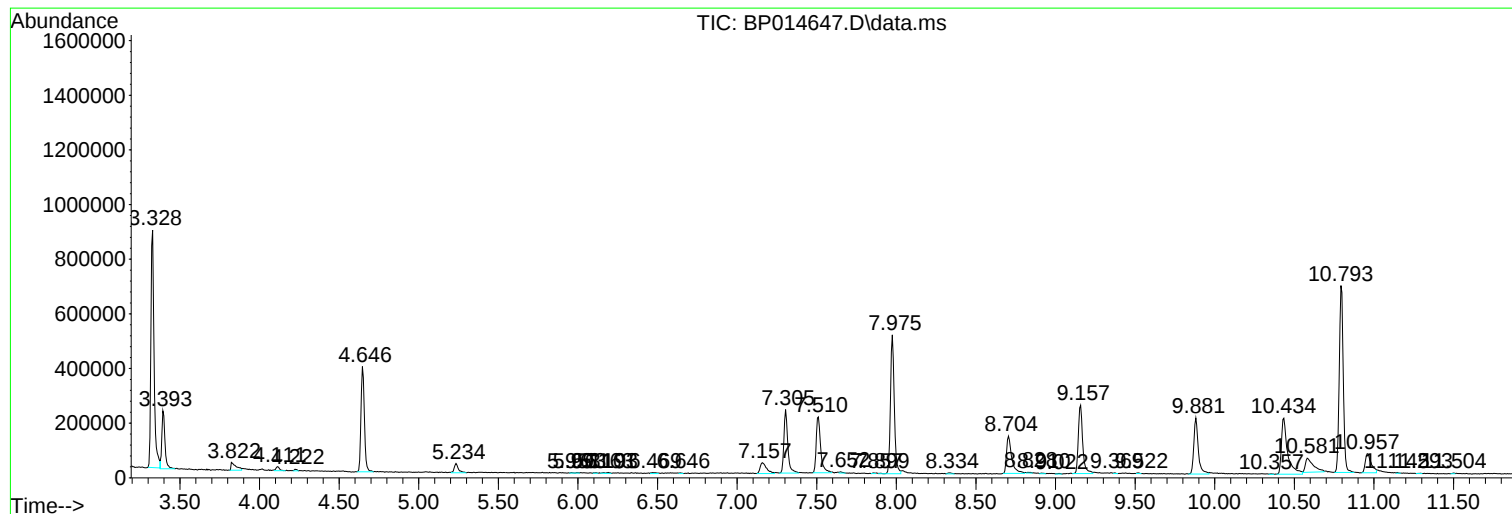

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014647.D
Acq On : 11 Apr 2023 10:02
Operator : CG/JU
Sample : 02250-05DL 2X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDx6DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.581	2.98 ng/ul	178049	Naphthalene-d8	10.793

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	86
2			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	86
3			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	83
4			Ethanol, 2-[2-(2-methylpropoxy)e...	162	C8H18O3	018912-80-6	72
5			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	72

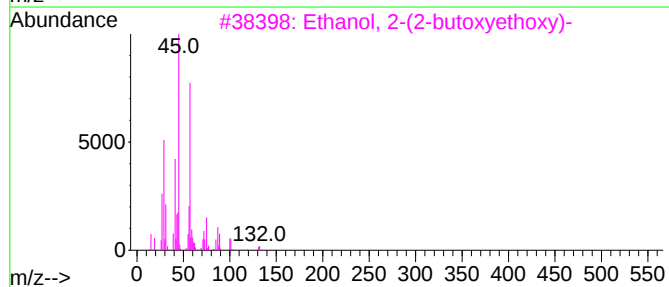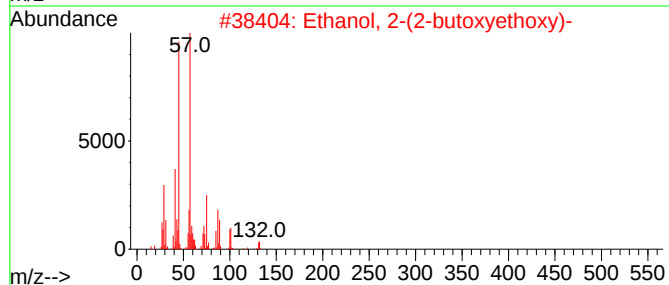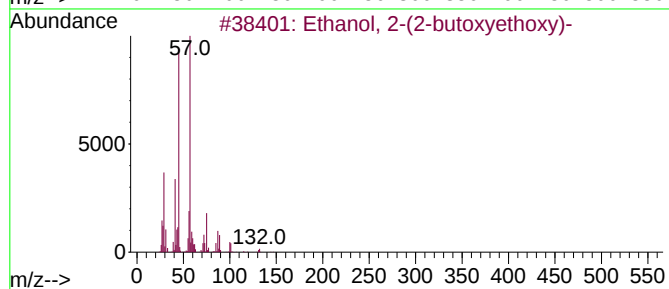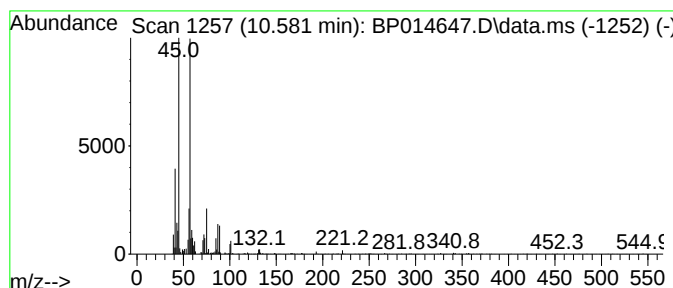

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014647.D
Acq On : 11 Apr 2023 10:02
Operator : CG/JU
Sample : 02250-05DL 2X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDx6DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.581	3.0	ng/u1	178049	2	10.793	1196820	20.0