

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
 Data File : BP014649.D
 Acq On : 11 Apr 2023 11:10
 Operator : CG/JU
 Sample : PB152026BL
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK026

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014649.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	26	30	36	rVB	48654	64352	1.78%	0.149%
2	3.793	101	103	131	rBV	508677	873841	24.11%	2.027%
3	4.117	154	158	162	rVB3	9663	13803	0.38%	0.032%
4	7.140	666	672	693	rBV	640827	1181763	32.61%	2.741%
5	7.305	693	700	710	rVV	578714	927040	25.58%	2.151%
6	7.505	727	734	752	rBV	722797	1212739	33.47%	2.813%
7	7.975	806	814	826	rBV	618273	1004954	27.73%	2.331%
8	8.693	929	936	953	rBV	803385	1500610	41.41%	3.481%
9	9.152	1006	1014	1030	rBV	729800	1274277	35.16%	2.956%
10	9.875	1129	1137	1150	rBV	624737	1111858	30.68%	2.579%
11	10.422	1220	1230	1252	rBV	743968	1518901	41.92%	3.524%
12	10.793	1285	1293	1304	rBV	909132	1531614	42.27%	3.553%
13	10.946	1310	1319	1343	rBV	762112	1662430	45.88%	3.857%
14	12.404	1559	1567	1576	rBV4	10141	24877	0.69%	0.058%
15	14.040	1838	1845	1860	rBV	1609220	2420708	66.80%	5.616%
16	14.322	1883	1893	1909	rBV	1859703	2765606	76.32%	6.416%
17	14.628	1938	1945	1957	rBV	1457324	2081709	57.45%	4.829%
18	14.863	1979	1985	2003	rBV	229826	741918	20.47%	1.721%
19	15.198	2040	2042	2049	rVB8	3000	5458	0.15%	0.013%
20	15.622	2108	2114	2131	rBV	2236035	3385446	93.42%	7.854%
21	15.757	2131	2137	2149	rVV	672676	1113868	30.74%	2.584%
22	15.863	2153	2155	2166	rVB8	14998	31703	0.87%	0.074%
23	16.416	2243	2249	2253	rVB9	3952	8182	0.23%	0.019%
24	17.128	2366	2370	2372	rBV5	2926	4286	0.12%	0.010%
25	17.186	2376	2380	2383	rVV5	4488	6079	0.17%	0.014%
26	17.392	2407	2415	2424	rBV	1629924	2388943	65.92%	5.542%
27	17.492	2425	2432	2448	rVV	2485817	3623755	100.00%	8.406%
28	17.933	2504	2507	2510	rVB5	2837	3727	0.10%	0.009%
29	19.298	2736	2739	2744	rBV3	26529	34415	0.95%	0.080%
30	19.375	2748	2752	2755	rBV	20909	30738	0.85%	0.071%
31	19.722	2805	2811	2827	rBV	2728882	3621469	99.94%	8.401%
32	21.480	3105	3110	3123	rBV	1184313	1895183	52.30%	4.396%
33	23.816	3501	3507	3522	rVB2	1510002	3179768	87.75%	7.376%
34	23.986	3529	3536	3548	rVB2	841557	1861178	51.36%	4.318%

Sum of corrected areas: 43107198




Instrument :
BNA_P
ClientSampleId :
SBLK026

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014649.D
Acq On : 11 Apr 2023 11:10
Operator : CG/JU
Sample : PB152026BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK026

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

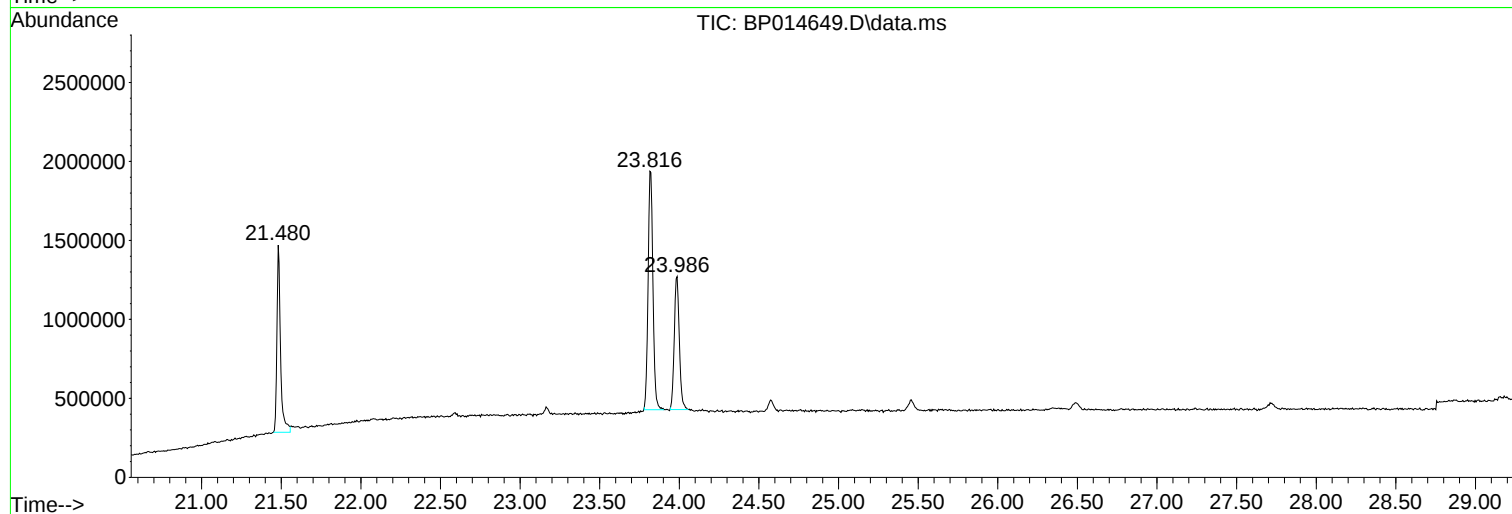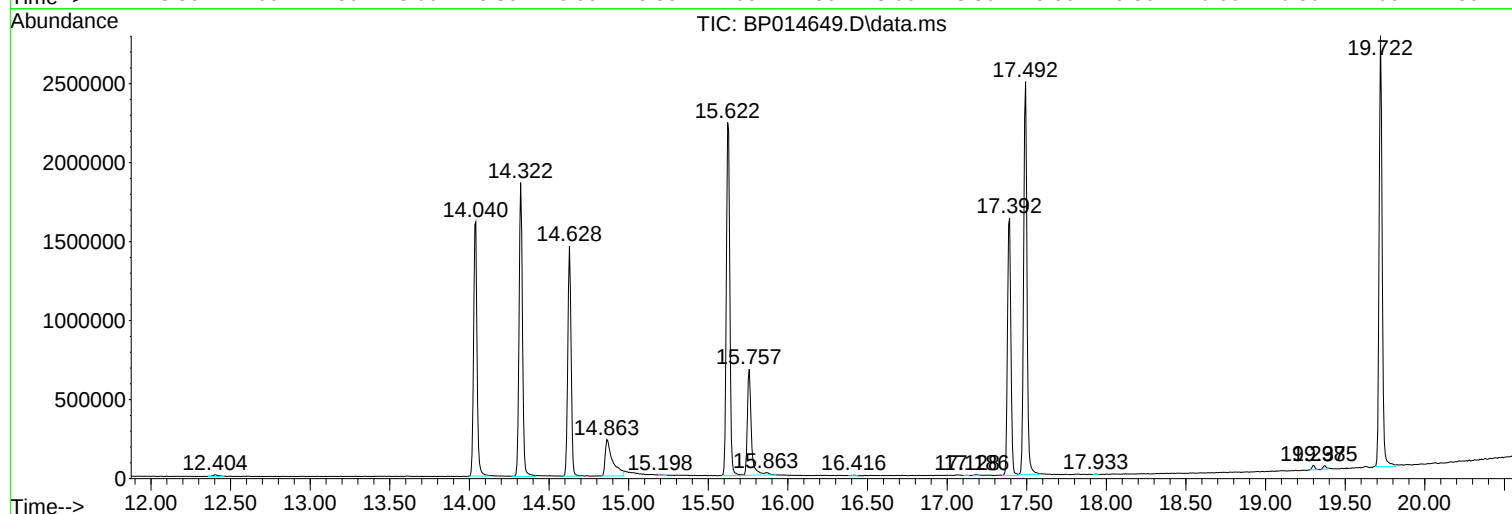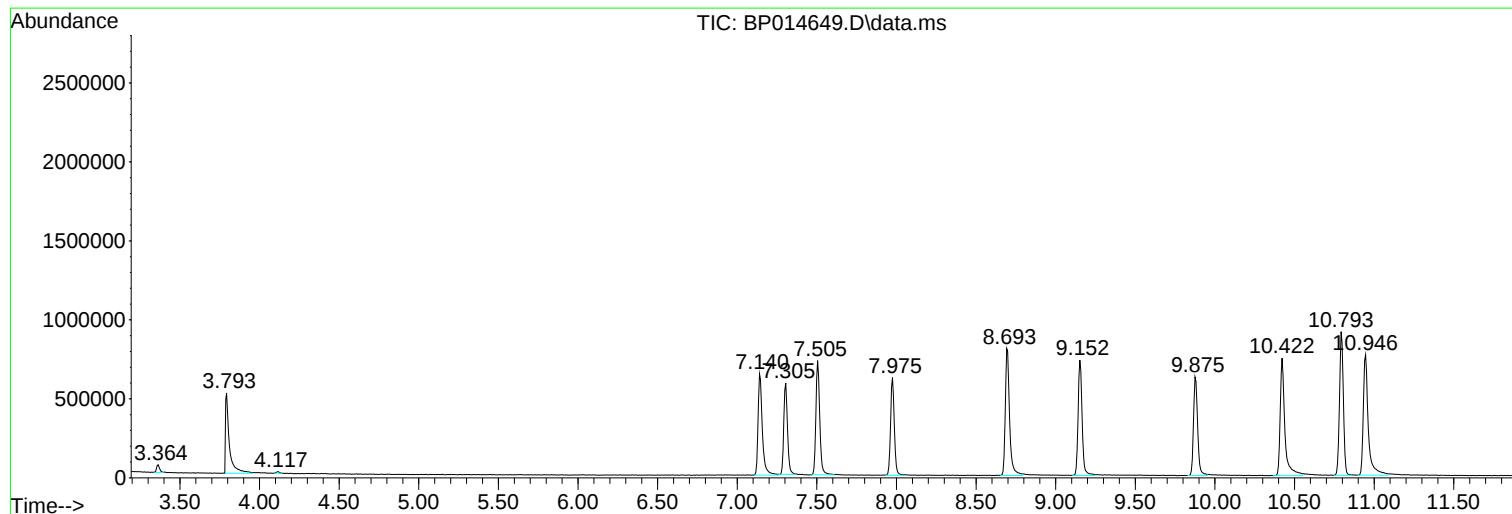

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014649.D
Acq On : 11 Apr 2023 11:10
Operator : CG/JU
Sample : PB152026BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK026

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014649.D
Acq On : 11 Apr 2023 11:10
Operator : CG/JU
Sample : PB152026BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK026

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc