

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
 Data File : BP014650.D
 Acq On : 11 Apr 2023 11:44
 Operator : CG/JU
 Sample : PB152027BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK027

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014650.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.363	26	30	38	rBV	49218	65551	1.97%	0.161%
2	3.793	100	103	120	rBV	529875	864115	25.95%	2.128%
3	4.063	147	149	153	rBV5	3289	4192	0.13%	0.010%
4	4.116	154	158	163	rVB	11520	15150	0.45%	0.037%
5	5.387	369	374	377	rVB7	2076	4180	0.13%	0.010%
6	7.140	666	672	686	rBV	642560	1195529	35.90%	2.944%
7	7.304	694	700	712	rBV	587188	942722	28.31%	2.322%
8	7.504	727	734	754	rBV	747844	1244199	37.36%	3.064%
9	7.975	807	814	828	rBV	596800	963901	28.94%	2.374%
10	8.692	930	936	955	rBV	817255	1511578	45.39%	3.722%
11	9.151	1005	1014	1030	rBV	737576	1277528	38.36%	3.146%
12	9.316	1040	1042	1046	rVB5	3881	4554	0.14%	0.011%
13	9.875	1130	1137	1156	rBV	622449	1133051	34.02%	2.790%
14	10.422	1223	1230	1254	rBV	738277	1521786	45.70%	3.748%
15	10.792	1286	1293	1310	rBV	852222	1441426	43.28%	3.550%
16	10.945	1312	1319	1346	rBV	796080	1663014	49.94%	4.095%
17	12.398	1560	1566	1575	rBV8	8657	23587	0.71%	0.058%
18	12.751	1623	1626	1631	rVB7	2485	3903	0.12%	0.010%
19	14.039	1835	1845	1861	rBV	1507445	2261104	67.90%	5.568%
20	14.322	1886	1893	1910	rBV	1750001	2595635	77.94%	6.392%
21	14.627	1936	1945	1962	rBV	1227347	1844290	55.38%	4.542%
22	14.869	1978	1986	2023	rBV	184926	771157	23.16%	1.899%
23	15.627	2107	2115	2130	rBV	1980753	3082109	92.55%	7.590%
24	15.757	2131	2137	2153	rVV	581064	966303	29.02%	2.380%
25	15.869	2153	2156	2161	rVB7	12801	24112	0.72%	0.059%
26	16.204	2210	2213	2217	rVB6	2299	3351	0.10%	0.008%
27	16.410	2242	2248	2249	rBV6	2631	4246	0.13%	0.010%
28	16.921	2332	2335	2338	rBV4	3342	4098	0.12%	0.010%
29	17.063	2356	2359	2365	rVB8	3629	6197	0.19%	0.015%
30	17.180	2375	2379	2384	rVB6	4296	7005	0.21%	0.017%
31	17.392	2407	2415	2425	rBV	1339560	1947661	58.48%	4.796%
32	17.492	2425	2432	2450	rVV	2149321	3152839	94.67%	7.764%
33	19.298	2736	2739	2746	rVB4	26269	40226	1.21%	0.099%
34	19.374	2748	2752	2759	rVB2	21007	40437	1.21%	0.100%
35	19.721	2805	2811	2825	rBV	2304855	3185583	95.66%	7.845%
36	21.486	3106	3111	3120	rBV	1007530	1623864	48.76%	3.999%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014650.D
Acq On : 11 Apr 2023 11:44
Operator : CG/JU
Sample : PB152027BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK027

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Title : SVOA CALIBRATION

37	23.821	3501	3508	3522	rVB2	1631249	3330249	100.00%	8.201%
38	23.986	3529	3536	3550	rVB2	819502	1836678	55.15%	4.523%




Sum of corrected areas: 40607110

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014650.D
Acq On : 11 Apr 2023 11:44
Operator : CG/JU
Sample : PB152027BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK027

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

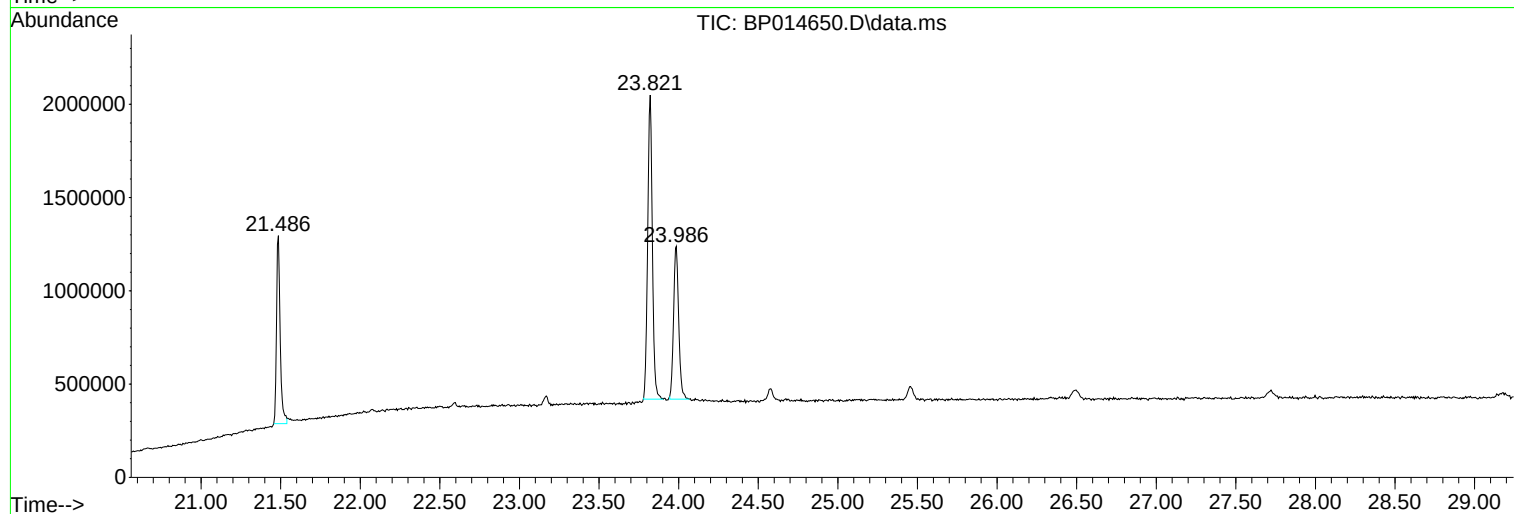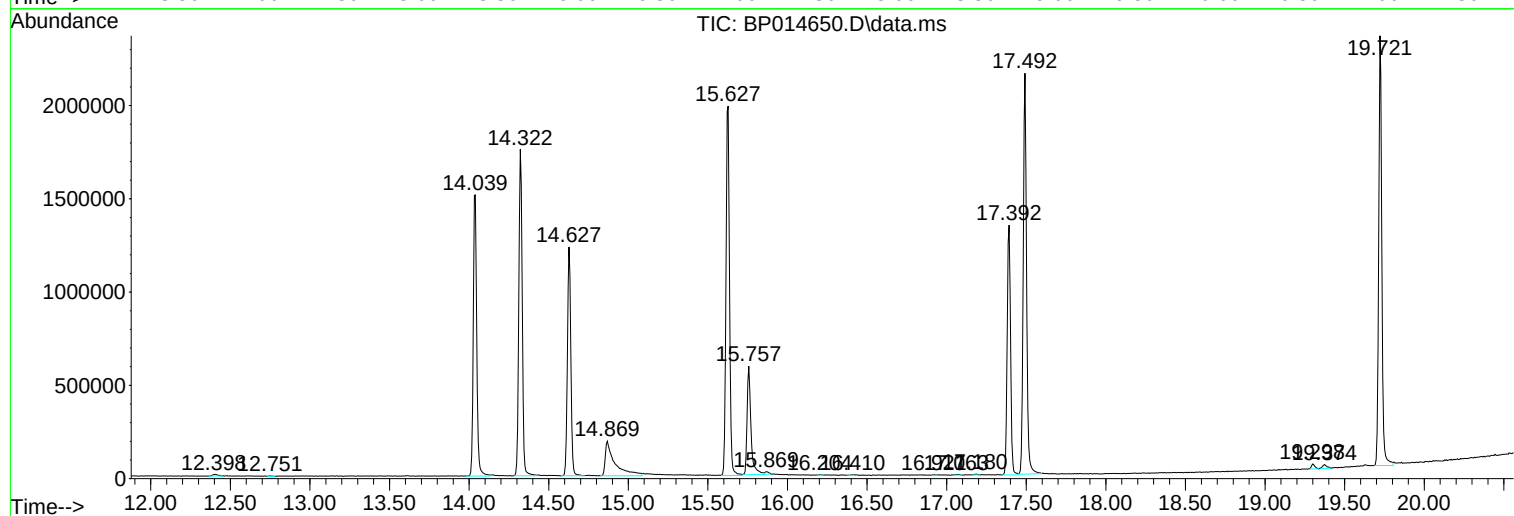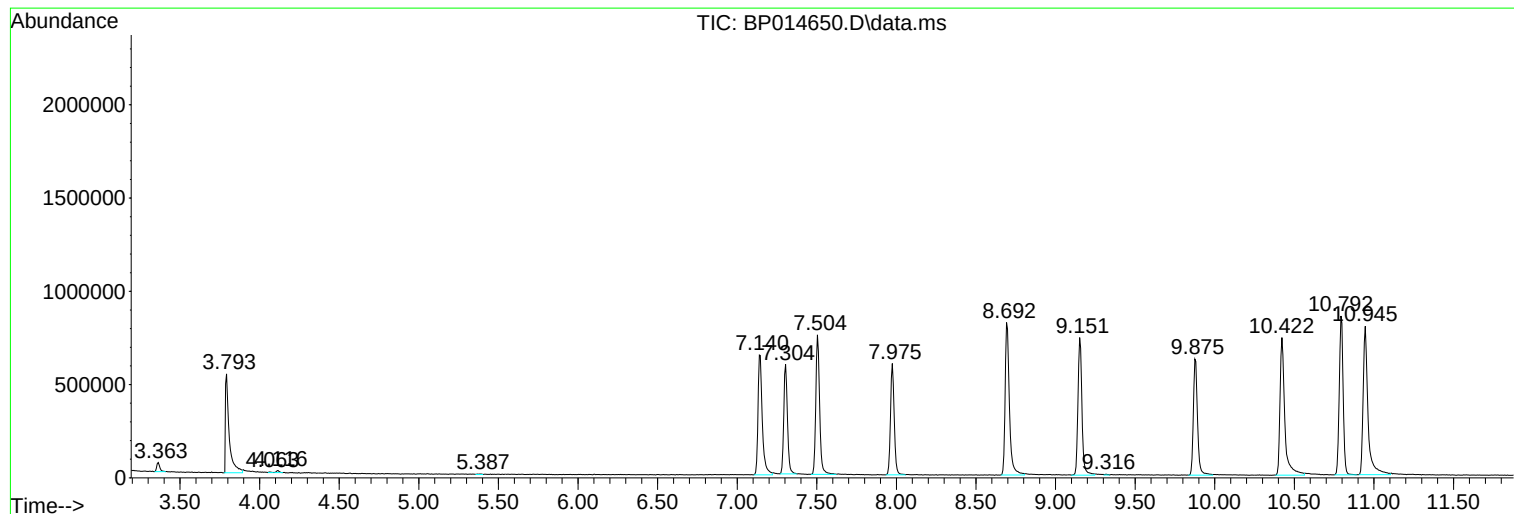

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014650.D
Acq On : 11 Apr 2023 11:44
Operator : CG/JU
Sample : PB152027BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK027

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014650.D
Acq On : 11 Apr 2023 11:44
Operator : CG/JU
Sample : PB152027BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK027

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------