

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
 Data File : BP014652.D
 Acq On : 11 Apr 2023 12:52
 Operator : CG/JU
 Sample : 02251-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COMB9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014652.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	27	30	37	rVB	34260	42943	1.20%	0.128%
2	4.017	136	141	146	rVB	16815	24842	0.69%	0.074%
3	4.117	155	158	164	rVB3	10505	16071	0.45%	0.048%
4	4.228	173	177	182	rVB5	10092	15283	0.43%	0.046%
5	5.046	311	316	324	rBV	11167	18376	0.51%	0.055%
6	6.358	533	539	544	rBV4	7361	11176	0.31%	0.033%
7	7.063	656	659	664	rVB7	3469	5028	0.14%	0.015%
8	7.152	667	674	689	rBV	83522	194953	5.45%	0.582%
9	7.305	693	700	711	rBV	524349	857687	23.99%	2.563%
10	7.505	726	734	755	rBV	470322	845823	23.66%	2.527%
11	7.975	806	814	833	rBV	520232	922736	25.81%	2.757%
12	8.340	870	876	881	rBV8	5397	10945	0.31%	0.033%
13	8.699	930	937	955	rBV	297101	590817	16.53%	1.765%
14	9.152	1006	1014	1032	rBV	648344	1133628	31.71%	3.387%
15	9.293	1033	1038	1040	rBV6	7929	10667	0.30%	0.032%
16	9.516	1074	1076	1082	rVB5	6391	9116	0.26%	0.027%
17	9.881	1125	1138	1149	rBV	499600	921649	25.78%	2.754%
18	10.428	1223	1231	1259	rBV	472426	1177428	32.94%	3.518%
19	10.793	1285	1293	1309	rBV	736603	1244027	34.80%	3.717%
20	10.963	1315	1322	1334	rBV2	58515	167932	4.70%	0.502%
21	11.551	1418	1422	1425	rBV5	2212	3972	0.11%	0.012%
22	12.016	1494	1501	1506	rVB4	6321	11442	0.32%	0.034%
23	12.193	1527	1531	1533	rBV5	3480	5165	0.14%	0.015%
24	12.404	1558	1567	1573	rBV5	9211	23577	0.66%	0.070%
25	13.434	1735	1742	1746	rBV10	4881	7980	0.22%	0.024%
26	13.504	1746	1754	1760	rBV2	10832	24122	0.67%	0.072%
27	14.034	1833	1844	1860	rBV	1257697	1954557	54.68%	5.840%
28	14.140	1860	1862	1868	rVB7	5164	7979	0.22%	0.024%
29	14.257	1880	1882	1886	rBV4	2864	4405	0.12%	0.013%
30	14.322	1886	1893	1912	rVV	1587485	2268072	63.45%	6.776%
31	14.628	1938	1945	1958	rBV	1054525	1573810	44.03%	4.702%
32	14.710	1958	1959	1964	rVB5	3700	4029	0.11%	0.012%
33	14.945	1992	1999	2000	rBV6	11756	23429	0.66%	0.070%
34	15.281	2050	2056	2060	rVB8	4115	7481	0.21%	0.022%
35	15.375	2066	2072	2076	rBV	102536	153400	4.29%	0.458%
36	15.628	2107	2115	2132	rBV	1797200	2746155	76.82%	8.205%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
 Data File : BP014652.D
 Acq On : 11 Apr 2023 12:52
 Operator : CG/JU
 Sample : 02251-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COMB9

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	15.757	2132	2137	2153	rVV	474223	844654	23.63%	2.524%
38	15.869	2153	2156	2166	rVB6	13807	25398	0.71%	0.076%
39	15.998	2172	2178	2187	rBV	30649	54237	1.52%	0.162%
40	17.069	2357	2360	2364	rVB6	2803	3832	0.11%	0.011%
41	17.122	2366	2369	2372	rBV4	2476	4360	0.12%	0.013%
42	17.392	2408	2415	2425	rBV	1211281	1699829	47.55%	5.079%
43	17.492	2425	2432	2447	rBV	1984563	2886451	80.75%	8.624%
44	18.263	2558	2563	2573	rBV3	84442	168855	4.72%	0.505%
45	19.304	2735	2740	2746	rBV4	27115	47245	1.32%	0.141%
46	19.375	2748	2752	2759	rVV2	19564	41168	1.15%	0.123%
47	19.492	2768	2772	2779	rBV4	56637	116856	3.27%	0.349%
48	19.722	2805	2811	2824	rBV	2305324	3196250	89.41%	9.550%
49	21.480	3105	3110	3120	rBV	1146141	1790388	50.08%	5.349%
50	21.563	3121	3124	3127	rVB2	85434	106990	2.99%	0.320%
51	23.821	3501	3508	3521	rVB2	1736021	3574764	100.00%	10.681%
52	23.986	3529	3536	3546	rVB2	859191	1867746	52.25%	5.580%




Sum of corrected areas: 33469725

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014652.D
Acq On : 11 Apr 2023 12:52
Operator : CG/JU
Sample : 02251-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMB9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

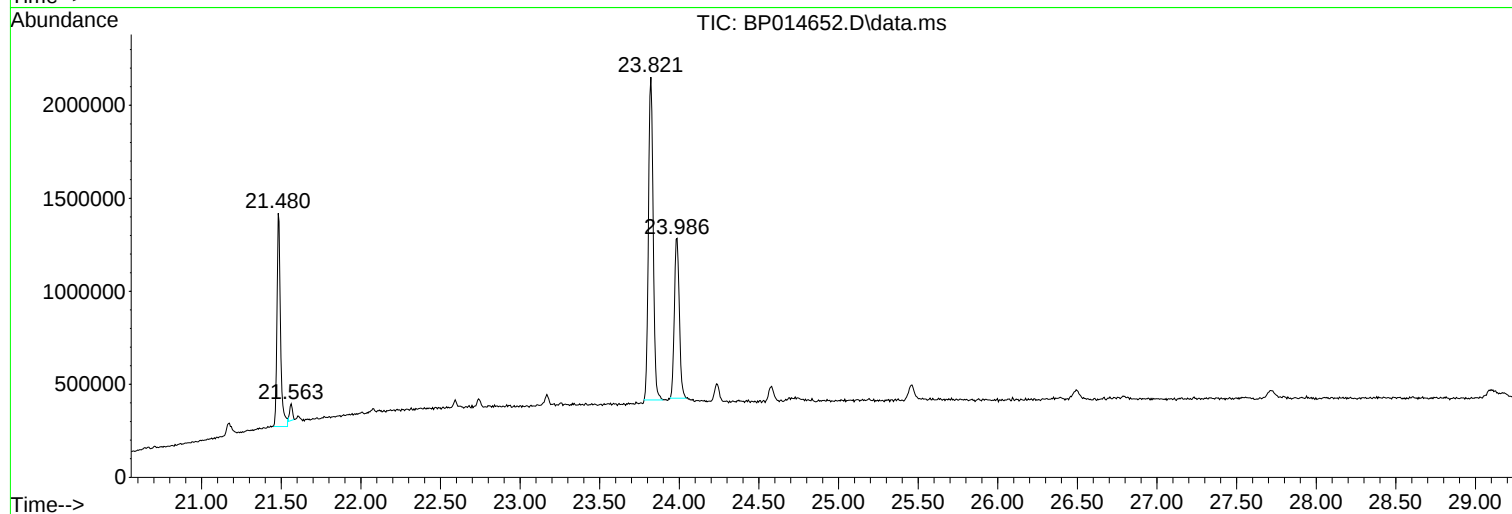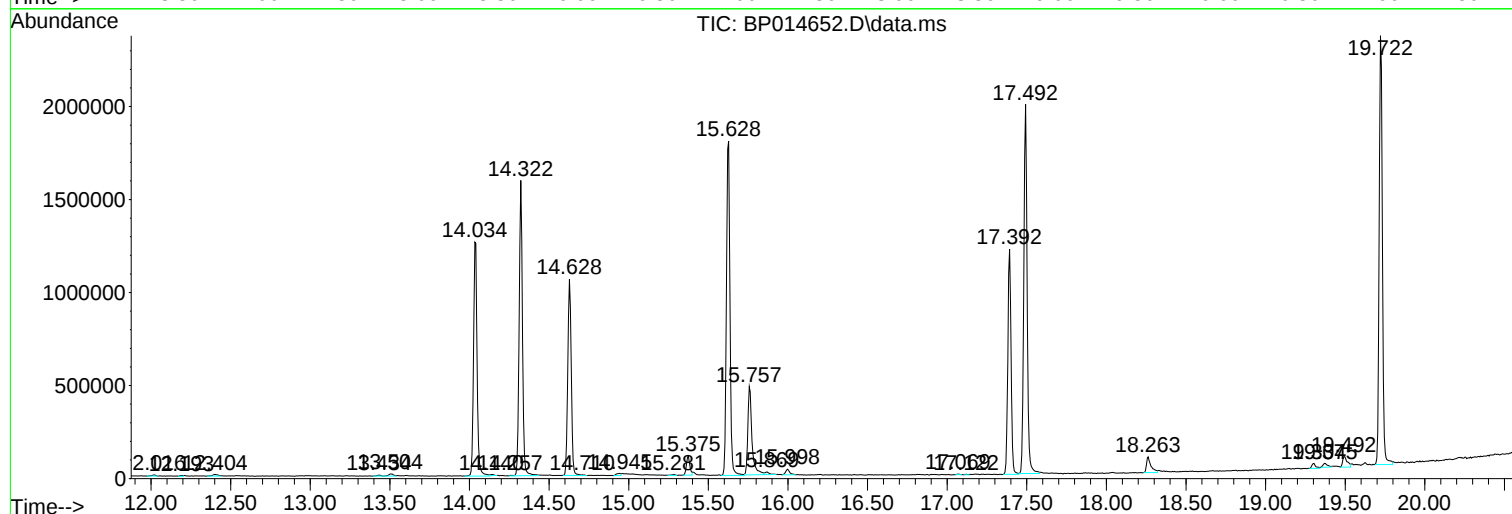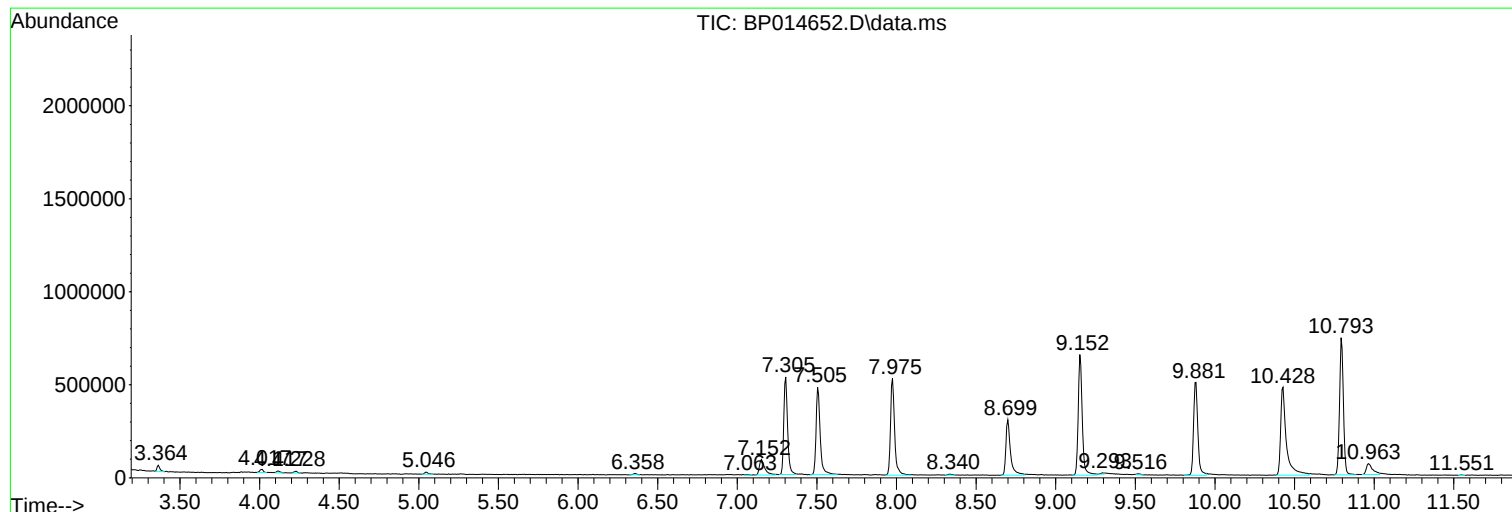

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014652.D
Acq On : 11 Apr 2023 12:52
Operator : CG/JU
Sample : 02251-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMB9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014652.D
Acq On : 11 Apr 2023 12:52
Operator : CG/JU
Sample : 02251-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0MB9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc