

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
 Data File : BP014656.D
 Acq On : 11 Apr 2023 15:09
 Operator : CG/JU
 Sample : 02251-05
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COMC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014656.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	27	30	35	rBV2	14975	20008	0.61%	0.064%
2	4.017	138	141	146	rVB3	11695	16340	0.50%	0.052%
3	4.111	154	157	164	rVB3	11057	17135	0.53%	0.055%
4	4.223	174	176	182	rVB7	5038	8245	0.25%	0.026%
5	5.046	312	316	321	rBV2	8451	11329	0.35%	0.036%
6	6.364	534	540	544	rBV7	4259	7235	0.22%	0.023%
7	7.152	667	674	686	rBV	75250	178495	5.48%	0.573%
8	7.305	693	700	715	rBV	448777	738825	22.69%	2.374%
9	7.505	728	734	749	rBV	407590	733604	22.52%	2.357%
10	7.975	807	814	823	rBV	553538	912975	28.03%	2.933%
11	8.699	931	937	956	rBV	264203	539015	16.55%	1.732%
12	9.152	1007	1014	1033	rBV	533157	965458	29.64%	3.102%
13	9.522	1072	1077	1084	rVB6	7066	11111	0.34%	0.036%
14	9.881	1131	1138	1157	rBV	420462	802744	24.65%	2.579%
15	10.428	1224	1231	1258	rBV	399119	1030487	31.64%	3.311%
16	10.793	1285	1293	1307	rBV	763727	1301462	39.96%	4.181%
17	10.969	1317	1323	1348	rBV	51421	174851	5.37%	0.562%
18	12.199	1525	1532	1540	rBV9	6178	13390	0.41%	0.043%
19	12.399	1559	1566	1567	rBV6	7052	8690	0.27%	0.028%
20	13.010	1666	1670	1675	rBV7	2545	3333	0.10%	0.011%
21	13.428	1736	1741	1745	rBV6	6684	10004	0.31%	0.032%
22	14.040	1838	1845	1858	rBV	1116904	1692882	51.98%	5.439%
23	14.140	1860	1862	1866	rVB5	6194	8403	0.26%	0.027%
24	14.322	1886	1893	1910	rVV	1308195	1960781	60.20%	6.299%
25	14.498	1921	1923	1931	rVB8	4198	6301	0.19%	0.020%
26	14.628	1938	1945	1957	rBV	1122712	1645105	50.51%	5.285%
27	14.940	1994	1998	2001	rBV4	9272	15532	0.48%	0.050%
28	15.316	2060	2062	2065	rBV4	3071	3822	0.12%	0.012%
29	15.451	2083	2085	2089	rBV5	3062	5142	0.16%	0.017%
30	15.622	2108	2114	2126	rBV	1563788	2398548	73.65%	7.706%
31	15.763	2132	2138	2153	rBV	387170	734239	22.54%	2.359%
32	15.863	2153	2155	2161	rVB6	8649	14262	0.44%	0.046%
33	15.998	2172	2178	2189	rVB	68495	122037	3.75%	0.392%
34	16.863	2323	2325	2329	rBV5	4753	6304	0.19%	0.020%
35	16.910	2329	2333	2339	rVB8	11660	18274	0.56%	0.059%
36	17.392	2408	2415	2425	rBV	1229806	1788708	54.92%	5.747%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
 Data File : BP014656.D
 Acq On : 11 Apr 2023 15:09
 Operator : CG/JU
 Sample : 02251-05
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COMC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	17.492	2425	2432	2450	rVV	1736022	2588100	79.47%	8.315%
38	17.869	2494	2496	2499	rBV3	3894	4592	0.14%	0.015%
39	18.263	2559	2563	2574	rBV2	72205	158381	4.86%	0.509%
40	19.304	2736	2740	2744	rVB6	19382	28863	0.89%	0.093%
41	19.375	2749	2752	2760	rVB2	17262	33664	1.03%	0.108%
42	19.504	2770	2774	2782	rBV8	23066	64396	1.98%	0.207%
43	19.722	2806	2811	2826	rBV	2046470	2829274	86.87%	9.090%
44	21.169	3052	3057	3066	rBV4	119377	309660	9.51%	0.995%
45	21.486	3106	3111	3122	rBV	1207708	1878908	57.69%	6.036%
46	23.822	3501	3508	3519	rBV2	1607059	3256860	100.00%	10.463%
47	23.986	3530	3536	3549	rVB2	932578	2048762	62.91%	6.582%




Sum of corrected areas: 31126536

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014656.D
Acq On : 11 Apr 2023 15:09
Operator : CG/JU
Sample : 02251-05
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

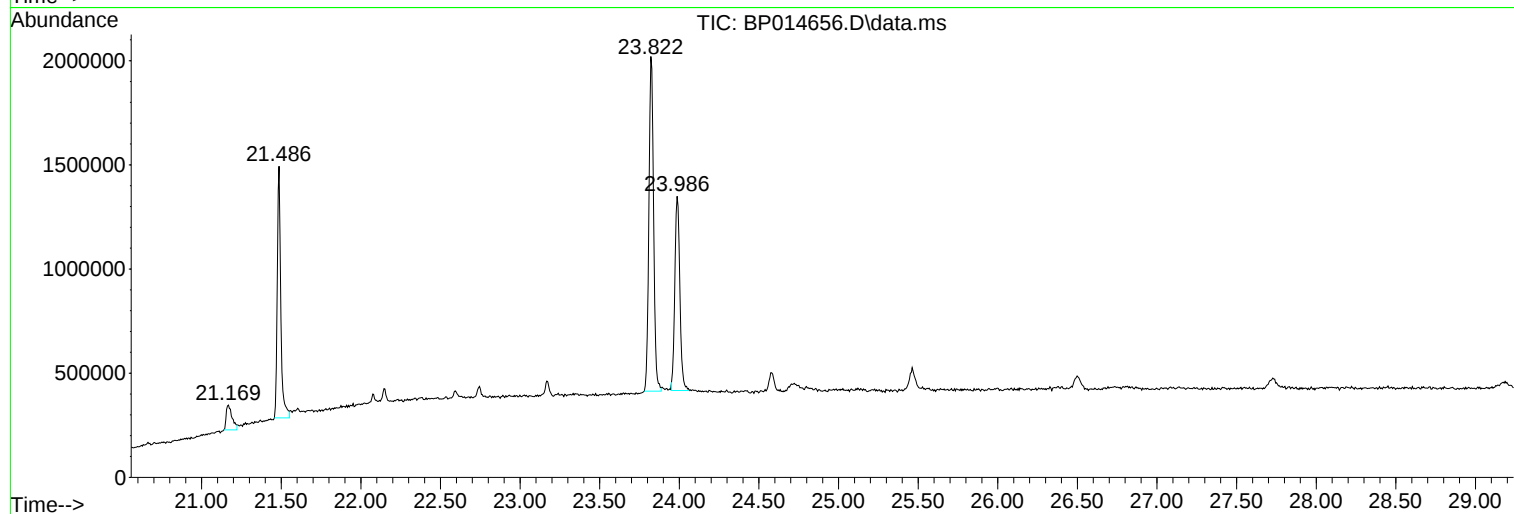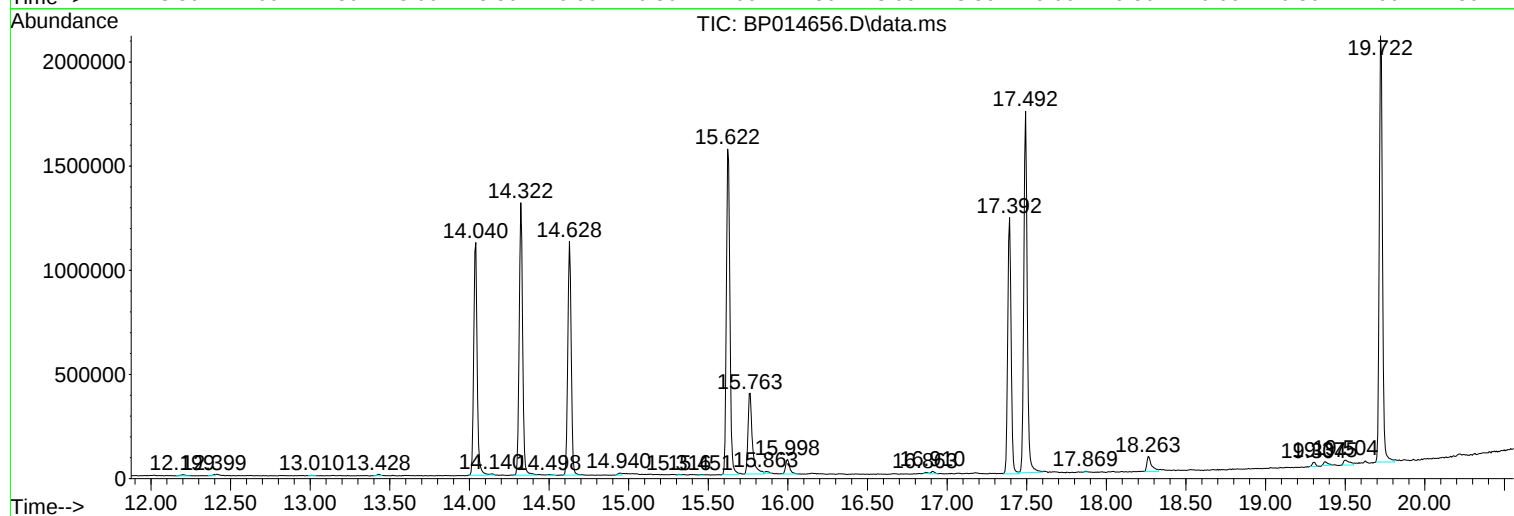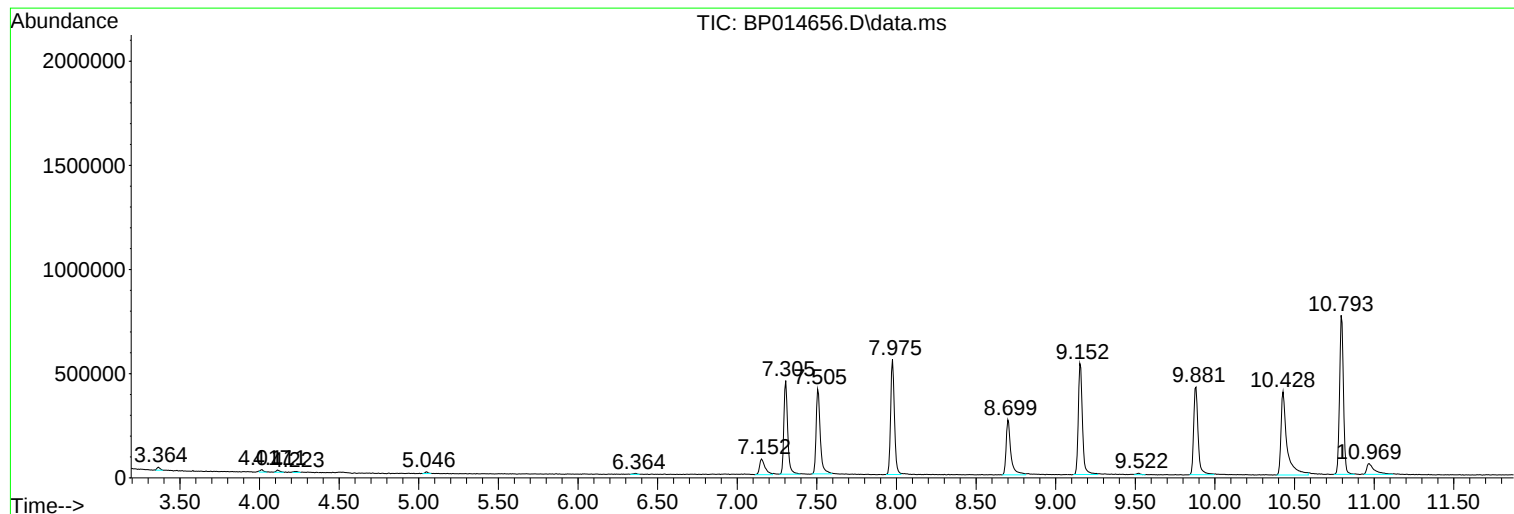

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014656.D
Acq On : 11 Apr 2023 15:09
Operator : CG/JU
Sample : 02251-05
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMC3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic21.169 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.169	3.30 ng/ul	309660	Chrysene-d12	21.486

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclotetracosane	336	C24H48	000297-03-0	95
2			Cyclotetracosane	336	C24H48	000297-03-0	93
3			1-Hexacosene	364	C26H52	018835-33-1	93
4			n-Tetracosanol-1	354	C24H50O	000506-51-4	90
5			Trichloroacetic acid, pentadecyl...	372	C17H31Cl3O2	074339-53-0	90

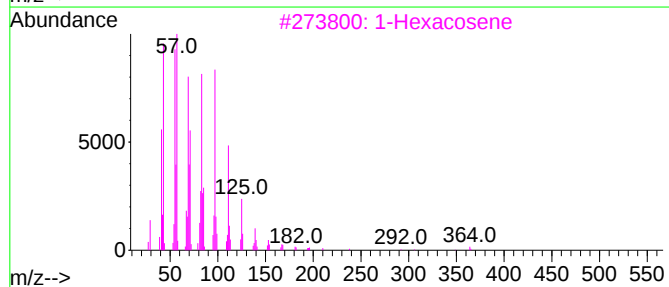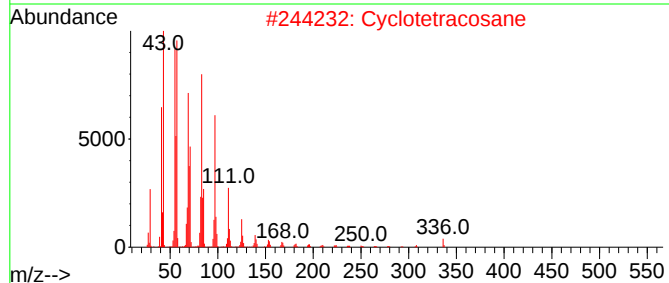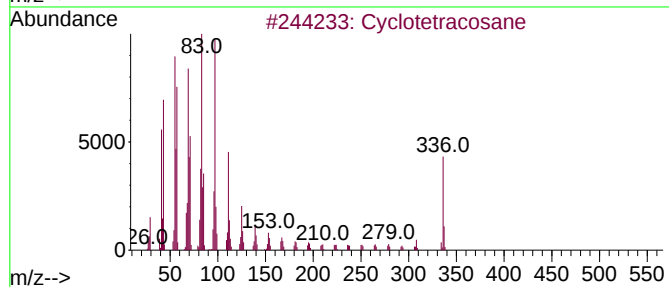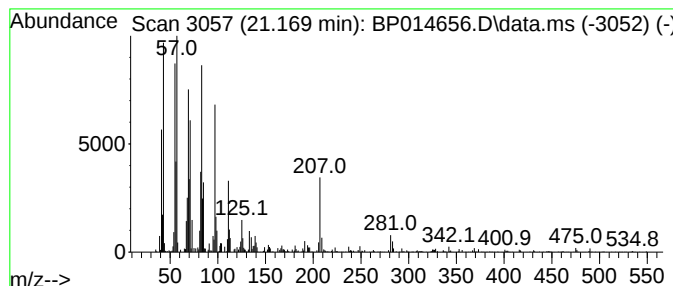

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014656.D
Acq On : 11 Apr 2023 15:09
Operator : CG/JU
Sample : 02251-05
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0MC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	21.169	3.3	ng/u1	309660	5	21.486	1878910	20.0