

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
 Data File : BP014660.D
 Acq On : 11 Apr 2023 17:26
 Operator : CG/JU
 Sample : 02251-09
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COMC7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014660.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	27	30	33	rBV	19638	23102	0.16%	0.032%
2	3.399	33	36	42	rVB	42236	55190	0.38%	0.078%
3	3.805	103	105	121	rBV	111845	208835	1.43%	0.294%
4	4.116	153	158	164	rBV2	11489	17243	0.12%	0.024%
5	5.263	345	353	368	rBV	9596989	14609229	100.00%	20.545%
6	7.146	668	673	689	rBV	148142	281978	1.93%	0.397%
7	7.310	692	701	719	rBV	7979071	13424774	91.89%	18.880%
8	7.504	728	734	750	rVB	587651	986957	6.76%	1.388%
9	7.863	788	795	805	rVB	234913	389890	2.67%	0.548%
10	7.975	807	814	816	rBV	602151	970220	6.64%	1.364%
11	8.010	816	820	836	rVB	3228197	4996091	34.20%	7.026%
12	8.328	867	874	884	rBV	1887475	3041561	20.82%	4.277%
13	8.699	929	937	955	rBV	389228	754512	5.16%	1.061%
14	9.151	1007	1014	1033	rBV	688100	1230665	8.42%	1.731%
15	9.822	1120	1128	1132	rBV	95532	162337	1.11%	0.228%
16	9.875	1132	1137	1152	rVB	547067	1006632	6.89%	1.416%
17	10.422	1223	1230	1254	rBV	683712	1384129	9.47%	1.947%
18	10.657	1263	1270	1277	rVB	147430	243894	1.67%	0.343%
19	10.793	1285	1293	1306	rBV	783969	1345013	9.21%	1.892%
20	10.916	1307	1314	1317	rBV	825878	1555415	10.65%	2.187%
21	11.181	1354	1359	1367	rVB2	24875	47469	0.32%	0.067%
22	12.404	1558	1567	1572	rBV6	9054	22638	0.15%	0.032%
23	13.722	1784	1791	1797	rBV6	5832	14702	0.10%	0.021%
24	14.039	1838	1845	1858	rBV	1457502	2093680	14.33%	2.944%
25	14.322	1886	1893	1910	rBV	1655470	2427997	16.62%	3.415%
26	14.628	1938	1945	1955	rBV	1134018	1650912	11.30%	2.322%
27	14.934	1990	1997	2001	rBV7	16000	41703	0.29%	0.059%
28	15.628	2108	2115	2131	rBV	1875466	2902988	19.87%	4.083%
29	15.757	2131	2137	2153	rVV	492600	875718	5.99%	1.232%
30	15.869	2153	2156	2162	rVB6	13055	19007	0.13%	0.027%
31	15.998	2172	2178	2187	rBV	61382	101709	0.70%	0.143%
32	17.392	2408	2415	2425	rBV	1189007	1706552	11.68%	2.400%
33	17.492	2425	2432	2453	rVV2	1877335	2887369	19.76%	4.061%
34	18.269	2559	2564	2572	rBV7	36185	81784	0.56%	0.115%
35	19.298	2736	2739	2747	rBV5	23850	34935	0.24%	0.049%
36	19.380	2748	2753	2757	rBV5	22178	42850	0.29%	0.060%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014660.D
Acq On : 11 Apr 2023 17:26
Operator : CG/JU
Sample : 02251-09
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0MC7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Title : SVOA CALIBRATION

37	19.504	2770	2774	2781	rBV7	21145	50222	0.34%	0.071%
38	19.721	2806	2811	2821	rBV	2067614	2890745	19.79%	4.065%
39	21.486	3106	3111	3122	rBV	1006439	1577483	10.80%	2.218%
40	23.821	3501	3508	3522	rVB2	1516190	3211658	21.98%	4.517%
41	23.986	3530	3536	3549	rVB2	782380	1737004	11.89%	2.443%




Sum of corrected areas: 71106792

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014660.D
Acq On : 11 Apr 2023 17:26
Operator : CG/JU
Sample : 02251-09
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMC7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

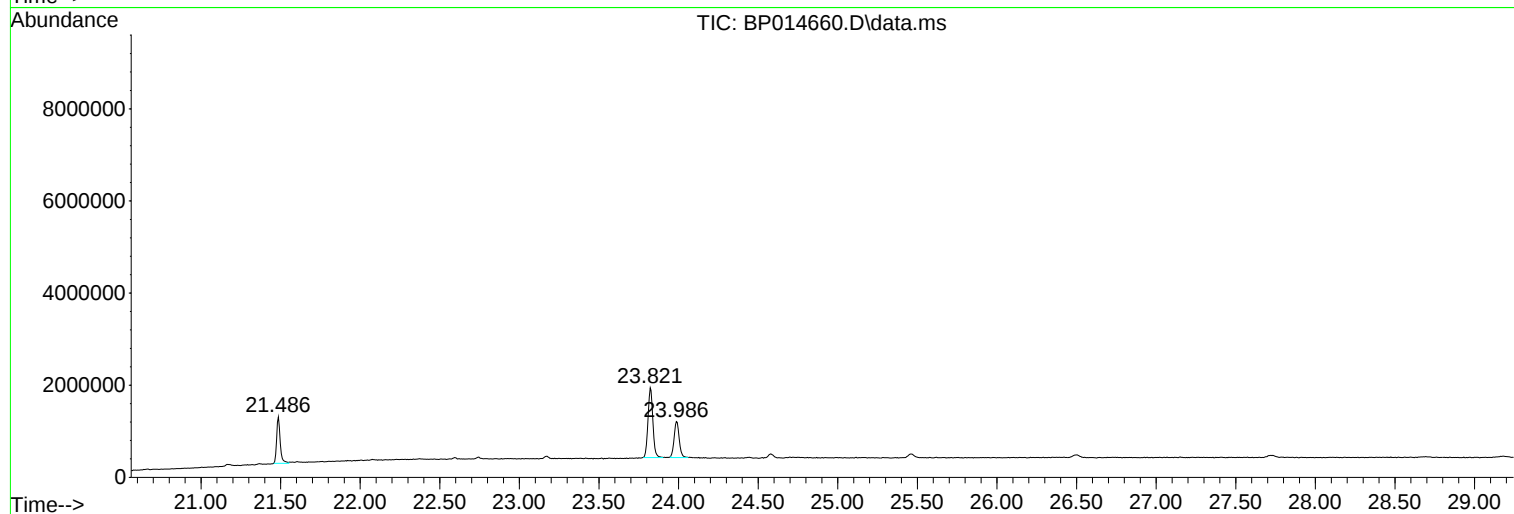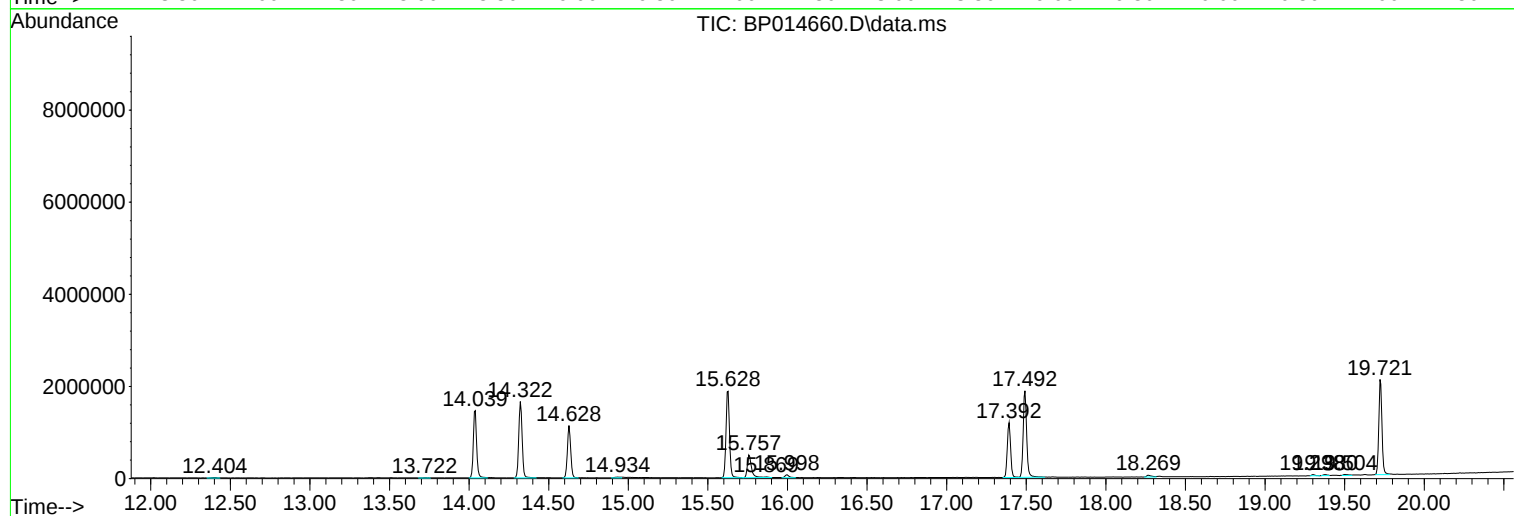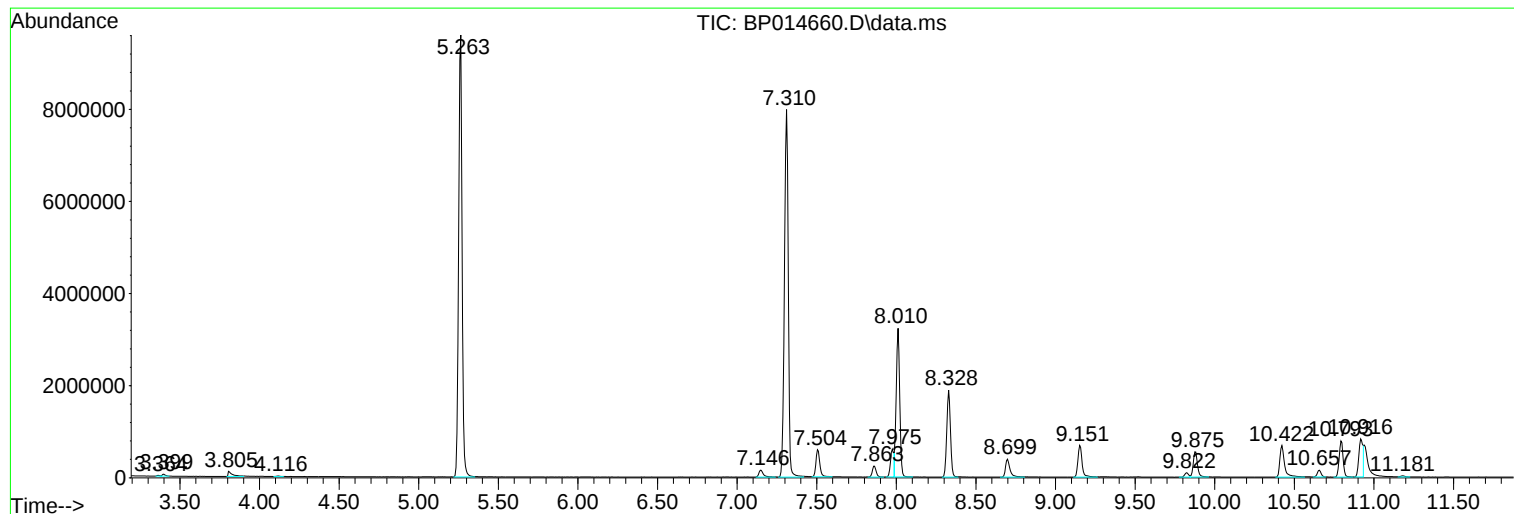

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014660.D
Acq On : 11 Apr 2023 17:26
Operator : CG/JU
Sample : 02251-09
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMC7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 m-Chloroaniline Concentration Rank 5

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.822	2.41 ng/ul	162337	Naphthalene-d8	10.793

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		m-Chloroaniline	127	C6H6ClN	000108-42-9	94
2		p-Chloroaniline	127	C6H6ClN	000106-47-8	94
3		o-Chloroaniline	127	C6H6ClN	000095-51-2	94
4		o-Chloroaniline	127	C6H6ClN	000095-51-2	93
5		m-Chloroaniline	127	C6H6ClN	000108-42-9	93

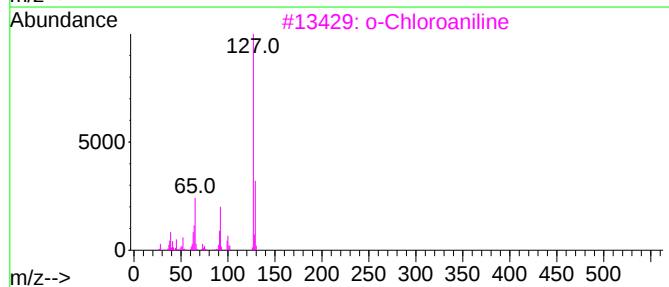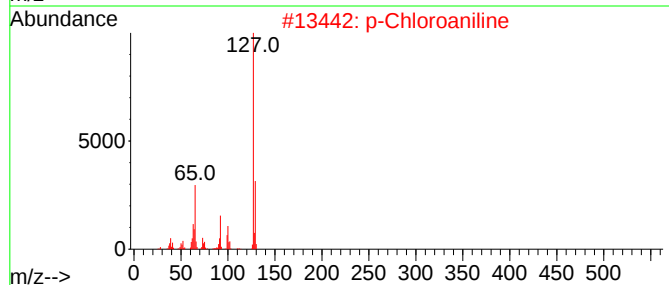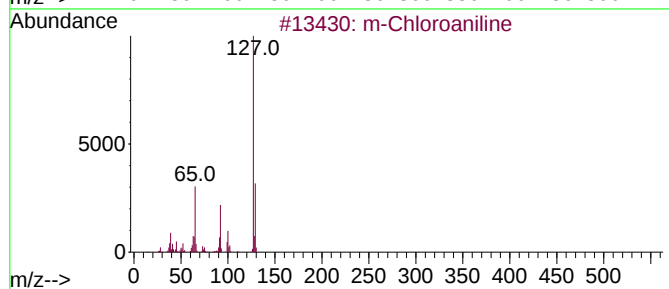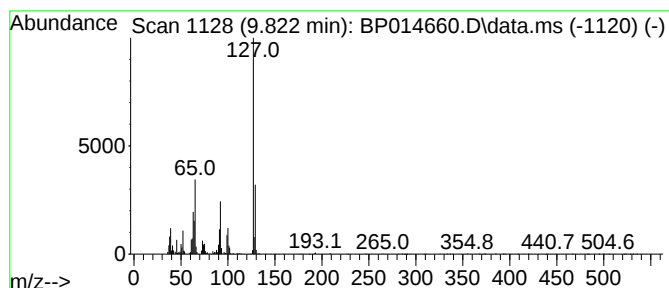

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041023\
Data File : BP014660.D
Acq On : 11 Apr 2023 17:26
Operator : CG/JU
Sample : 02251-09
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0MC7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
m-Chloroaniline	9.822	2.4	ng/u1	162337	2	10.793	1345010	20.0