




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
 Data File : BP009781.D
 Acq On : 12 Apr 2022 13:29
 Operator : CG/JU
 Sample : N2338-11
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J73

Manual IntegrationsAPPROVED

Quant Time: Apr 13 02:20:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 13 02:15:22 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/13/2022

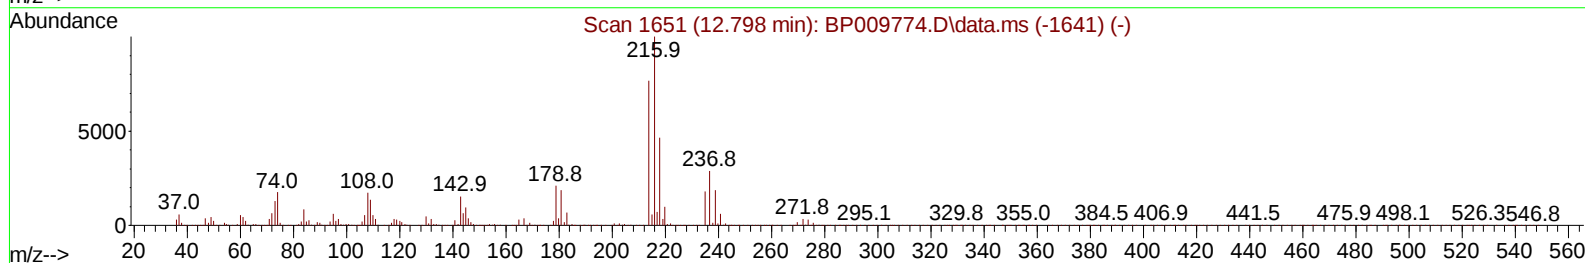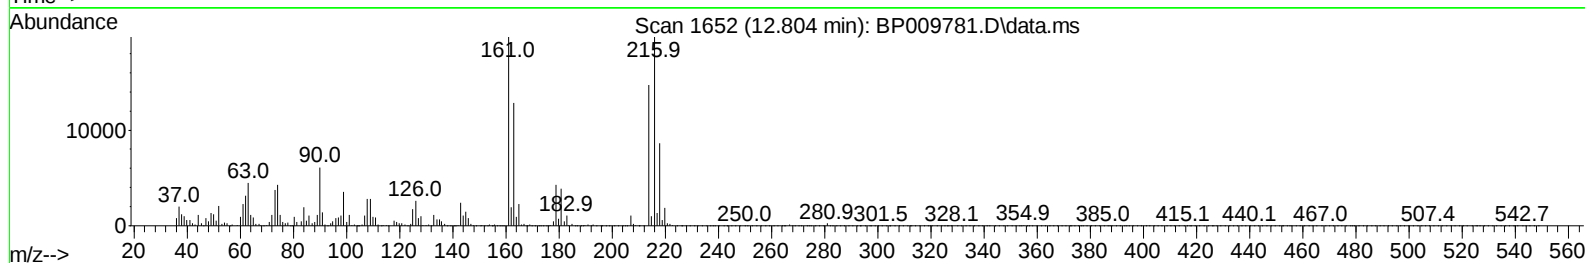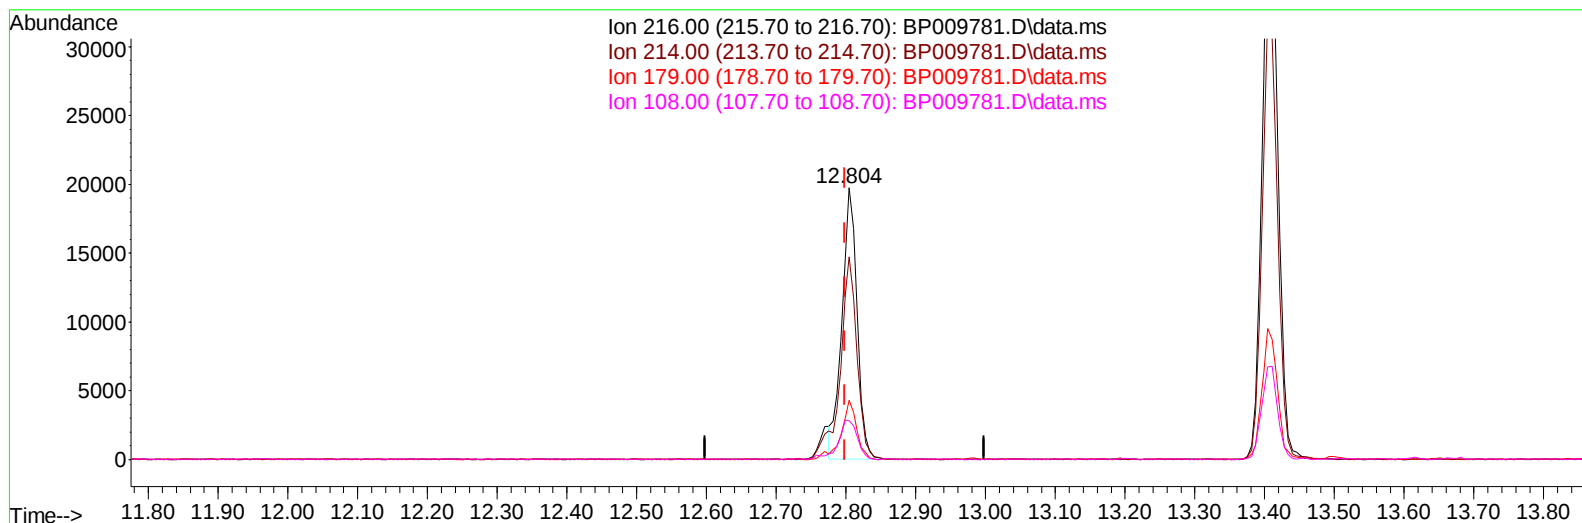

TIC: BP009781.D\data.ms

(39) 1,2,4,5-Tetrachlorobenzene

12.804min (+ 0.006) 3.03 ng/u1

response 29756

Ion	Exp%	Act%
216.00	100.00	100.00
214.00	72.70	74.54
179.00	17.70	21.84#
108.00	19.10	14.35#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009781.D
Acq On : 12 Apr 2022 13:29
Operator : CG/JU
Sample : N2338-11
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J73

Manual IntegrationsAPPROVED

Quant Time: Apr 13 02:20:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 13 02:15:22 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
Supervised By :Yogesh Patel 04/13/2022

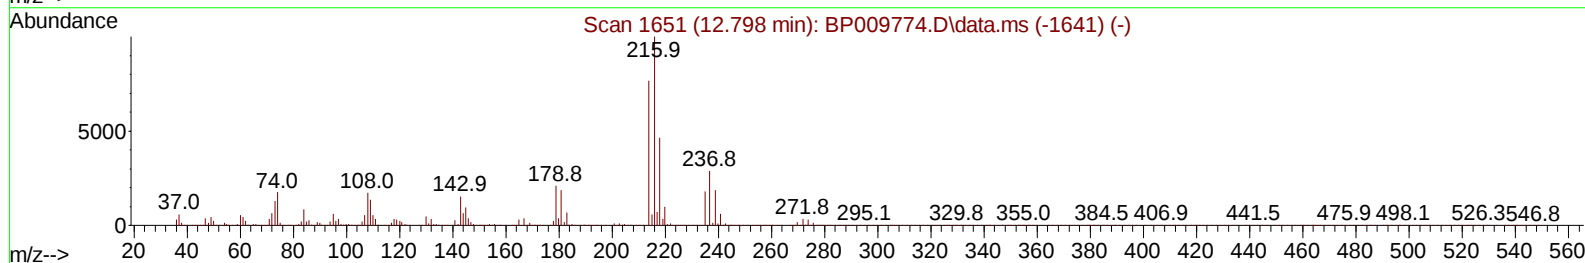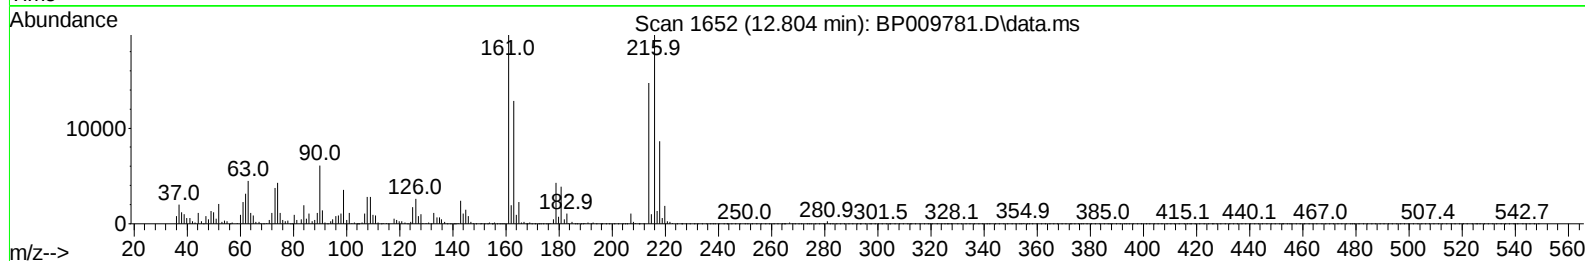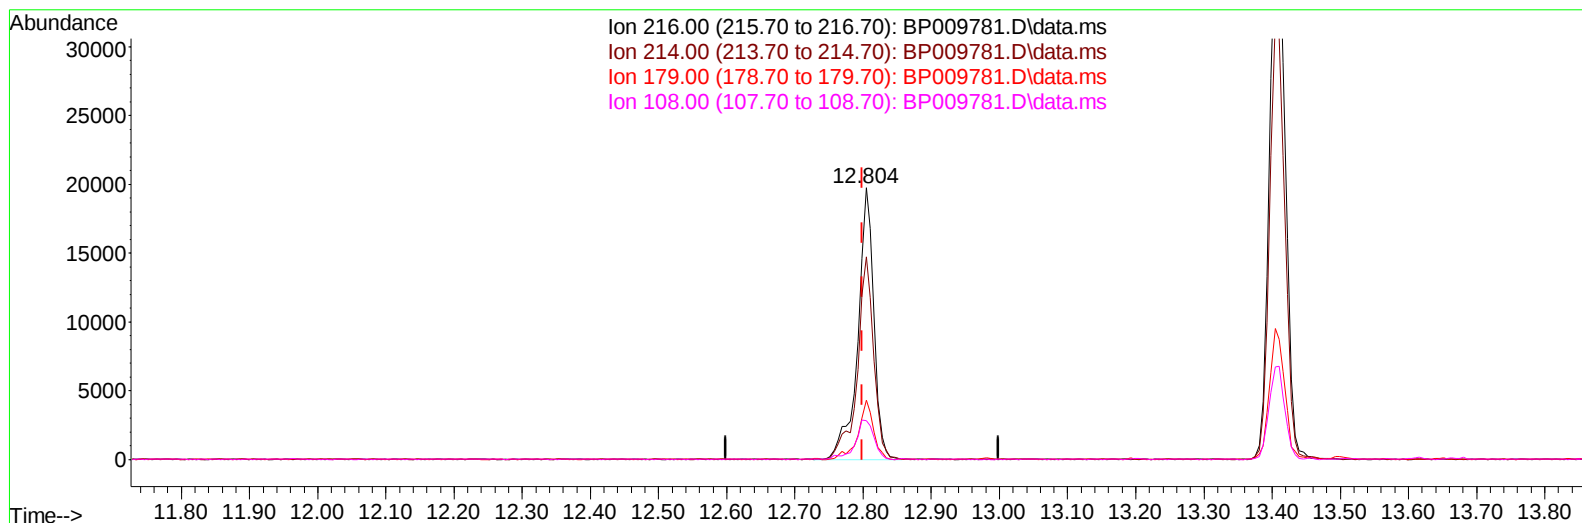

TIC: BP009781.D\data.ms

(39) 1,2,4,5-Tetrachlorobenzene

12.804min (+ 0.006) 3.29 ng/ul m

response 32338

Ion	Exp%	Act%
216.00	100.00	100.00
214.00	72.70	74.54
179.00	17.70	21.84#
108.00	19.10	14.35#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
 Data File : BP009781.D
 Acq On : 12 Apr 2022 13:29
 Operator : CG/JU
 Sample : N2338-11
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J73

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/13/2022

Quant Time: Apr 13 02:20:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 13 02:15:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.981	152	105938	20.000	ng/ul	0.01
20) Naphthalene-d8	10.787	136	445954	20.000	ng/ul	0.01
38) Acenaphthene-d10	14.604	164	320992	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.357	188	718851	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.433	240	788763	20.000	ng/ul	# 0.00
88) Perylene-d12	23.910	264	783752	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	13068	5.505	ng/uL	0.00
4) Pyridine-d5	3.811	84	81306	12.423	ng/ul	0.00
7) Phenol-d5	7.128	99	75466	8.114	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.299	67	250582	45.256	ng/ul	0.00
11) 2-Chlorophenol-d4	7.505	132	219303	31.259	ng/ul	0.00
15) 4-Methylphenol-d8	8.675	113	146703	18.895	ng/ul	0.00
21) Nitrobenzene-d5	9.134	128	150028	46.652	ng/ul	0.00
24) 2-Nitrophenol-d4	9.858	143	159879	45.346	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.399	165	260808	35.350	ng/ul	0.00
31) 4-Chloroaniline-d4	10.910	131	352830	33.577	ng/ul	0.00
46) Dimethylphthalate-d6	14.010	166	1062786	42.150	ng/ul	0.00
49) Acenaphthylene-d8	14.299	160	1209622	40.494	ng/ul	0.00
54) 4-Nitrophenol-d4	14.781	143	38062	8.324	ng/ul	0.00
60) Fluorene-d10	15.598	176	923589	43.542	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.704	200	174721	41.029	ng/ul	0.00
73) Anthracene-d10	17.457	188	1599115	46.462	ng/ul	0.00
81) Pyrene-d10	19.686	212	2001329	46.458	ng/ul	0.01
92) Benzo(a)pyrene-d12	23.751	264	1984349	48.618	ng/ul	0.01
Target Compounds						
					Qvalue	
22) Nitrobenzene	9.187	77	2374111	287.613	ng/ul#	85
32) 4-Chloroaniline	10.934	127	19371	1.863	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.804	216	32338m	3.293	ng/ul	
75) 1,2,3,4-Tetrachloroben...	13.404	216	63883	6.147	ng/uL#	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009781.D
Acq On : 12 Apr 2022 13:29
Operator : CG/JU
Sample : N2338-11
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J73

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/13/2022
Supervised By :Yogesh Patel 04/13/2022

Quant Time: Apr 13 02:20:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 13 02:15:22 2022
Response via : Initial Calibration

