




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
 Data File : BP009792.D
 Acq On : 12 Apr 2022 20:24
 Operator : CG/JU
 Sample : N2342-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J85

Manual IntegrationsAPPROVED

Quant Time: Apr 13 02:25:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 13 02:15:22 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/13/2022

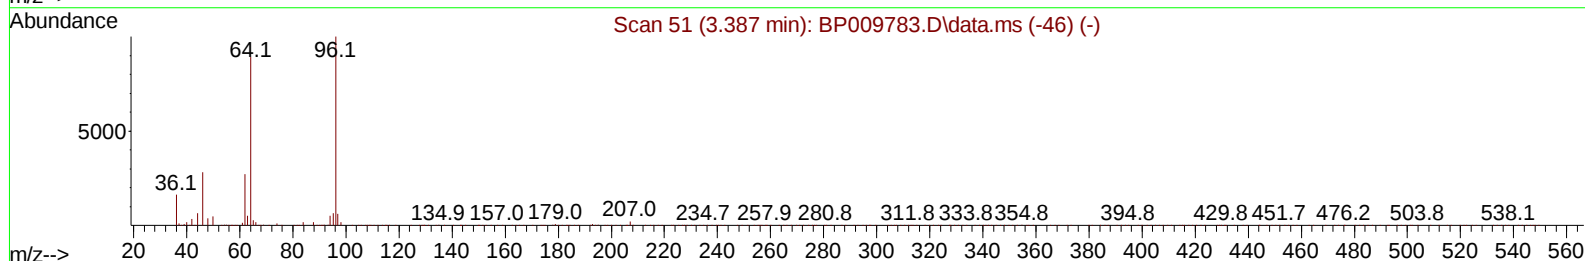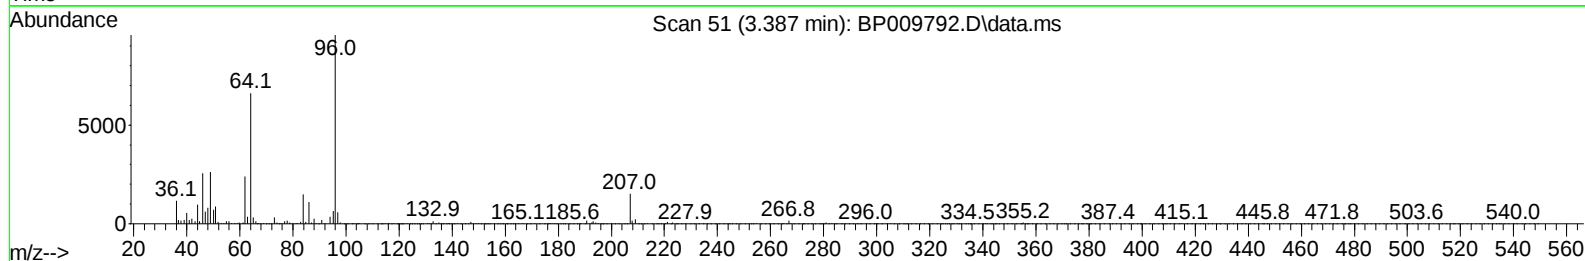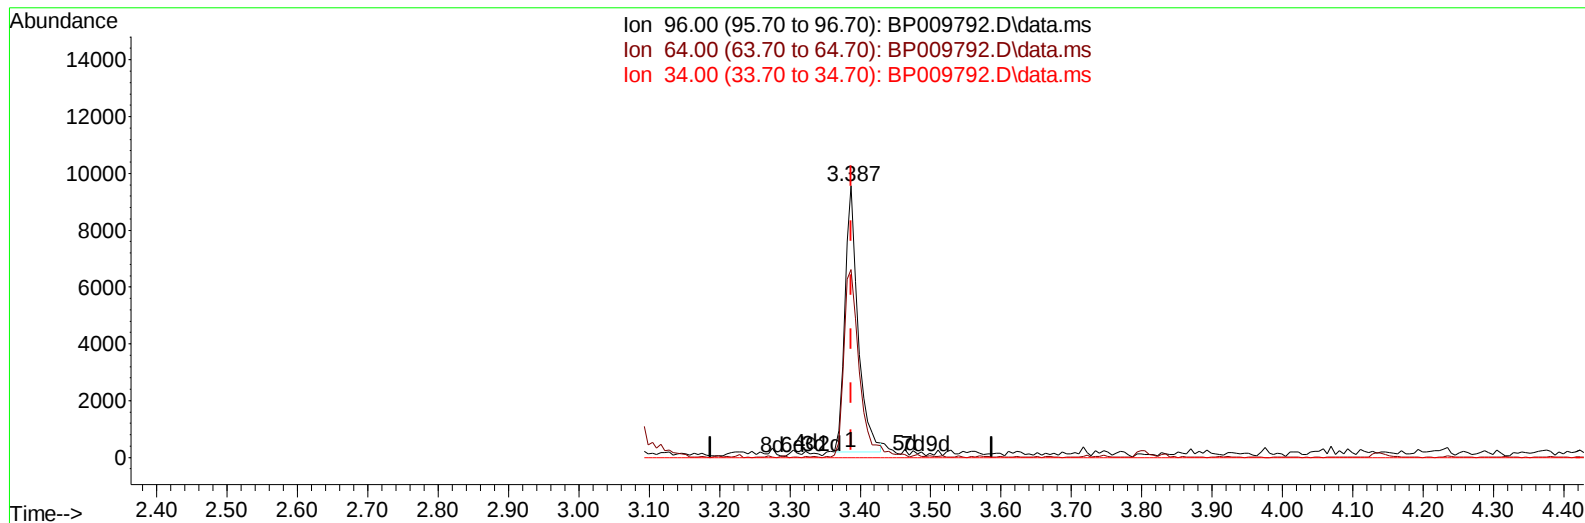

TIC: BP009792.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.387min (+ 0.000) 4.47 ng/uL

response 12087

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	69.18#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
 Data File : BP009792.D
 Acq On : 12 Apr 2022 20:24
 Operator : CG/JU
 Sample : N2342-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J85

Manual IntegrationsAPPROVED

Quant Time: Apr 13 02:25:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 13 02:15:22 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/13/2022

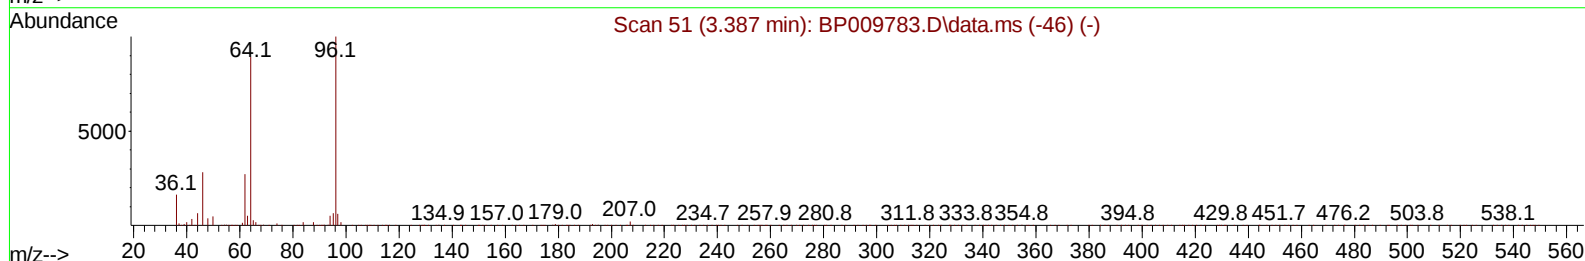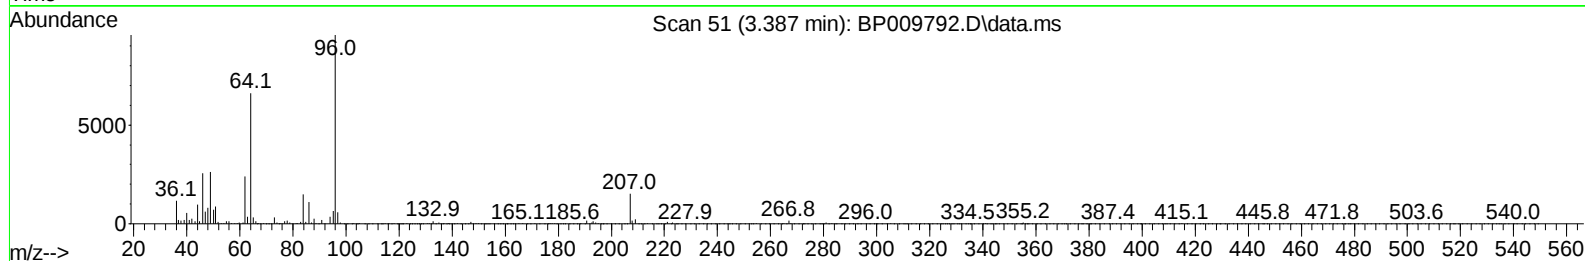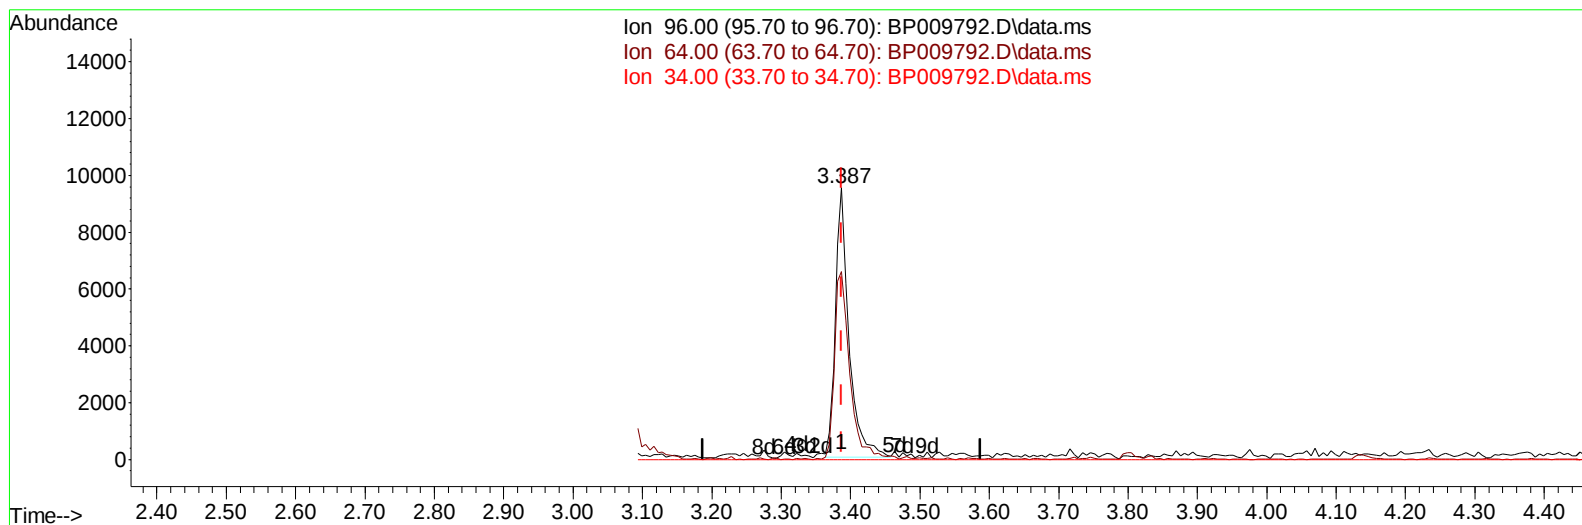

TIC: BP009792.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.387min (+ 0.000) 4.74 ng/uL m

response 12826

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	69.18#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009792.D
Acq On : 12 Apr 2022 20:24
Operator : CG/JU
Sample : N2342-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J85

Manual IntegrationsAPPROVED

Quant Time: Apr 13 02:25:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 13 02:15:22 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
Supervised By :Yogesh Patel 04/13/2022

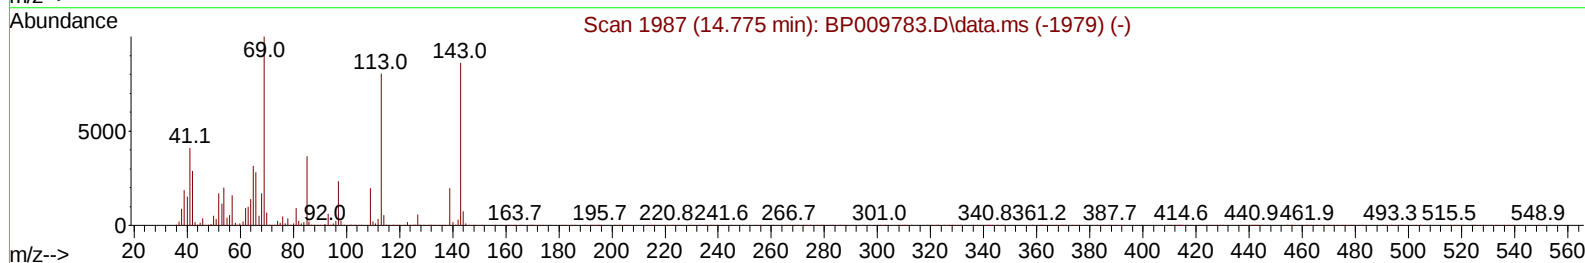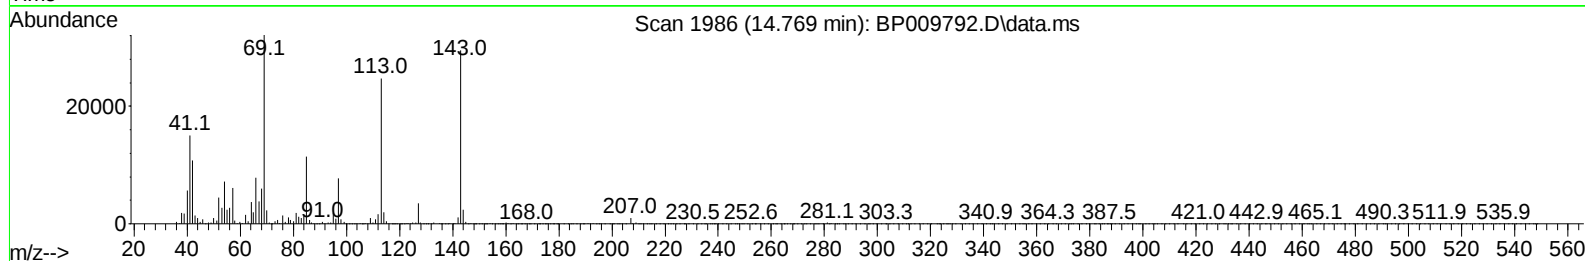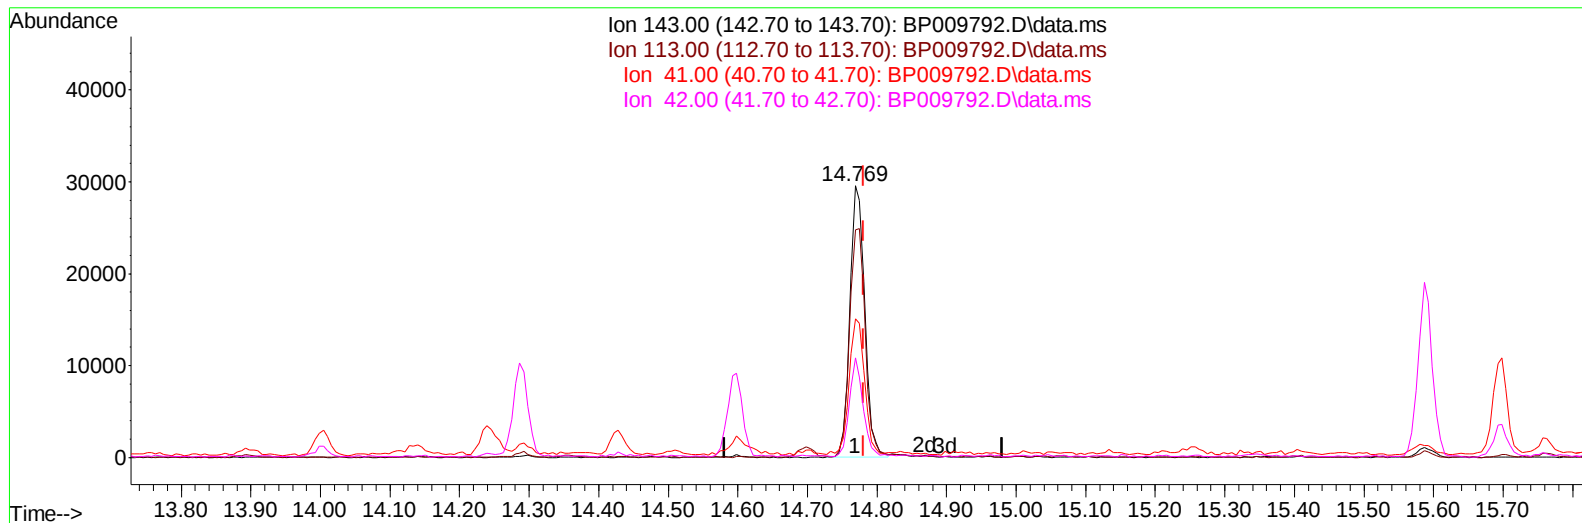

TIC: BP009792.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.769min (-0.012) 7.89 ng/u1

response 43687

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	83.84#
41.00	23.20	51.05#
42.00	18.00	36.63#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009792.D
Acq On : 12 Apr 2022 20:24
Operator : CG/JU
Sample : N2342-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J85

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/13/2022
Supervised By :Yogesh Patel 04/13/2022

Quant Time: Apr 13 02:25:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 13 02:15:22 2022
Response via : Initial Calibration

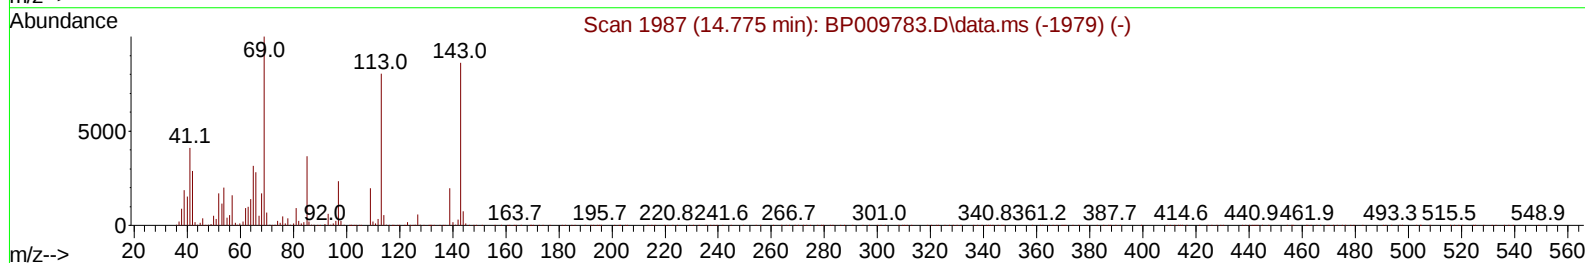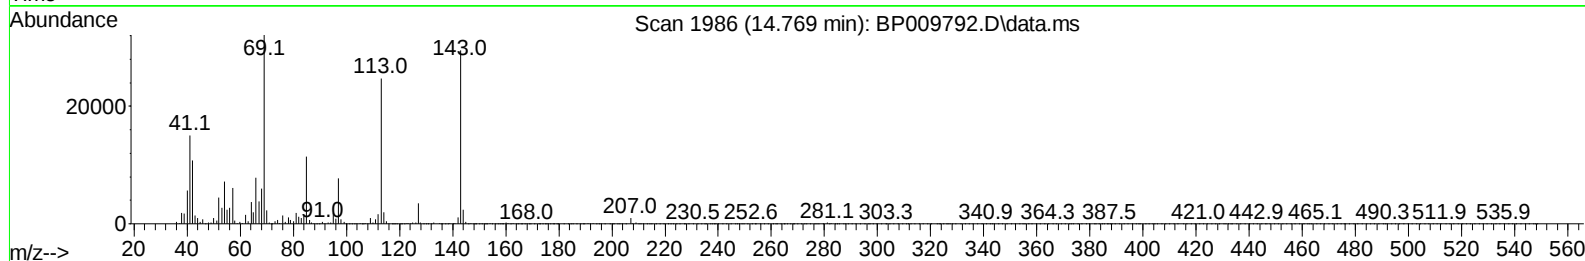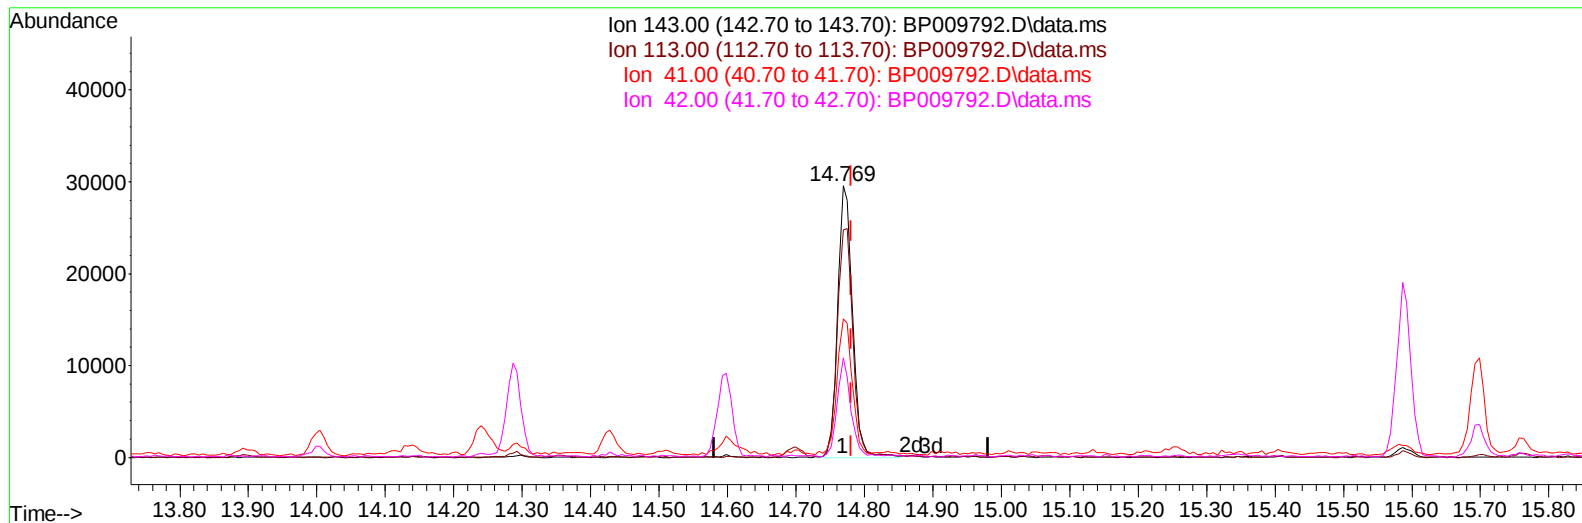

TIC: BP009792.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.769min (-0.012) 8.00 ng/ul m

response 44299

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	83.84#
41.00	23.20	51.05#
42.00	18.00	36.63#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
 Data File : BP009792.D
 Acq On : 12 Apr 2022 20:24
 Operator : CG/JU
 Sample : N2342-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J85

Manual IntegrationsAPPROVED

Quant Time: Apr 13 02:25:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 13 02:15:22 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/13/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.969	152	120699	20.000	ng/ul	0.00
20) Naphthalene-d8	10.775	136	535349	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.598	164	388858	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.345	188	865495	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.427	240	922350	20.000	ng/ul	# 0.00
88) Perylene-d12	23.892	264	890090	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	12826m	4.743	ng/uL	0.00
4) Pyridine-d5	3.805	84	96310	12.916	ng/ul	0.00
7) Phenol-d5	7.122	99	81584	7.699	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.293	67	351048	55.647	ng/ul	0.00
11) 2-Chlorophenol-d4	7.499	132	208087	26.033	ng/ul	0.00
15) 4-Methylphenol-d8	8.669	113	158119	17.875	ng/ul	0.00
21) Nitrobenzene-d5	9.122	128	135104	34.996	ng/ul	0.00
24) 2-Nitrophenol-d4	9.851	143	140622	33.224	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.387	165	252358	28.493	ng/ul	0.00
31) 4-Chloroaniline-d4	10.904	131	348498	27.626	ng/ul	0.00
46) Dimethylphthalate-d6	14.004	166	1050439	34.390	ng/ul	0.00
49) Acenaphthylene-d8	14.292	160	1117108	30.870	ng/ul	0.00
54) 4-Nitrophenol-d4	14.769	143	44299m	7.997	ng/ul	-0.01
60) Fluorene-d10	15.592	176	891686	34.702	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.698	200	155536	30.335	ng/ul	0.00
73) Anthracene-d10	17.445	188	1550158	37.408	ng/ul	0.00
81) Pyrene-d10	19.674	212	1958669	38.882	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.739	264	1856650	40.055	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.152	94	119164	11.235	ng/ul#	91
12) 2-Chlorophenol	7.528	128	27415	3.402	ng/ul	98
32) 4-Chloroaniline	10.928	127	30480	2.442	ng/ul	98
34) Caprolactam	11.687	113	72243	25.441	ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
 Data File : BP009792.D
 Acq On : 12 Apr 2022 20:24
 Operator : CG/JU
 Sample : N2342-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J85

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/13/2022

Quant Time: Apr 13 02:25:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 13 02:15:22 2022
 Response via : Initial Calibration

