




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
 Data File : BP009796.D
 Acq On : 12 Apr 2022 23:13
 Operator : CG/JU
 Sample : PB144076BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK076

Manual IntegrationsAPPROVED

Quant Time: Apr 13 04:15:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 13 02:15:22 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/13/2022

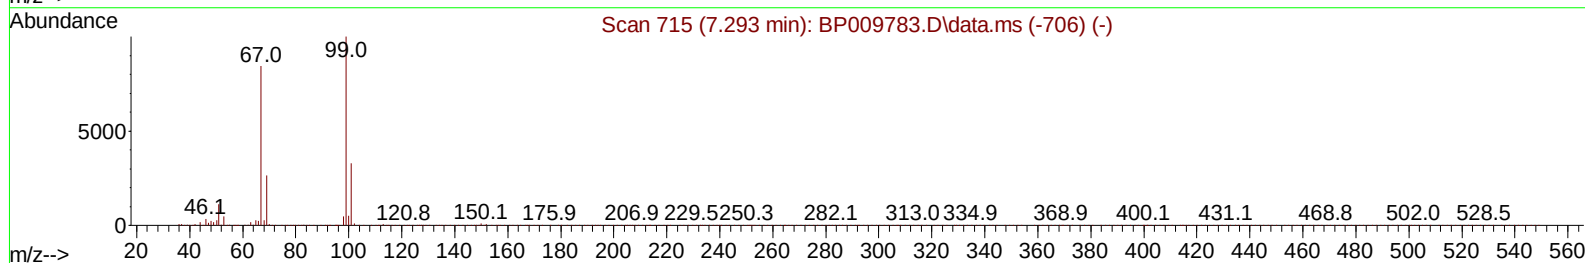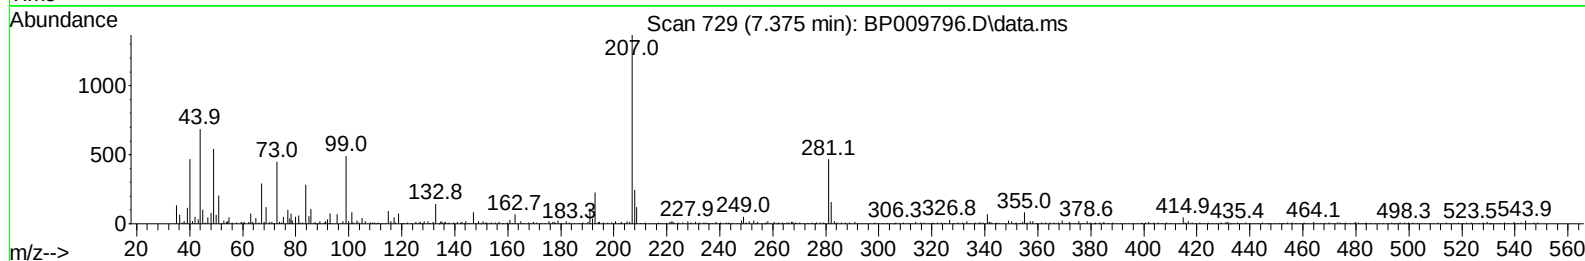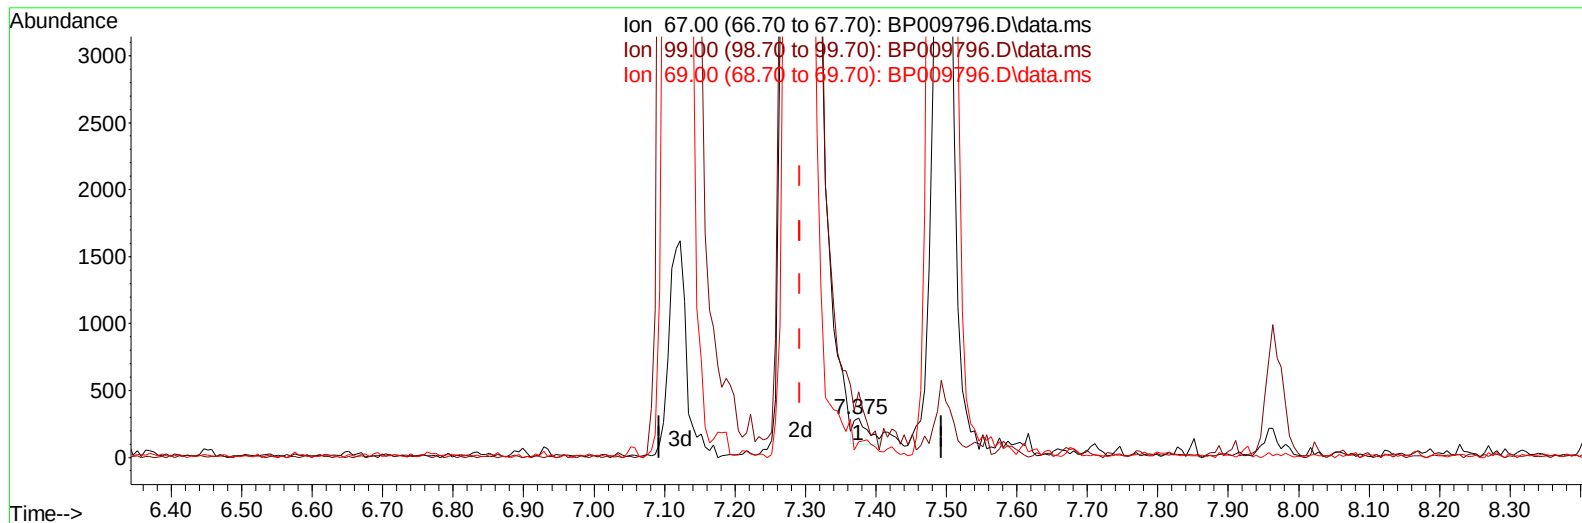

TIC: BP009796.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.375min (+ 0.083) 0.05 ng/uL

response 278

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	165.50	168.49
69.00	40.10	40.75
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
 Data File : BP009796.D
 Acq On : 12 Apr 2022 23:13
 Operator : CG/JU
 Sample : PB144076BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK076

Manual IntegrationsAPPROVED

Quant Time: Apr 13 04:15:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 13 02:15:22 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/13/2022

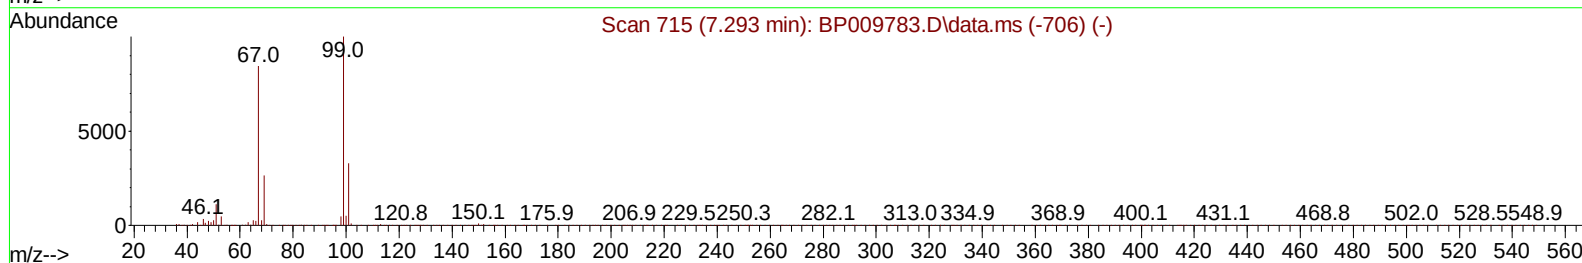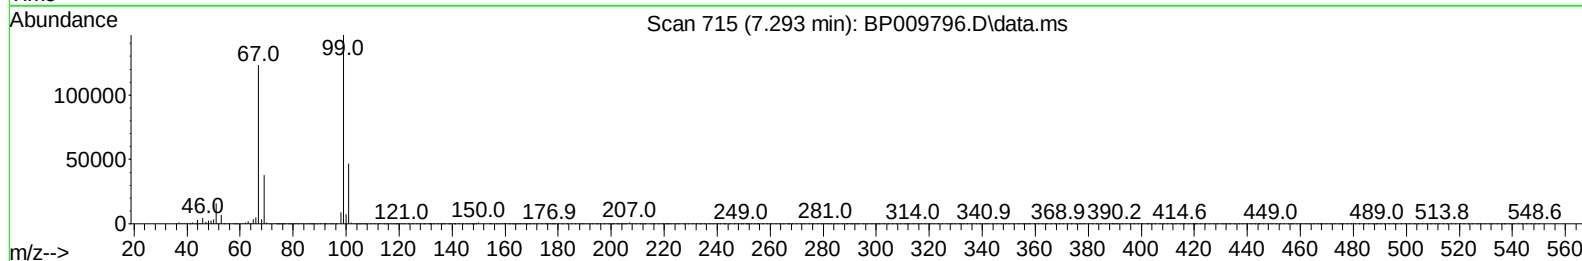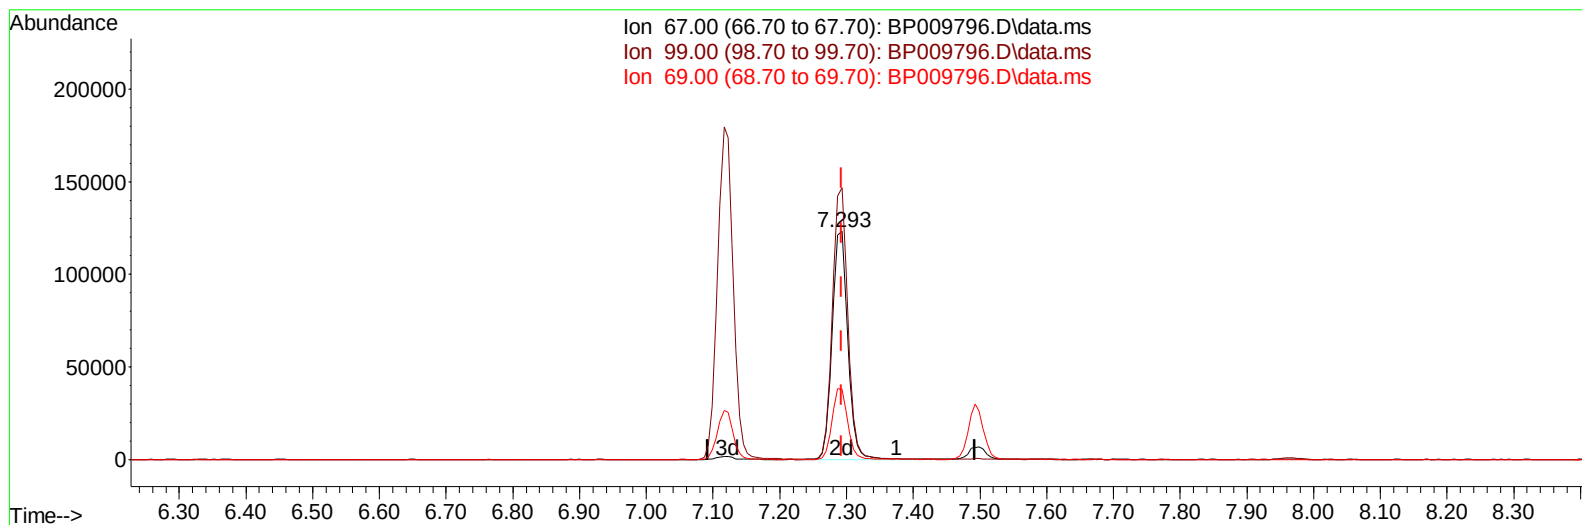

TIC: BP009796.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.293min (+ 0.000) 36.21 ng/ul m

response 198237

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	165.50	119.03#
69.00	40.10	30.63#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
 Data File : BP009796.D
 Acq On : 12 Apr 2022 23:13
 Operator : CG/JU
 Sample : PB144076BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK076

Manual IntegrationsAPPROVED

Quant Time: Apr 13 04:15:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 13 02:15:22 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/13/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.969	152	104747	20.000	ng/ul	0.00
20) Naphthalene-d8	10.775	136	482368	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.598	164	357649	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.345	188	813074	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.422	240	846147	20.000	ng/ul	#-0.01
88) Perylene-d12	23.892	264	767673	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	16417	6.995	ng/uL	0.00
4) Pyridine-d5	3.805	84	233972	36.156	ng/ul	0.00
7) Phenol-d5	7.116	99	289814	31.515	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.293	67	198237m	36.209	ng/ul	0.00
11) 2-Chlorophenol-d4	7.493	132	236163	34.045	ng/ul	0.00
15) 4-Methylphenol-d8	8.663	113	258351	33.653	ng/ul	0.00
21) Nitrobenzene-d5	9.122	128	127954	36.784	ng/ul	0.00
24) 2-Nitrophenol-d4	9.846	143	138789	36.393	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.387	165	248581	31.149	ng/ul	0.00
31) 4-Chloroaniline-d4	10.899	131	388308	34.163	ng/ul	0.00
46) Dimethylphthalate-d6	14.004	166	997059	35.490	ng/ul	0.00
49) Acenaphthylene-d8	14.287	160	1077321	32.368	ng/ul	0.00
54) 4-Nitrophenol-d4	14.775	143	167782	32.931	ng/ul	0.00
60) Fluorene-d10	15.587	176	842763	35.660	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.698	200	139195	28.899	ng/ul	0.00
73) Anthracene-d10	17.445	188	1373405	35.279	ng/ul	0.00
81) Pyrene-d10	19.675	212	1683160	36.422	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.733	264	1460121	36.523	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009796.D
Acq On : 12 Apr 2022 23:13
Operator : CG/JU
Sample : PB144076BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK076

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/13/2022
Supervised By :Yogesh Patel 04/13/2022

Quant Time: Apr 13 04:15:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 13 02:15:22 2022
Response via : Initial Calibration

