

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
 Data File : BP009751.D
 Acq On : 11 Apr 2022 14:49
 Operator : CG/JU
 Sample : N2338-12
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J81

Quant Time: Apr 12 01:31:39 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 07 19:16:52 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.969	152	144048	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.781	136	618995	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.604	164	427732	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.351	188	951771	20.000	ng/ul	#-0.01
79) Chrysene-d12	21.433	240	978928	20.000	ng/ul	#-0.01
88) Perylene-d12	23.910	264	940892	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	12878	3.990	ng/uL	0.00
4) Pyridine-d5	3.811	84	70205	7.889	ng/ul	0.00
7) Phenol-d5	7.122	99	78689	6.222	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.293	67	246644	32.760	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.499	132	230691	24.183	ng/ul	0.00
15) 4-Methylphenol-d8	8.669	113	161867	15.332	ng/ul	-0.01
21) Nitrobenzene-d5	9.128	128	159999	35.844	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.857	143	164229	33.558	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.393	165	275354	26.888	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.904	131	378947	25.981	ng/ul	-0.01
46) Dimethylphthalate-d6	14.010	166	1219091	36.284	ng/ul	-0.01
49) Acenaphthylene-d8	14.298	160	1318003	33.111	ng/ul	0.00
54) 4-Nitrophenol-d4	14.775	143	42101	6.909	ng/ul	-0.01
60) Fluorene-d10	15.598	176	1033702	36.572	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.704	200	195853	34.736	ng/ul	0.00
73) Anthracene-d10	17.451	188	1825642	40.062	ng/ul	-0.01
81) Pyrene-d10	19.680	212	2273093	42.516	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.751	264	2101737	42.894	ng/ul	-0.01
Target Compounds						
8) Phenol	7.152	94	29649	2.342	ng/ul#	90
86) Bis(2-ethylhexyl)phtha...	21.351	149	41104	1.068	ng/ul#	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009751.D
Acq On : 11 Apr 2022 14:49
Operator : CG/JU
Sample : N2338-12
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J81

Quant Time: Apr 12 01:31:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 07 19:16:52 2022
Response via : Initial Calibration




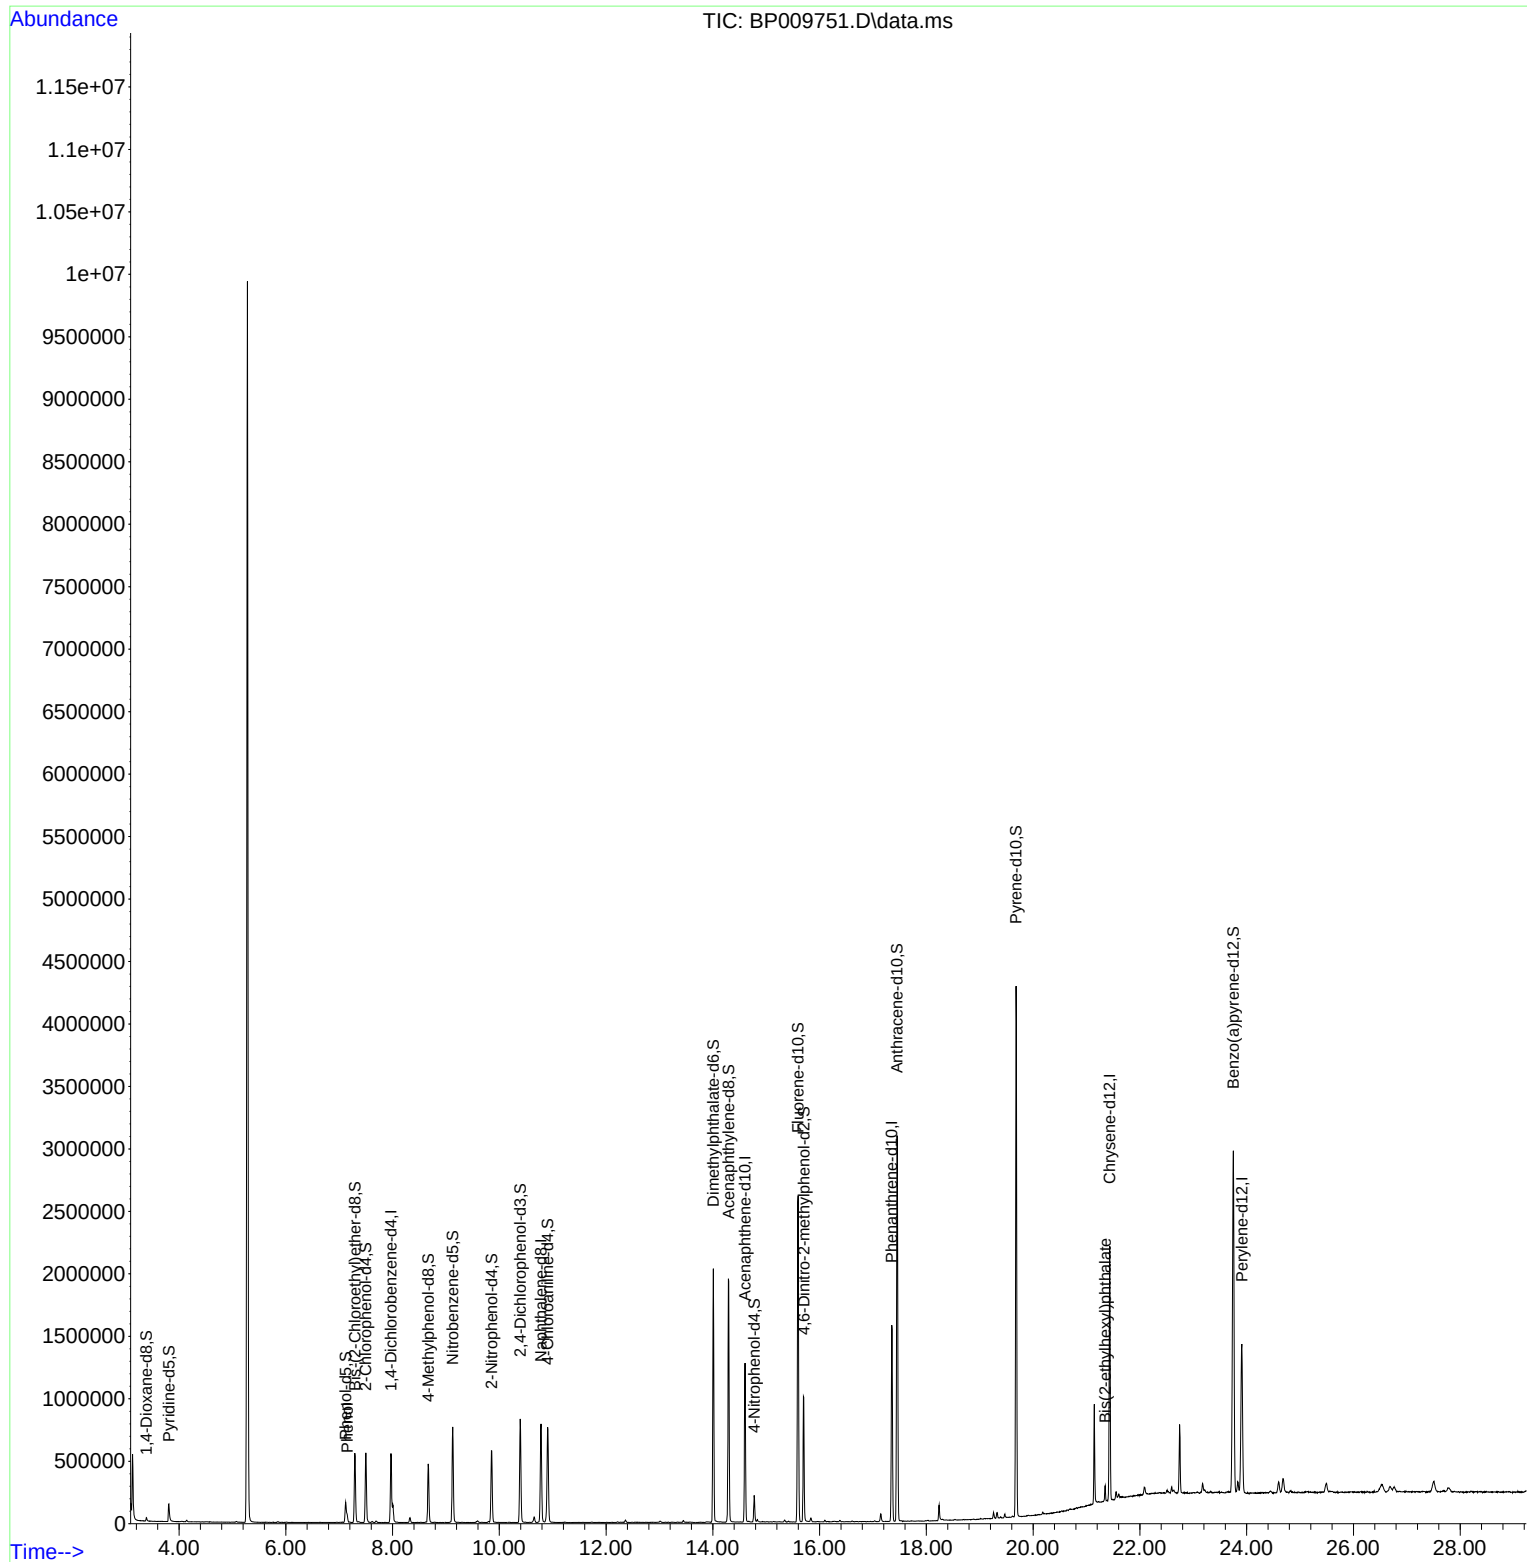


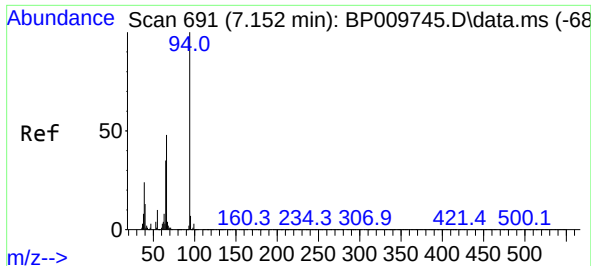

#8
Phenol
Concen: 2.342 ng/ul
RT: 7.152 min Scan# 691
Delta R.T. -0.006 min
Lab File: BP009751.D
Acq: 11 Apr 2022 14:49

Instrument :
BNA_P
ClientSampleId :
C0J81

Tgt Ion: 94 Resp: 29649
Ion Ratio Lower Upper
94 100
65 33.8 19.0 28.6#
66 45.5 34.6 51.8

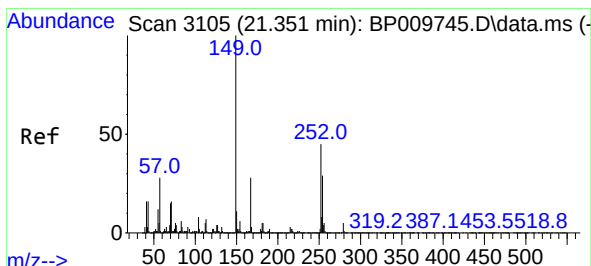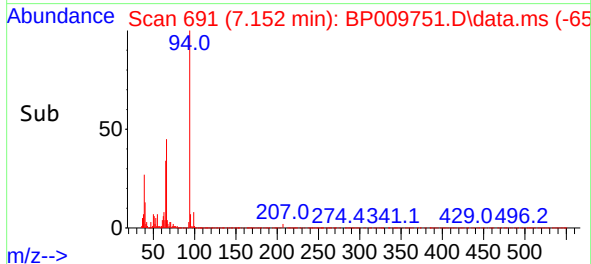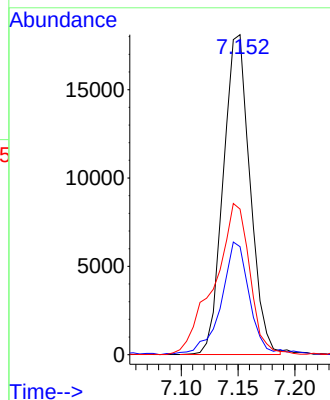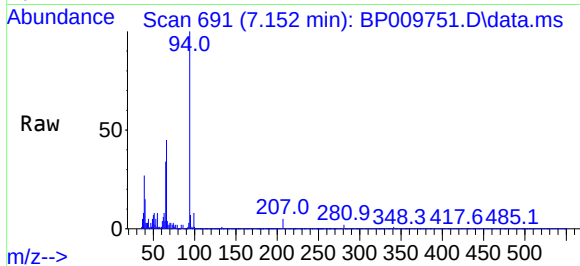

#86
Bis(2-ethylhexyl)phthalate
Concen: 1.068 ng/ul
RT: 21.351 min Scan# 3105
Delta R.T. -0.012 min
Lab File: BP009751.D
Acq: 11 Apr 2022 14:49

Tgt Ion:149 Resp: 41104
Ion Ratio Lower Upper
149 100
167 28.3 32.8 49.2#
279 4.6 5.6 8.4#

