

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
 Data File : BP009769.D
 Acq On : 12 Apr 2022 01:31
 Operator : CG/JU
 Sample : N2342-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0HY2

Quant Time: Apr 12 02:45:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 07 19:16:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.969	152	111949	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.775	136	497628	20.000	ng/u1	-0.02
38) Acenaphthene-d10	14.598	164	355213	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.351	188	791525	20.000	ng/u1	#-0.01
79) Chrysene-d12	21.427	240	873688	20.000	ng/u1	#-0.02
88) Perylene-d12	23.898	264	886816	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	14226	5.671	ng/uL	0.00
4) Pyridine-d5	3.805	84	55965	8.092	ng/u1	0.00
7) Phenol-d5	7.122	99	52072	5.298	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.293	67	188485	32.213	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.499	132	170620	23.014	ng/u1	0.00
15) 4-Methylphenol-d8	8.669	113	75769	9.235	ng/u1	-0.01
21) Nitrobenzene-d5	9.128	128	123969	34.546	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.852	143	134676	34.231	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.393	165	205408	24.950	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.904	131	97616	8.325	ng/u1	-0.01
46) Dimethylphthalate-d6	14.004	166	946359	33.917	ng/u1	-0.02
49) Acenaphthylene-d8	14.292	160	1013626	30.663	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.775	143	34597	6.837	ng/u1	-0.01
60) Fluorene-d10	15.592	176	821583	35.002	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.698	200	153111	32.653	ng/u1	-0.01
73) Anthracene-d10	17.451	188	1371057	36.178	ng/u1	-0.01
81) Pyrene-d10	19.675	212	1756285	36.806	ng/u1	-0.01
92) Benzo(a)pyrene-d12	23.739	264	1697837	36.764	ng/u1	-0.02


Target Compounds				Qvalue	
2) 1,4-Dioxane	3.422	88	3968	1.552 ng/uL#	40


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009769.D
Acq On : 12 Apr 2022 01:31
Operator : CG/JU
Sample : N2342-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HY2


Quant Time: Apr 12 02:45:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 07 19:16:52 2022
Response via : Initial Calibration

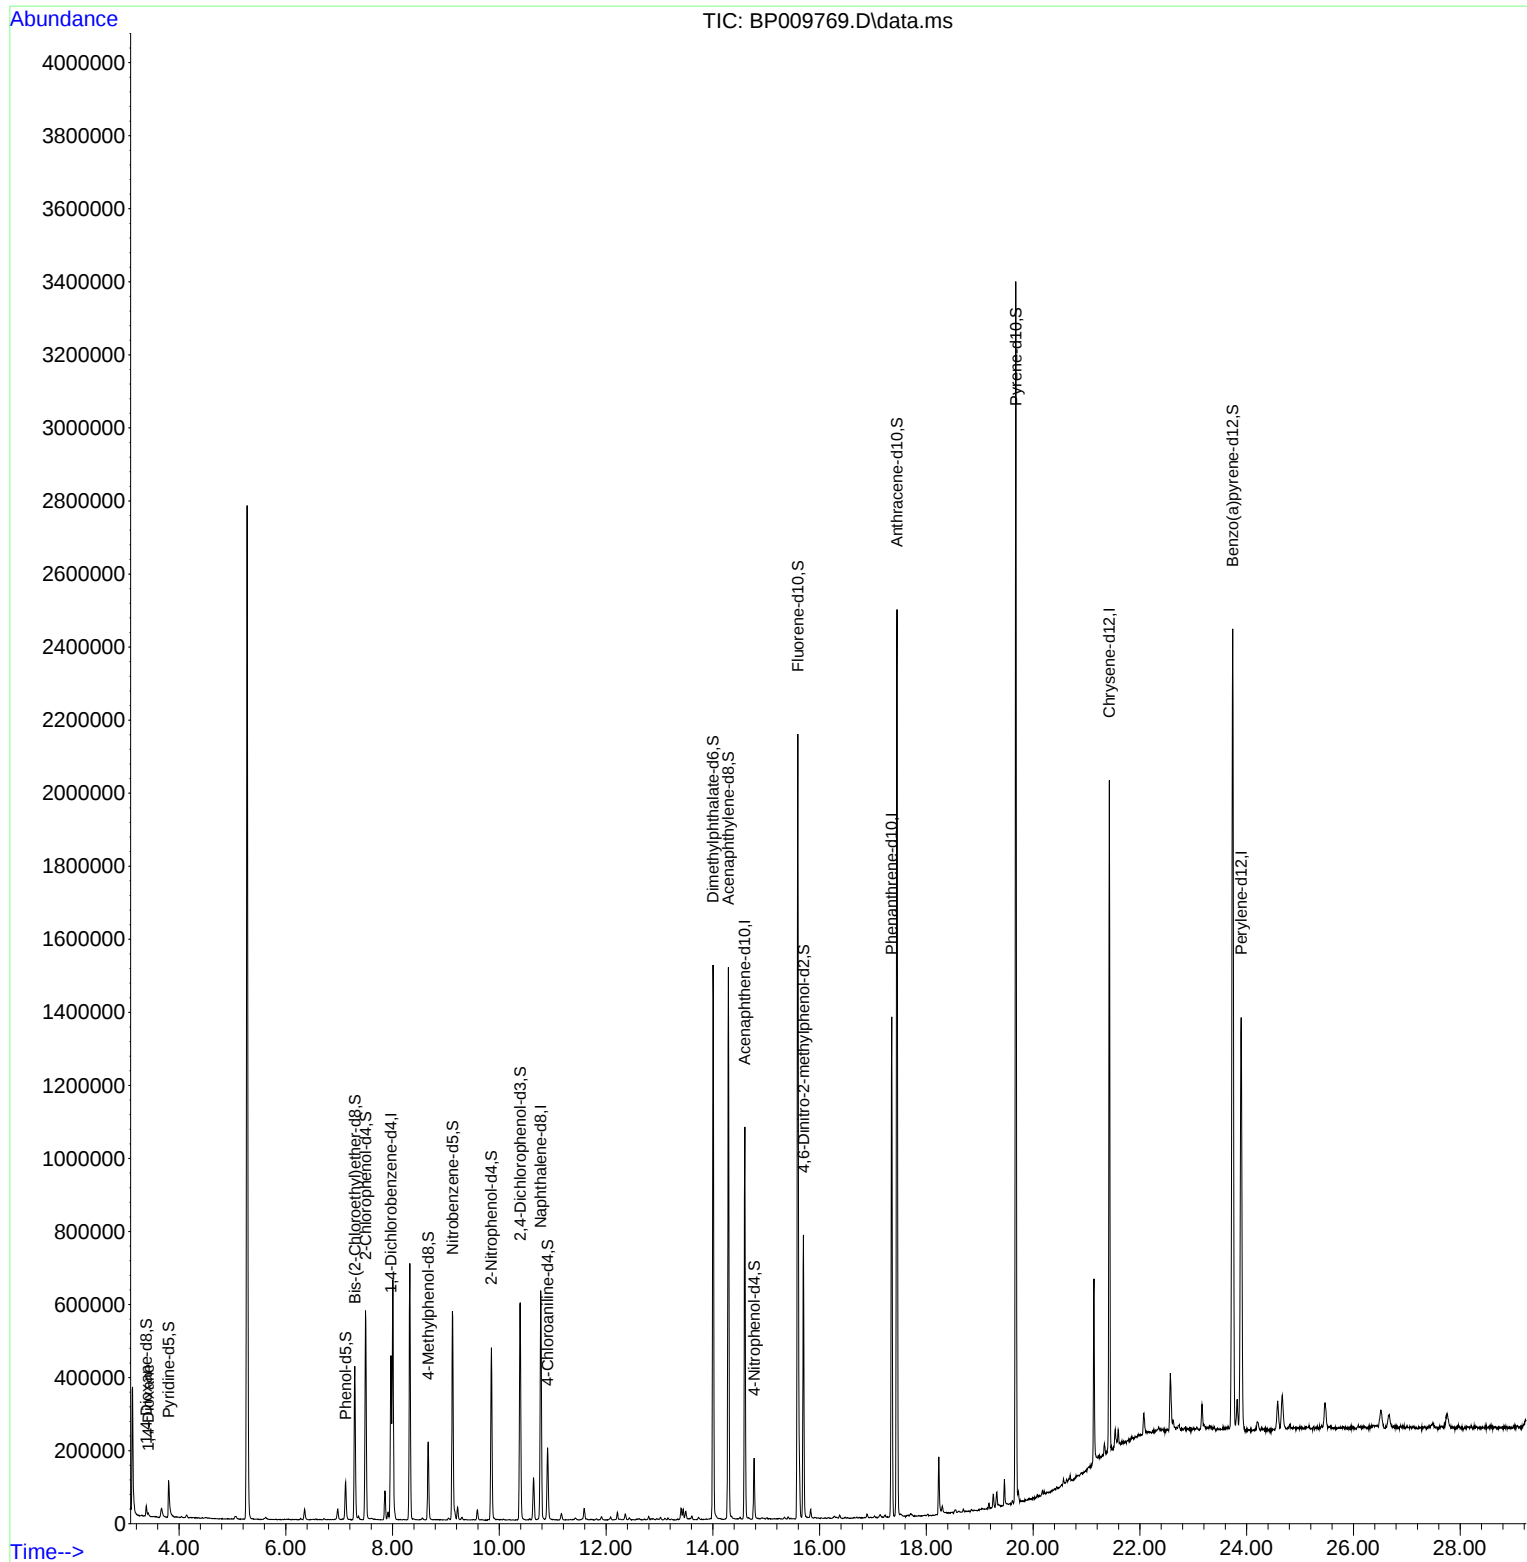

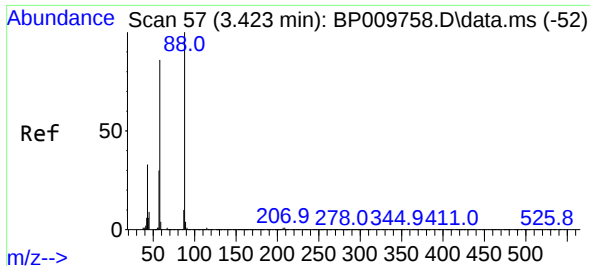

#2
 1,4-Dioxane
 Concen: 1.552 ng/uL
 RT: 3.422 min Scan# 51
 Delta R.T. -0.006 min
 Lab File: BP009769.D
 Acq: 12 Apr 2022 01:31

Instrument :
 BNA_P
 ClientSampleId :
 C0HY2

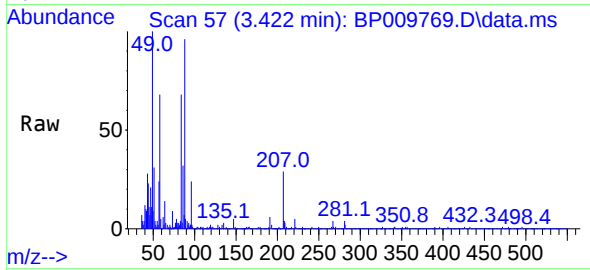

Tgt Ion: 88 Resp: 3968

Ion	Ratio	Lower	Upper
88	100		
43	28.8	6.8	10.2#
58	70.8	28.4	42.6#

