

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
 Data File : BP009779.D
 Acq On : 12 Apr 2022 12:03
 Operator : CG/JU
 Sample : N2338-17DL 5X
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J69DL

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/13/2022

Quant Time: Apr 13 02:20:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 13 02:15:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.975	152	108624	20.000	ng/u1	0.00
20) Naphthalene-d8	10.781	136	460802	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.604	164	331876	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.357	188	750125m	20.000	ng/u1	0.00
79) Chrysene-d12	21.433	240	769825	20.000	ng/u1	# 0.00
88) Perylene-d12	23.910	264	728283	20.000	ng/u1	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	3.817	84	15730	2.344	ng/u1	0.01
7) Phenol-d5	7.128	99	15535	1.629	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.293	67	64423m	11.347	ng/u1	0.00
11) 2-Chlorophenol-d4	7.505	132	40240	5.594	ng/u1	0.00
15) 4-Methylphenol-d8	8.675	113	28172	3.539	ng/u1	0.00
21) Nitrobenzene-d5	9.128	128	23300	7.012	ng/u1	0.00
24) 2-Nitrophenol-d4	9.857	143	24726	6.787	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.399	165	44393	5.823	ng/u1	0.00
31) 4-Chloroaniline-d4	10.910	131	66562	6.130	ng/u1	0.00
46) Dimethylphthalate-d6	14.010	166	189947	7.286	ng/u1	0.00
49) Acenaphthylene-d8	14.298	160	193559m	6.267	ng/u1	0.00
54) 4-Nitrophenol-d4	14.781	143	6674m	1.412	ng/u1	0.00
60) Fluorene-d10	15.598	176	166867	7.609	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.704	200	21825m	4.911	ng/u1	0.00
73) Anthracene-d10	17.457	188	277501	7.727	ng/u1	0.00
81) Pyrene-d10	19.680	212	350561	8.338	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.745	264	299592	7.899	ng/u1	0.00
Target Compounds						
					Qvalue	
22) Nitrobenzene	9.175	77	406595	47.670	ng/u1#	83

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009779.D
Acq On : 12 Apr 2022 12:03
Operator : CG/JU
Sample : N2338-17DL 5X
Misc :
ALS Vial : 37 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
C0J69DL

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 04/13/2022
Supervised By :Yogesh Patel 04/13/2022


Quant Time: Apr 13 02:20:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 13 02:15:22 2022
Response via : Initial Calibration

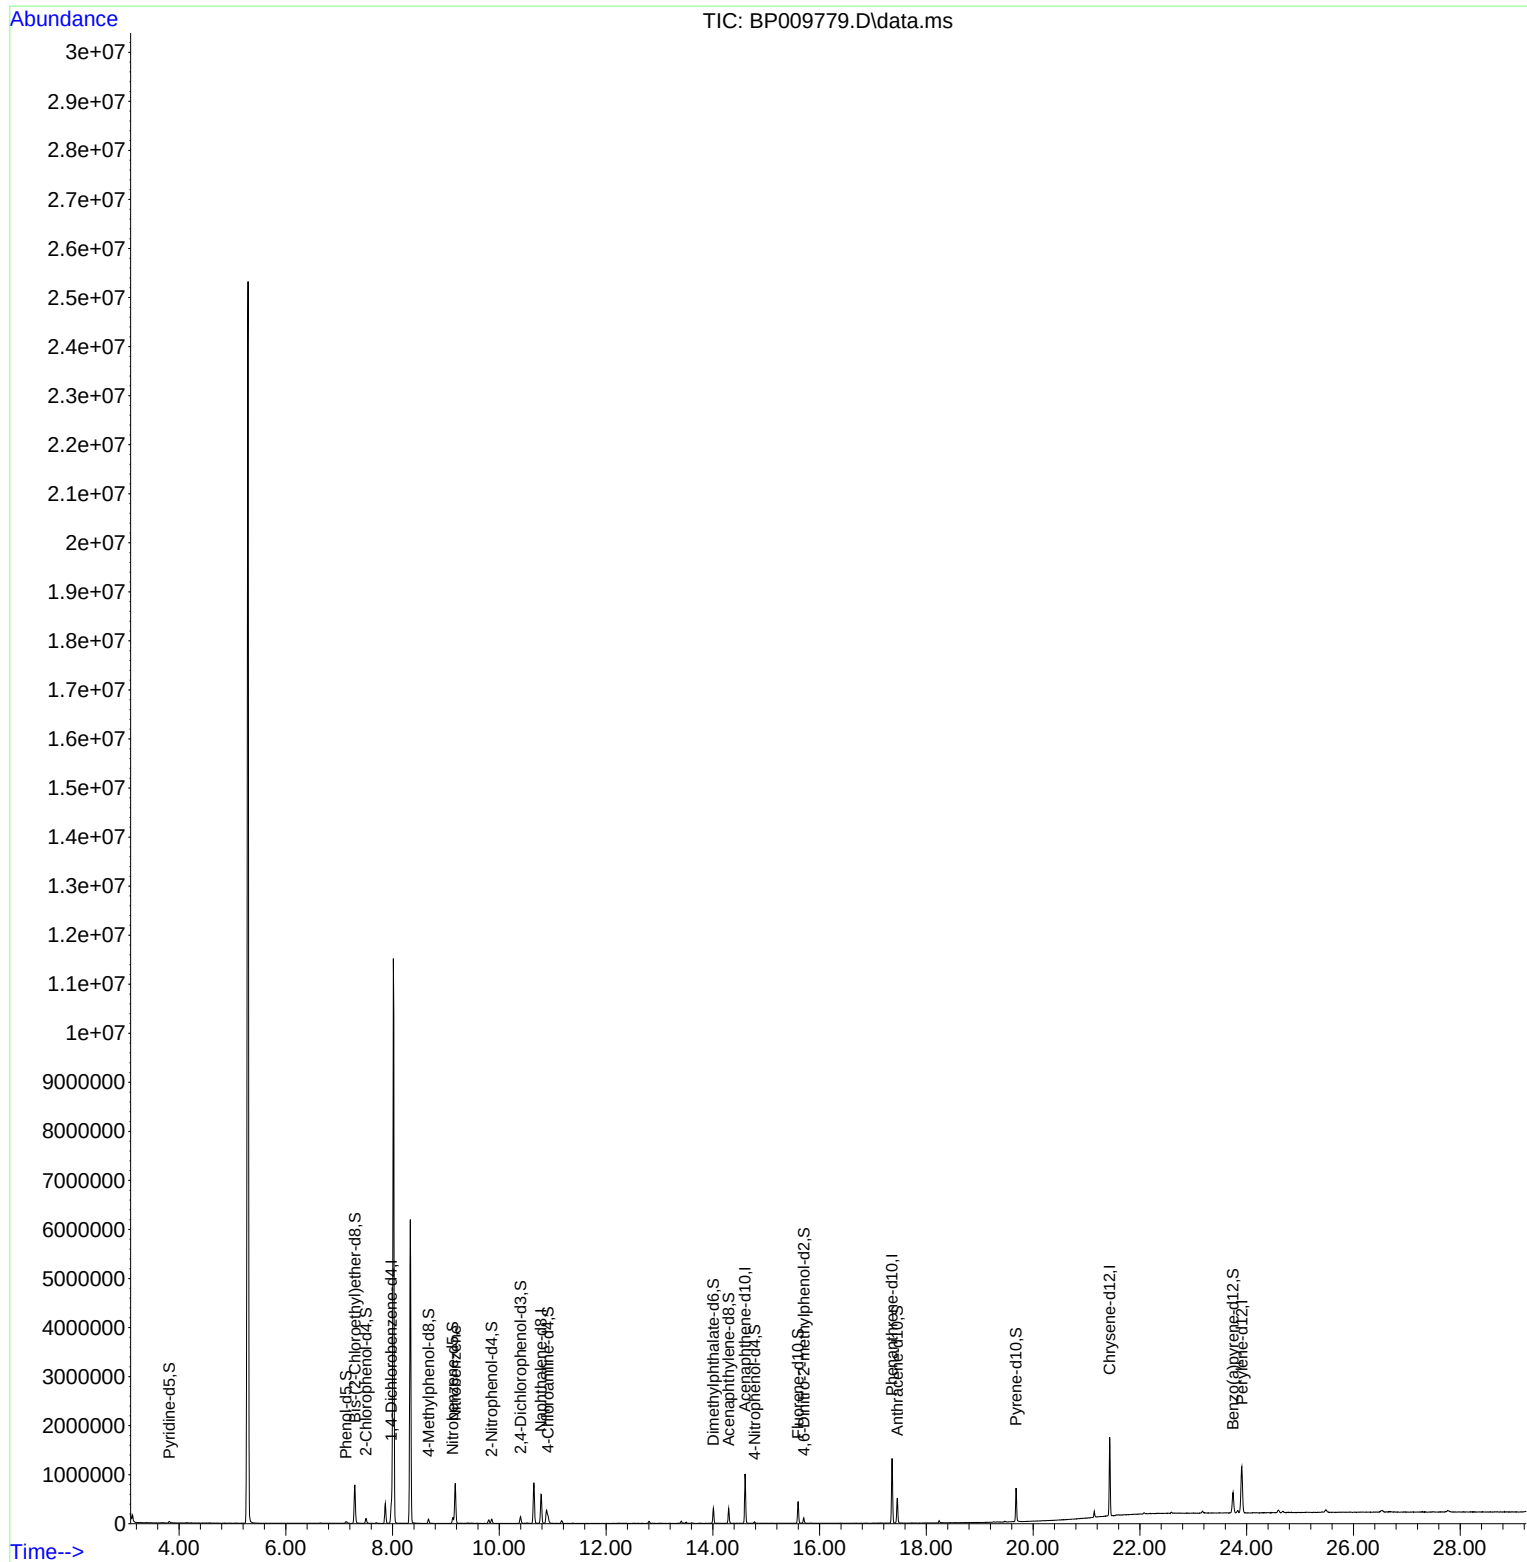

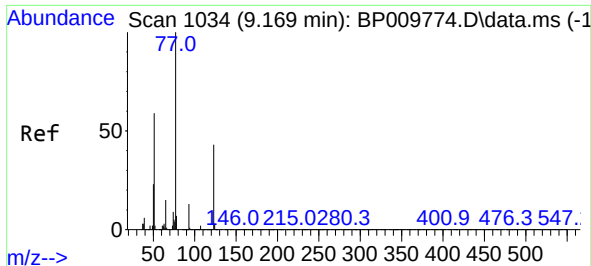

#22
Nitrobenzene
Concen: 47.670 ng/ul
RT: 9.175 min Scan# 1035
Delta R.T. 0.006 min
Lab File: BP009779.D
Acq: 12 Apr 2022 12:03

Instrument :
BNA_P
ClientSampleId :
C0J69DL

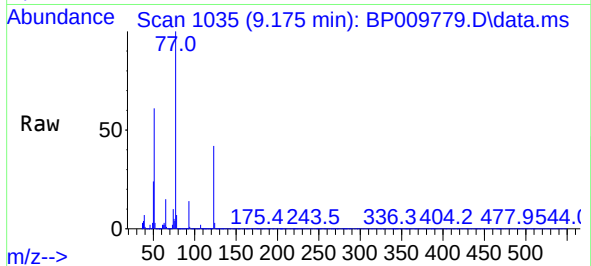

Tgt Ion: 77 Resp: 40659
Ion Ratio Lower Upper
77 100
123 41.6 42.3 63.5
65 15.1 5.8 8.8

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 04/13/2022
Supervised By :Yogesh Patel 04/13/2022

