

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
 Data File : BP009798.D
 Acq On : 13 Apr 2022 00:21
 Operator : CG/JU
 Sample : N2342-12
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0J09

Quant Time: Apr 13 04:27:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 13 02:15:22 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.963	152	124022	20.000	ng/ul	0.00
20) Naphthalene-d8	10.775	136	560884	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.598	164	416288	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.345	188	941229	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.422	240	999237	20.000	ng/ul	-0.01
88) Perylene-d12	23.892	264	960137	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	18213	6.554	ng/uL	0.00
4) Pyridine-d5	3.805	84	137261	17.915	ng/ul	0.00
7) Phenol-d5	7.116	99	146491	13.454	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.287	67	255402	39.400	ng/ul	0.00
11) 2-Chlorophenol-d4	7.493	132	257357	31.334	ng/ul	0.00
15) 4-Methylphenol-d8	8.663	113	202397	22.267	ng/ul	0.00
21) Nitrobenzene-d5	9.122	128	170168	42.072	ng/ul	0.00
24) 2-Nitrophenol-d4	9.852	143	182177	41.083	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.387	165	310150	33.424	ng/ul	0.00
31) 4-Chloroaniline-d4	10.899	131	376977	28.524	ng/ul	0.00
46) Dimethylphthalate-d6	14.004	166	1384292	42.333	ng/ul	0.00
49) Acenaphthylene-d8	14.293	160	1481324	38.237	ng/ul	0.00
54) 4-Nitrophenol-d4	14.769	143	87615	14.774	ng/ul	-0.01
60) Fluorene-d10	15.587	176	1177769	42.815	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.698	200	217756	39.053	ng/ul	0.00
73) Anthracene-d10	17.445	188	1983187	44.007	ng/ul	0.00
81) Pyrene-d10	19.675	212	2478021	45.407	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.733	264	2340800	46.816	ng/ul	0.00
Target Compounds						
8) Phenol	7.146	94	23397	2.147	ng/ul#	90
22) Nitrobenzene	9.163	77	12978	1.250	ng/ul#	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009798.D
Acq On : 13 Apr 2022 00:21
Operator : CG/JU
Sample : N2342-12
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0J09

Quant Time: Apr 13 04:27:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 13 02:15:22 2022
Response via : Initial Calibration




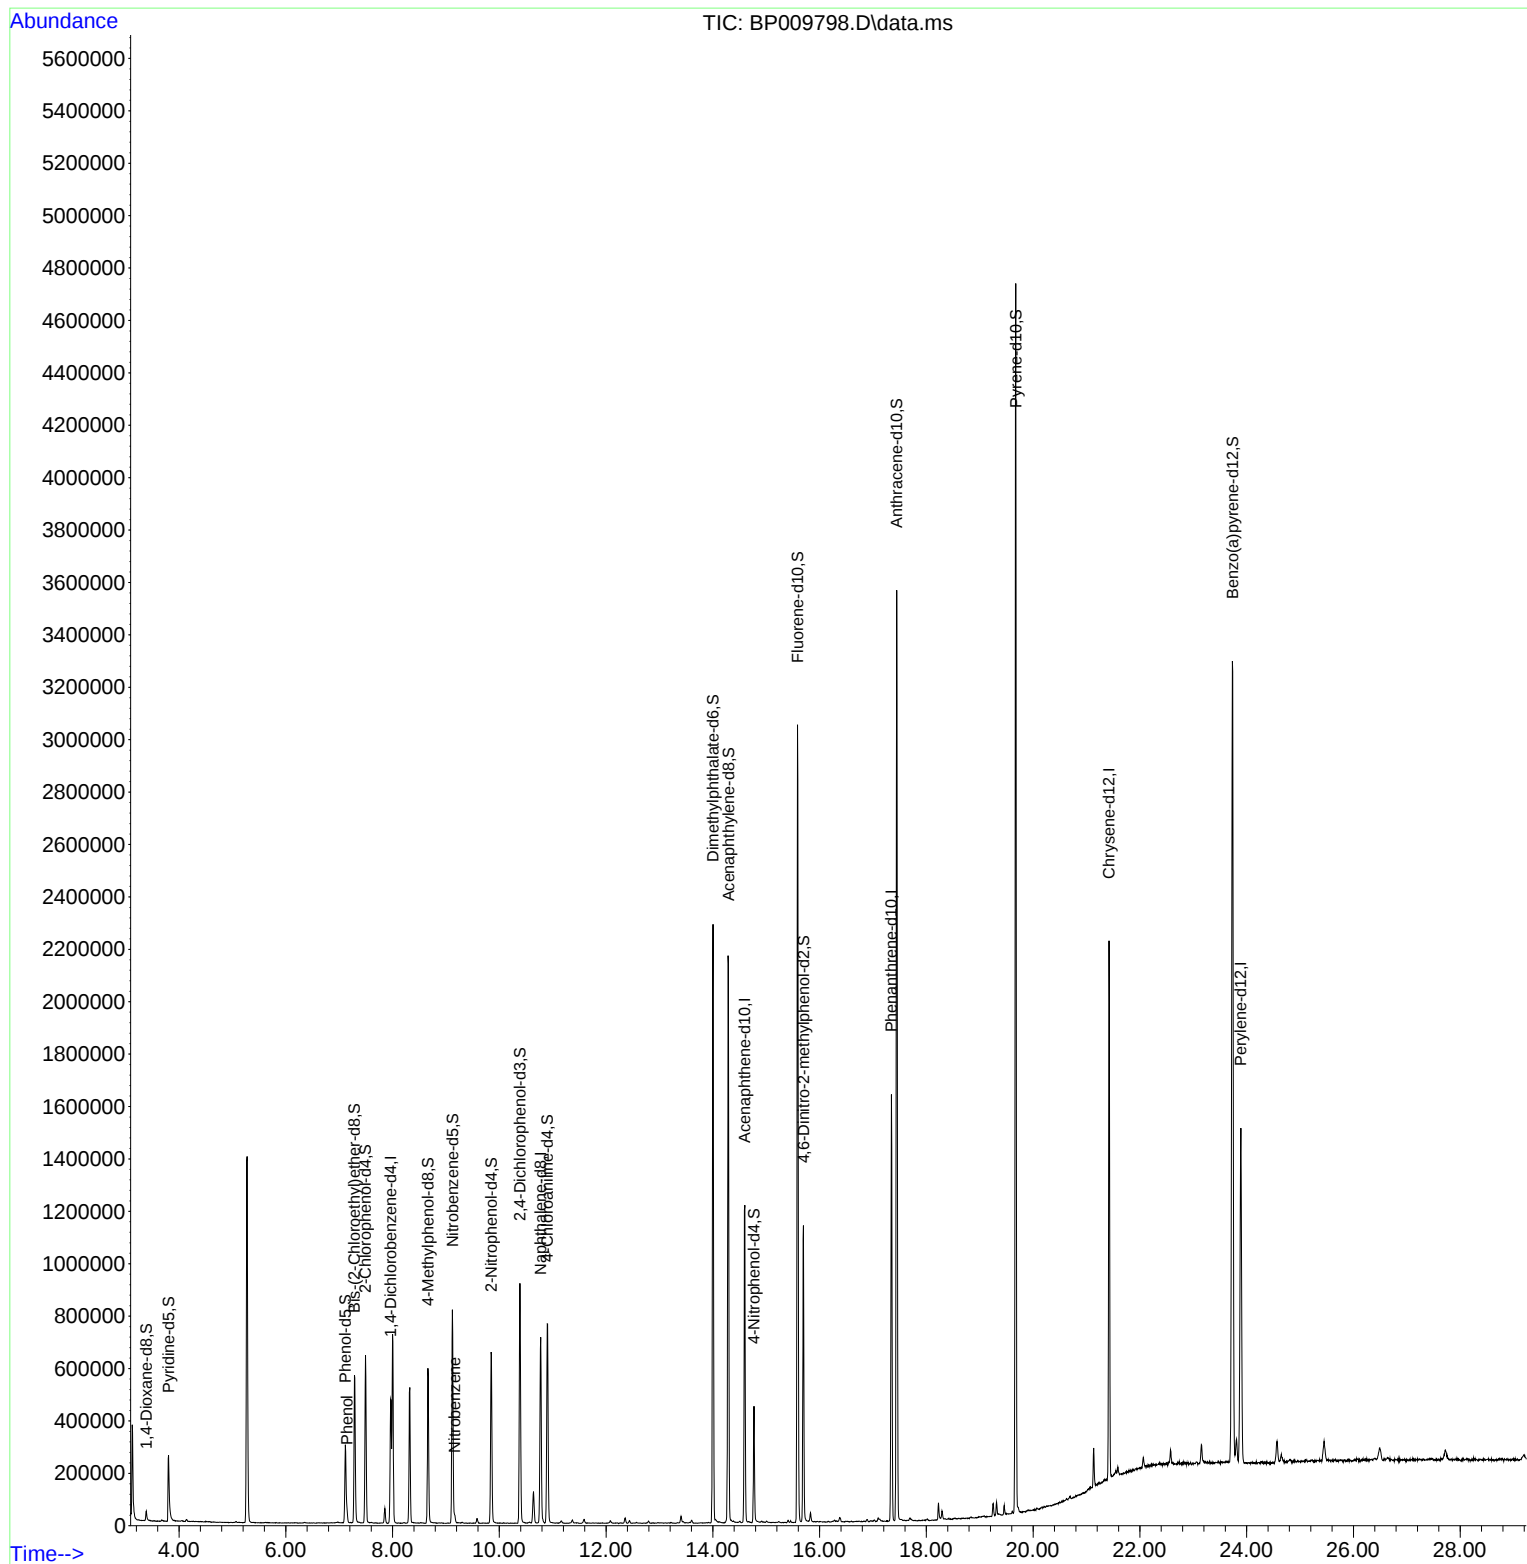


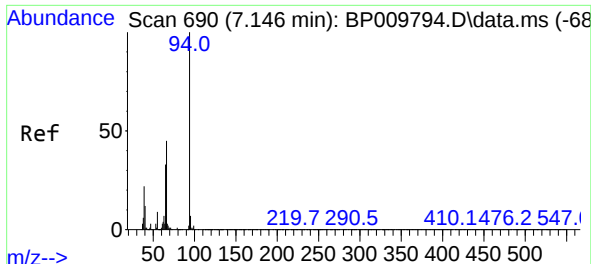

#8
Phenol
Concen: 2.147 ng/ul
RT: 7.146 min Scan# 690
Delta R.T. 0.000 min
Lab File: BP009798.D
Acq: 13 Apr 2022 00:21

Instrument :
BNA_P
ClientSampleId :
C0J09

Tgt Ion: 94 Resp: 23397
Ion Ratio Lower Upper
94 100
65 32.3 19.0 28.6#
66 47.0 34.6 51.8

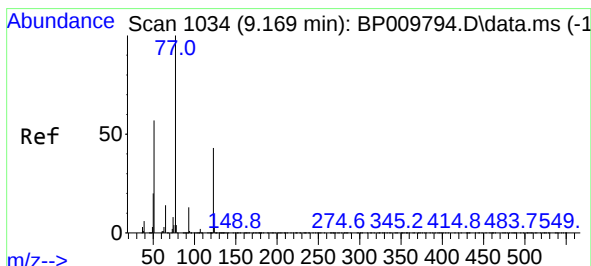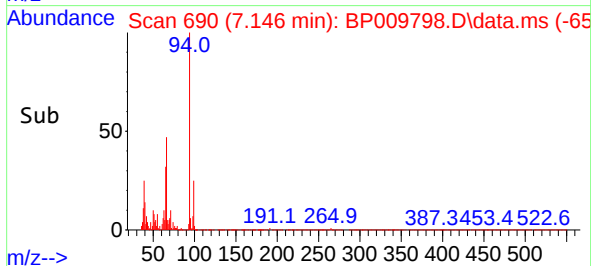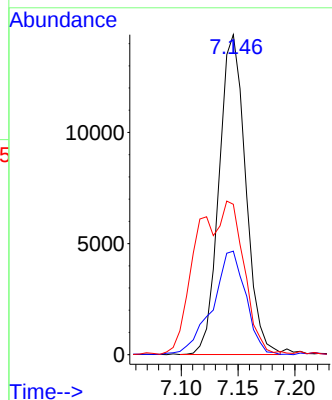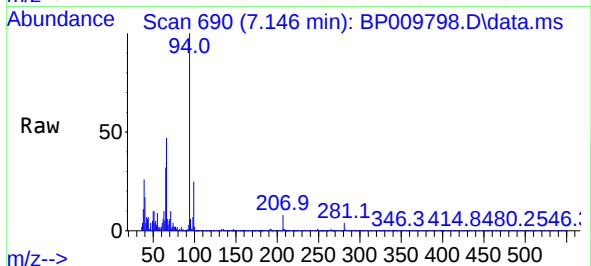

#22
Nitrobenzene
Concen: 1.250 ng/ul
RT: 9.163 min Scan# 1033
Delta R.T. -0.006 min
Lab File: BP009798.D
Acq: 13 Apr 2022 00:21

Tgt Ion: 77 Resp: 12978
Ion Ratio Lower Upper
77 100
123 39.7 42.3 63.5#
65 13.3 5.8 8.8#

