

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
 Data File : BP009746.D
 Acq On : 11 Apr 2022 11:48
 Operator : CG/JU
 Sample : PB144004BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK004

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009746.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	4	7	12	rVB	10478	14463	0.41%	0.042%
2	3.387	47	51	61	rVB	29733	43473	1.22%	0.126%
3	3.805	118	122	140	rBV	369167	617317	17.39%	1.794%
4	4.140	176	179	185	rBV5	4785	7790	0.22%	0.023%
5	7.122	679	686	704	rVB	504004	792282	22.32%	2.302%
6	7.293	709	715	729	rVB	374555	619960	17.47%	1.801%
7	7.499	742	750	766	rBV	495049	796976	22.46%	2.316%
8	7.969	824	830	844	rVB	360435	607074	17.10%	1.764%
9	8.669	941	949	965	rBV	632276	1029451	29.01%	2.991%
10	9.128	1019	1027	1040	rBV	510174	854115	24.07%	2.482%
11	9.857	1142	1151	1159	rBV	402623	682646	19.23%	1.983%
12	10.393	1233	1242	1259	rBV	640583	1049747	29.58%	3.050%
13	10.781	1300	1308	1321	rVB	539516	922190	25.98%	2.679%
14	10.904	1321	1329	1346	rBV	640858	1145294	32.27%	3.328%
15	12.363	1571	1577	1586	rVB2	14222	24649	0.69%	0.072%
16	14.010	1848	1857	1873	rBV	1377670	1861619	52.45%	5.409%
17	14.298	1897	1906	1916	rBV	1267490	1959975	55.22%	5.695%
18	14.604	1949	1958	1970	rBV	890886	1350418	38.05%	3.924%
19	14.775	1980	1987	1997	rBV	677094	982111	27.67%	2.854%
20	15.598	2120	2127	2138	rBV	1739989	2557754	72.07%	7.432%
21	15.704	2138	2145	2159	rVV	592004	849491	23.93%	2.468%
22	15.834	2162	2167	2174	rVB2	19017	30878	0.87%	0.090%
23	16.381	2256	2260	2264	rVB5	6022	8538	0.24%	0.025%
24	17.034	2368	2371	2379	rVB9	3094	4193	0.12%	0.012%
25	17.145	2385	2390	2392	rVB3	4514	5436	0.15%	0.016%
26	17.351	2417	2425	2434	rBV	1151489	1681527	47.38%	4.886%
27	17.451	2436	2442	2457	rVB	2054511	2925228	82.42%	8.499%
28	19.257	2745	2749	2753	rVB4	26760	35577	1.00%	0.103%
29	19.328	2756	2761	2767	rVB	26514	38203	1.08%	0.111%
30	19.680	2815	2821	2832	rBV	2756682	3518193	99.13%	10.222%
31	21.433	3114	3119	3125	rVB	1467189	1934238	54.50%	5.620%
32	23.745	3505	3512	3522	rVB2	1740967	3549199	100.00%	10.312%
33	23.904	3532	3539	3550	rVB2	917035	1917000	54.01%	5.570%




Sum of corrected areas: 34417005

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009746.D
Acq On : 11 Apr 2022 11:48
Operator : CG/JU
Sample : PB144004BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK004

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

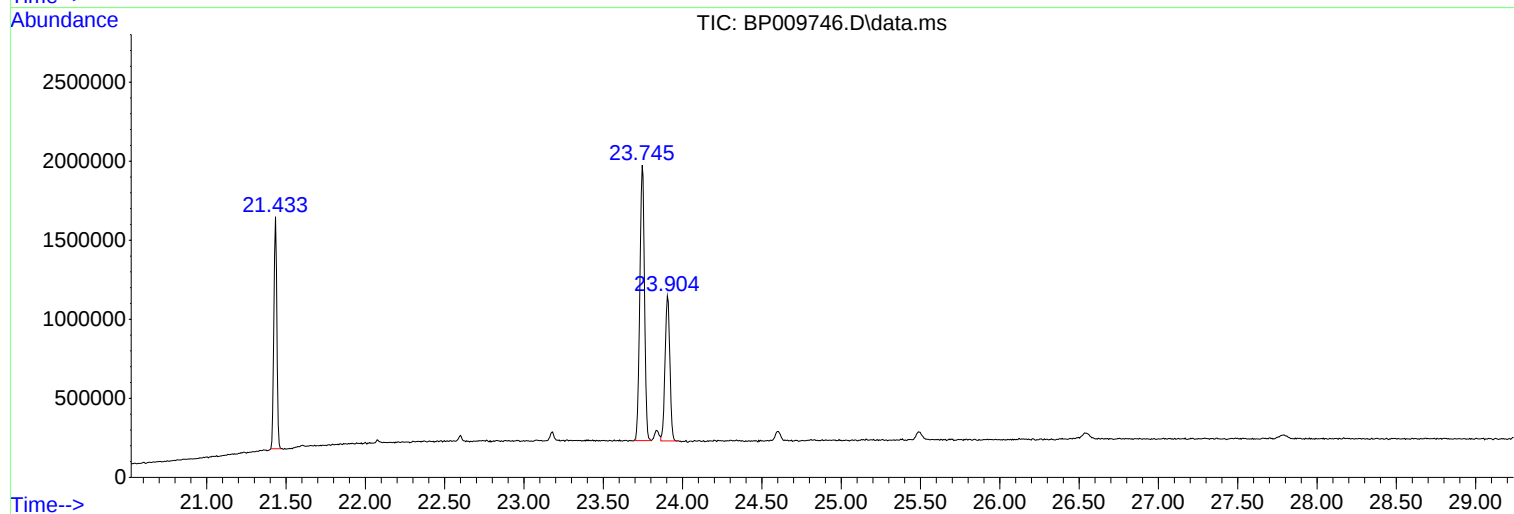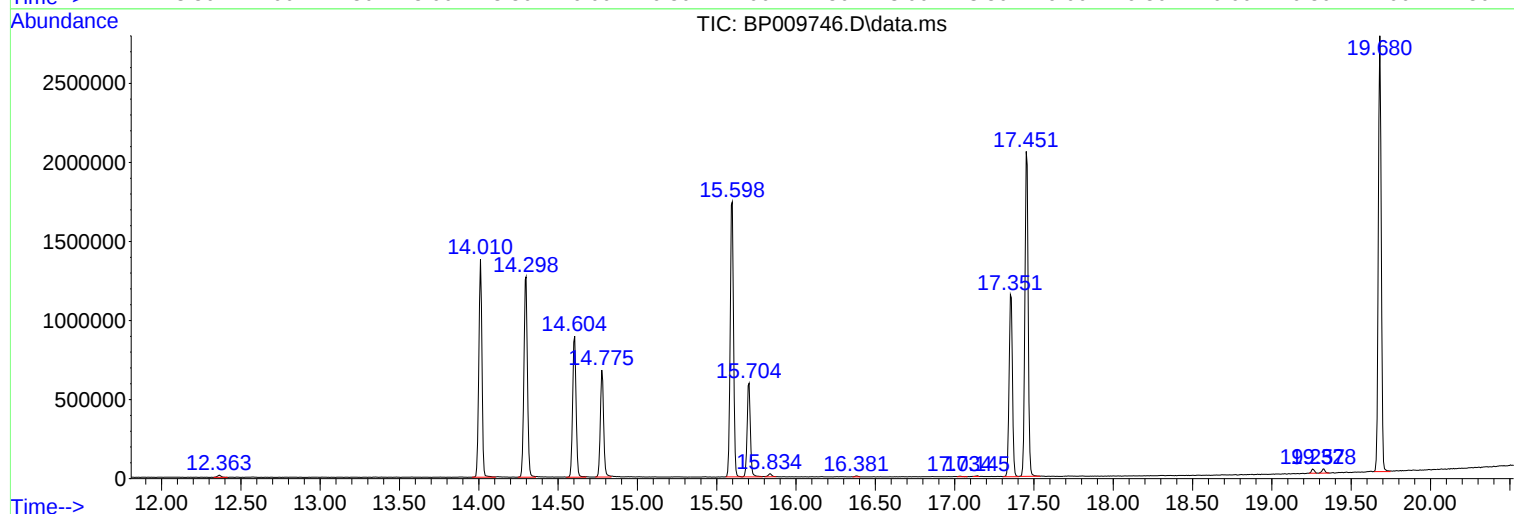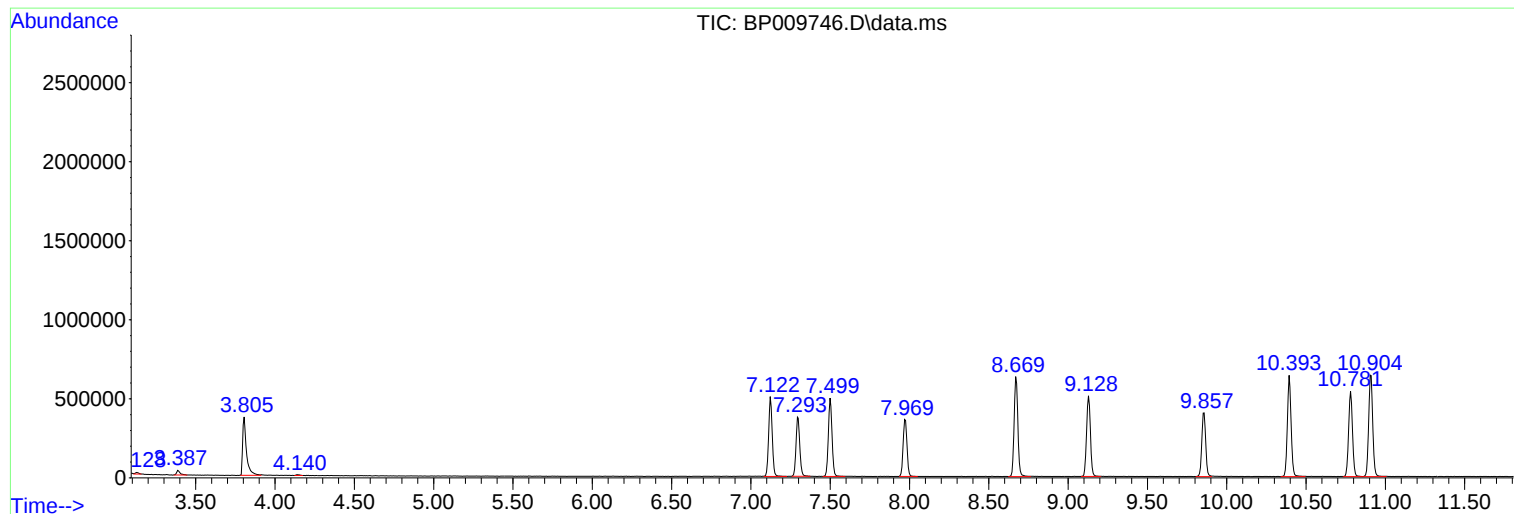

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009746.D
Acq On : 11 Apr 2022 11:48
Operator : CG/JU
Sample : PB144004BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK004

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009746.D
Acq On : 11 Apr 2022 11:48
Operator : CG/JU
Sample : PB144004BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK004

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc