

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
 Data File : BP009759.D
 Acq On : 11 Apr 2022 19:53
 Operator : CG/JU
 Sample : PB144014BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK014

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009759.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.129	4	7	16	rVB2	20220	32654	0.74%	0.077%
2	3.387	47	51	61	rVB	38433	56443	1.27%	0.133%
3	3.805	118	122	141	rBV	476990	758925	17.14%	1.787%
4	4.140	176	179	183	rVB	8057	9724	0.22%	0.023%
5	7.122	679	686	696	rBV	608871	963714	21.77%	2.269%
6	7.293	708	715	725	rBV	480335	755123	17.06%	1.778%
7	7.499	742	750	764	rBV	630049	988773	22.33%	2.328%
8	7.969	823	830	843	rBV	435273	706671	15.96%	1.664%
9	8.669	939	949	964	rBV	786989	1286802	29.07%	3.029%
10	9.128	1019	1027	1038	rBV	661136	1076160	24.31%	2.534%
11	9.852	1142	1150	1161	rBV	536647	892772	20.17%	2.102%
12	10.393	1234	1242	1252	rBV	761056	1306497	29.51%	3.076%
13	10.781	1297	1308	1317	rBV	638336	1075243	24.29%	2.531%
14	10.905	1322	1329	1345	rVV	836688	1443480	32.61%	3.398%
15	12.363	1571	1577	1585	rVB2	16377	28068	0.63%	0.066%
16	12.575	1608	1613	1616	rBV7	2657	4518	0.10%	0.011%
17	14.010	1849	1857	1870	rBV	1710639	2406355	54.36%	5.665%
18	14.293	1894	1905	1920	rBV	1707999	2521483	56.96%	5.936%
19	14.598	1951	1957	1968	rBV	1042297	1605913	36.27%	3.781%
20	14.775	1980	1987	2003	rBV	897442	1311176	29.62%	3.087%
21	15.240	2060	2066	2068	rBV7	2555	4929	0.11%	0.012%
22	15.593	2119	2126	2138	rBV	2238130	3283032	74.16%	7.729%
23	15.698	2138	2144	2156	rBV	790735	1145981	25.89%	2.698%
24	15.834	2162	2167	2172	rVB2	26326	35529	0.80%	0.084%
25	16.157	2218	2222	2227	rBV7	2174	4546	0.10%	0.011%
26	16.381	2255	2260	2267	rVB6	8260	12777	0.29%	0.030%
27	17.028	2367	2370	2375	rBV7	4805	7394	0.17%	0.017%
28	17.134	2382	2388	2393	rBV3	6479	12349	0.28%	0.029%
29	17.351	2418	2425	2433	rBV	1384989	2016918	45.56%	4.748%
30	17.451	2435	2442	2454	rBV	2673186	3784021	85.47%	8.909%
31	19.257	2745	2749	2754	rBV4	33003	45482	1.03%	0.107%
32	19.322	2756	2760	2765	rBV	32908	48366	1.09%	0.114%
33	19.681	2815	2821	2832	rBV	3336906	4427056	100.00%	10.423%
34	21.433	3113	3119	3126	rBV	1677552	2278428	51.47%	5.364%
35	23.745	3504	3512	3520	rVB2	2016649	4057356	91.65%	9.552%
36	23.904	3532	3539	3548	rVB2	1009359	2081141	47.01%	4.900%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009759.D
Acq On : 11 Apr 2022 19:53
Operator : CG/JU
Sample : PB144014BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK014

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Title : SVOA CALIBRATION




Sum of corrected areas: 42475799

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009759.D
Acq On : 11 Apr 2022 19:53
Operator : CG/JU
Sample : PB144014BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK014

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

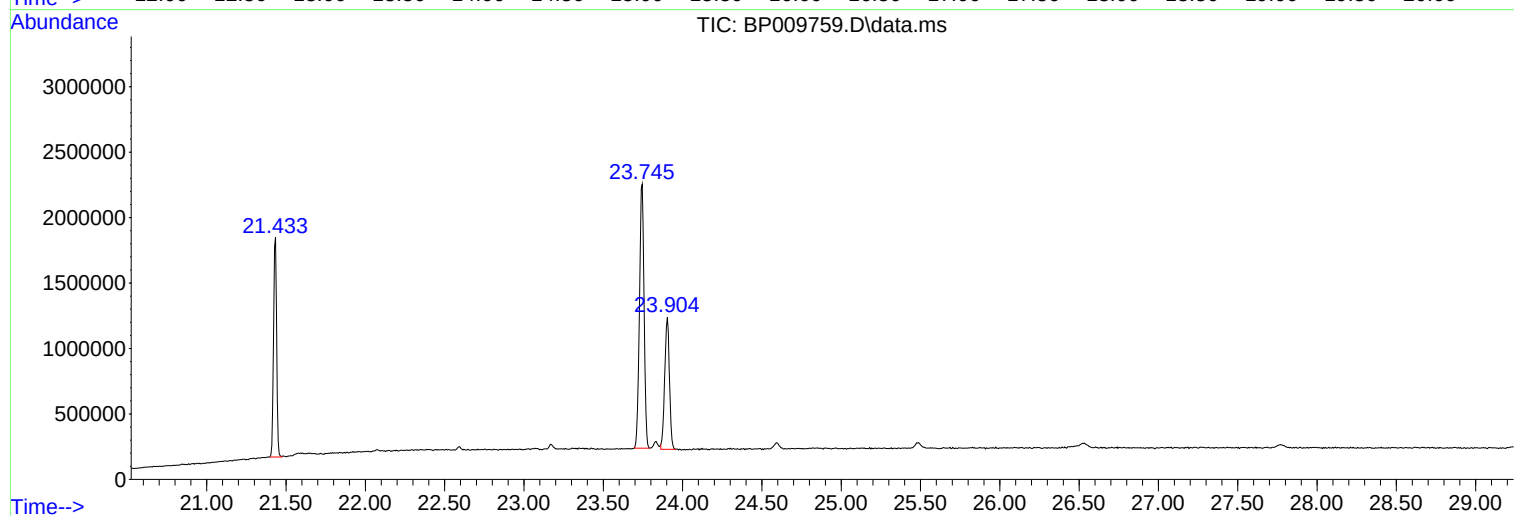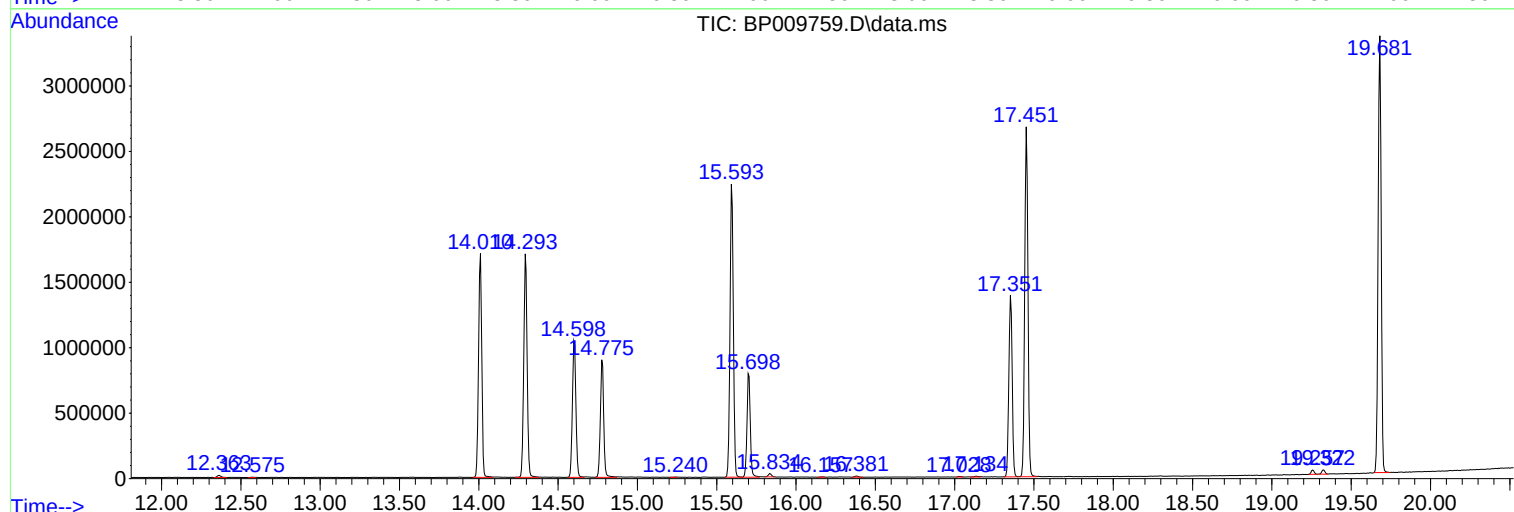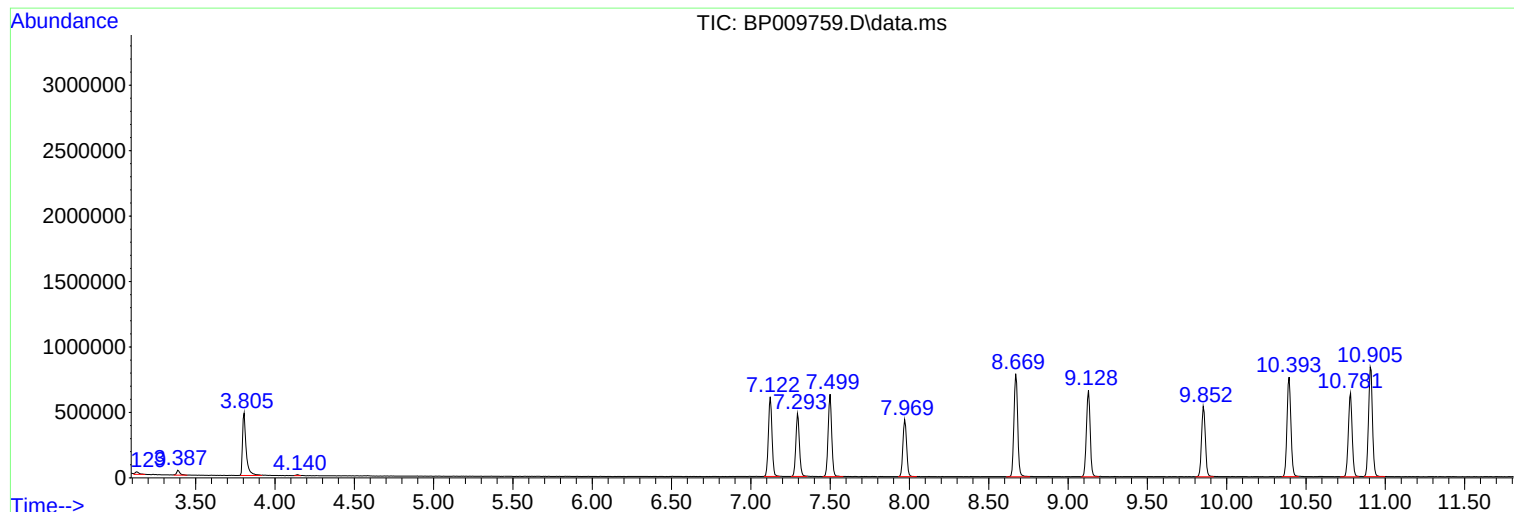

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009759.D
Acq On : 11 Apr 2022 19:53
Operator : CG/JU
Sample : PB144014BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK014

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009759.D
Acq On : 11 Apr 2022 19:53
Operator : CG/JU
Sample : PB144014BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK014

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc