

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
 Data File : BP009760.D
 Acq On : 11 Apr 2022 20:27
 Operator : CG/JU
 Sample : PB144015BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK015

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009760.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	4	7	13	rVB2	11515	15786	0.44%	0.048%
2	3.387	47	51	63	rVB	26210	42408	1.19%	0.130%
3	3.805	118	122	138	rBV	324725	562305	15.76%	1.720%
4	4.140	176	179	186	rVB	5405	7725	0.22%	0.024%
5	7.122	678	686	696	rBV	461875	730909	20.48%	2.236%
6	7.293	708	715	729	rVB	360795	568814	15.94%	1.740%
7	7.499	743	750	761	rBV	455575	729730	20.45%	2.233%
8	7.969	823	830	842	rVB	315185	514004	14.40%	1.573%
9	8.669	942	949	965	rBV	612429	963169	26.99%	2.947%
10	9.128	1019	1027	1042	rBV	486014	814705	22.83%	2.493%
11	9.852	1141	1150	1161	rBV	402509	665124	18.64%	2.035%
12	10.393	1233	1242	1252	rBV	582196	982904	27.54%	3.007%
13	10.781	1300	1308	1317	rBV	452395	776916	21.77%	2.377%
14	10.904	1320	1329	1342	rBV	639384	1092380	30.61%	3.342%
15	12.363	1569	1577	1582	rBV2	12732	21062	0.59%	0.064%
16	14.004	1850	1856	1864	rBV	1254949	1826194	51.17%	5.587%
17	14.292	1895	1905	1914	rBV	1256752	1884260	52.80%	5.765%
18	14.428	1921	1928	1930	rBV7	5089	7861	0.22%	0.024%
19	14.598	1950	1957	1967	rBV	770888	1161522	32.55%	3.554%
20	14.775	1978	1987	2001	rBV	710490	992337	27.81%	3.036%
21	15.422	2091	2097	2102	rBV8	2140	4448	0.12%	0.014%
22	15.592	2119	2126	2135	rBV	1716502	2490503	69.79%	7.620%
23	15.698	2138	2144	2160	rVV	631367	860248	24.11%	2.632%
24	15.834	2162	2167	2174	rVB2	19346	30207	0.85%	0.092%
25	16.381	2254	2260	2264	rBV6	7780	11007	0.31%	0.034%
26	17.028	2366	2370	2374	rBV7	2665	4157	0.12%	0.013%
27	17.134	2384	2388	2392	rBV4	4130	6787	0.19%	0.021%
28	17.351	2418	2425	2433	rBV	1045434	1478797	41.44%	4.524%
29	17.451	2435	2442	2455	rVV	1980559	2851626	79.91%	8.724%
30	17.722	2483	2488	2492	rBV8	3397	7054	0.20%	0.022%
31	19.257	2745	2749	2754	rBV4	26484	35555	1.00%	0.109%
32	19.322	2756	2760	2765	rVV2	25075	35459	0.99%	0.108%
33	19.680	2814	2821	2830	rBV	2582296	3432353	96.18%	10.501%
34	21.433	3113	3119	3125	rBV	1350733	1736331	48.65%	5.312%
35	23.745	3504	3512	3521	rVB2	1803216	3568722	100.00%	10.918%
36	23.904	3532	3539	3547	rVB	871389	1772106	49.66%	5.422%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009760.D
Acq On : 11 Apr 2022 20:27
Operator : CG/JU
Sample : PB144015BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK015

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Title : SVOA CALIBRATION




Sum of corrected areas: 32685475

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009760.D
Acq On : 11 Apr 2022 20:27
Operator : CG/JU
Sample : PB144015BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK015

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

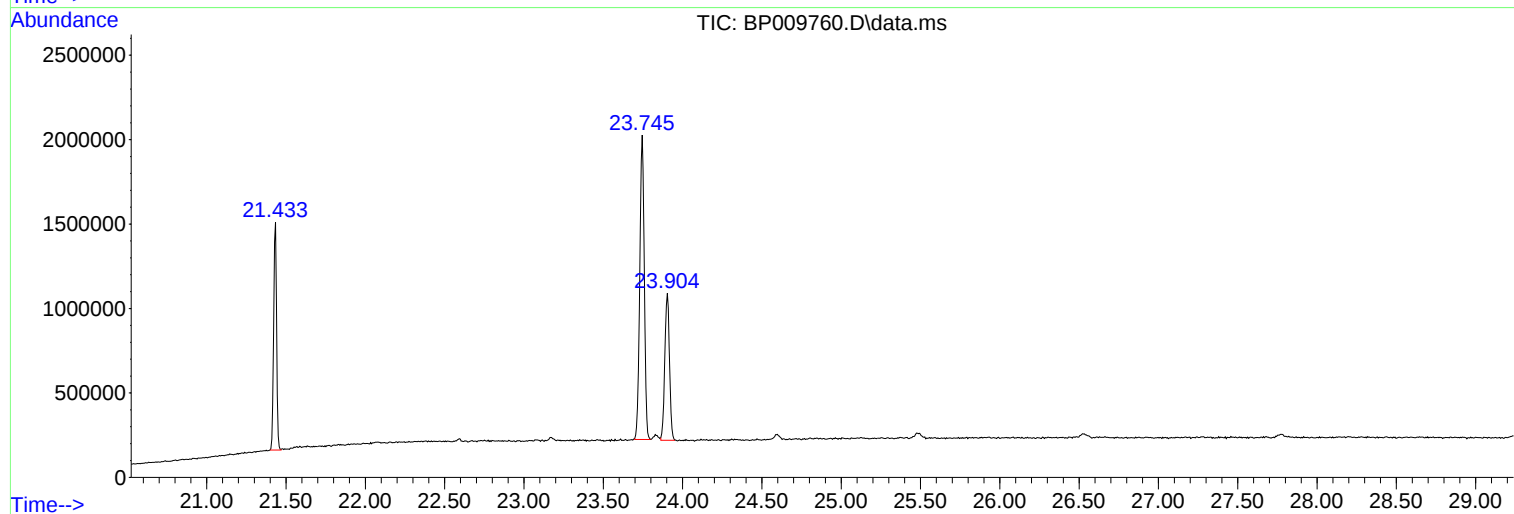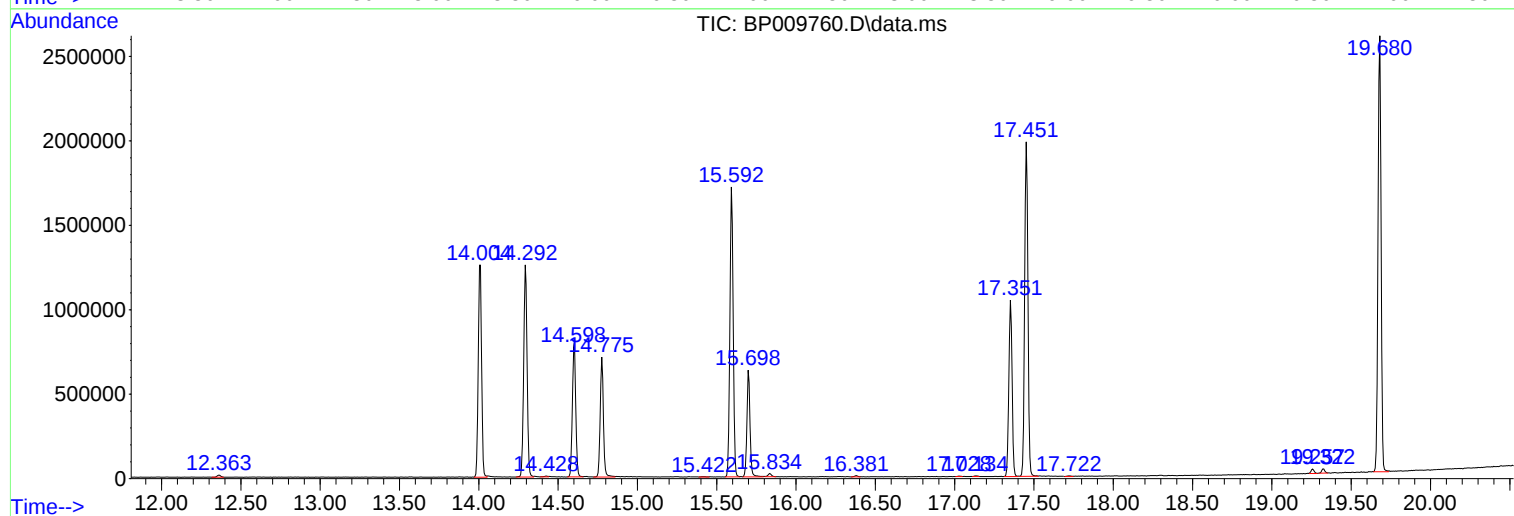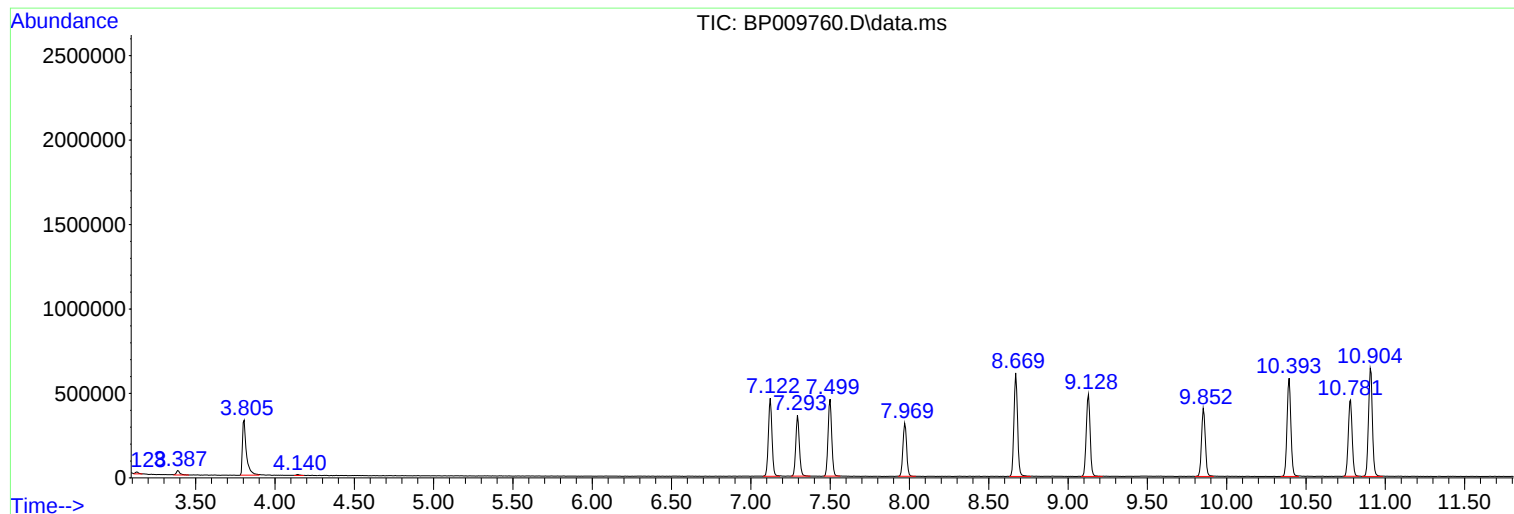

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009760.D
Acq On : 11 Apr 2022 20:27
Operator : CG/JU
Sample : PB144015BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK015

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009760.D
Acq On : 11 Apr 2022 20:27
Operator : CG/JU
Sample : PB144015BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK015

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
