

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
 Data File : BP009785.D
 Acq On : 12 Apr 2022 16:27
 Operator : CG/JU
 Sample : PB144055BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK055

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009785.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	4	7	13	rVB2	14496	17608	0.46%	0.045%
2	3.387	47	51	61	rVB	35396	52389	1.38%	0.133%
3	3.805	118	122	140	rBV	438518	728482	19.22%	1.849%
4	4.140	175	179	185	rVB	12862	19637	0.52%	0.050%
5	7.122	679	686	695	rBV	554440	898751	23.72%	2.281%
6	7.293	708	715	727	rBV	435877	688719	18.18%	1.748%
7	7.493	741	749	761	rBV	558990	917070	24.20%	2.328%
8	7.969	822	830	837	rBV	495974	806607	21.29%	2.047%
9	8.669	941	949	961	rBV	725954	1176474	31.05%	2.986%
10	9.122	1019	1026	1040	rBV	597019	991490	26.17%	2.516%
11	9.852	1141	1150	1160	rBV	480869	805877	21.27%	2.045%
12	10.387	1233	1241	1256	rBV	695212	1201007	31.69%	3.048%
13	10.775	1298	1307	1318	rBV	712335	1219754	32.19%	3.096%
14	10.905	1321	1329	1340	rBV	774570	1300012	34.31%	3.299%
15	12.357	1572	1576	1582	rVB3	14673	24125	0.64%	0.061%
16	14.004	1848	1856	1870	rBV	1482651	2044280	53.95%	5.188%
17	14.122	1872	1876	1882	rVB9	2403	5112	0.13%	0.013%
18	14.293	1897	1905	1915	rBV	1470174	2200213	58.06%	5.584%
19	14.598	1950	1957	1966	rBV	1194374	1768491	46.67%	4.488%
20	14.663	1966	1968	1973	rVB6	2945	4489	0.12%	0.011%
21	14.775	1980	1987	1998	rBV	761862	1116446	29.46%	2.834%
22	15.593	2118	2126	2136	rBV	1963131	2856197	75.38%	7.249%
23	15.698	2137	2144	2159	rVV	673419	936902	24.73%	2.378%
24	15.834	2162	2167	2172	rVB	22540	35133	0.93%	0.089%
25	16.375	2255	2259	2264	rVB5	8604	10735	0.28%	0.027%
26	17.028	2365	2370	2376	rBV9	5656	9951	0.26%	0.025%
27	17.128	2383	2387	2393	rBV3	5792	9567	0.25%	0.024%
28	17.345	2417	2424	2434	rBV	1527673	2213822	58.42%	5.619%
29	17.445	2434	2441	2451	rBV	2192164	3197731	84.39%	8.116%
30	17.598	2463	2467	2471	rBV7	2580	5605	0.15%	0.014%
31	19.251	2744	2748	2754	rBV3	31247	44692	1.18%	0.113%
32	19.322	2756	2760	2767	rVV	28894	40549	1.07%	0.103%
33	19.675	2814	2820	2829	rBV	2976756	3789276	100.00%	9.617%
34	21.428	3113	3118	3125	rVB	1978405	2504602	66.10%	6.357%
35	23.739	3503	3511	3519	rBV	1713531	3453689	91.14%	8.766%
36	23.898	3531	3538	3550	rVB2	1130420	2305417	60.84%	5.851%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009785.D
Acq On : 12 Apr 2022 16:27
Operator : CG/JU
Sample : PB144055BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK055

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Title : SVOA CALIBRATION


Sum of corrected areas: 39400901

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009785.D
Acq On : 12 Apr 2022 16:27
Operator : CG/JU
Sample : PB144055BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK055

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

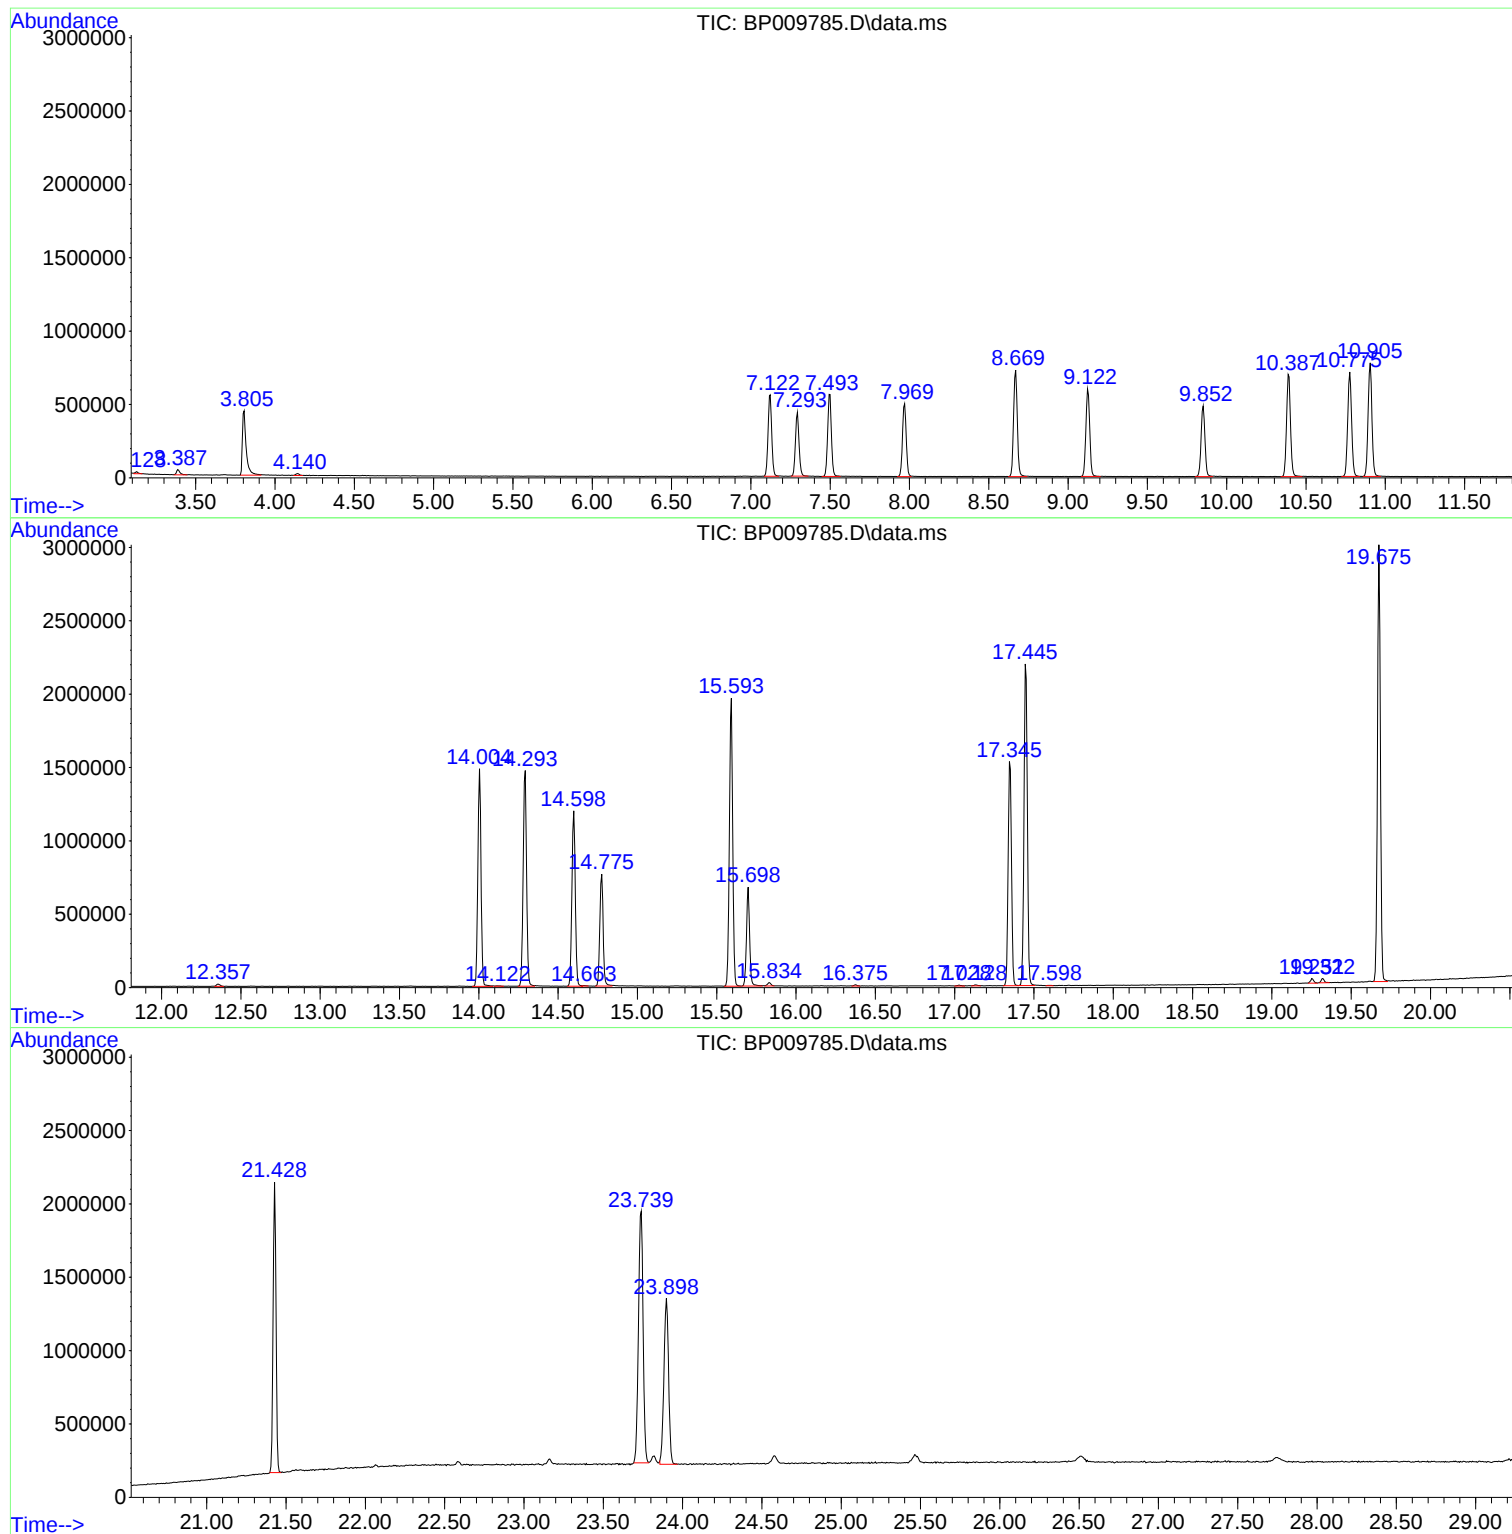

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009785.D
Acq On : 12 Apr 2022 16:27
Operator : CG/JU
Sample : PB144055BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK055

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009785.D
Acq On : 12 Apr 2022 16:27
Operator : CG/JU
Sample : PB144055BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK055

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc