

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
 Data File : BP009789.D
 Acq On : 12 Apr 2022 18:42
 Operator : CG/JU
 Sample : N2316-17
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 ETNR5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009789.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.123	3	6	18	rVB	341222	443737	10.49%	1.263%
2	3.387	46	51	62	rVB	24072	39926	0.94%	0.114%
3	3.805	119	122	139	rBV	105922	175717	4.15%	0.500%
4	4.140	174	179	187	rVB2	7995	14951	0.35%	0.043%
5	7.117	675	685	695	rBV	114162	193796	4.58%	0.552%
6	7.287	708	714	731	rVB	354932	592921	14.01%	1.688%
7	7.493	742	749	759	rBV	381601	612897	14.48%	1.745%
8	7.964	821	829	838	rBV	406927	668195	15.79%	1.902%
9	8.211	866	871	878	rBV9	4254	8875	0.21%	0.025%
10	8.534	921	926	928	rBV5	3607	5677	0.13%	0.016%
11	8.663	941	948	962	rBV	320117	521160	12.32%	1.484%
12	8.881	980	985	990	rBV6	3309	6665	0.16%	0.019%
13	9.122	1018	1026	1033	rBV	508447	835478	19.74%	2.379%
14	9.234	1042	1045	1051	rVV6	3919	5515	0.13%	0.016%
15	9.299	1051	1056	1064	rVB8	9490	16398	0.39%	0.047%
16	9.852	1140	1150	1159	rBV	371952	648364	15.32%	1.846%
17	10.387	1233	1241	1262	rVB	546604	930945	22.00%	2.650%
18	10.775	1299	1307	1316	rBV	590537	1004979	23.75%	2.861%
19	10.905	1321	1329	1341	rVV	567107	994591	23.50%	2.832%
20	11.334	1397	1402	1407	rVB6	2410	4238	0.10%	0.012%
21	11.569	1436	1442	1450	rBV7	8146	16886	0.40%	0.048%
22	12.357	1570	1576	1583	rVB	12537	21732	0.51%	0.062%
23	12.975	1675	1681	1684	rBV7	2875	6003	0.14%	0.017%
24	13.222	1715	1723	1727	rBV9	3120	6443	0.15%	0.018%
25	14.004	1849	1856	1864	rBV	1342116	1872143	44.24%	5.330%
26	14.287	1894	1904	1922	rBV	1296217	1943840	45.94%	5.534%
27	14.598	1949	1957	1967	rBV	961640	1483272	35.05%	4.223%
28	14.669	1967	1969	1976	rVB8	3750	5384	0.13%	0.015%
29	14.769	1979	1986	2001	rBV	156511	247221	5.84%	0.704%
30	15.010	2022	2027	2031	rVB7	4526	5665	0.13%	0.016%
31	15.281	2069	2073	2078	rVB3	4242	6591	0.16%	0.019%
32	15.410	2088	2095	2102	rVB4	8012	12367	0.29%	0.035%
33	15.587	2116	2125	2136	rBV	1859740	2790909	65.96%	7.946%
34	15.698	2137	2144	2160	rVV	698843	1018817	24.08%	2.901%
35	15.828	2162	2166	2172	rVB2	23585	36951	0.87%	0.105%
36	16.275	2237	2242	2250	rBV2	3769	8397	0.20%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
 Data File : BP009789.D
 Acq On : 12 Apr 2022 18:42
 Operator : CG/JU
 Sample : N2316-17
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 ETNR5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

37	16.375	2253	2259	2267	rVB8	7165	12902	0.30%	0.037%
38	17.028	2365	2370	2374	rBV8	4558	5616	0.13%	0.016%
39	17.128	2384	2387	2392	rVB4	5482	7914	0.19%	0.023%
40	17.345	2418	2424	2433	rBV	1303818	1877633	44.37%	5.346%
41	17.445	2435	2441	2451	rVV	2423592	3502404	82.77%	9.972%
42	17.534	2453	2456	2462	rVB7	10867	14673	0.35%	0.042%
43	17.639	2472	2474	2478	rVB5	3824	4565	0.11%	0.013%
44	18.022	2533	2539	2541	rBV6	5905	8073	0.19%	0.023%
45	18.228	2570	2574	2582	rBV10	11832	22603	0.53%	0.064%
46	18.304	2582	2587	2590	rVV2	7837	9569	0.23%	0.027%
47	18.645	2643	2645	2649	rBV4	3586	5404	0.13%	0.015%
48	18.698	2651	2654	2657	rBV5	3500	5211	0.12%	0.015%
49	18.839	2676	2678	2681	rBV4	3257	4468	0.11%	0.013%
50	19.251	2744	2748	2753	rVB3	29821	40350	0.95%	0.115%
51	19.316	2755	2759	2763	rBV	32940	46978	1.11%	0.134%
52	19.598	2805	2807	2814	rBV7	8684	16624	0.39%	0.047%
53	19.675	2814	2820	2832	rVV	3198257	4231433	100.00%	12.047%
54	21.428	3112	3118	3124	rBV	1608502	2161788	51.09%	6.155%
55	23.733	3503	3510	3519	rVB2	1935238	3925411	92.77%	11.176%
56	23.892	3530	3537	3547	rVB2	963282	2012799	47.57%	5.731%


Sum of corrected areas: 35124064

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009789.D
Acq On : 12 Apr 2022 18:42
Operator : CG/JU
Sample : N2316-17
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
ETNR5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

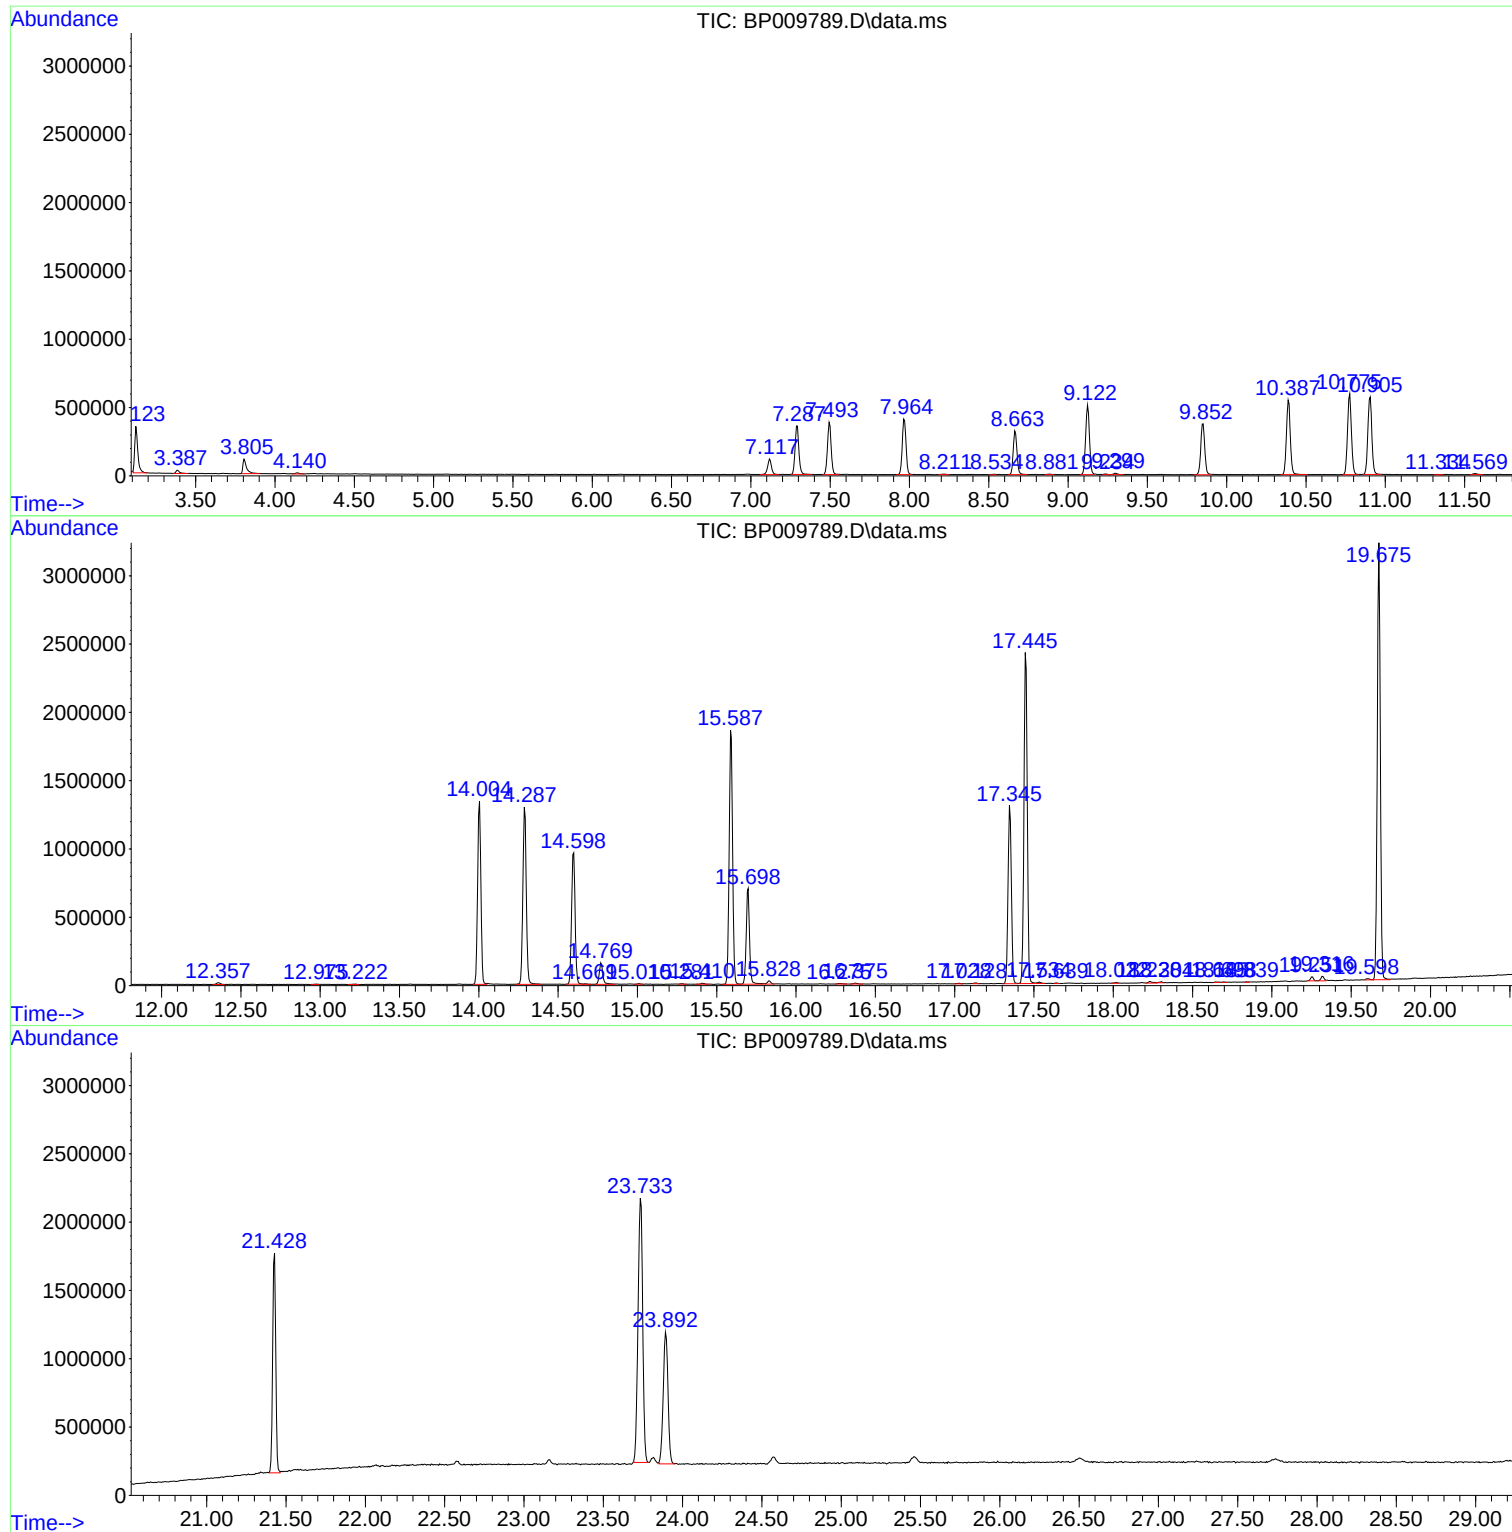

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009789.D
Acq On : 12 Apr 2022 18:42
Operator : CG/JU
Sample : N2316-17
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
ETNR5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.123	13.28 ng/ul	443737	1,4-Dichlorobenzene-d4	7.969

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	72
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
4			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	27
5			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	25

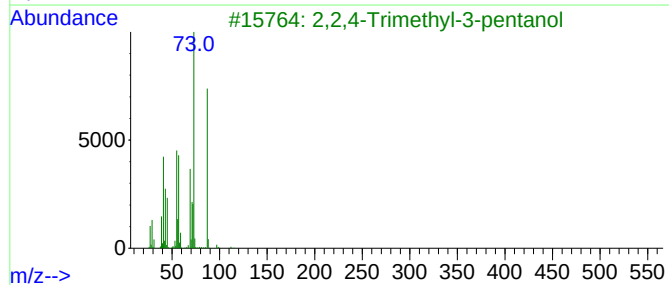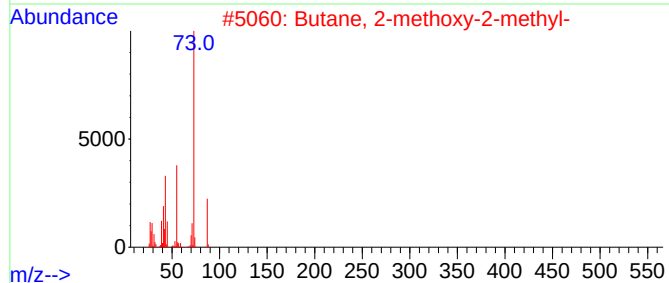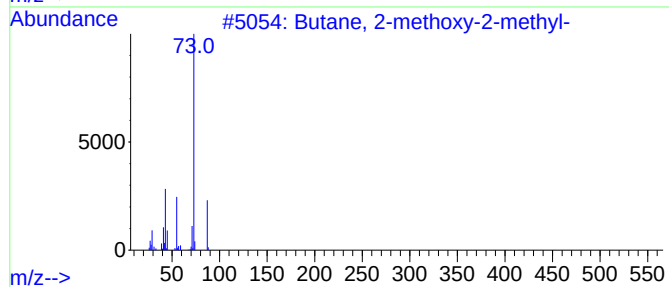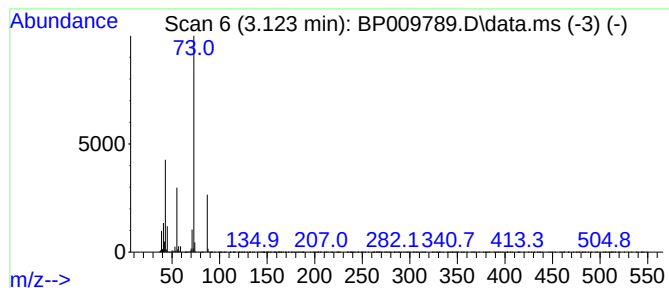

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009789.D
Acq On : 12 Apr 2022 18:42
Operator : CG/JU
Sample : N2316-17
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
ETNR5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.123	13.3	ng/ul	443737	1	7.969	668195	20.0