

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
 Data File : BP009795.D
 Acq On : 12 Apr 2022 22:40
 Operator : CG/JU
 Sample : PB144055BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK055

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009795.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	4	6	13	rVB2	11274	14105	0.32%	0.032%
2	3.387	47	51	63	rVB	37961	60384	1.36%	0.135%
3	3.799	118	121	141	rBV	475686	786795	17.72%	1.763%
4	4.140	175	179	187	rVB2	13284	21744	0.49%	0.049%
5	7.116	678	685	695	rBV	617439	978379	22.03%	2.192%
6	7.287	705	714	723	rBV	474924	772607	17.40%	1.731%
7	7.493	742	749	762	rBV	632586	1001858	22.56%	2.245%
8	7.963	821	829	838	rBV	506714	832128	18.74%	1.865%
9	8.663	941	948	961	rBV	785411	1296043	29.19%	2.904%
10	9.122	1017	1026	1036	rBV	656072	1084912	24.43%	2.431%
11	9.846	1141	1149	1164	rVB	523214	882418	19.87%	1.977%
12	10.387	1234	1241	1257	rBV	793762	1314286	29.60%	2.945%
13	10.775	1298	1307	1321	rBV	738605	1284381	28.93%	2.878%
14	10.899	1321	1328	1343	rVV	841280	1451193	32.68%	3.252%
15	12.357	1569	1576	1585	rBV3	17404	30167	0.68%	0.068%
16	13.875	1829	1834	1840	rVB9	2816	5312	0.12%	0.012%
17	14.004	1846	1856	1868	rBV	1684105	2353273	53.00%	5.274%
18	14.287	1895	1904	1921	rBV	1672590	2538623	57.17%	5.689%
19	14.598	1948	1957	1967	rBV	1252151	1908352	42.98%	4.277%
20	14.669	1967	1969	1974	rVB6	3673	5770	0.13%	0.013%
21	14.775	1979	1987	2001	rBV	878063	1279429	28.81%	2.867%
22	15.587	2118	2125	2136	rBV	2267717	3271867	73.69%	7.332%
23	15.692	2137	2143	2155	rBV	756299	1085321	24.44%	2.432%
24	15.828	2161	2166	2172	rVB2	24786	36056	0.81%	0.081%
25	16.375	2254	2259	2265	rVB5	8799	13156	0.30%	0.029%
26	17.022	2367	2369	2377	rVB9	4216	6759	0.15%	0.015%
27	17.128	2381	2387	2392	rBV3	8206	12977	0.29%	0.029%
28	17.345	2417	2424	2434	rBV	1659335	2378992	53.58%	5.331%
29	17.445	2434	2441	2451	rVV	2554742	3696251	83.24%	8.283%
30	17.592	2462	2466	2471	rBV6	3476	6189	0.14%	0.014%
31	17.716	2483	2487	2491	rBV5	3628	6621	0.15%	0.015%
32	19.251	2743	2748	2752	rBV2	34808	49628	1.12%	0.111%
33	19.316	2755	2759	2765	rVV2	37445	55624	1.25%	0.125%
34	19.675	2814	2820	2826	rBV	3296243	4440213	100.00%	9.950%
35	21.422	3112	3117	3124	rBV	2063804	2747997	61.89%	6.158%
36	23.733	3502	3510	3519	rBV	2178267	4306546	96.99%	9.651%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009795.D
Acq On : 12 Apr 2022 22:40
Operator : CG/JU
Sample : PB144055BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK055

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Title : SVOA CALIBRATION

37	23.892	3530	3537	3546	rVB2	1259542	2607559	58.73%	5.843%
----	--------	------	------	------	------	---------	---------	--------	--------




Sum of corrected areas: 44623915

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009795.D
Acq On : 12 Apr 2022 22:40
Operator : CG/JU
Sample : PB144055BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK055

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

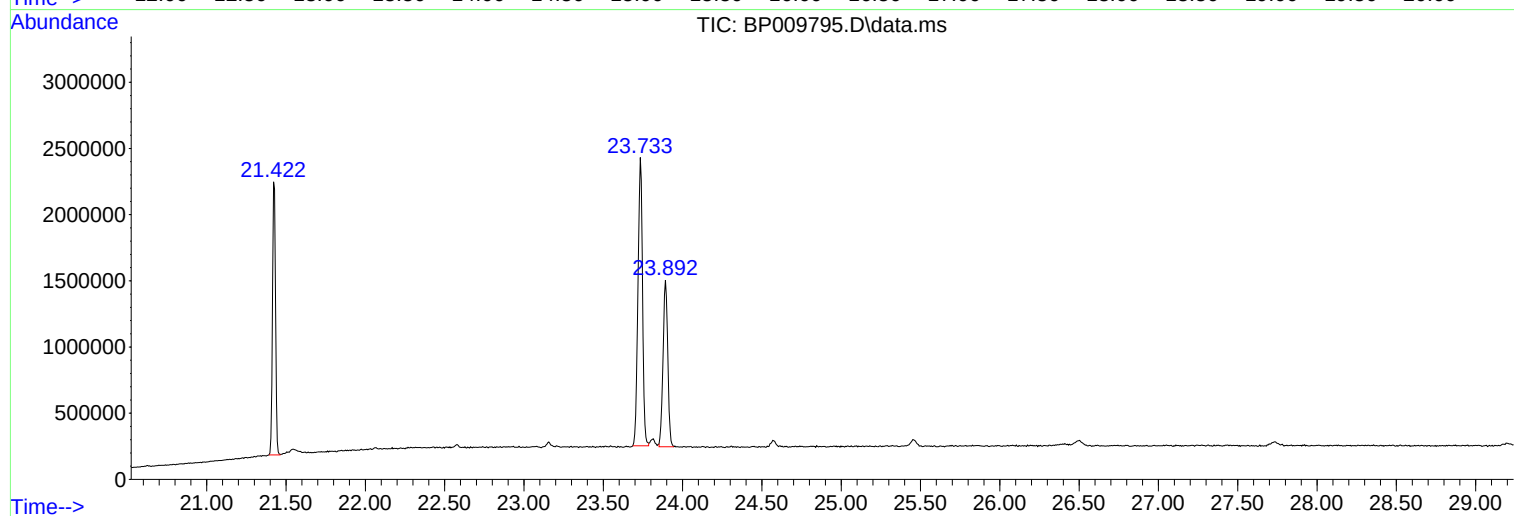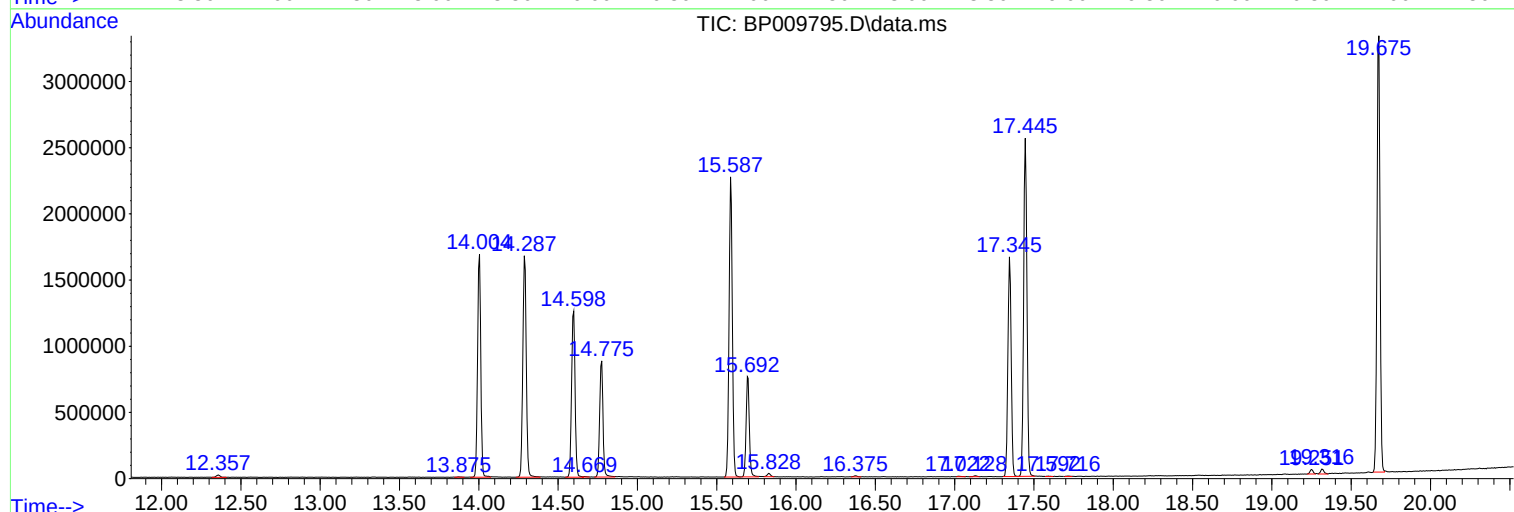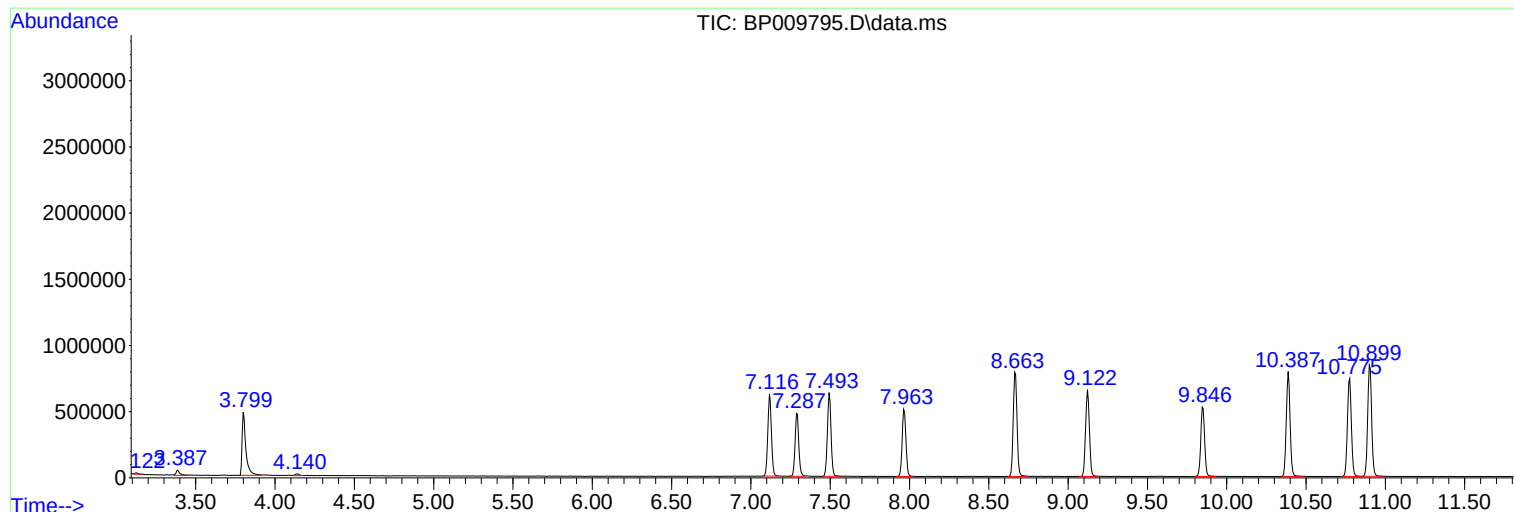

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009795.D
Acq On : 12 Apr 2022 22:40
Operator : CG/JU
Sample : PB144055BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK055

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009795.D
Acq On : 12 Apr 2022 22:40
Operator : CG/JU
Sample : PB144055BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK055

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc