

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
 Data File : BP009796.D
 Acq On : 12 Apr 2022 23:13
 Operator : CG/JU
 Sample : PB144076BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK076

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009796.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	3	7	12	rVB3	13128	18925	0.44%	0.046%
2	3.387	47	51	60	rVB	32110	48567	1.14%	0.119%
3	3.805	118	122	140	rBV	420015	744038	17.41%	1.827%
4	4.140	175	179	186	rVB2	11324	18882	0.44%	0.046%
5	4.581	252	254	259	rVB6	3421	4320	0.10%	0.011%
6	7.116	678	685	693	rBV	566726	912817	21.35%	2.242%
7	7.293	708	715	727	rVB	436681	708046	16.56%	1.739%
8	7.493	741	749	759	rBV	582011	921676	21.56%	2.263%
9	7.963	821	829	841	rBV	404019	665308	15.56%	1.634%
10	8.663	939	948	958	rBV	746941	1220571	28.55%	2.997%
11	9.122	1018	1026	1041	rBV	618337	1020939	23.88%	2.507%
12	9.846	1140	1149	1160	rBV	497218	835530	19.55%	2.052%
13	10.387	1233	1241	1258	rBV	757888	1253935	29.33%	3.079%
14	10.775	1299	1307	1319	rVB	603978	1039905	24.33%	2.554%
15	10.899	1319	1328	1342	rBV	784360	1385887	32.42%	3.403%
16	12.357	1569	1576	1582	rBV2	15942	25770	0.60%	0.063%
17	14.004	1846	1856	1872	rBV	1666399	2247921	52.59%	5.520%
18	14.287	1896	1904	1920	rBV	1616638	2398511	56.11%	5.890%
19	14.598	1950	1957	1965	rBV	1025178	1564611	36.60%	3.842%
20	14.775	1979	1987	2003	rBV	835493	1245352	29.13%	3.058%
21	15.587	2117	2125	2137	rBV	2216273	3160353	73.93%	7.761%
22	15.692	2137	2143	2156	rBV	716196	1029648	24.09%	2.528%
23	15.828	2161	2166	2172	rVB2	25101	40618	0.95%	0.100%
24	16.145	2217	2220	2227	rVB8	2493	6020	0.14%	0.015%
25	16.375	2254	2259	2266	rBV5	8393	14614	0.34%	0.036%
26	17.028	2365	2370	2373	rBV5	4297	6892	0.16%	0.017%
27	17.134	2380	2388	2393	rVB3	6568	12406	0.29%	0.030%
28	17.345	2417	2424	2433	rBV	1385902	2002802	46.85%	4.918%
29	17.445	2433	2441	2453	rBV	2470784	3563802	83.37%	8.751%
30	17.716	2484	2487	2492	rVB6	2980	5049	0.12%	0.012%
31	19.251	2744	2748	2754	rVB3	35267	46286	1.08%	0.114%
32	19.316	2754	2759	2765	rBV	36042	54204	1.27%	0.133%
33	19.675	2813	2820	2831	rBV	3261436	4274687	100.00%	10.497%
34	21.422	3112	3117	3125	rBV	1742349	2284504	53.44%	5.610%
35	23.733	3502	3510	3518	rBV2	1918889	3841103	89.86%	9.432%
36	23.892	3529	3537	3549	rVB	993015	2098264	49.09%	5.153%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009796.D
Acq On : 12 Apr 2022 23:13
Operator : CG/JU
Sample : PB144076BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK076

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Title : SVOA CALIBRATION




Sum of corrected areas: 40722763

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009796.D
Acq On : 12 Apr 2022 23:13
Operator : CG/JU
Sample : PB144076BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK076

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

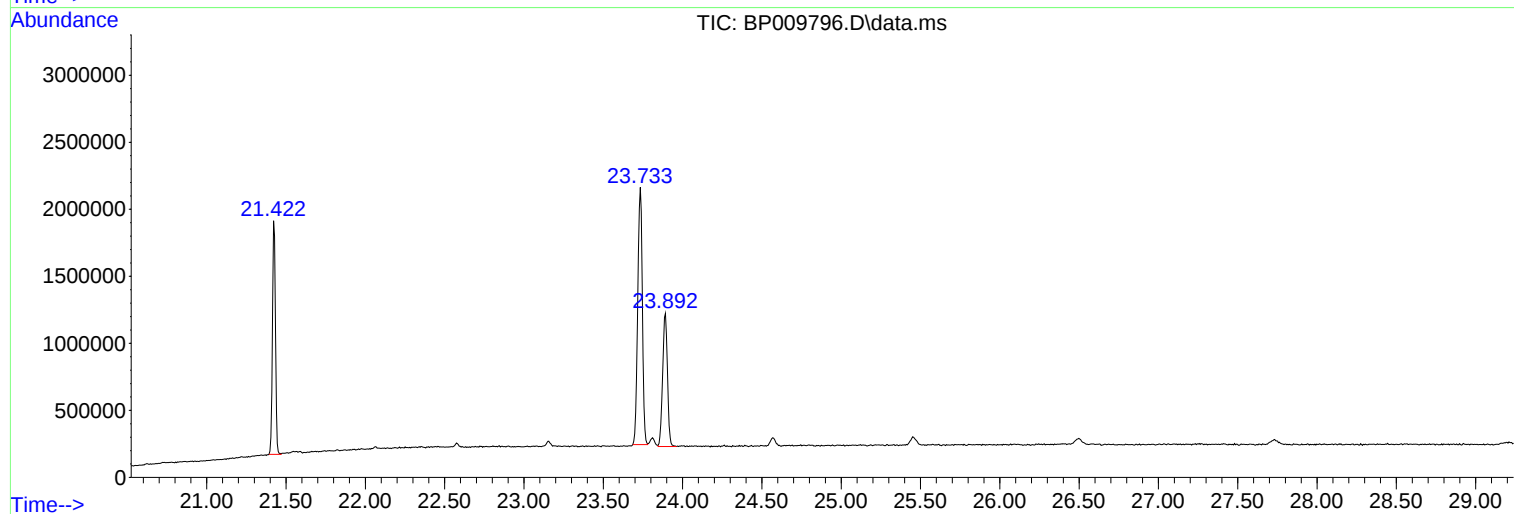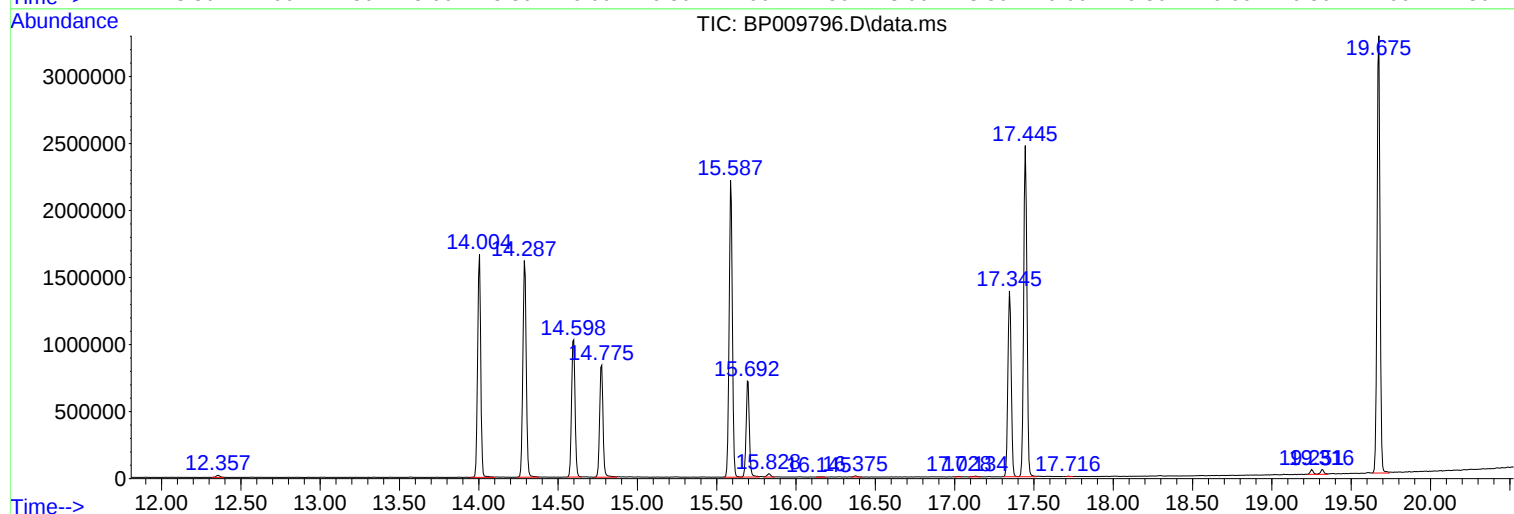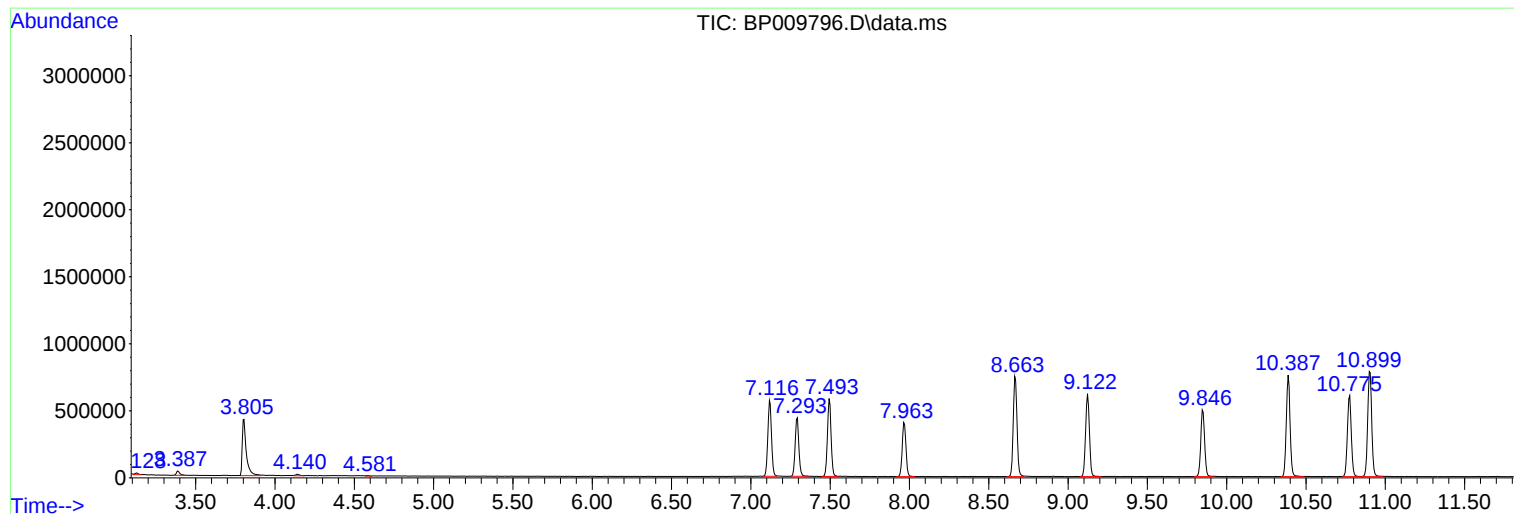

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009796.D
Acq On : 12 Apr 2022 23:13
Operator : CG/JU
Sample : PB144076BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK076

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009796.D
Acq On : 12 Apr 2022 23:13
Operator : CG/JU
Sample : PB144076BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK076

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc