

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
 Data File : BP009801.D
 Acq On : 13 Apr 2022 02:02
 Operator : CG/JU
 Sample : N2342-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COHZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009801.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.123	3	6	21	rVB	410385	583470	12.01%	1.370%
2	3.381	47	50	60	rVB	26153	38318	0.79%	0.090%
3	3.675	97	100	110	rVB10	5616	12941	0.27%	0.030%
4	3.805	118	122	137	rBV	155425	263116	5.42%	0.618%
5	4.140	175	179	183	rBV4	6961	9313	0.19%	0.022%
6	5.069	333	337	343	rBV2	8318	12212	0.25%	0.029%
7	5.269	367	371	376	rVB2	8973	13873	0.29%	0.033%
8	7.116	677	685	692	rBV	156899	252586	5.20%	0.593%
9	7.287	707	714	724	rBV	452217	719223	14.81%	1.689%
10	7.363	724	727	733	rVB2	5533	8858	0.18%	0.021%
11	7.493	741	749	758	rBV	495439	784483	16.15%	1.843%
12	7.599	762	767	773	rVB8	4031	6896	0.14%	0.016%
13	7.963	822	829	838	rBV	456175	746855	15.37%	1.754%
14	8.034	838	841	848	rVB	9434	15379	0.32%	0.036%
15	8.663	941	948	957	rBV	450509	713124	14.68%	1.675%
16	9.122	1019	1026	1040	rBV	618528	1031105	21.23%	2.422%
17	9.587	1097	1105	1111	rVB3	12322	21534	0.44%	0.051%
18	9.846	1140	1149	1166	rBV	509711	826550	17.01%	1.941%
19	10.387	1233	1241	1252	rBV	729156	1226700	25.25%	2.881%
20	10.769	1296	1306	1315	rBV	650179	1133125	23.33%	2.662%
21	10.899	1320	1328	1342	rBV	738198	1247220	25.67%	2.930%
22	12.087	1524	1530	1534	rVB8	3156	4977	0.10%	0.012%
23	12.210	1545	1551	1558	rVB4	7352	12699	0.26%	0.030%
24	12.293	1560	1565	1570	rVV	35328	56058	1.15%	0.132%
25	12.357	1570	1576	1581	rVB3	14922	26120	0.54%	0.061%
26	13.222	1719	1723	1728	rVB4	6497	10588	0.22%	0.025%
27	13.440	1755	1760	1766	rBV2	13355	18877	0.39%	0.044%
28	13.998	1849	1855	1863	rBV	1619295	2286827	47.07%	5.371%
29	14.287	1897	1904	1921	rVB	1701173	2464865	50.74%	5.790%
30	14.593	1950	1956	1967	rBV	1146234	1708060	35.16%	4.012%
31	14.769	1979	1986	1996	rBV	191873	290297	5.98%	0.682%
32	15.010	2023	2027	2031	rVB7	4057	6112	0.13%	0.014%
33	15.134	2044	2048	2056	rBV9	3231	5825	0.12%	0.014%
34	15.240	2062	2066	2075	rVB9	3439	9896	0.20%	0.023%
35	15.410	2090	2095	2101	rBV6	5000	9877	0.20%	0.023%
36	15.587	2118	2125	2136	rBV	2354728	3338887	68.73%	7.843%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
 Data File : BP009801.D
 Acq On : 13 Apr 2022 02:02
 Operator : CG/JU
 Sample : N2342-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0HZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
 Title : SVOA CALIBRATION

37	15.692	2136	2143	2155	rBV	843463	1153890	23.75%	2.710%
38	15.828	2161	2166	2172	rVB2	25263	38577	0.79%	0.091%
39	16.375	2255	2259	2265	rVB5	9102	12385	0.25%	0.029%
40	17.022	2364	2369	2374	rBV9	5906	9313	0.19%	0.022%
41	17.128	2380	2387	2392	rBV4	6910	13494	0.28%	0.032%
42	17.345	2416	2424	2434	rBV	1539627	2201881	45.33%	5.172%
43	17.445	2434	2441	2451	rVV	2786780	4001867	82.38%	9.400%
44	17.528	2451	2455	2462	rVB10	14616	25726	0.53%	0.060%
45	18.228	2569	2574	2579	rBV	60030	81247	1.67%	0.191%
46	18.528	2622	2625	2627	rBV4	5362	6548	0.13%	0.015%
47	19.251	2743	2748	2753	rBV2	39752	58079	1.20%	0.136%
48	19.316	2755	2759	2763	rVV	42482	52501	1.08%	0.123%
49	19.457	2780	2783	2787	rBV5	11766	16134	0.33%	0.038%
50	19.669	2813	2819	2830	rBV	3561380	4857963	100.00%	11.411%
51	21.127	3064	3067	3075	rBV	182935	239342	4.93%	0.562%
52	21.422	3112	3117	3125	rBV	2006817	2549471	52.48%	5.988%
53	23.733	3502	3510	3518	rBV2	2364840	4786898	98.54%	11.244%
54	23.892	3529	3537	3548	rVB2	1193862	2551771	52.53%	5.994%




Sum of corrected areas: 42573933

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009801.D
Acq On : 13 Apr 2022 02:02
Operator : CG/JU
Sample : N2342-10
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HZ3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

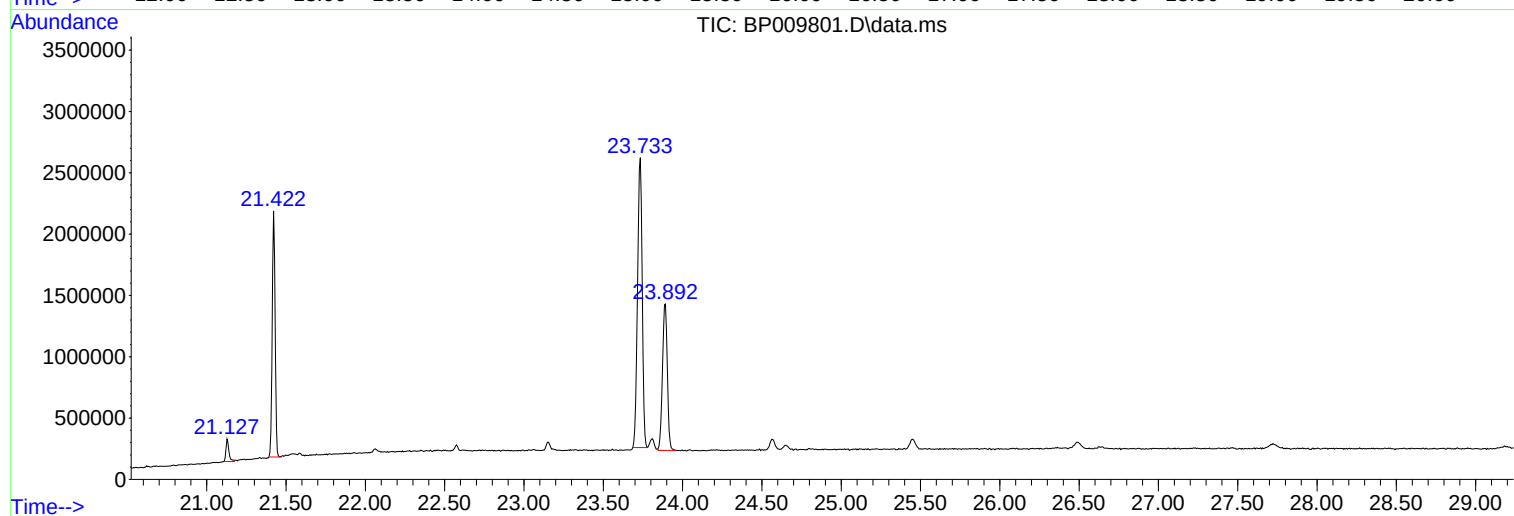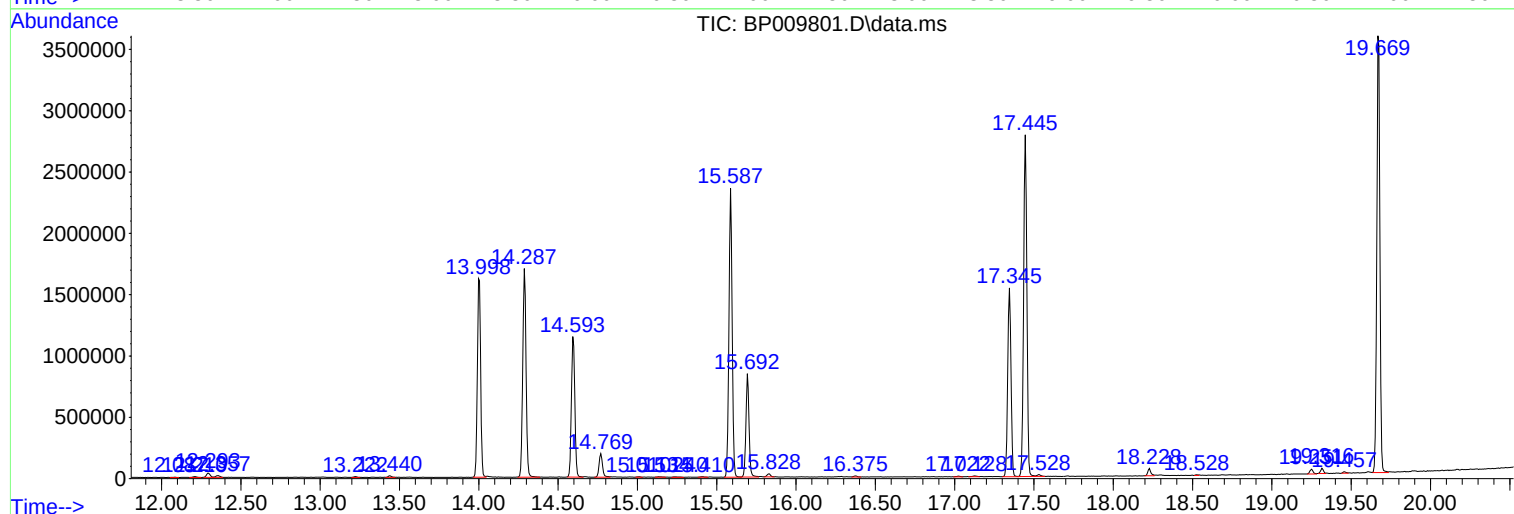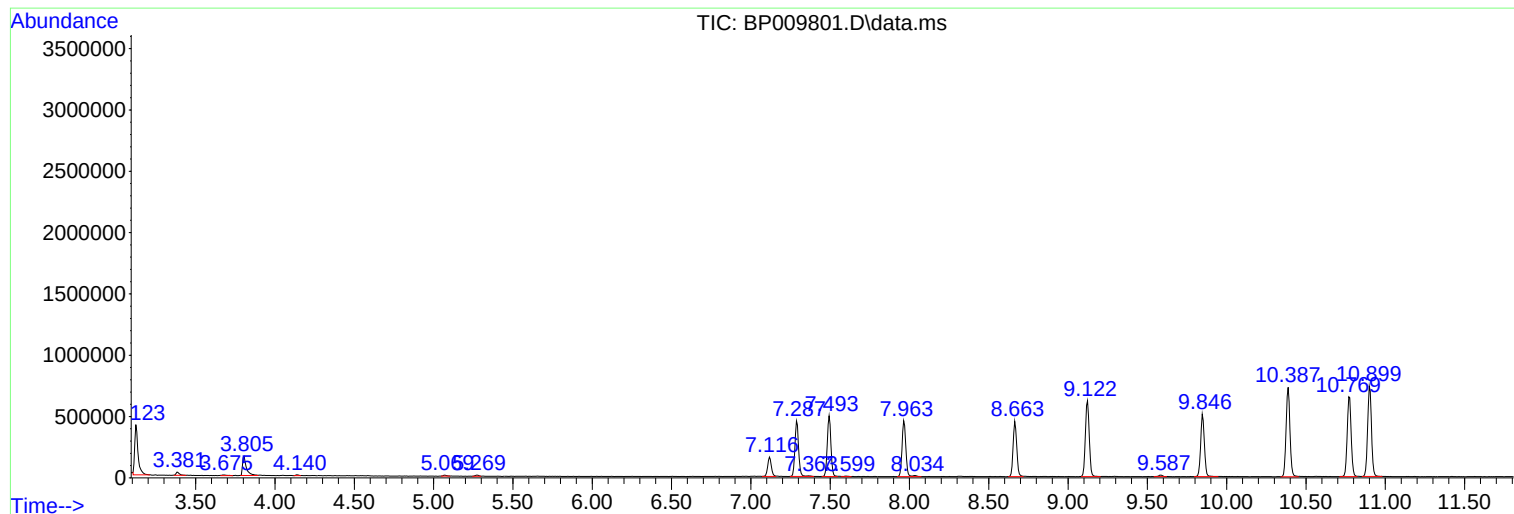

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009801.D
Acq On : 13 Apr 2022 02:02
Operator : CG/JU
Sample : N2342-10
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HZ3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.123	15.62 ng/ul	583470	1,4-Dichlorobenzene-d4	7.963

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
4			1,3-Dioxolane, 2-propyl-	116	C6H12O2	003390-13-4	23
5			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	23

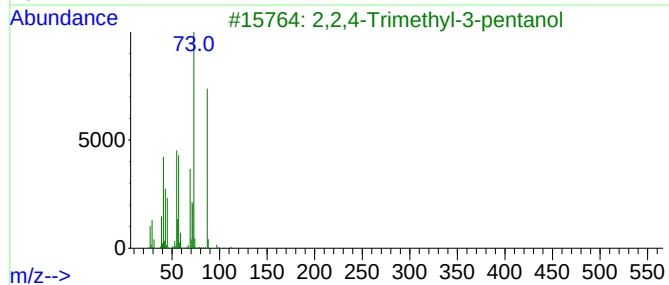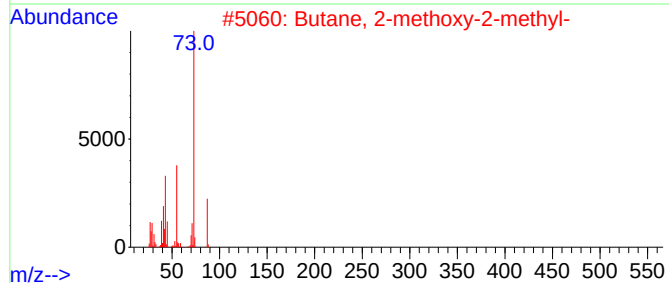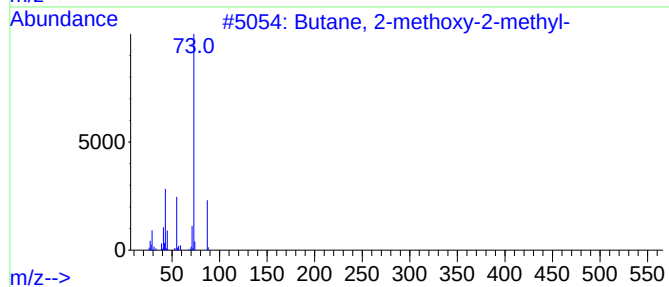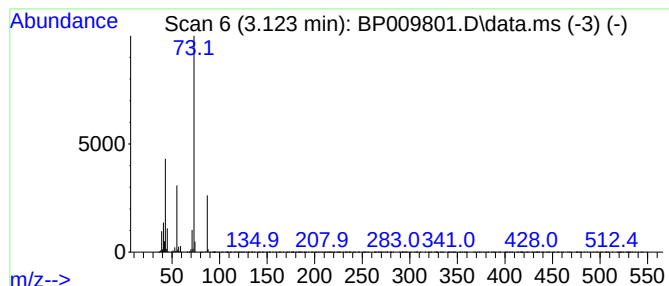

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041122\
Data File : BP009801.D
Acq On : 13 Apr 2022 02:02
Operator : CG/JU
Sample : N2342-10
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0HZ3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP040722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.123	15.6	ng/ul	583470	1	7.963	746855	20.0