
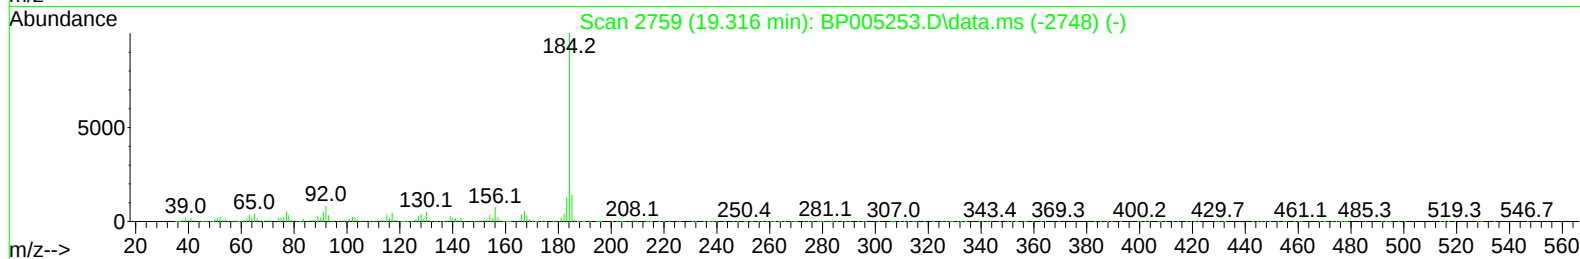
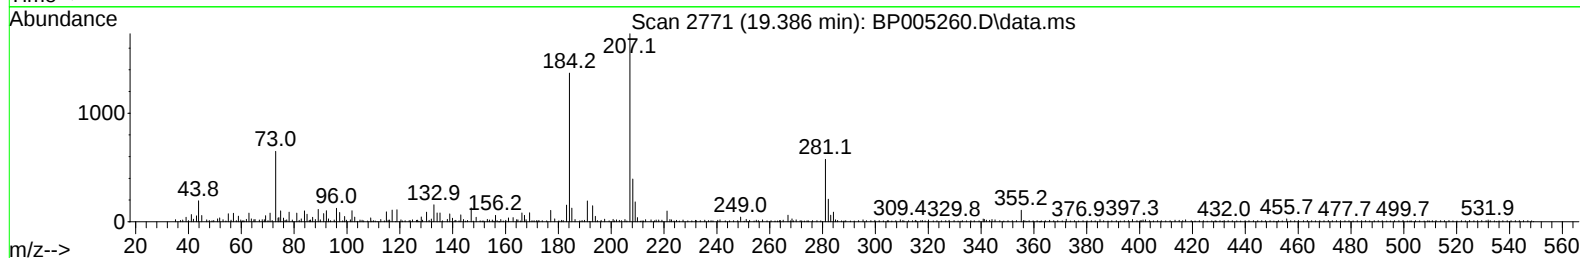


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041221\
Data File : BP005260.D
Acq On : 12 Apr 2021 09:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 10:52:30 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP040921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 18:44:11 2021
Response via : Initial Calibration

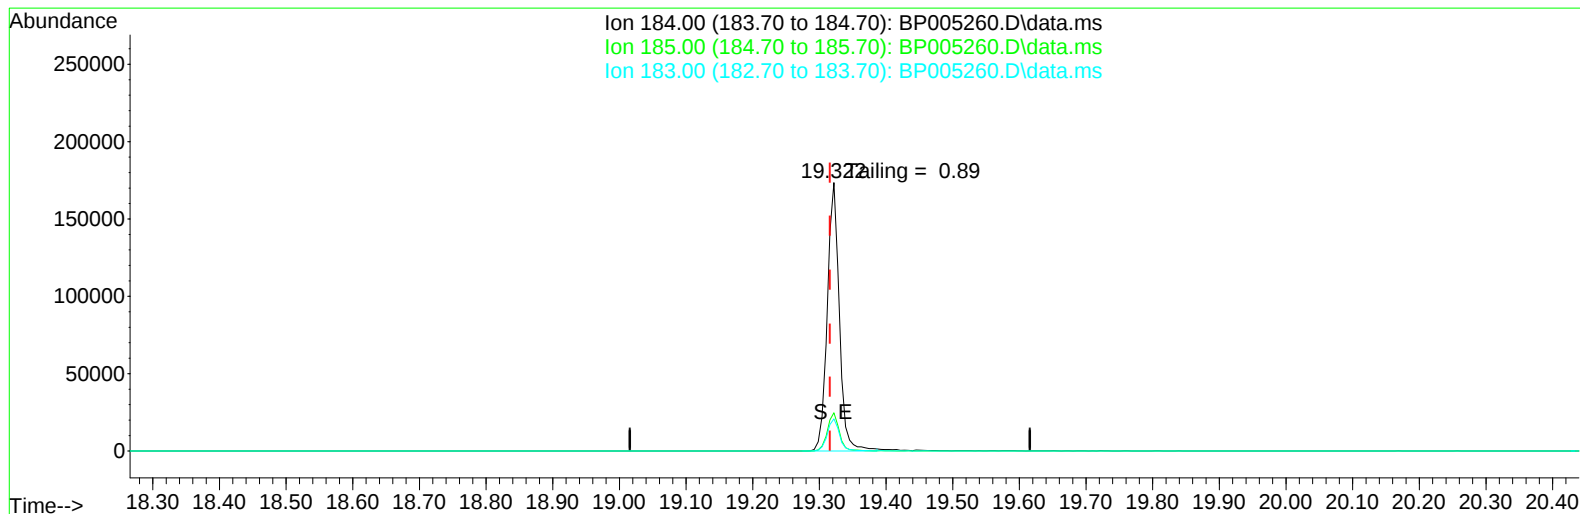




TIC: BP005260.D\data.ms

(77) Benzidine**19.322min (+ 0.006) 1206063.11 ng****response 220726**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.26
183.00	12.00	12.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041221\
Data File : BP005260.D
Acq On : 12 Apr 2021 09:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 10:52:30 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP040921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 18:44:11 2021
Response via : Initial Calibration

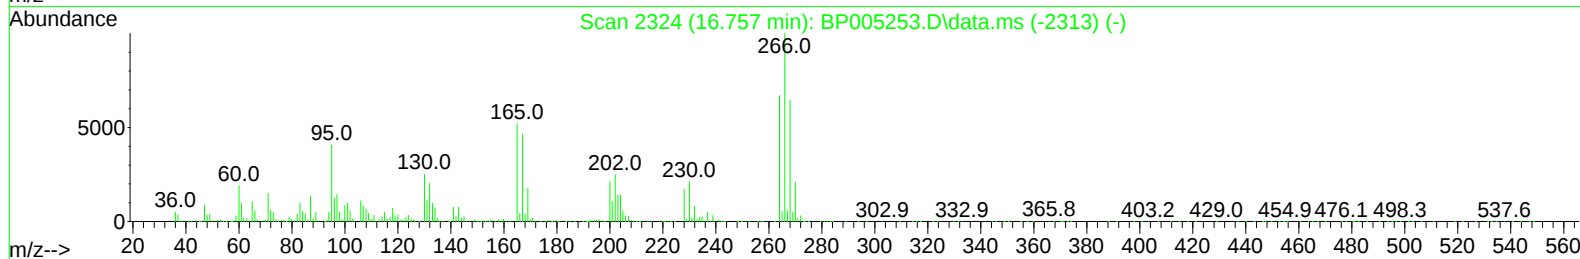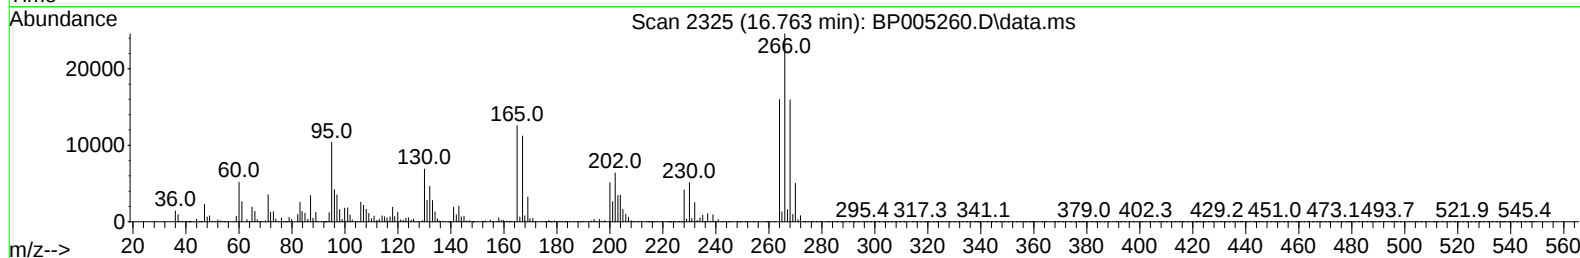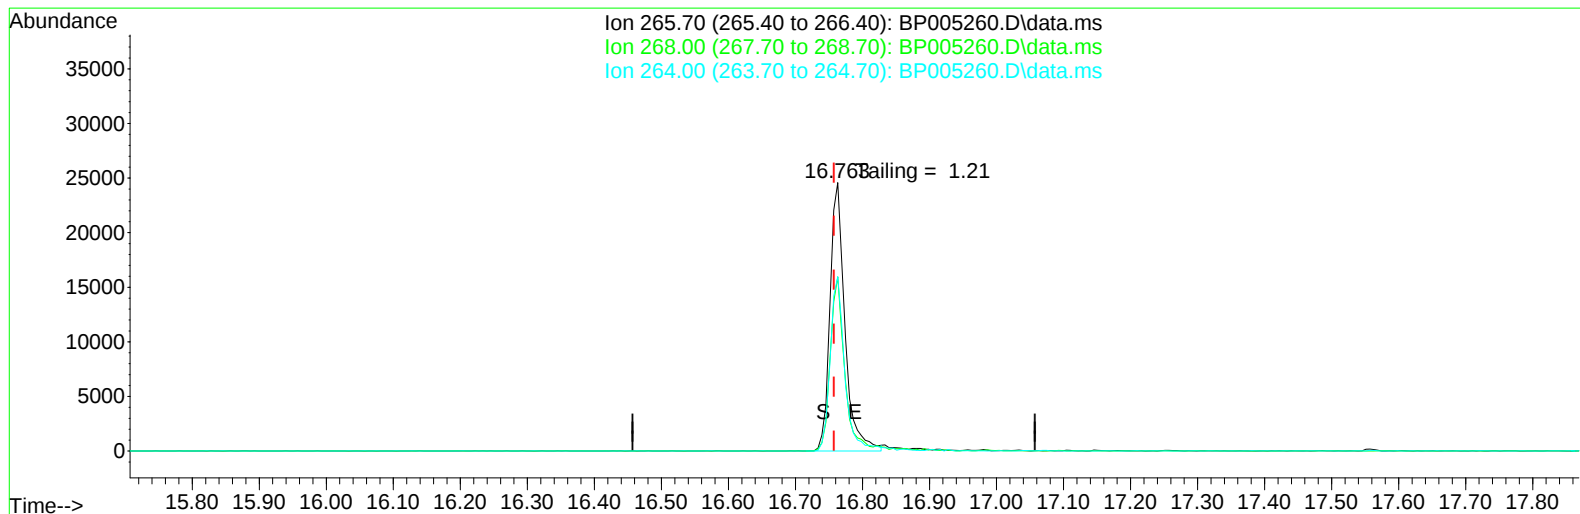

TIC: BP005260.D\data.ms

(70) Pentachlorophenol (C)

16.763min (+ 0.006) 329469.56 ng

response 38845

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	64.85
264.00	63.30	64.95
0.00	0.00	0.00