

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041221\
 Data File : BP005271.D
 Acq On : 12 Apr 2021 17:59
 Operator : CG/JU
 Sample : M1967-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SB2-A

Manual Integrations
 APPROVED

mohammad
 4/14/2021 11:49:26 AM

Quant Time: Apr 12 18:38:27 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP040921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 09 18:44:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.675	152	31634	20.00	ng	# 0.00
21) Naphthalene-d8	10.469	136	109706	20.00	ng	# 0.00
39) Acenaphthene-d10	14.340	164	65797	20.00	ng	0.00
64) Phenanthrene-d10	17.098	188	156615	20.00	ng	# 0.00
76) Chrysene-d12	21.204	240	178309	20.00	ng	0.00
86) Perylene-d12	23.474	264	179137	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.275	112	207716	68.91	ng	0.00
7) Phenol-d6	6.864	99	338311	98.37	ng	0.00
23) Nitrobenzene-d5	8.840	82	244993	70.42	ng	0.00
42) 2,4,6-Tribromophenol	15.839	330	16847	20.28	ng	0.00
45) 2-Fluorobiphenyl	12.951	172	346298	71.05	ng	0.00
79) Terphenyl-d14	19.680	244	613005	67.54	ng	0.00
Target Compounds						
						Qvalue
10) Phenol	6.893	94	8363	2.37	ng	75
50) Dimethylphthalate	13.798	163	11105	2.30	ng	97
71) Phenanthrene	17.145	178	20620	2.33	ng	97
75) Fluoranthene	19.128	202	56528	5.21	ng	99
78) Pyrene	19.480	202	64772	5.84	ng	97
81) Benzo(a)anthracene	21.186	228	46116	3.92	ng	94
83) Chrysene	21.239	228	46454	4.06	ng	97
84) Bis(2-ethylhexyl)phtha...	21.116	149	18016	2.77	ng	95
88) Benzo(b)fluoranthene	22.786	252	57982m	4.94	ng	
89) Benzo(k)fluoranthene	22.827	252	22586m	2.01	ng	
90) Benzo(a)pyrene	23.374	252	51881	4.78	ng	95
92) Benzo(g,h,i)perylene	26.510	276	29505	2.56	ng	# 87

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041221\
Data File : BP005271.D
Acq On : 12 Apr 2021 17:59
Operator : CG/JU
Sample : M1967-06
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampled :
SB2-A

Manual Integrations
APPROVED

mohammad
4/14/2021 11:49:26 AM

Quant Time: Apr 12 18:38:27 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP040921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 18:44:11 2021
Response via : Initial Calibration

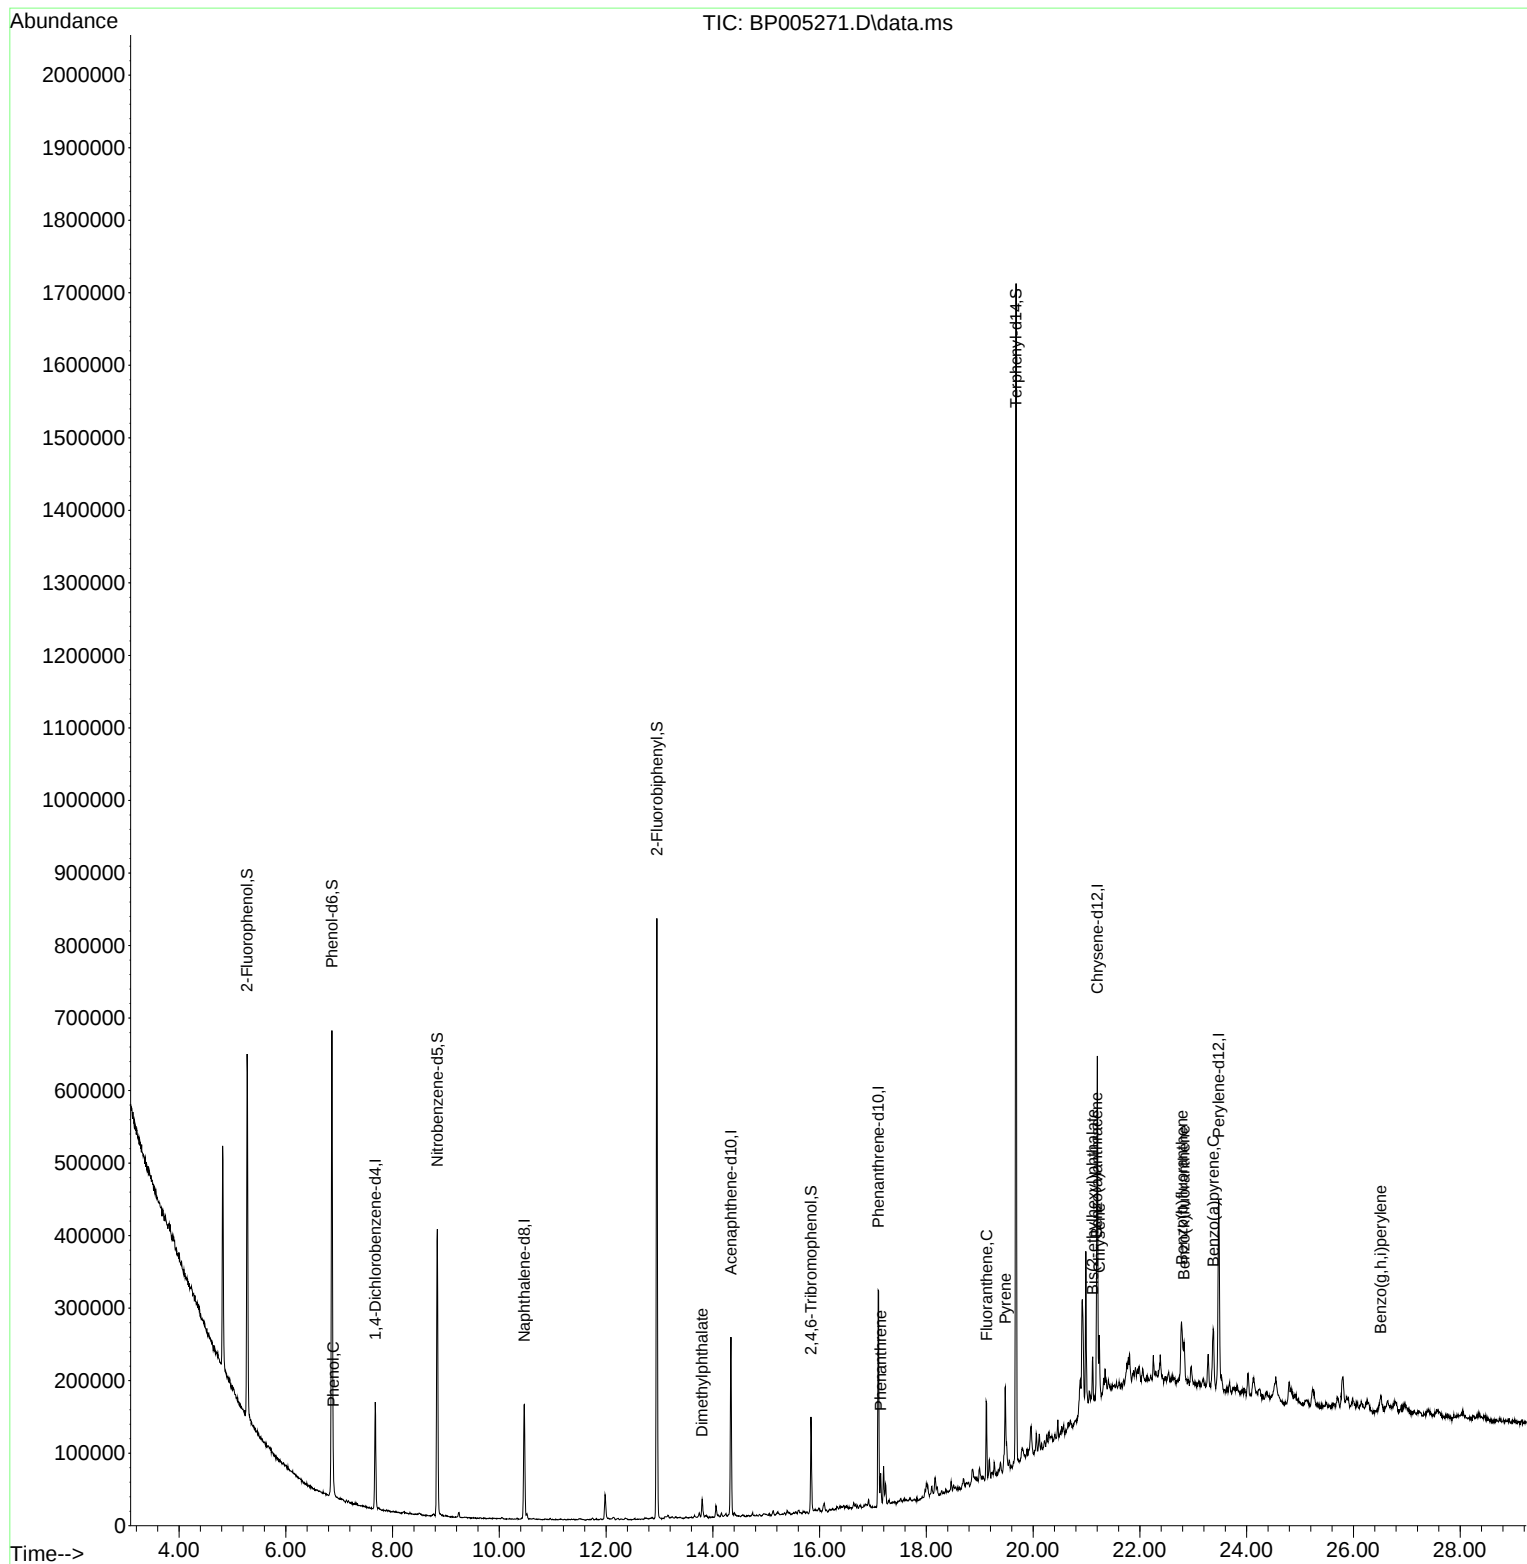







#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.675 min Scan# 780
Delta R.T. -0.006 min
Lab File: BP005271.D
Acq: 12 Apr 2021 17:59

Tgt Ion:152 Resp: 31634
Ion Ratio Lower Upper
152 100
150 163.3 123.8 185.6
115 78.0 43.8 65.6#

Instrument :
BNA_P
ClientSampled :
SB2-A




Manual Integrations
APPROVED


mohammad
4/14/2021 11:49:26 AM



#5
2-Fluorophenol
Concen: 68.91 ng
RT: 5.275 min Scan# 372
Delta R.T. -0.000 min
Lab File: BP005271.D
Acq: 12 Apr 2021 17:59


Tgt Ion:112 Resp: 207716
Ion Ratio Lower Upper
112 100
64 59.5 32.8 49.2#
63 32.3 17.0 25.4#

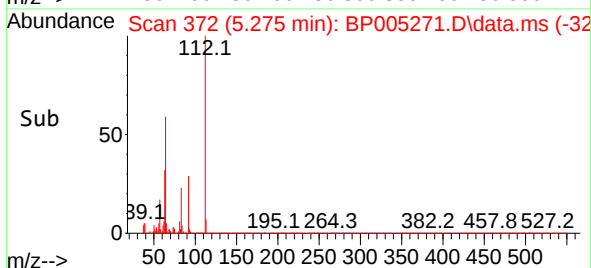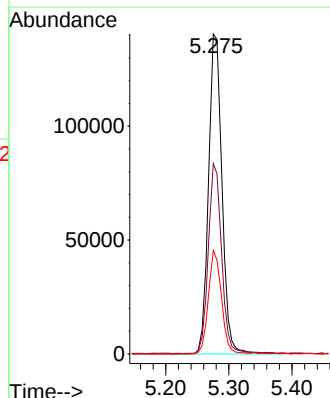

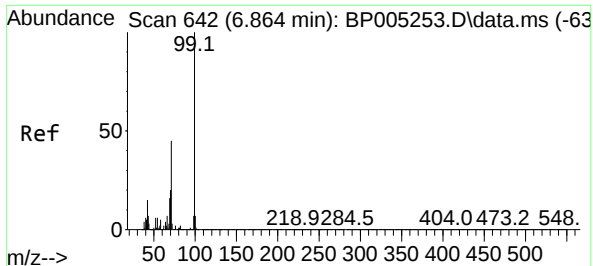

#7
Phenol-d6
Concen: 98.37 ng
RT: 6.864 min Scan# 642
Delta R.T. -0.000 min
Lab File: BP005271.D
Acq: 12 Apr 2021 17:59




Instrument :
BNA_P
ClientSampleId :
SB2-A

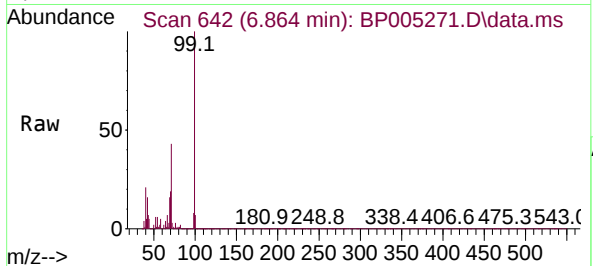


Tgt Ion: 99 Resp: 338311
Ion Ratio Lower Upper
99 100
42 15.6 8.6 13.0#
71 43.0 23.4 35.2#

Manual Integrations
APPROVED



mohammad
4/14/2021 11:49:26 AM

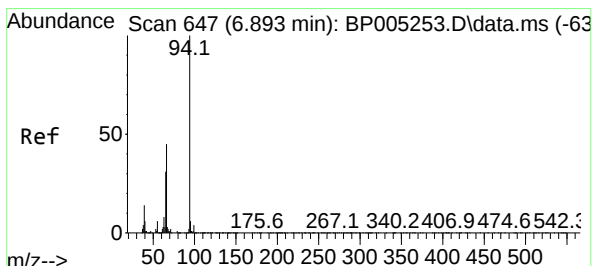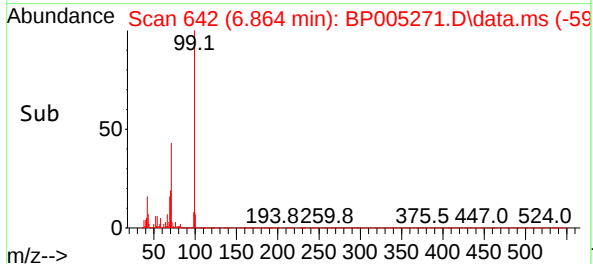


#10
Phenol
Concen: 2.37 ng
RT: 6.893 min Scan# 647
Delta R.T. -0.000 min
Lab File: BP005271.D
Acq: 12 Apr 2021 17:59

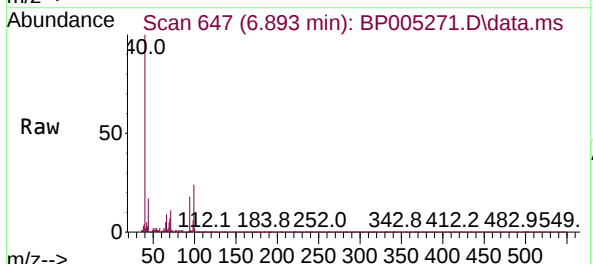


Tgt Ion: 94 Resp: 8363
Ion Ratio Lower Upper
94 100
65 28.7 2.3 42.3
66 48.9 10.9 50.9

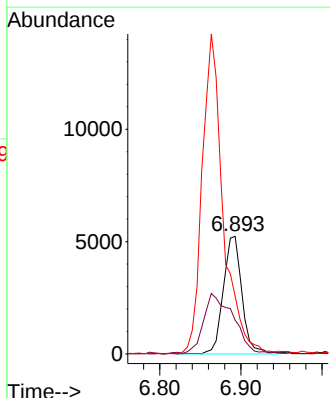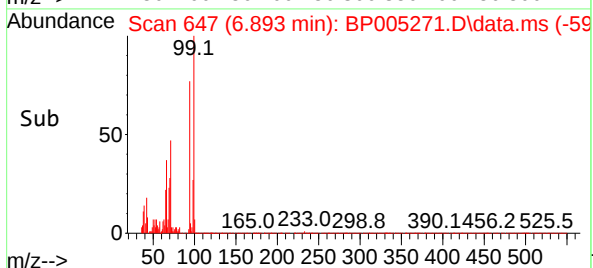



#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.469 min Scan# 1255
Delta R.T. -0.000 min
Lab File: BP005271.D
Acq: 12 Apr 2021 17:59




Instrument :
BNA_P
ClientSampled :
SB2-A



Tgt Ion	Ratio	Lower	Upper
136	100		
137	10.9	8.6	13.0
54	7.2	3.6	5.4#
68	7.6	3.3	4.9#




Manual Integrations
APPROVED


mohammad
4/14/2021 11:49:26 AM

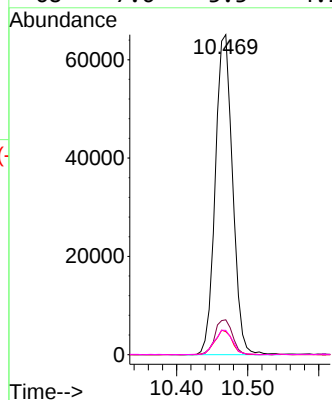

#23
Nitrobenzene-d5
Concen: 70.42 ng
RT: 8.840 min Scan# 978
Delta R.T. -0.000 min
Lab File: BP005271.D
Acq: 12 Apr 2021 17:59


Tgt Ion	Ratio	Lower	Upper
82	100		
128	29.6	45.6	68.4#
54	40.0	30.1	45.1

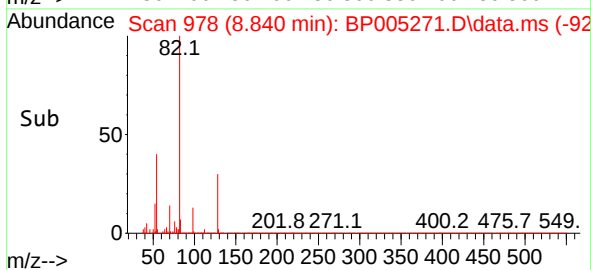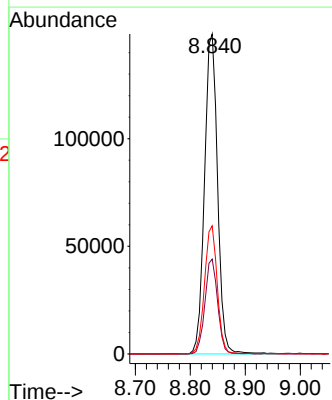

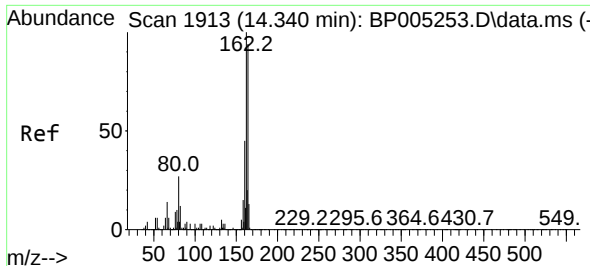

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.340 min Scan# 1913
Delta R.T. -0.000 min
Lab File: BP005271.D
Acq: 12 Apr 2021 17:59




Instrument :
BNA_P
ClientSampleId :
SB2-A

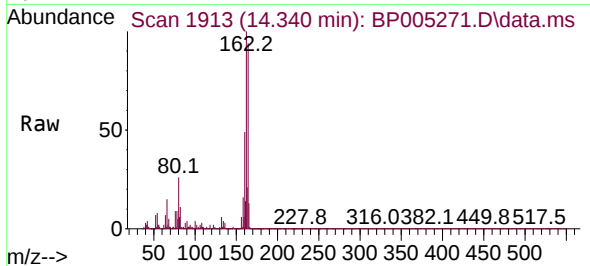


Tgt Ion:164 Resp: 65797
Ion Ratio Lower Upper
164 100
162 106.8 79.4 119.2
160 52.5 36.1 54.1

Manual Integrations
APPROVED



mohammad
4/14/2021 11:49:26 AM

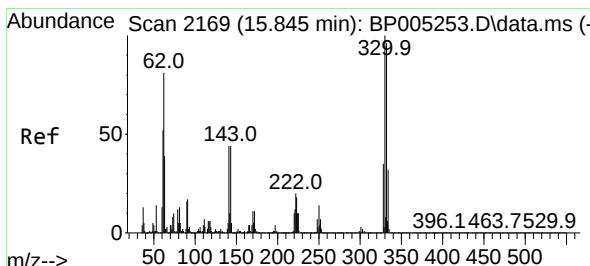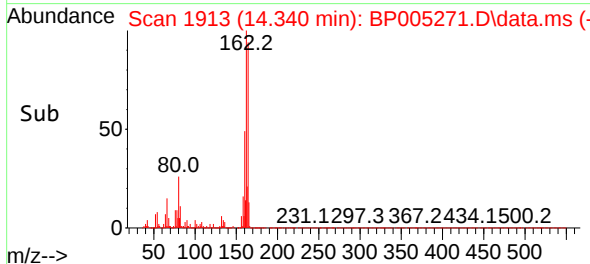


#42
2,4,6-Tribromophenol
Concen: 20.28 ng
RT: 15.839 min Scan# 2168
Delta R.T. -0.006 min
Lab File: BP005271.D
Acq: 12 Apr 2021 17:59

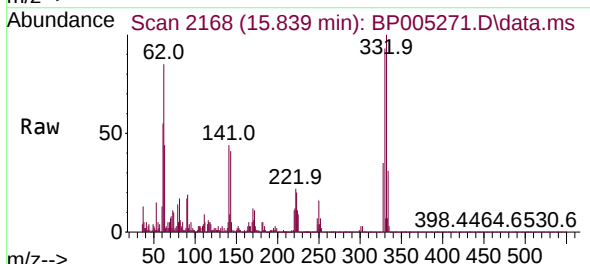


Tgt Ion:330 Resp: 16847
Ion Ratio Lower Upper
330 100
332 102.8 77.1 115.7
141 45.3 23.4 35.2#

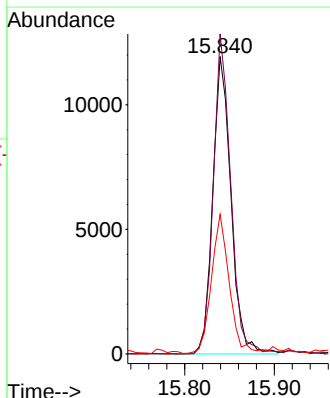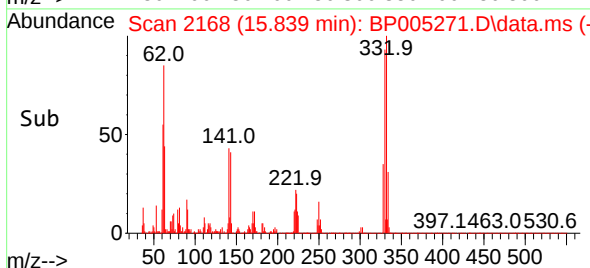



#45
2-Fluorobiphenyl
Concen: 71.05 ng
RT: 12.951 min Scan# 1677
Delta R.T. -0.000 min
Lab File: BP005271.D
Acq: 12 Apr 2021 17:59




Instrument :
BNA_P
ClientSampled :
SB2-A




Tgt Ion:172 Resp: 346298
Ion Ratio Lower Upper
172 100
171 36.1 28.5 42.7
170 23.2 19.2 28.8

Manual Integrations
APPROVED



mohammad
4/14/2021 11:49:26 AM

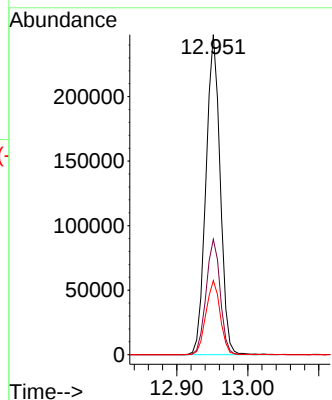


#50
Dimethylphthalate
Concen: 2.30 ng
RT: 13.798 min Scan# 1821
Delta R.T. -0.006 min
Lab File: BP005271.D
Acq: 12 Apr 2021 17:59



Tgt Ion:163 Resp: 11105
Ion Ratio Lower Upper
163 100
194 3.9 3.3 4.9
164 8.9 8.2 12.2

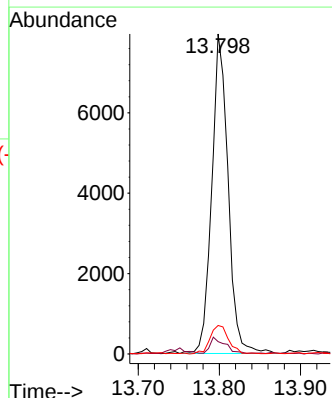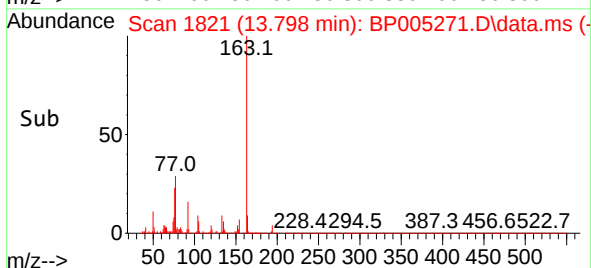







#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.098 min Scan# 2382
Delta R.T. -0.006 min
Lab File: BP005271.D
Acq: 12 Apr 2021 17:59

Tgt Ion	Ratio	Lower	Upper
188	100		
94	10.5	6.2	9.2#
80	13.1	6.2	9.2#

Instrument :
BNA_P
ClientSampled :
SB2-A




Manual Integrations
APPROVED


mohammad
4/14/2021 11:49:26 AM

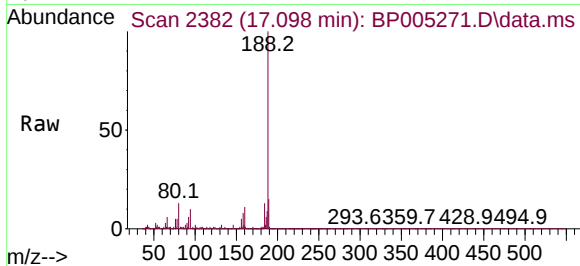

#71
Phenanthrene
Concen: 2.33 ng
RT: 17.145 min Scan# 2390
Delta R.T. -0.000 min
Lab File: BP005271.D
Acq: 12 Apr 2021 17:59

Tgt Ion	Ratio	Lower	Upper
178	100		
176	19.7	15.3	22.9
179	13.1	12.5	18.7

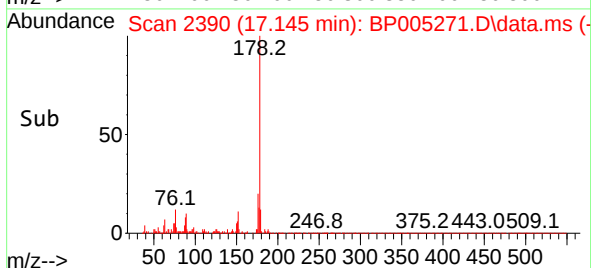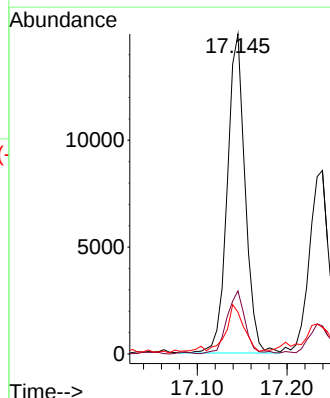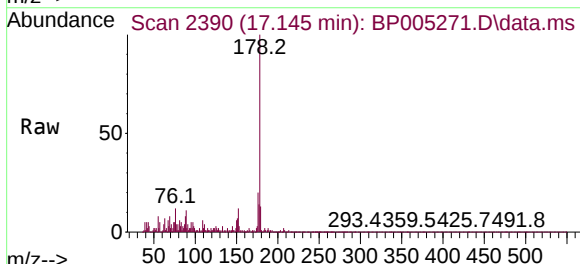







#75
Fluoranthene
Concen: 5.21 ng
RT: 19.128 min Scan# 2727
Delta R.T. -0.000 min
Lab File: BP005271.D
Acq: 12 Apr 2021 17:59

Instrument :
BNA_P
ClientSampleId :
SB2-A

Tgt Ion:	202	Resp:	56528
Ion Ratio	Lower	Upper	
202	100		
101	9.3	0.0	29.4
203	18.2	0.0	37.8




Manual Integrations
APPROVED


mohammad
4/14/2021 11:49:26 AM

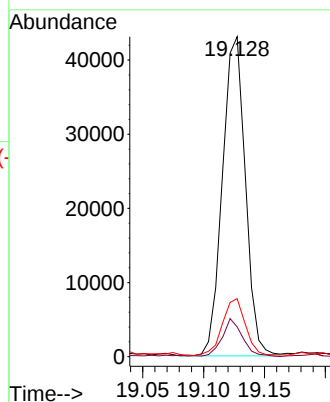

#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.204 min Scan# 3080
Delta R.T. -0.000 min
Lab File: BP005271.D
Acq: 12 Apr 2021 17:59

Tgt Ion:	240	Resp:	178309
Ion Ratio	Lower	Upper	
240	100		
120	8.8	7.8	11.6
236	25.8	20.8	31.2

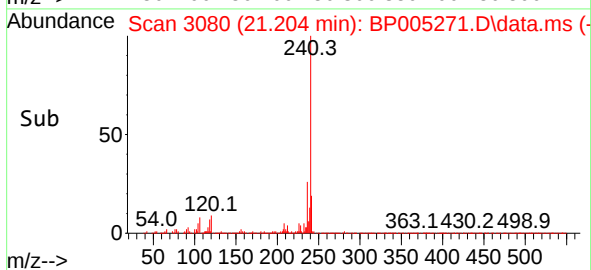







#78
Pyrene
Concen: 5.84 ng
RT: 19.480 min Scan# 2787
Delta R.T. -0.000 min
Lab File: BP005271.D
Acq: 12 Apr 2021 17:59

Instrument :
BNA_P
ClientSampleId :
SB2-A

Tgt Ion	Ratio	Lower	Upper
202	100		
200	19.4	17.1	25.7
203	18.0	14.2	21.2




Manual Integrations
APPROVED


mohammad
4/14/2021 11:49:26 AM



#79
Terphenyl-d14
Concen: 67.54 ng
RT: 19.680 min Scan# 2821
Delta R.T. -0.000 min
Lab File: BP005271.D
Acq: 12 Apr 2021 17:59

Tgt Ion	Ratio	Lower	Upper
244	100		
212	7.8	5.8	8.6
122	9.3	7.8	11.8

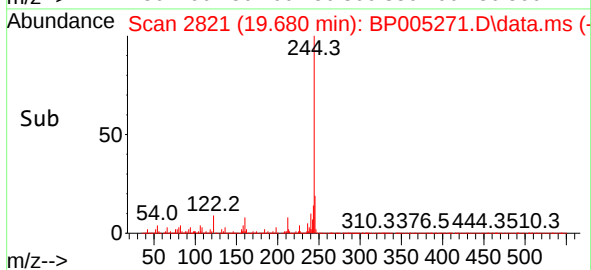







#81
Benzo(a)anthracene
Concen: 3.92 ng
RT: 21.186 min Scan# 3077
Delta R.T. -0.000 min
Lab File: BP005271.D
Acq: 12 Apr 2021 17:59

Instrument :
BNA_P
ClientSampleId :
SB2-A

Tgt Ion:	228	Resp:	46116
Ion Ratio	Lower	Upper	
228	100		
226	31.8	22.1	33.1
229	21.6	15.9	23.9




Manual Integrations
APPROVED


mohammad
4/14/2021 11:49:26 AM

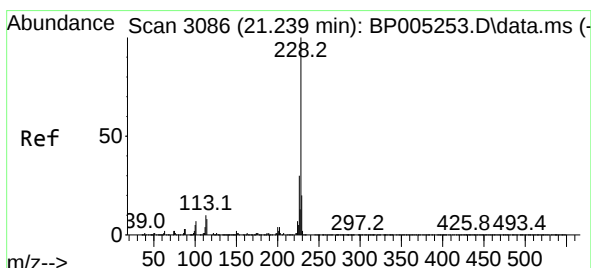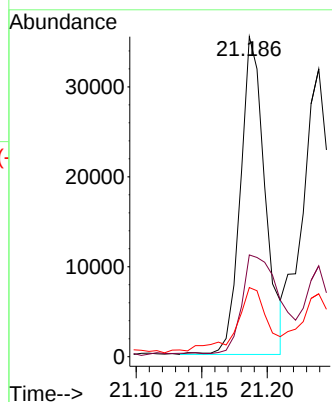

#83
Chrysene
Concen: 4.06 ng
RT: 21.239 min Scan# 3086
Delta R.T. -0.000 min
Lab File: BP005271.D
Acq: 12 Apr 2021 17:59


Tgt Ion:	228	Resp:	46454
Ion Ratio	Lower	Upper	
228	100		
226	31.6	24.4	36.6
229	21.8	15.8	23.6

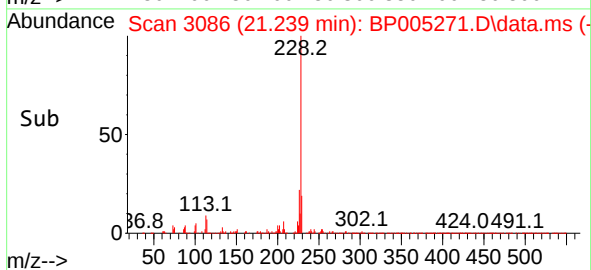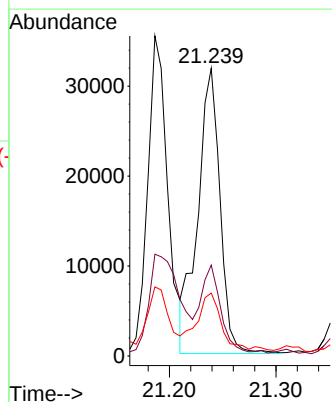



#84
Bis(2-ethylhexyl)phthalate
Concen: 2.77 ng
RT: 21.116 min Scan# 3065
Delta R.T. -0.000 min
Lab File: BP005271.D
Acq: 12 Apr 2021 17:59




Instrument :
BNA_P
ClientSampleId :
SB2-A




Tgt Ion:149 Resp: 18016
Ion Ratio Lower Upper
149 100
167 25.0 22.6 34.0
279 4.9 4.2 6.2

Manual Integrations
APPROVED



mohammad
4/14/2021 11:49:26 AM




#86
Perylene-d12
Concen: 20.00 ng
RT: 23.474 min Scan# 3466
Delta R.T. -0.000 min
Lab File: BP005271.D
Acq: 12 Apr 2021 17:59



Tgt Ion:264 Resp: 179137
Ion Ratio Lower Upper
264 100
260 22.3 18.8 28.2
265 21.5 17.4 26.2

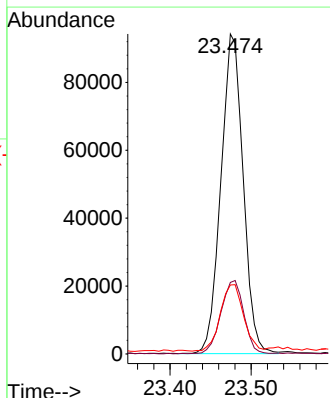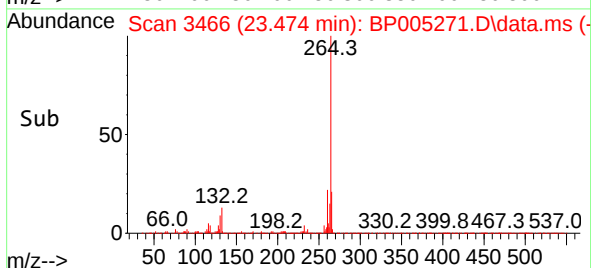







#88
Benzo(b)fluoranthene
Concen: 4.94 ng m
RT: 22.786 min Scan# 3349
Delta R.T. -0.000 min
Lab File: BP005271.D
Acq: 12 Apr 2021 17:59

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.8	17.6	26.4
125	11.3	7.3	10.9#

Instrument :
BNA_P
ClientSampled :
SB2-A




Manual Integrations
APPROVED


mohammad
4/14/2021 11:49:26 AM

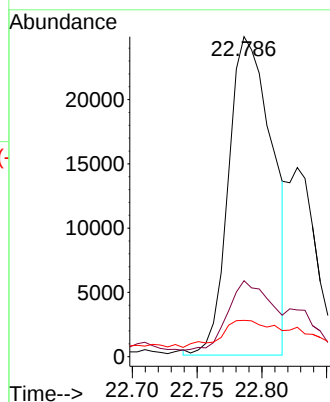

#89
Benzo(k)fluoranthene
Concen: 2.01 ng m
RT: 22.827 min Scan# 3356
Delta R.T. -0.006 min
Lab File: BP005271.D
Acq: 12 Apr 2021 17:59

Tgt Ion	Ratio	Lower	Upper
252	100		
253	24.7	17.8	26.8
125	15.5	7.4	11.2#

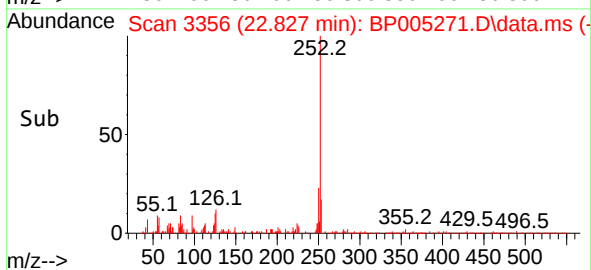







#90
Benzo(a)pyrene
Concen: 4.78 ng
RT: 23.374 min Scan# 3449
Delta R.T. -0.000 min
Lab File: BP005271.D
Acq: 12 Apr 2021 17:59

Tgt Ion:	252	Resp:	51881
Ion Ratio	Lower	Upper	
252	100		
253	24.8	17.4	26.0
125	11.1	8.2	12.4

Instrument :
BNA_P
ClientSampleId :
SB2-A

Manual Integrations
APPROVED

mohammad
4/14/2021 11:49:26 AM



#92
Benzo(g,h,i)perylene
Concen: 2.56 ng
RT: 26.510 min Scan# 3982
Delta R.T. -0.006 min
Lab File: BP005271.D
Acq: 12 Apr 2021 17:59

Tgt Ion:	276	Resp:	29505
Ion Ratio	Lower	Upper	
276	100		
277	26.3	19.0	28.6
138	10.6	16.6	24.8#

