


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041221\
 Data File : BP005260.D
 Acq On : 12 Apr 2021 09:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP040921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 09 18:44:11 2021

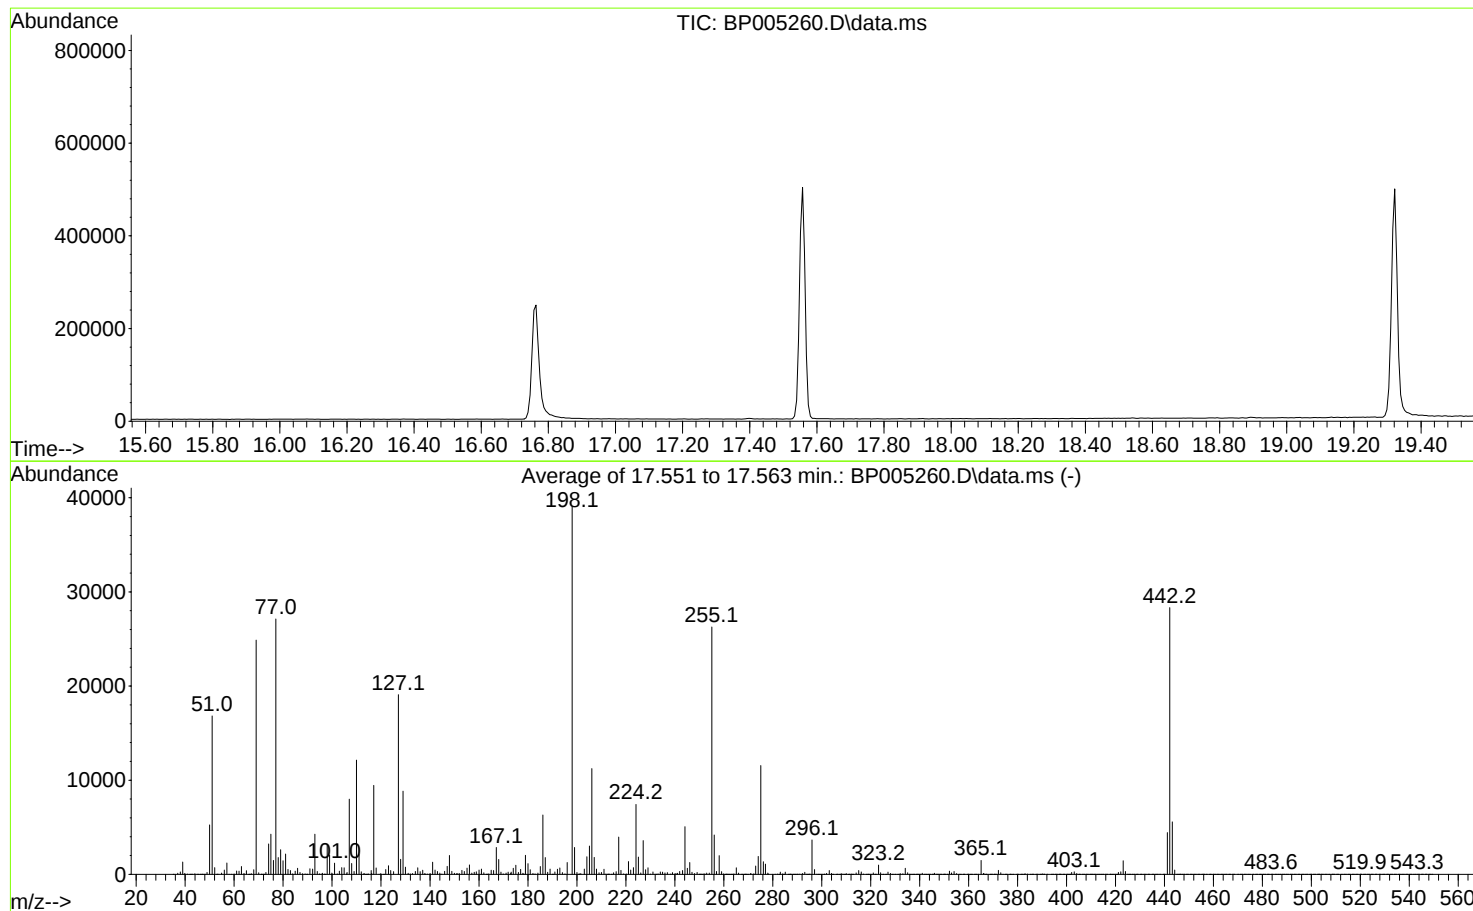

AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.1	16824	PASS
68	69	0.00	2	2.0	493	PASS
69	198	0.00	100	63.7	24872	PASS
70	69	0.00	2	0.7	167	PASS
127	198	10	80	48.8	19086	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	39071	PASS
199	198	5	9	7.3	2861	PASS
275	198	10	60	29.6	11555	PASS
365	198	1	100	3.8	1485	PASS
441	198	0.01	100	11.4	4435	PASS
442	442	100	100	100.0	28339	PASS
443	442	15	24	19.7	5572	PASS

Instrument :
BNA_P
ClientSampleId :
DFTPP

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/12/2021	BNA_P	<u>BP005260.D</u>
Compound Name	Response	Retention Time
DDT	141161	20.51
DDD	808	20.09
DDE	278	19.59
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1086	142247	0.76

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041221\
 Data File : BP005260.D
 Acq On : 12 Apr 2021 09:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Apr 12 10:52:30 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP040921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 09 18:44:11 2021
 Response via : Initial Calibration

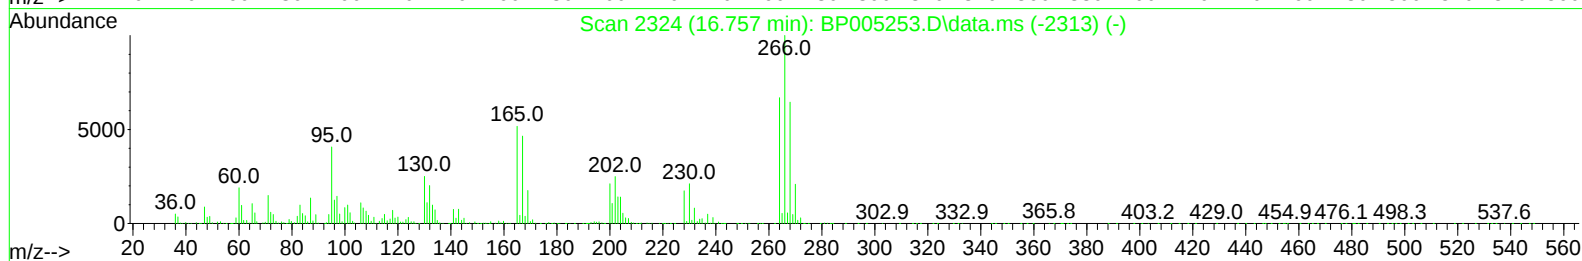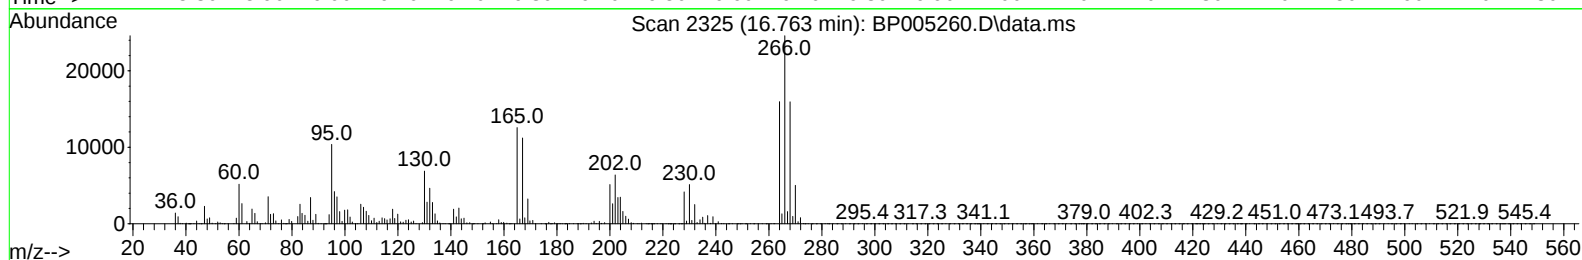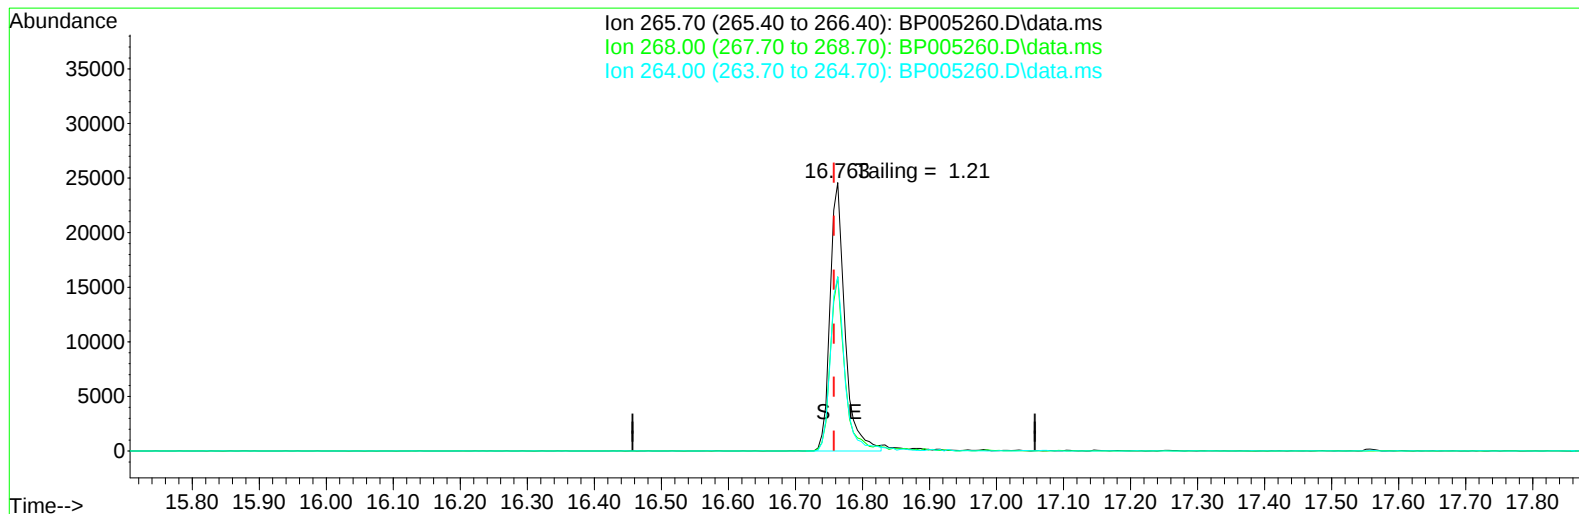

TIC: BP005260.D\data.ms

(70) Pentachlorophenol (C)

16.763min (+ 0.006) 329469.56 ng




response 38845

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	64.85
264.00	63.30	64.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041221\
Data File : BP005260.D
Acq On : 12 Apr 2021 09:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 12 10:52:30 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP040921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 18:44:11 2021
Response via : Initial Calibration

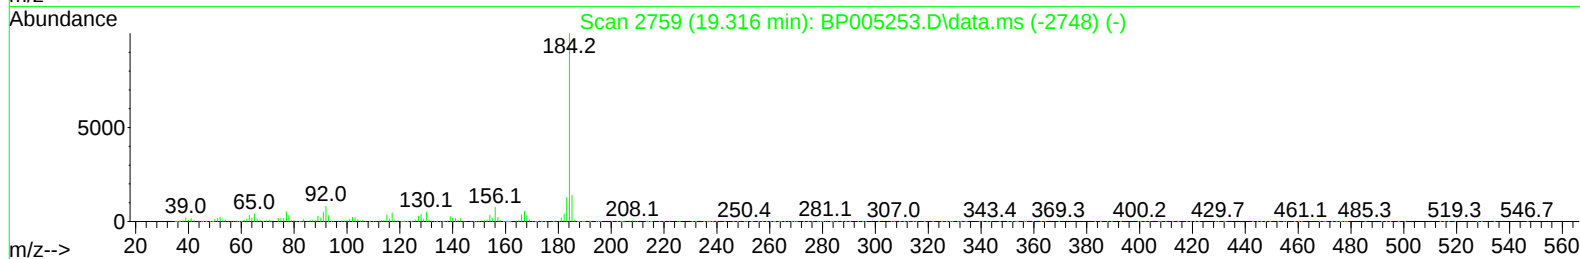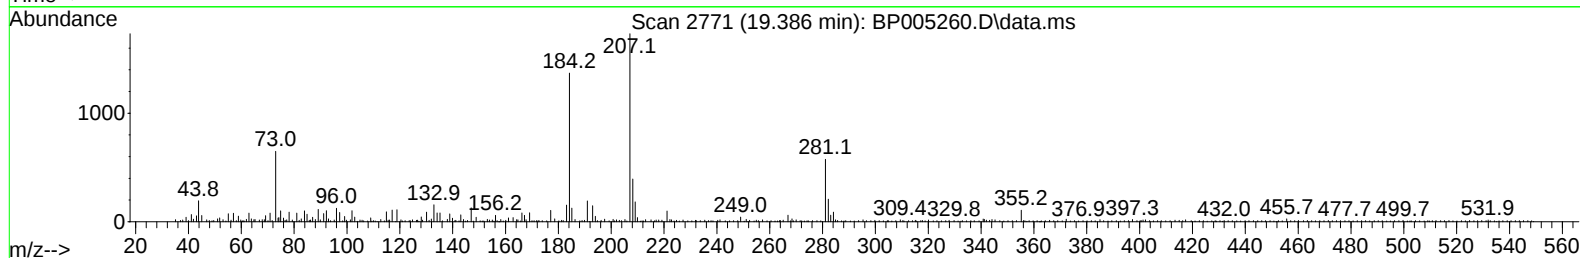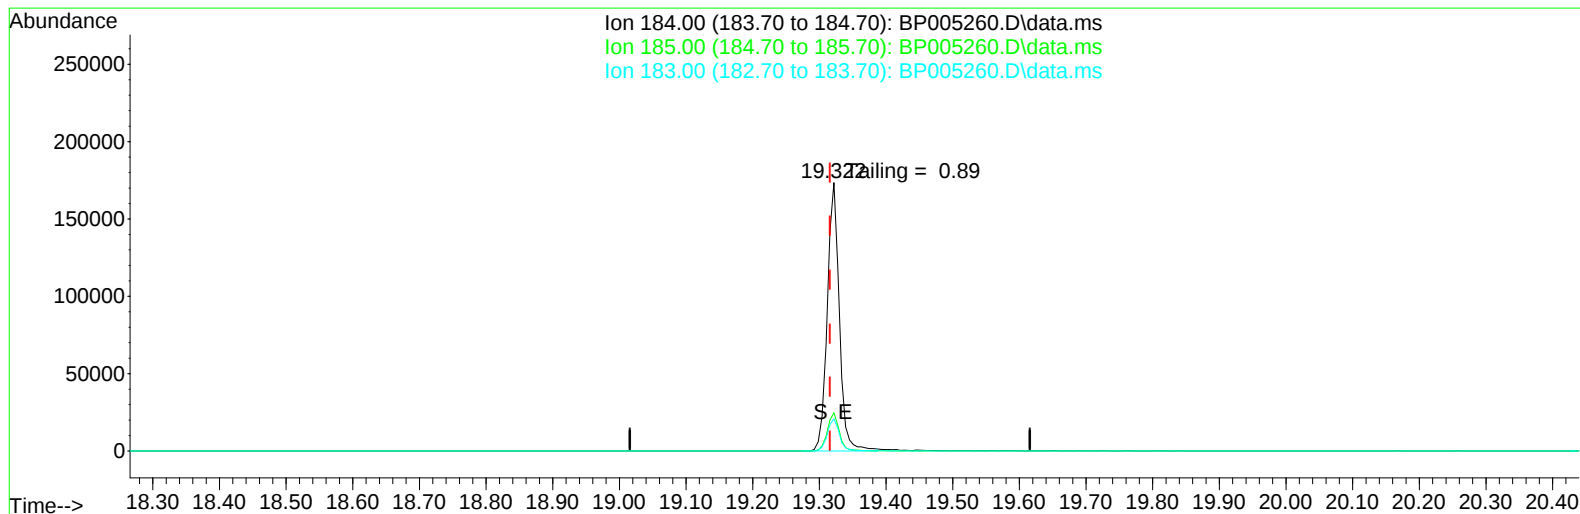

TIC: BP005260.D\data.ms

(77) Benzidine

19.322min (+ 0.006) 1206063.11 ng

response 220726

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.26
183.00	12.00	12.03
0.00	0.00	0.00