

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014704.D
 Acq On : 13 Apr 2023 09:52
 Operator : CG/JU
 Sample : 02282-01DL2 50X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG3DL2

Quant Time: Apr 14 00:54:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 13 02:01:50 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.969	152	87384	20.000	ng/ul	0.00
20) Naphthalene-d8	10.787	136	355402	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.622	164	215462	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.387	188	424897	20.000	ng/ul	0.00
79) Chrysene-d12	21.475	240	415254	20.000	ng/ul	0.00
88) Perylene-d12	23.974	264	501873	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	258	0.114	ng/uL	0.00
4) Pyridine-d5	3.799	84	361	0.063	ng/ul	0.00
7) Phenol-d5	7.140	99	7	0.001	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.322	67	1012	0.196	ng/ul	0.02
11) 2-Chlorophenol-d4	7.493	132	15	0.003	ng/ul	-0.01
15) 4-Methylphenol-d8	8.699	113	14	0.002	ng/ul	0.00
21) Nitrobenzene-d5	9.205	128	501	0.175	ng/ul	0.05
24) 2-Nitrophenol-d4	9.869	143	17	0.005	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.405	165	78	0.013	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.934	131	64	0.008	ng/ul	0.00
46) Dimethylphthalate-d6	14.063	166	7806	0.447	ng/ul	0.03
49) Acenaphthylene-d8	14.169	160	29	0.001	ng/ul	-0.15
54) 4-Nitrophenol-d4	14.851	143	5	0.002	ng/ul	0.00
60) Fluorene-d10	15.640	176	7697	0.528	ng/ul	0.02
65) 4,6-Dinitro-2-methylph...	15.740	200	3	0.001	ng/ul	-0.01
73) Anthracene-d10	17.387	188	424897	20.663	ng/ul	-0.10
81) Pyrene-d10	19.734	212	15229	0.546	ng/ul	0.01
92) Benzo(a)pyrene-d12	23.810	264	8125	0.305	ng/ul	0.00
Target Compounds						
					Qvalue	
30) Naphthalene	10.840	128	101552	5.130	ng/ul	99
71) Pentachlorophenol	17.040	266	91859	26.108	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014704.D
Acq On : 13 Apr 2023 09:52
Operator : CG/JU
Sample : 02282-01DL2 50X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG3DL2

Quant Time: Apr 14 00:54:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 13 02:01:50 2023
Response via : Initial Calibration




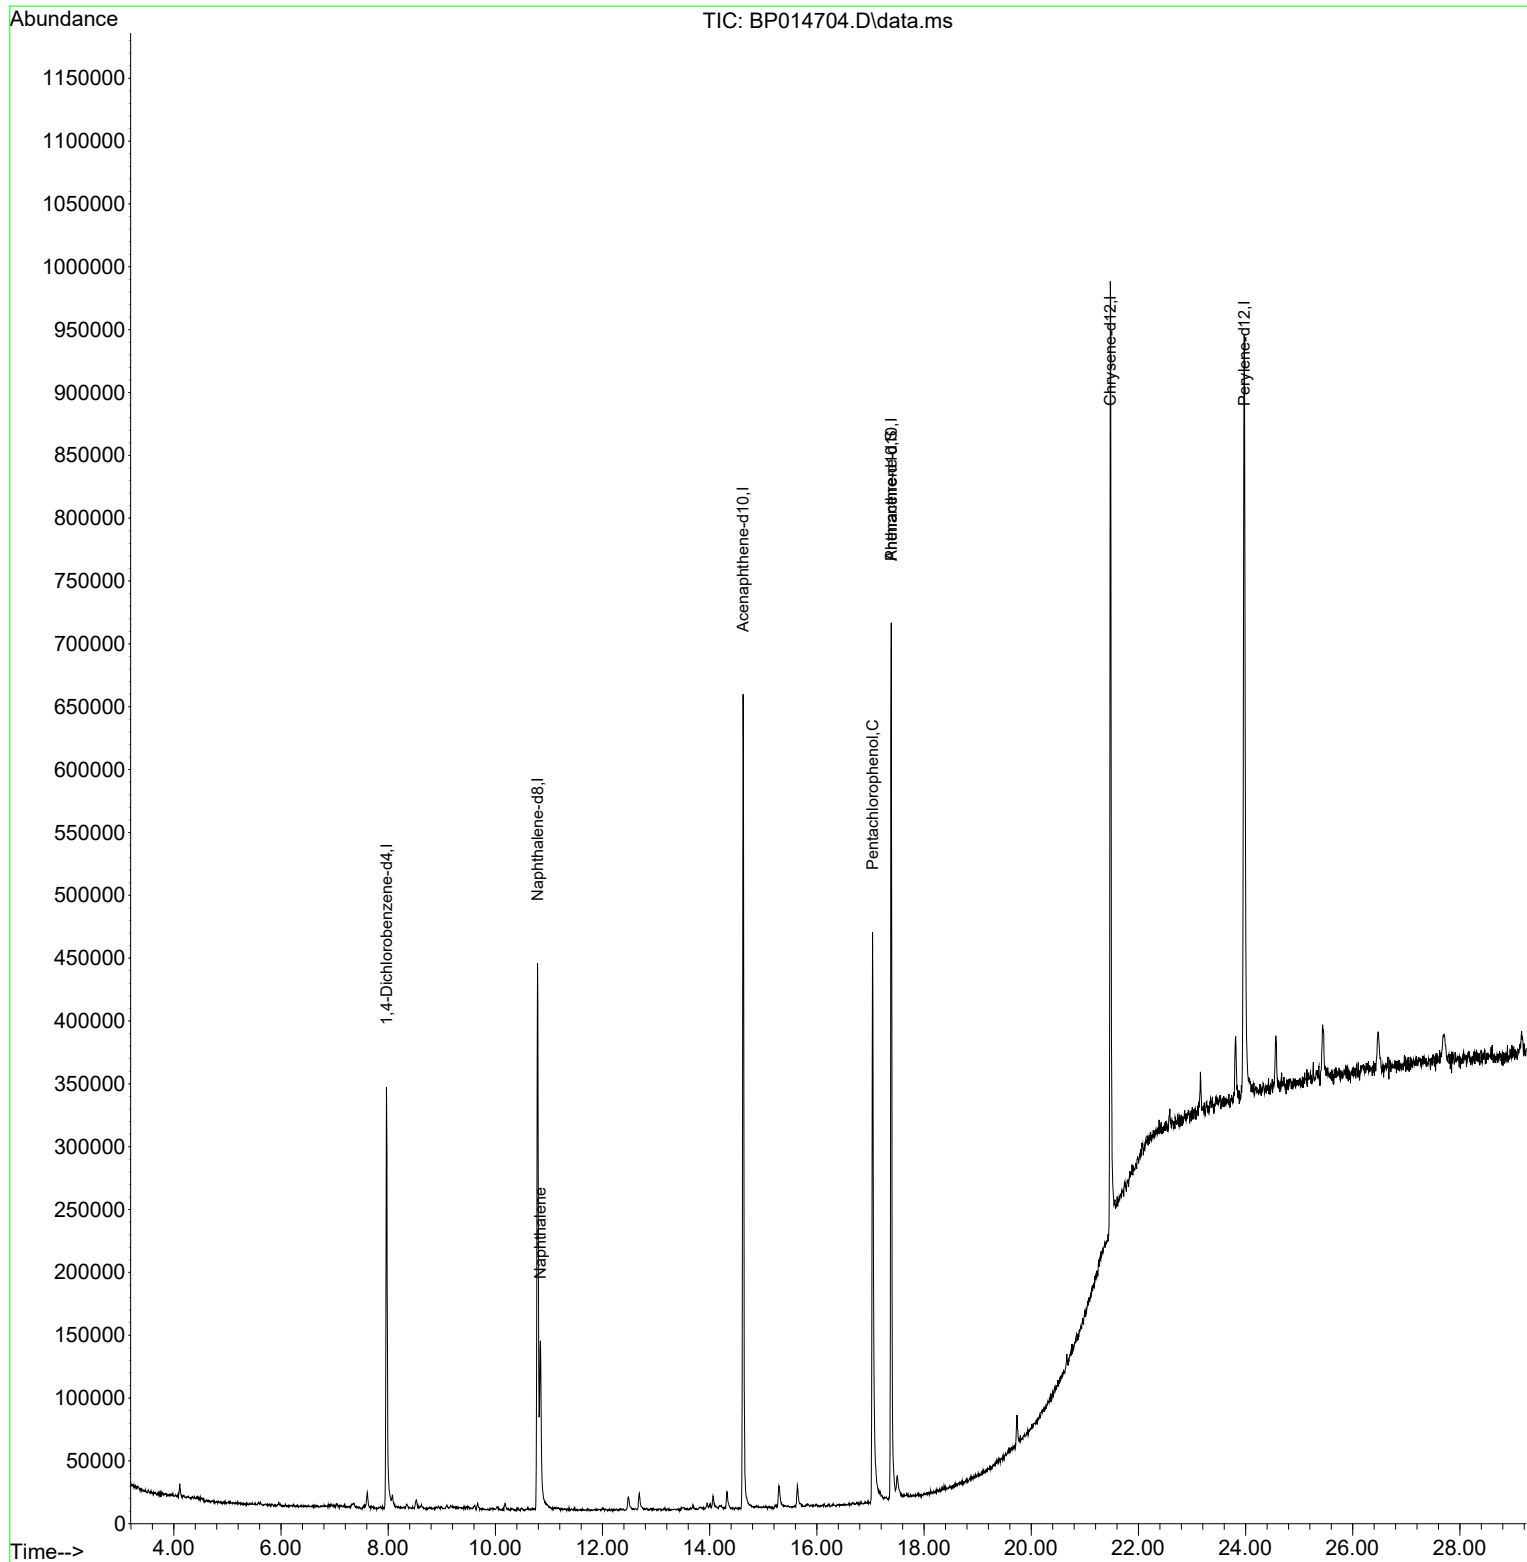


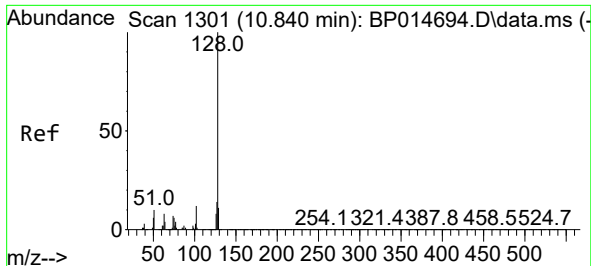

#30
Naphthalene
Concen: 5.130 ng/ul
RT: 10.840 min Scan# 11
Delta R.T. 0.000 min
Lab File: BP014704.D
Acq: 13 Apr 2023 09:52

Instrument :
BNA_P
ClientSampleId :
C0QG3DL2

Tgt Ion:128 Resp: 101552
Ion Ratio Lower Upper
128 100
129 12.0 8.9 13.3
127 14.0 11.0 16.6

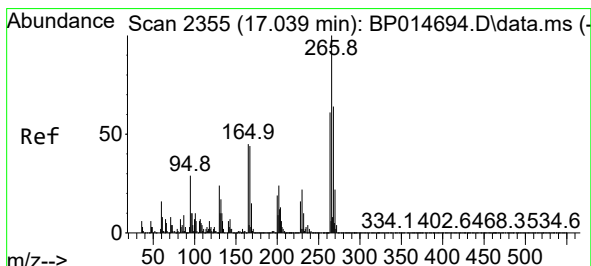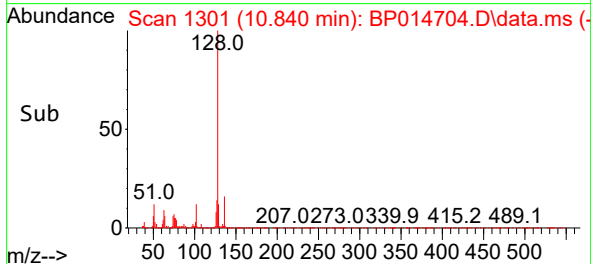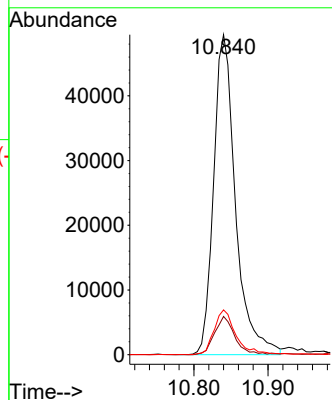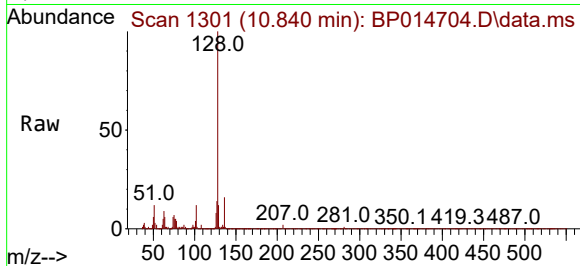

#71
Pentachlorophenol
Concen: 26.108 ng/ul
RT: 17.040 min Scan# 2355
Delta R.T. 0.000 min
Lab File: BP014704.D
Acq: 13 Apr 2023 09:52

Tgt Ion:266 Resp: 91859
Ion Ratio Lower Upper
266 100
264 63.3 51.0 76.4
268 65.7 51.4 77.2

