




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014672.D
 Acq On : 12 Apr 2023 14:17
 Operator : CG/JU
 Sample : 02251-16
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COMD4

Manual IntegrationsAPPROVED

Reviewed By :Christian
 Giraldo
 04/13/2023
 Supervised By :Jagrut
 Upadhyay
 04/13/2023

Quant Time: Apr 13 00:49:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 11 01:21:43 2023
 Response via : Initial Calibration

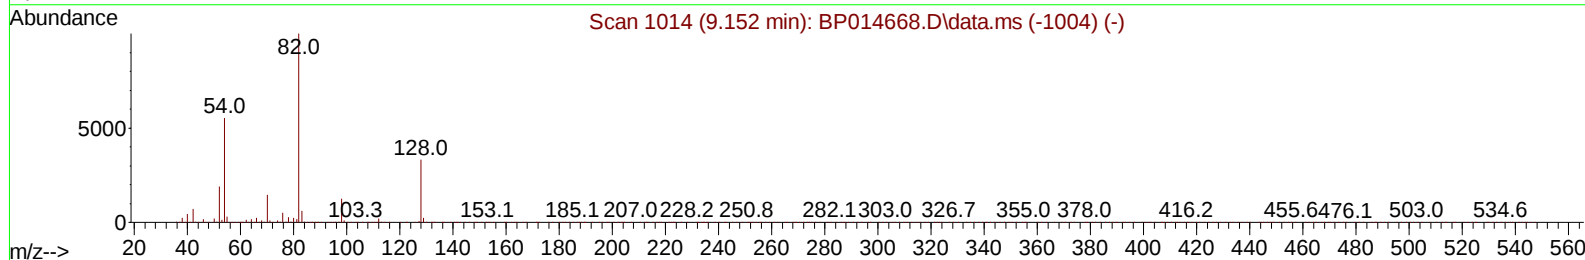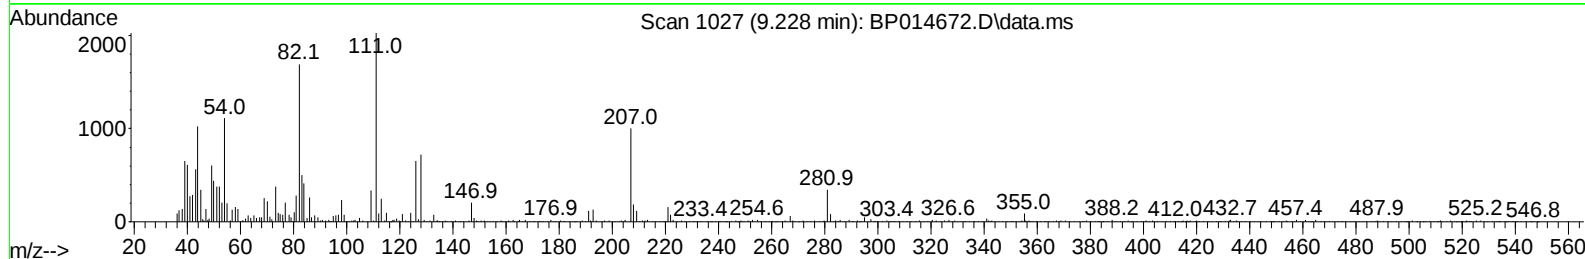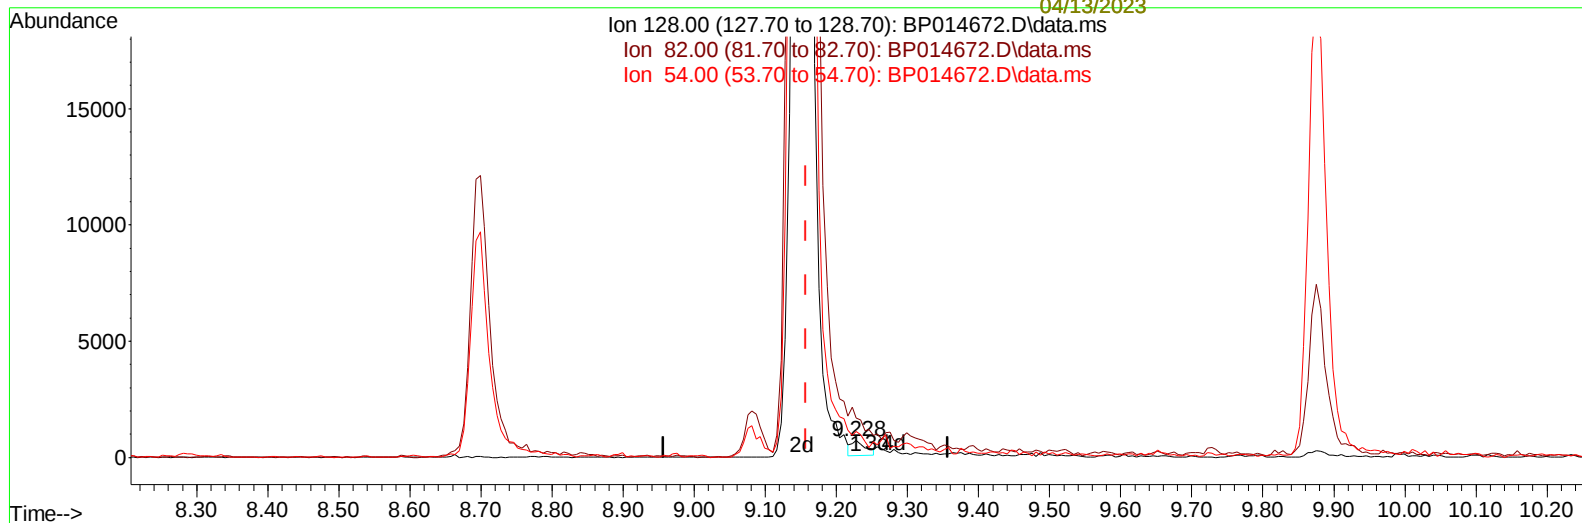

TIC: BP014672.D\data.ms

(21) Nitrobenzene-d5 (S)

9.228min (+ 0.071) 0.21 ng/u1

response 876

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	278.40	235.14
54.00	139.60	154.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014672.D
 Acq On : 12 Apr 2023 14:17
 Operator : CG/JU
 Sample : 02251-16
 Misc :
 ALS Vial : 6 Sample Multiplier: 1




Instrument :
 BNA_P
 ClientSampleId :
 COMD4

Manual IntegrationsAPPROVED

Reviewed By :Christian
 Giraldo
 04/13/2023
 Supervised By :Jagrut
 Upadhyay
 04/13/2023

Quant Time: Apr 13 00:49:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 11 01:21:43 2023
 Response via : Initial Calibration

Ion 128.00 (127.70 to 128.70): BP014672.D\data.ms
 Ion 82.00 (81.70 to 82.70): BP014672.D\data.ms
 Ion 54.00 (53.70 to 54.70): BP014672.D\data.ms

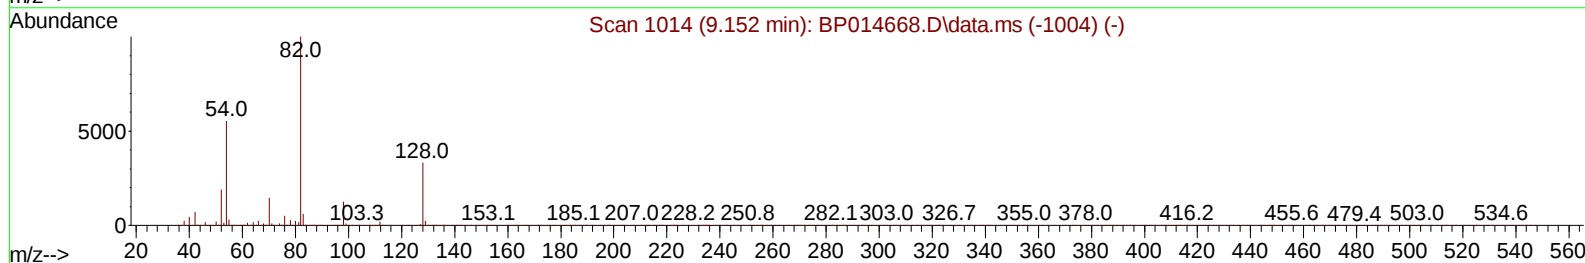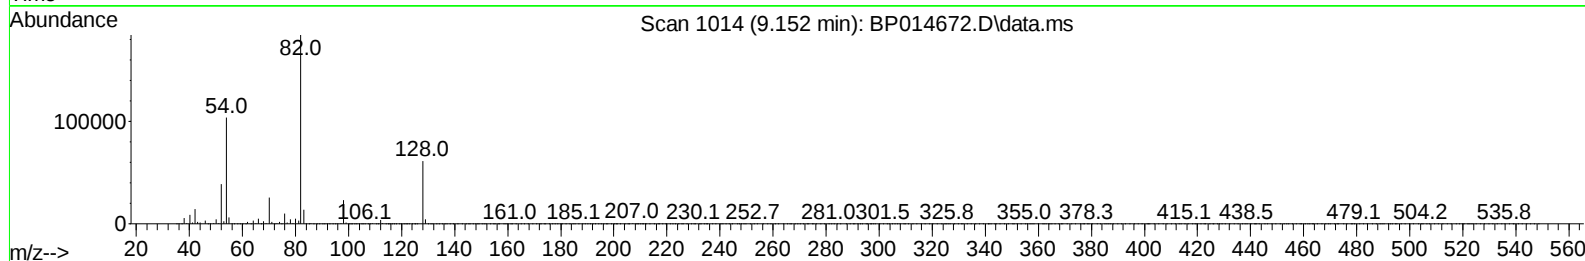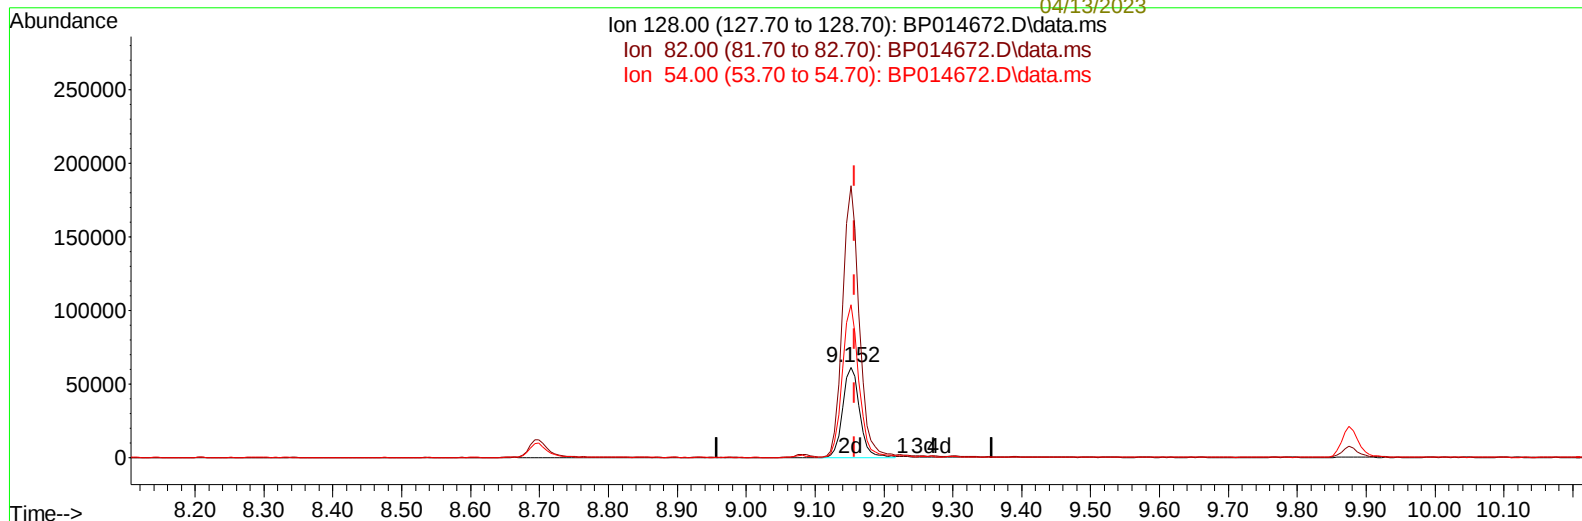

TIC: BP014672.D\data.ms

(21) Nitrobenzene-d5 (S)

9.152min (-0.006) 24.57 ng/ul m

response 104932

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	278.40	300.94
54.00	139.60	169.19#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014672.D
Acq On : 12 Apr 2023 14:17
Operator : CG/JU
Sample : 02251-16
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMD4

Manual IntegrationsAPPROVED

Quant Time: Apr 13 00:49:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

Reviewed By :Christian
Giraldo
04/13/2023
Supervised By :Jagrut
Upadhyay
04/13/2023

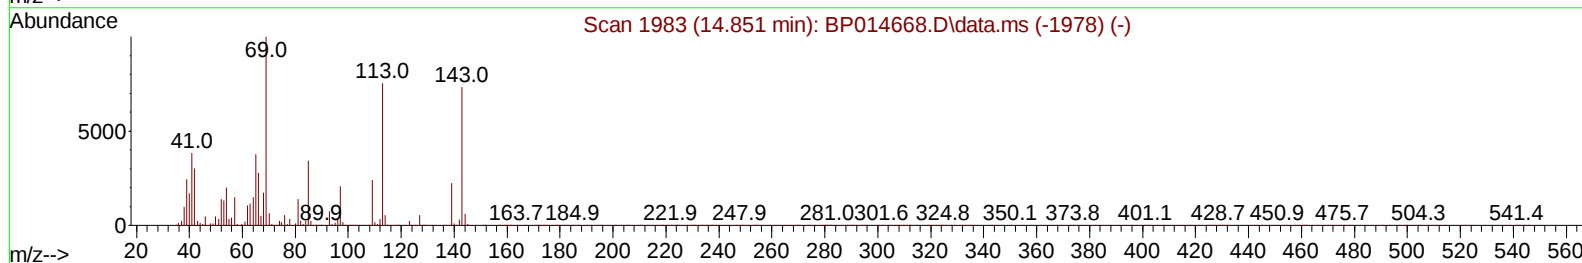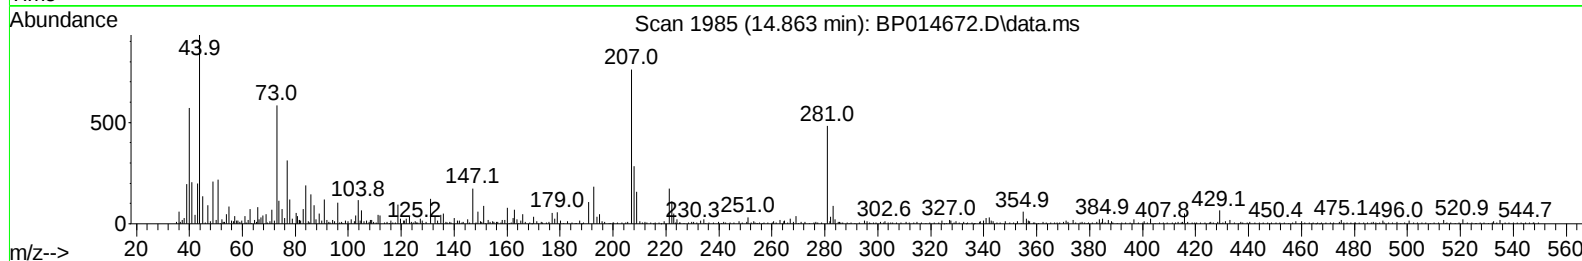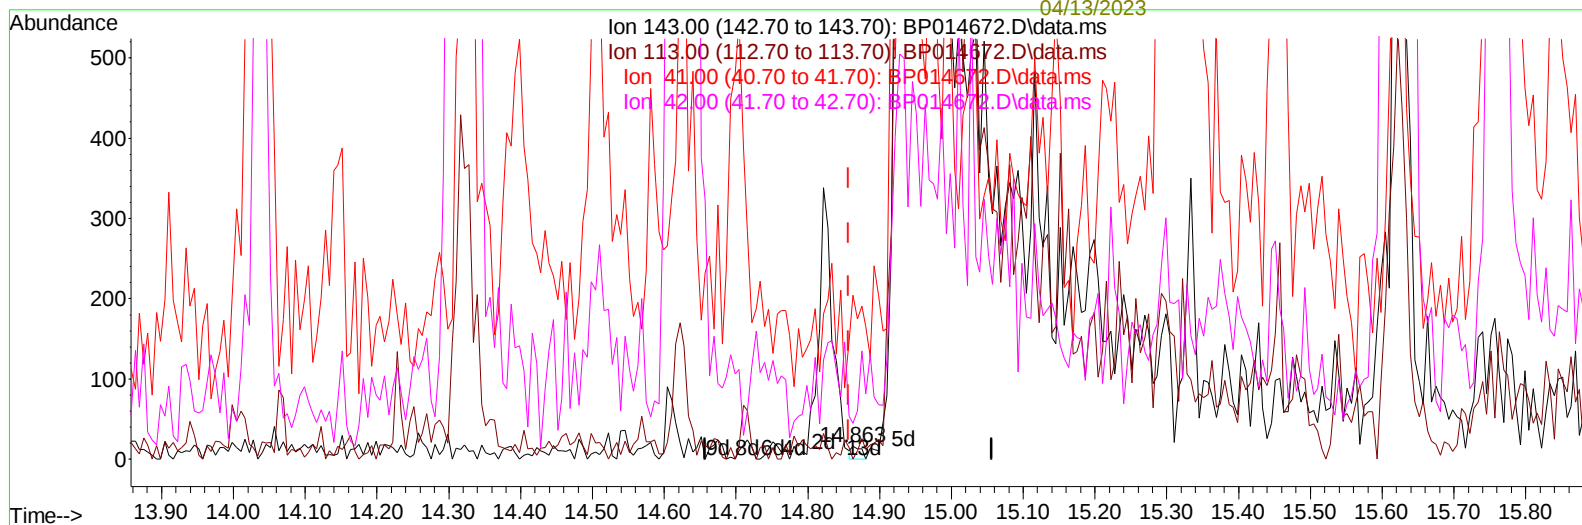

TIC: BP014672.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.863min (+ 0.006) 0.00 ng/u1

response 15

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	37.50#
41.00	44.20	1275.00#
42.00	31.50	281.25#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014672.D
 Acq On : 12 Apr 2023 14:17
 Operator : CG/JU
 Sample : 02251-16
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COMD4

Quant Time: Apr 13 00:49:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 11 01:21:43 2023
 Response via : Initial Calibration

Manual IntegrationsAPPROVED

Reviewed By :Christian
 Giraldo
 04/13/2023
 Supervised By :Jagrut
 Upadhyay
 04/13/2023

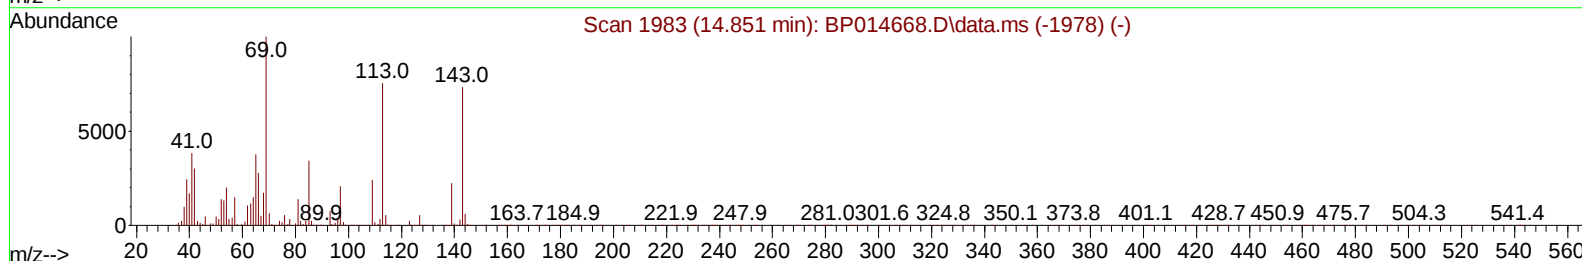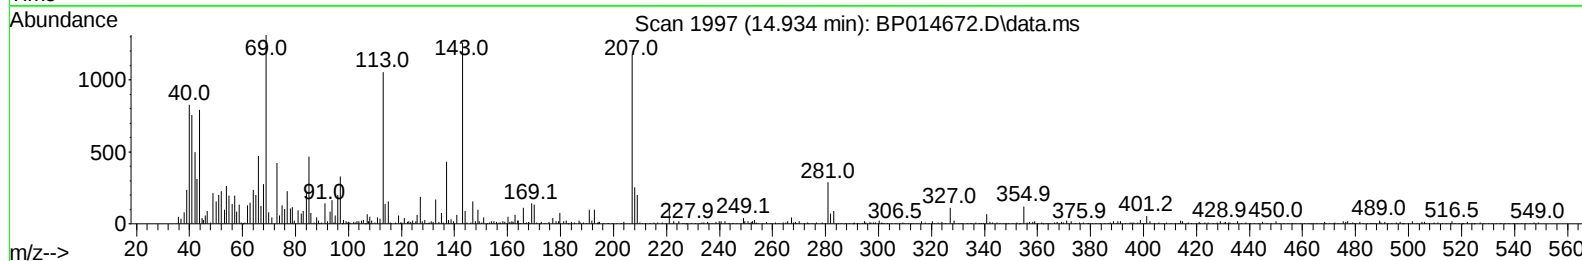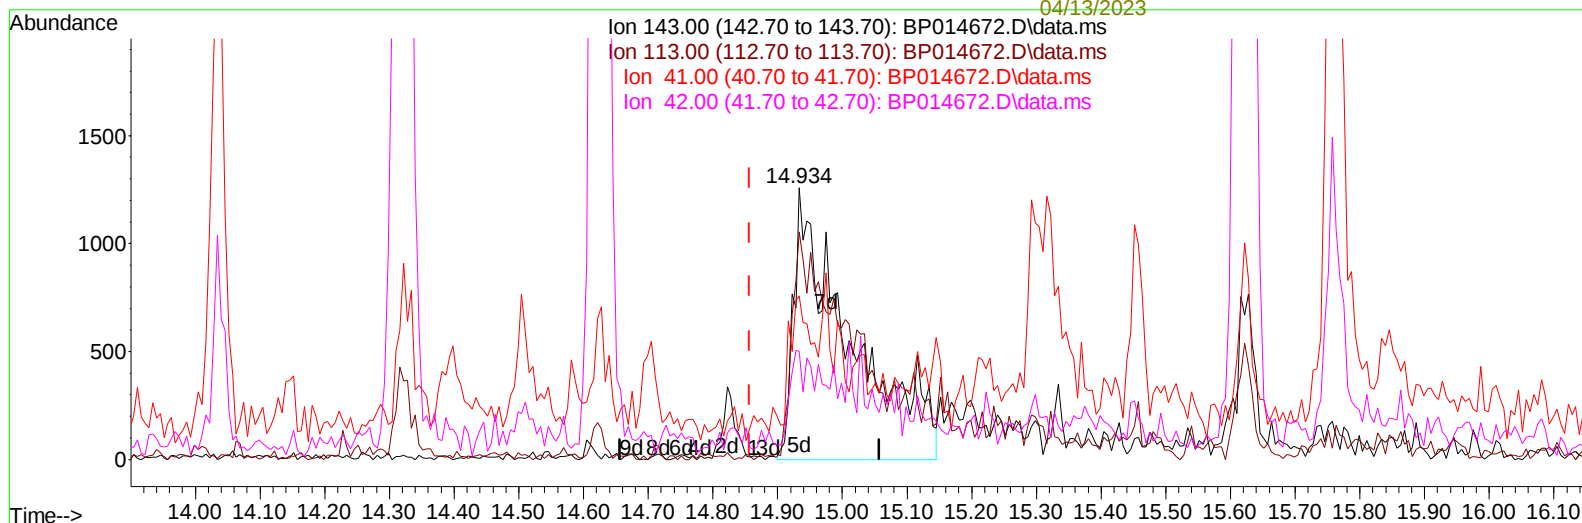

TIC: BP014672.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.934min (+ 0.077) 1.95 ng/ul m

response 7557

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	83.86
41.00	44.20	60.33#
42.00	31.50	39.67#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014672.D
 Acq On : 12 Apr 2023 14:17
 Operator : CG/JU
 Sample : 02251-16
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COMD4

Manual IntegrationsAPPROVED

Reviewed By :Christian
 Giraldo
 04/13/2023
 Supervised By :Jagrut
 Upadhyay
 04/13/2023

Quant Time: Apr 13 00:49:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 11 01:21:43 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.975	152		113534	20.000	ng/ul	0.00
20) Naphthalene-d8	10.793	136		528999	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.628	164		315800	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.392	188		682344	20.000	ng/ul	0.00
79) Chrysene-d12	21.486	240		445303	20.000	ng/ul	0.00
88) Perylene-d12	23.986	264		483514	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.364	96		13966	4.770	ng/uL	0.00
4) Pyridine-d5	3.811	84		42889	5.717	ng/ul	0.02
7) Phenol-d5	7.152	99		39401	3.763	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.299	67		198702	29.577	ng/ul	0.00
11) 2-Chlorophenol-d4	7.505	132		137180	18.127	ng/ul	0.00
15) 4-Methylphenol-d8	8.699	113		93497	11.070	ng/ul	0.00
21) Nitrobenzene-d5	9.152	128		104932m	24.571	ng/ul	0.00
24) 2-Nitrophenol-d4	9.875	143		100244	20.500	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.422	165		167899	18.853	ng/ul	0.00
31) 4-Chloroaniline-d4	10.946	131		229774	19.587	ng/ul	0.00
46) Dimethylphthalate-d6	14.034	166		684972	26.751	ng/ul	0.00
49) Acenaphthylene-d8	14.322	160		733559	25.819	ng/ul	0.00
54) 4-Nitrophenol-d4	14.934	143		7557m	1.954	ng/ul	0.08
60) Fluorene-d10	15.622	176		586808	27.481	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.763	200		55747	11.103	ng/ul	0.00
73) Anthracene-d10	17.492	188		955872	28.946	ng/ul	0.00
81) Pyrene-d10	19.722	212		1016247	33.976	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.822	264		740014	28.807	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014672.D
Acq On : 12 Apr 2023 14:17
Operator : CG/JU
Sample : 02251-16
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0MD4

Manual IntegrationsAPPROVED

Reviewed By :Christian
Giraldo
04/13/2023
Supervised By :Jagrut
Upadhyay
04/13/2023

Quant Time: Apr 13 00:49:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

