




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014677.D
Acq On : 12 Apr 2023 17:14
Operator : CG/JU
Sample : 02251-18
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMD6

Manual IntegrationsAPPROVED

Quant Time: Apr 13 00:50:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/13/2023
Supervised By :Jagrut Upadhyay 04/13/2023

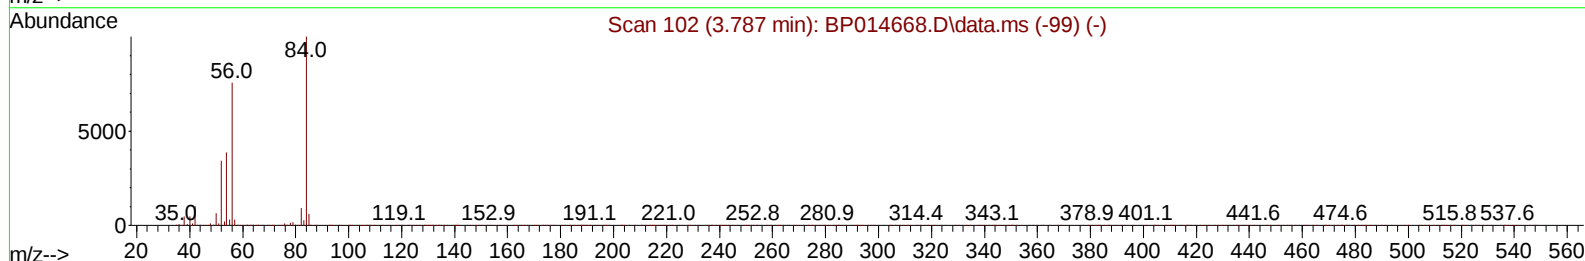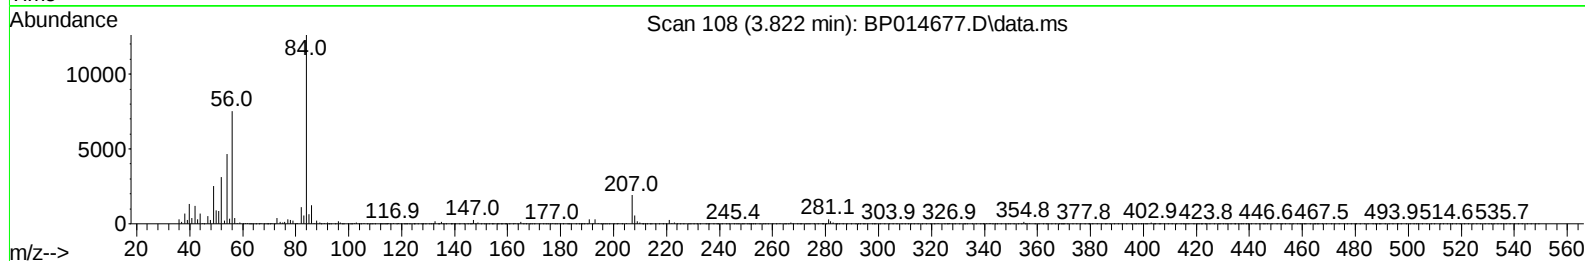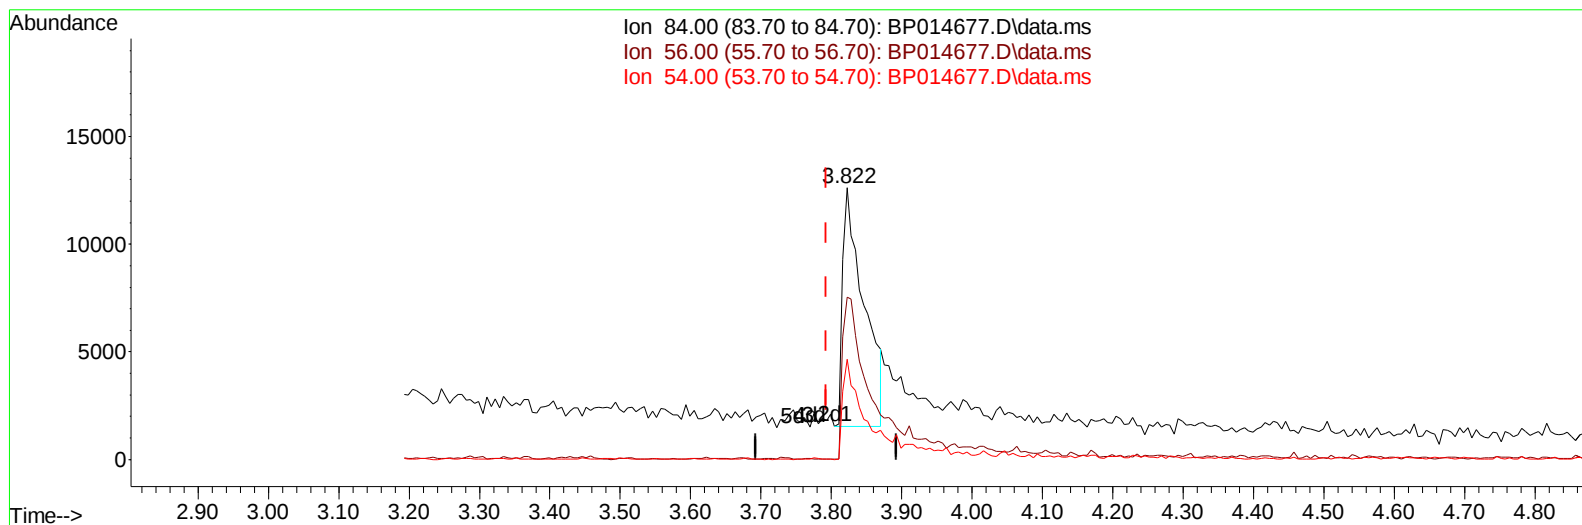

TIC: BP014677.D\data.ms

(4) Pyridine-d5 (S)

3.822min (+ 0.029) 3.08 ng/u1

response 22941

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.70	59.78
54.00	32.60	36.94
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014677.D
 Acq On : 12 Apr 2023 17:14
 Operator : CG/JU
 Sample : 02251-18
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COMD6

Manual IntegrationsAPPROVED

Quant Time: Apr 13 00:50:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 11 01:21:43 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/13/2023
 Supervised By :Jagrut Upadhyay 04/13/2023

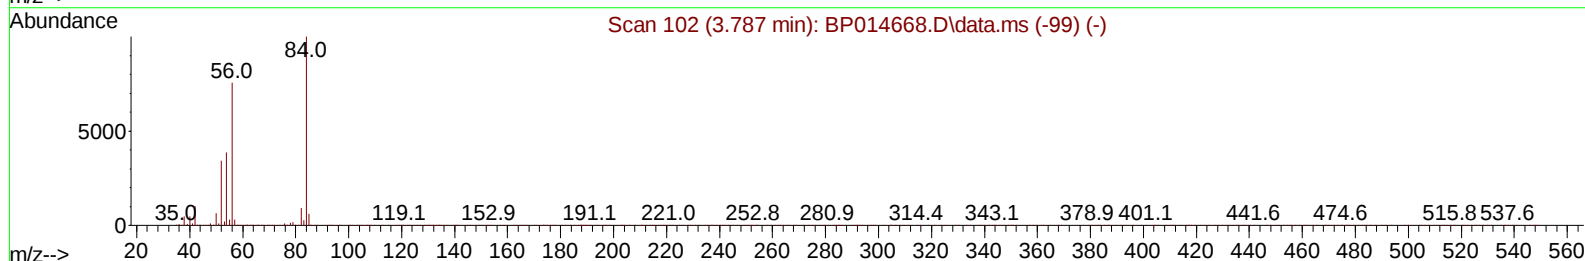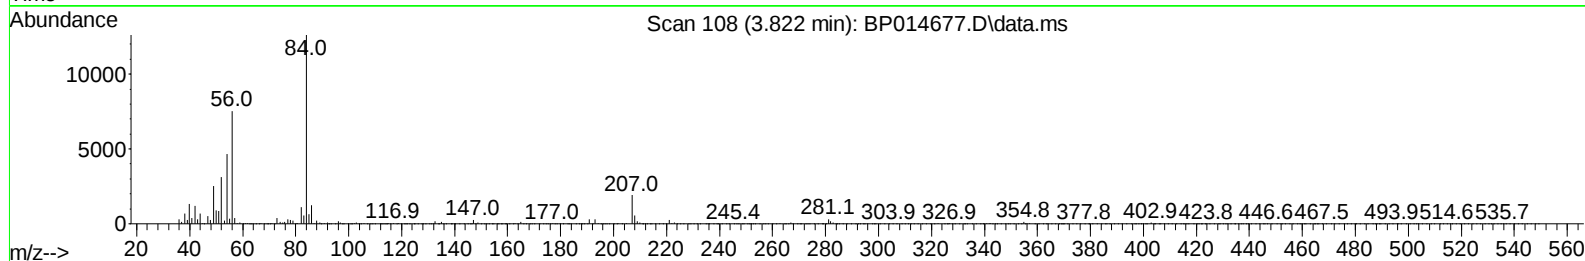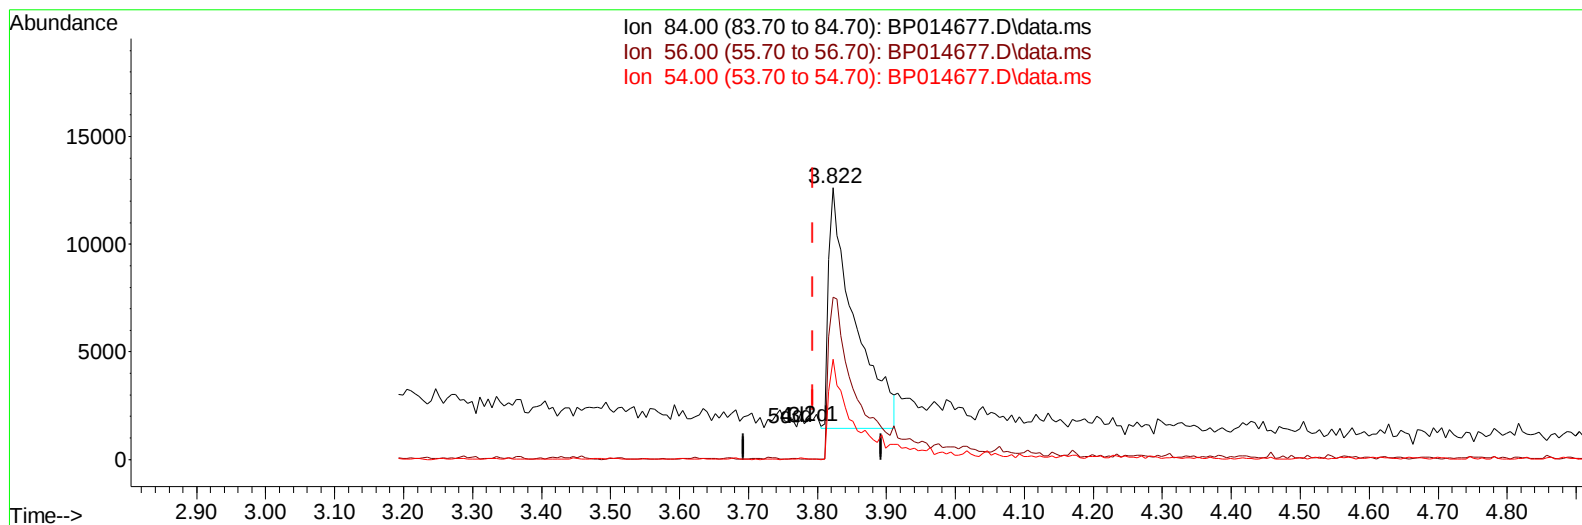

TIC: BP014677.D\data.ms

(4) Pyridine-d5 (S)

3.822min (+ 0.029) 3.89 ng/u1 m

response 28938

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.70	59.78
54.00	32.60	36.94
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014677.D
Acq On : 12 Apr 2023 17:14
Operator : CG/JU
Sample : 02251-18
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMD6

Manual IntegrationsAPPROVED

Quant Time: Apr 13 00:50:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/13/2023
Supervised By :Jagrut Upadhyay 04/13/2023

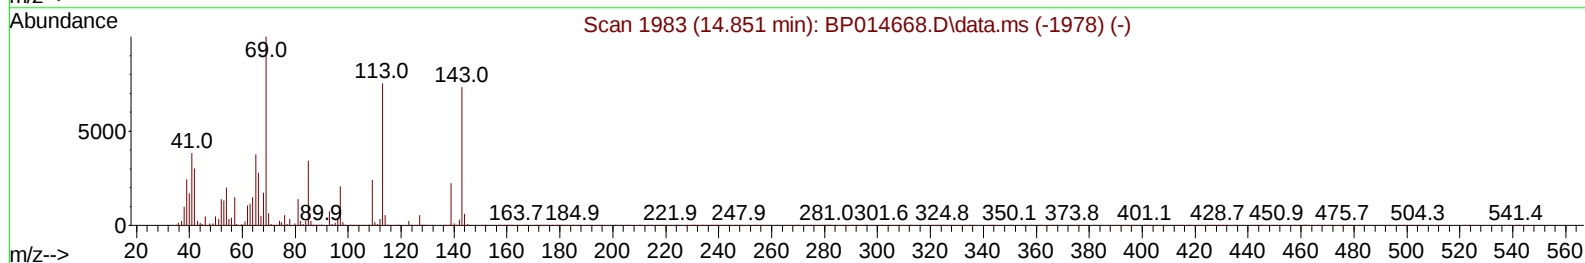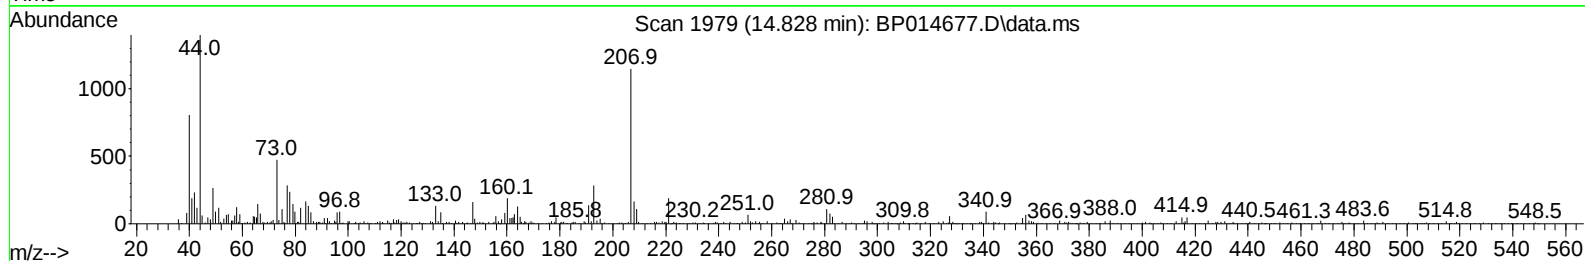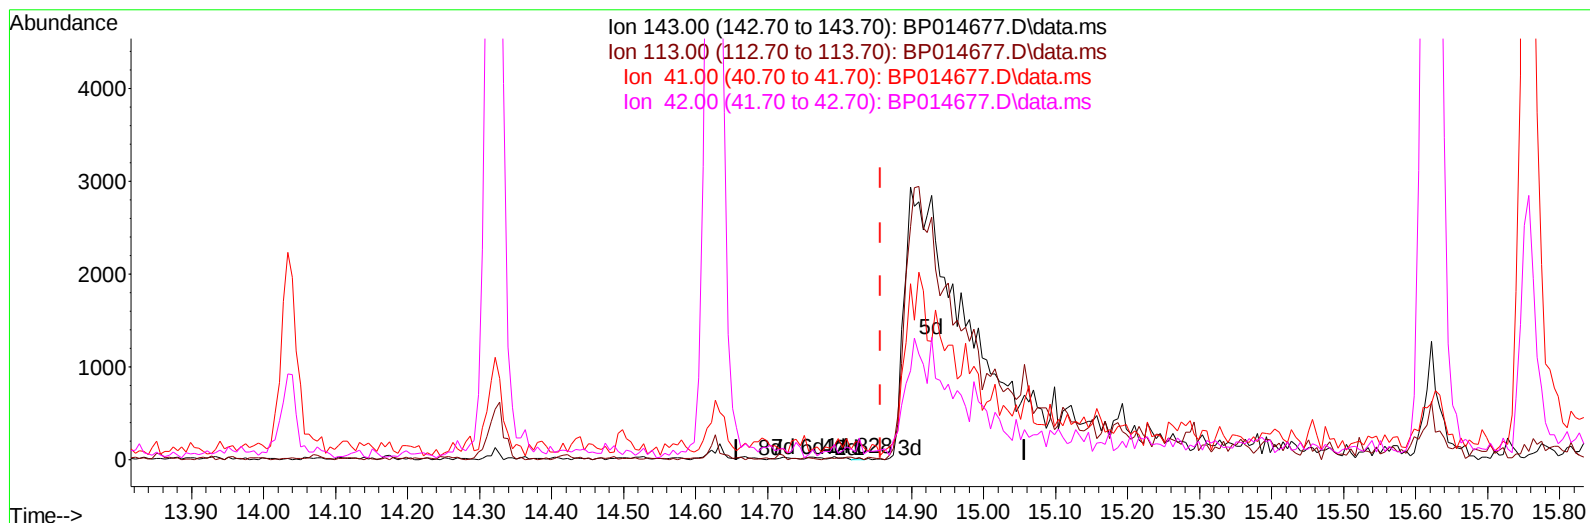

TIC: BP014677.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.828min (-0.029) 0.00 ng/u1

response 8

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	125.00#
41.00	44.20	1193.75#
42.00	31.50	1456.25#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014677.D
 Acq On : 12 Apr 2023 17:14
 Operator : CG/JU
 Sample : 02251-18
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COMD6

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/13/2023
 Supervised By :Jagrut Upadhyay 04/13/2023

Quant Time: Apr 13 00:50:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 11 01:21:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.975	152	112698	20.000	ng/ul	0.00
20) Naphthalene-d8	10.793	136	506626	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.628	164	345199	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.386	188	766187	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	522361	20.000	ng/ul	0.00
88) Perylene-d12	23.986	264	523219	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.358	96	14568	5.013	ng/uL	0.00
4) Pyridine-d5	3.822	84	28938m	3.886	ng/ul	0.03
7) Phenol-d5	7.146	99	69662	6.702	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.299	67	199912	29.978	ng/ul	0.00
11) 2-Chlorophenol-d4	7.505	132	171696	22.856	ng/ul	0.00
15) 4-Methylphenol-d8	8.699	113	129727	15.474	ng/ul	0.00
21) Nitrobenzene-d5	9.152	128	106862	26.128	ng/ul	0.00
24) 2-Nitrophenol-d4	9.875	143	119303	25.474	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.422	165	188270	22.074	ng/ul	0.00
31) 4-Chloroaniline-d4	10.946	131	182973	16.287	ng/ul	0.00
46) Dimethylphthalate-d6	14.034	166	780439	27.883	ng/ul	0.00
49) Acenaphthylene-d8	14.322	160	835266	26.895	ng/ul	0.00
54) 4-Nitrophenol-d4	14.898	143	18511m	4.378	ng/ul	0.04
60) Fluorene-d10	15.622	176	677248	29.015	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	118770	21.067	ng/ul	0.00
73) Anthracene-d10	17.492	188	1102814	29.741	ng/ul	0.00
81) Pyrene-d10	19.722	212	1208451	34.442	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.815	264	880400	31.671	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014677.D
Acq On : 12 Apr 2023 17:14
Operator : CG/JU
Sample : 02251-18
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMD6

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/13/2023
Supervised By :Jagrut Upadhyay 04/13/2023

Quant Time: Apr 13 00:50:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

