




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014678.D
Acq On : 12 Apr 2023 17:48
Operator : CG/JU
Sample : 02251-19
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMD7

Manual IntegrationsAPPROVED

Quant Time: Apr 13 00:50:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/13/2023
Supervised By :Jagrut Upadhyay 04/13/2023

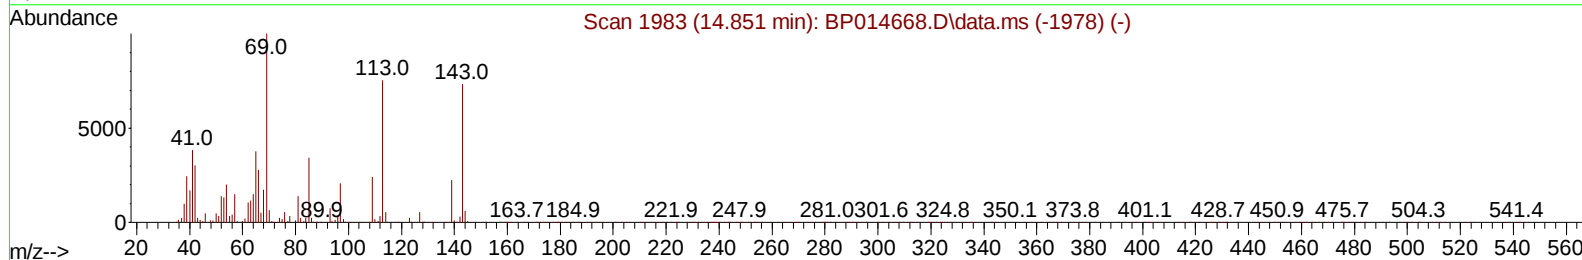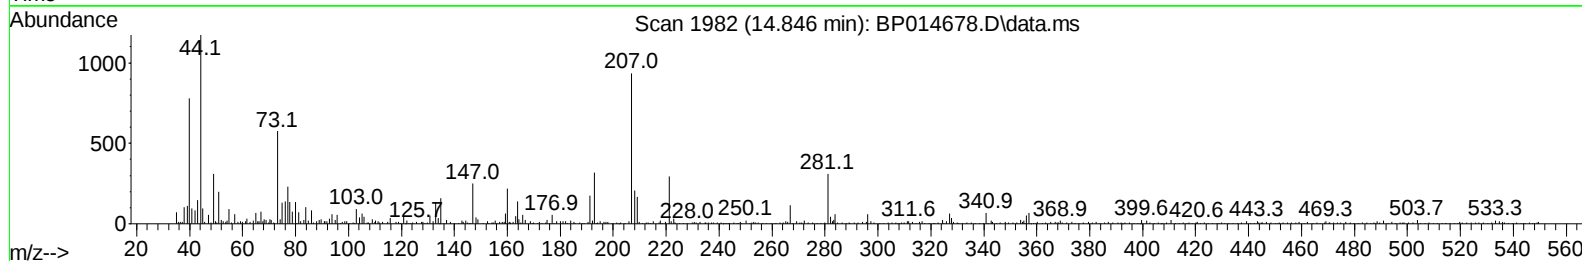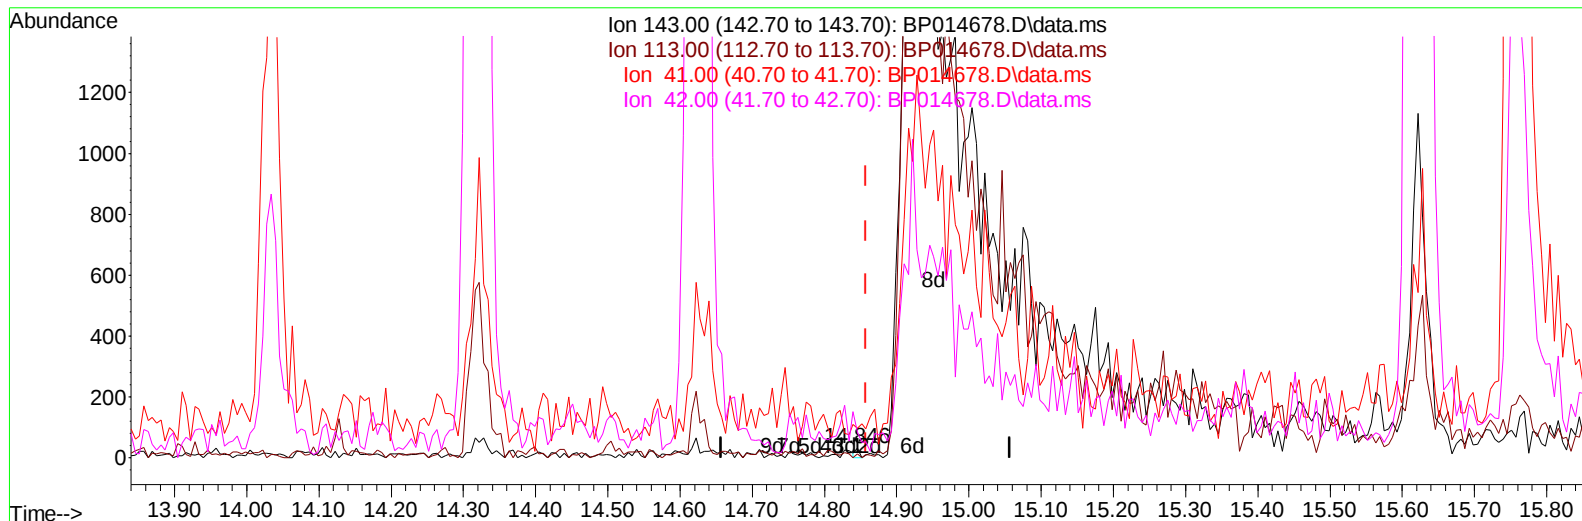

TIC: BP014678.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.846min (-0.012) 0.00 ng/u1

response 11

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	41.94#
41.00	44.20	312.90#
42.00	31.50	270.97#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014678.D
Acq On : 12 Apr 2023 17:48
Operator : CG/JU
Sample : 02251-19
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMD7

Manual IntegrationsAPPROVED

Quant Time: Apr 13 00:50:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/13/2023
Supervised By :Jagrut Upadhyay 04/13/2023

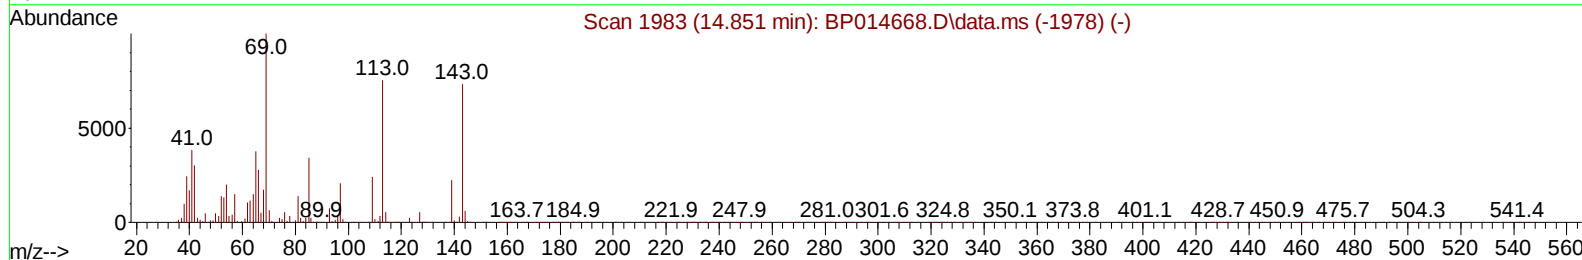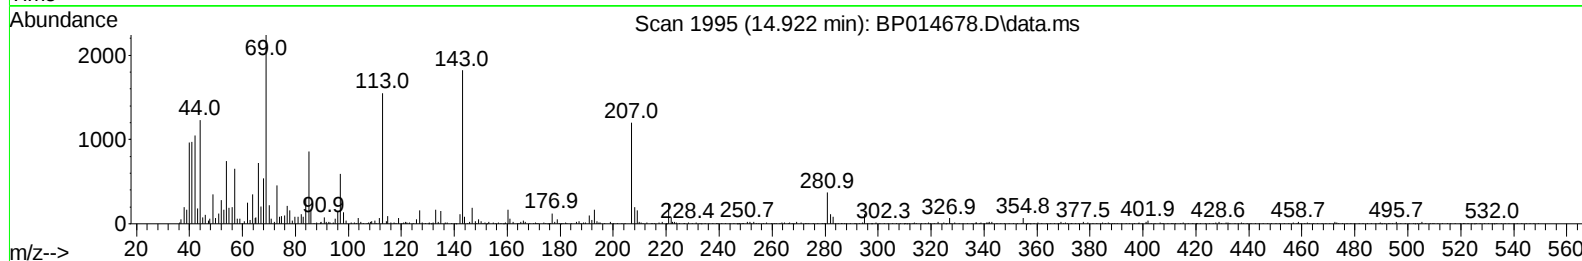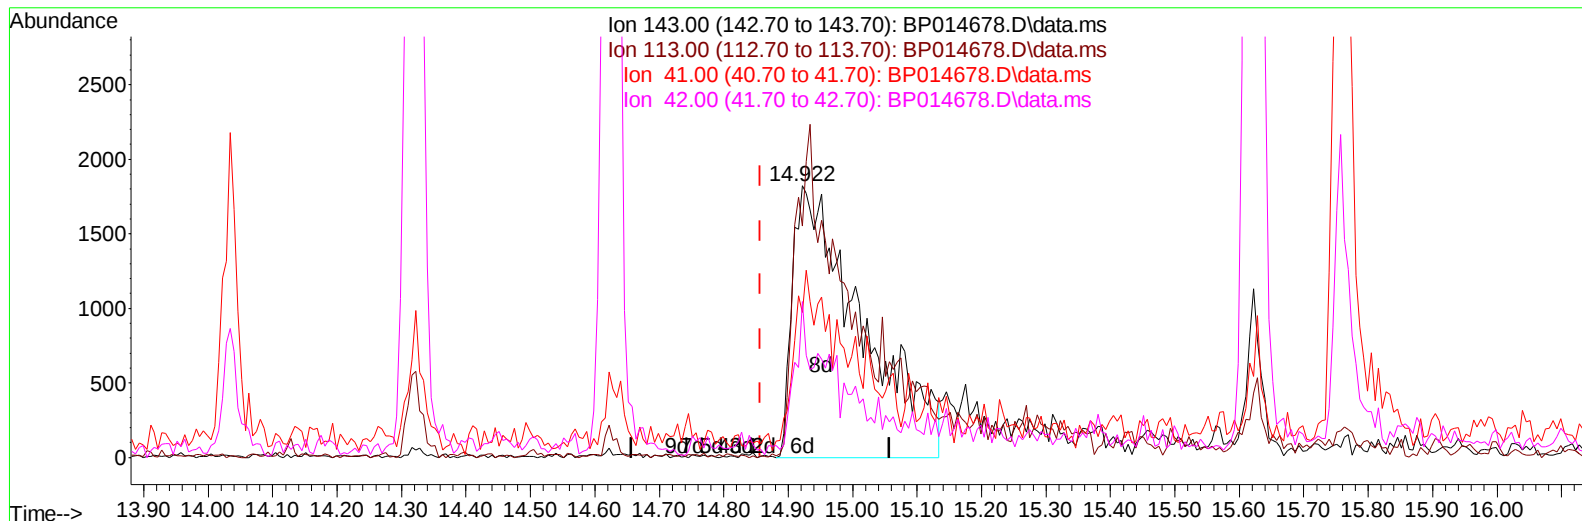

TIC: BP014678.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.922min (+ 0.065) 3.13 ng/ul m

response 13584

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	85.23
41.00	44.20	53.49#
42.00	31.50	57.50#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014678.D
 Acq On : 12 Apr 2023 17:48
 Operator : CG/JU
 Sample : 02251-19
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COMD7

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/13/2023
 Supervised By :Jagrut Upadhyay 04/13/2023

Quant Time: Apr 13 00:50:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 11 01:21:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.975	152	121561	20.000	ng/ul	0.00
20) Naphthalene-d8	10.793	136	536791	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.628	164	353938	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.392	188	721255	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	497936	20.000	ng/ul	0.00
88) Perylene-d12	23.980	264	591183	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	13884	4.429	ng/uL	0.00
4) Pyridine-d5	3.805	84	66072	8.225	ng/ul	0.01
7) Phenol-d5	7.146	99	66879	5.966	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.299	67	216820	30.143	ng/ul	0.00
11) 2-Chlorophenol-d4	7.505	132	181627	22.415	ng/ul	0.00
15) 4-Methylphenol-d8	8.693	113	129913	14.366	ng/ul	0.00
21) Nitrobenzene-d5	9.152	128	108938	25.139	ng/ul	0.00
24) 2-Nitrophenol-d4	9.875	143	122154	24.617	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.422	165	191633	21.206	ng/ul	0.00
31) 4-Chloroaniline-d4	10.946	131	223901	18.810	ng/ul	0.00
46) Dimethylphthalate-d6	14.034	166	738892	25.747	ng/ul	0.00
49) Acenaphthylene-d8	14.322	160	834258	26.199	ng/ul	0.00
54) 4-Nitrophenol-d4	14.922	143	13584m	3.133	ng/ul	0.06
60) Fluorene-d10	15.622	176	643755	26.899	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	100539	18.944	ng/ul	0.00
73) Anthracene-d10	17.492	188	960099	27.506	ng/ul	0.00
81) Pyrene-d10	19.722	212	967902	28.939	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.822	264	884030	28.146	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014678.D
Acq On : 12 Apr 2023 17:48
Operator : CG/JU
Sample : 02251-19
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMD7

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/13/2023
Supervised By :Jagrut Upadhyay 04/13/2023

Quant Time: Apr 13 00:50:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

