




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014679.D
Acq On : 12 Apr 2023 18:23
Operator : CG/JU
Sample : 02251-20
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMD8

Manual IntegrationsAPPROVED

Quant Time: Apr 13 00:50:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/13/2023
Supervised By :Jagrut Upadhyay 04/13/2023

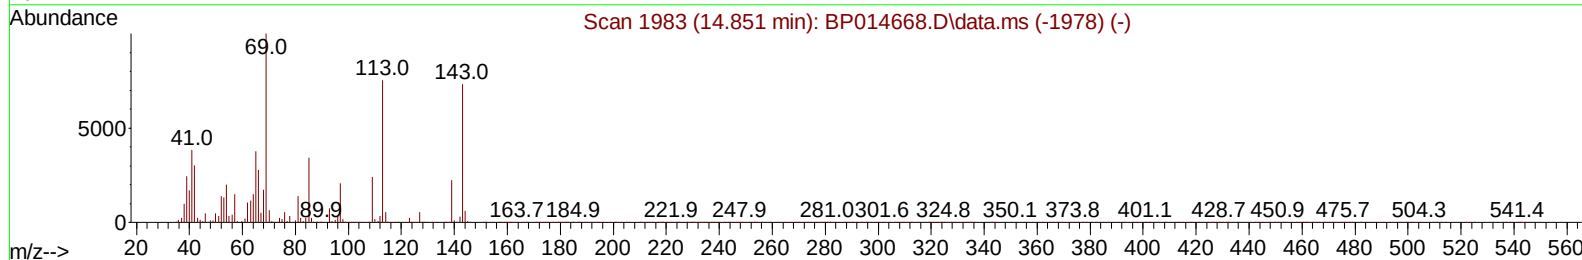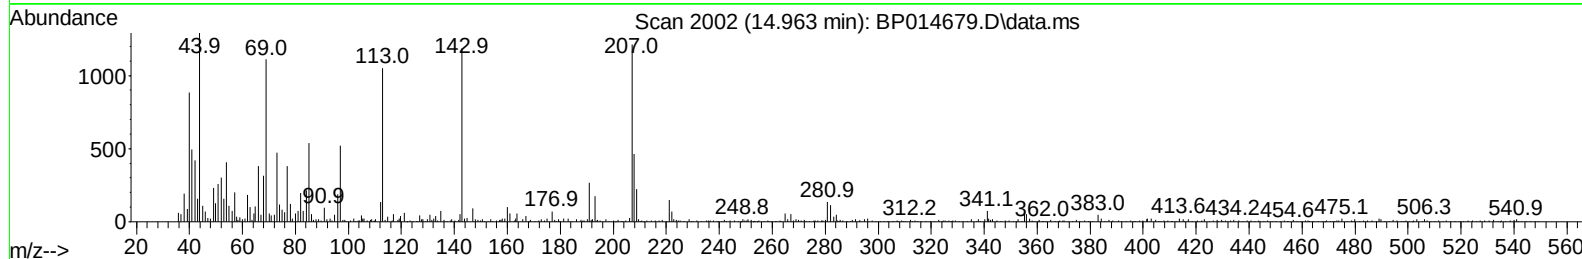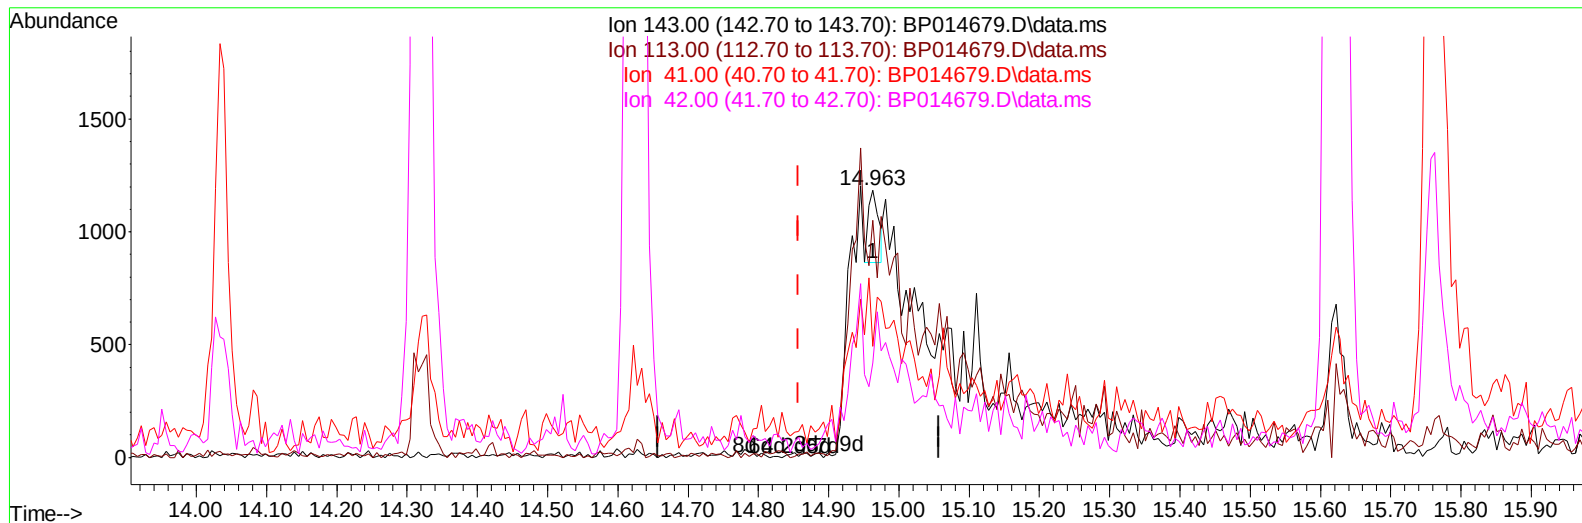

TIC: BP014679.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.963min (+ 0.106) 0.11 ng/ul

response 332

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	88.69
41.00	44.20	41.69
42.00	31.50	35.36




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014679.D
Acq On : 12 Apr 2023 18:23
Operator : CG/JU
Sample : 02251-20
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMD8

Manual IntegrationsAPPROVED

Quant Time: Apr 13 00:50:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/13/2023
Supervised By :Jagrut Upadhyay 04/13/2023

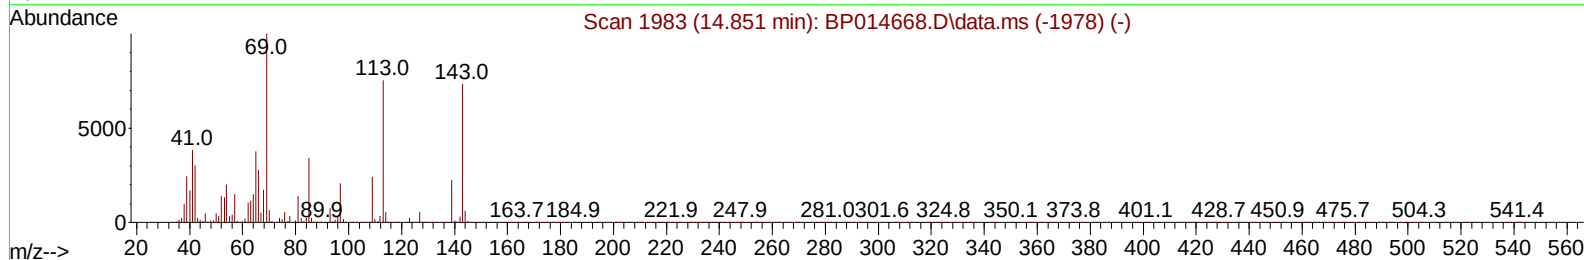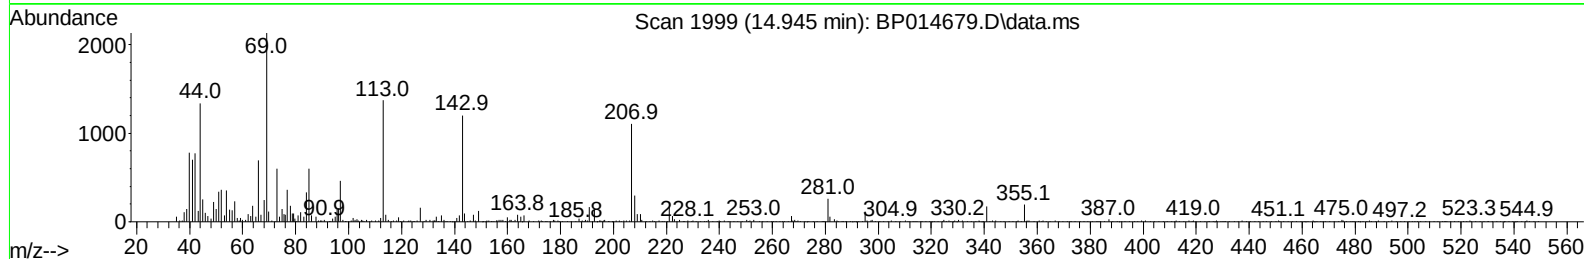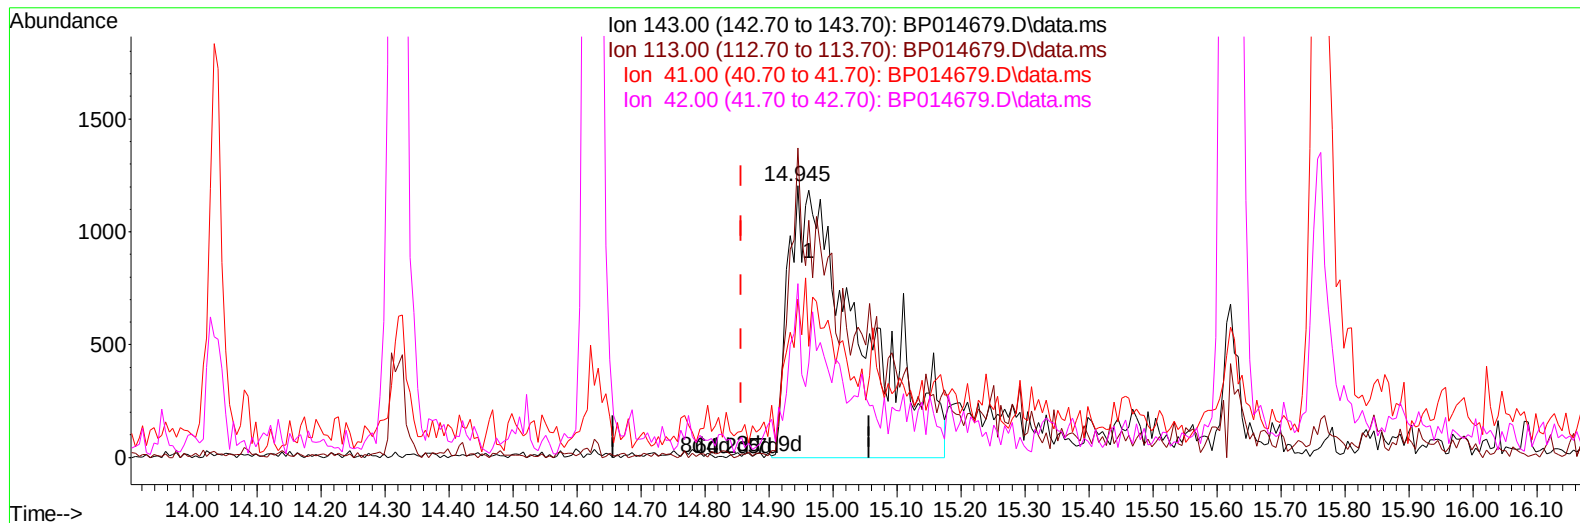

TIC: BP014679.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.945min (+ 0.088) 3.13 ng/ul m

response 9434

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	114.05
41.00	44.20	58.44#
42.00	31.50	64.09#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014679.D
 Acq On : 12 Apr 2023 18:23
 Operator : CG/JU
 Sample : 02251-20
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COMD8

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/13/2023
 Supervised By :Jagrut Upadhyay 04/13/2023

Quant Time: Apr 13 00:50:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 11 01:21:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.975	152	98748	20.000	ng/ul	0.00
20) Naphthalene-d8	10.793	136	418323	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.628	164	246259	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.392	188	479711	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	419014	20.000	ng/ul	0.00
88) Perylene-d12	23.980	264	516429	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	11899	4.673	ng/uL	0.00
4) Pyridine-d5	3.805	84	48687	7.461	ng/ul	0.01
7) Phenol-d5	7.152	99	57492	6.313	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.305	67	184648	31.601	ng/ul	0.00
11) 2-Chlorophenol-d4	7.505	132	152057	23.101	ng/ul	0.00
15) 4-Methylphenol-d8	8.699	113	103213	14.050	ng/ul	0.00
21) Nitrobenzene-d5	9.152	128	95694	28.337	ng/ul	0.00
24) 2-Nitrophenol-d4	9.875	143	101054	26.133	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.422	165	150180	21.325	ng/ul	0.00
31) 4-Chloroaniline-d4	10.946	131	175006	18.866	ng/ul	0.00
46) Dimethylphthalate-d6	14.040	166	555587	27.825	ng/ul	0.00
49) Acenaphthylene-d8	14.322	160	626899	28.295	ng/ul	0.00
54) 4-Nitrophenol-d4	14.945	143	9434m	3.127	ng/ul	0.09
60) Fluorene-d10	15.622	176	466842	28.037	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.763	200	66528	18.848	ng/ul	0.00
73) Anthracene-d10	17.492	188	693551	29.874	ng/ul	0.00
81) Pyrene-d10	19.722	212	773997	27.500	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.815	264	849975	30.978	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014679.D
Acq On : 12 Apr 2023 18:23
Operator : CG/JU
Sample : 02251-20
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMD8

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/13/2023
Supervised By :Jagrut Upadhyay 04/13/2023

Quant Time: Apr 13 00:50:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

