




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014683.D
 Acq On : 12 Apr 2023 20:41
 Operator : CG/JU
 Sample : PB152055BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK055

Manual IntegrationsAPPROVED

Quant Time: Apr 13 00:52:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 11 01:21:43 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/13/2023
 Supervised By :Jagrut Upadhyay 04/13/2023

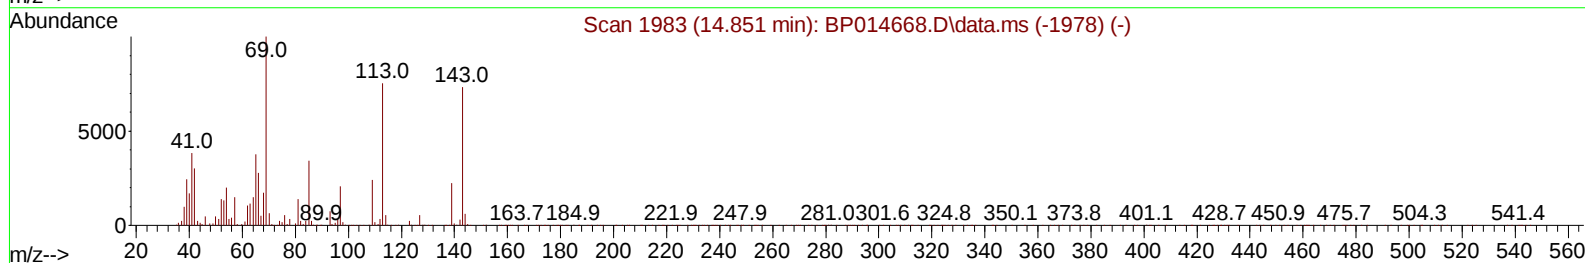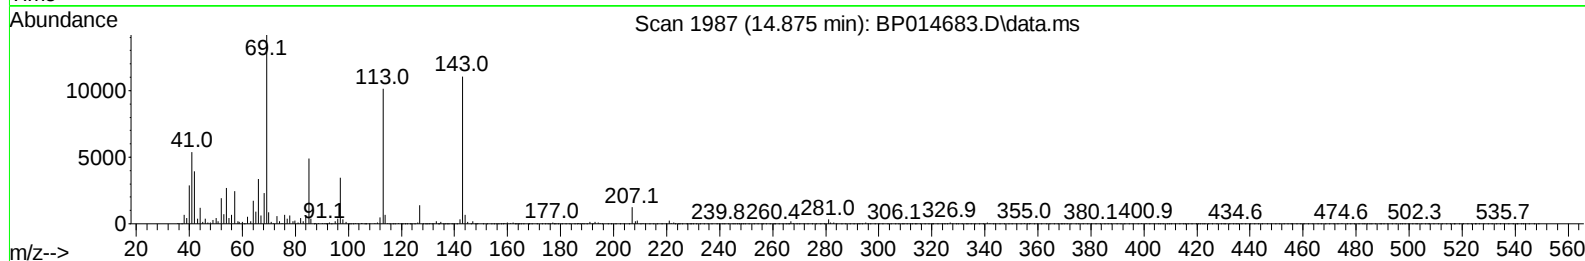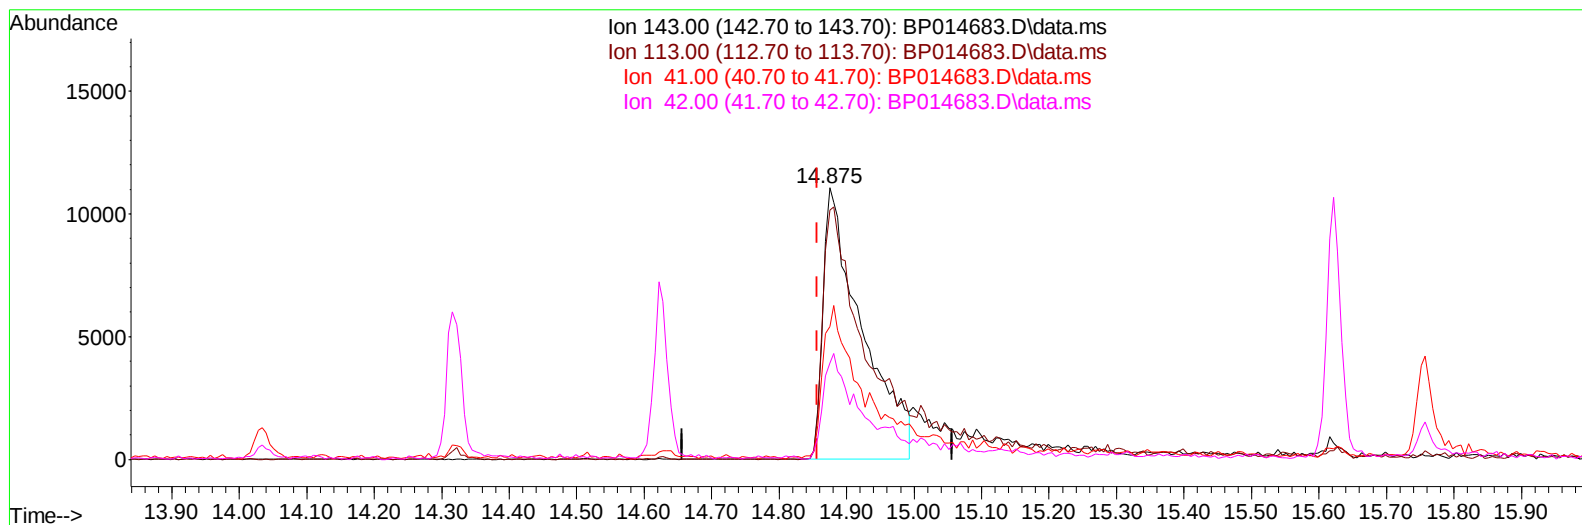

TIC: BP014683.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.875min (+ 0.018) 15.69 ng/u1

response 44037

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	91.84
41.00	44.20	48.85
42.00	31.50	35.61




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014683.D
Acq On : 12 Apr 2023 20:41
Operator : CG/JU
Sample : PB152055BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK055

Manual IntegrationsAPPROVED

Quant Time: Apr 13 00:52:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/13/2023
Supervised By :Jagrut Upadhyay 04/13/2023

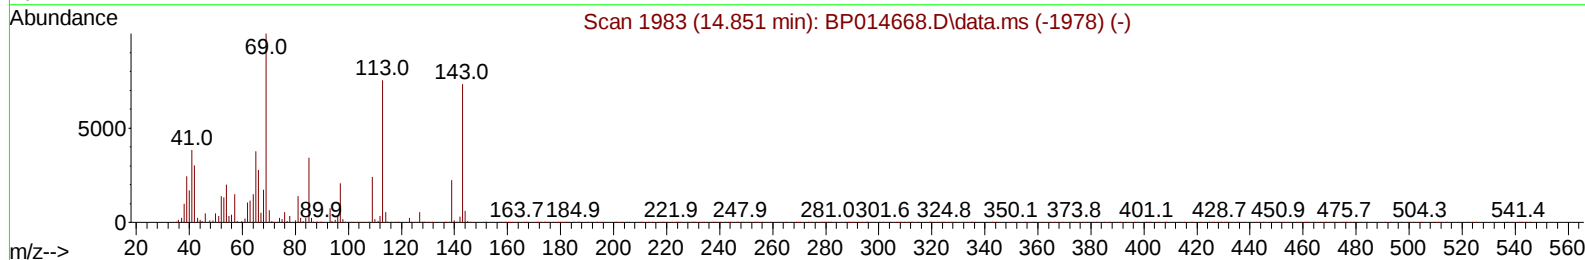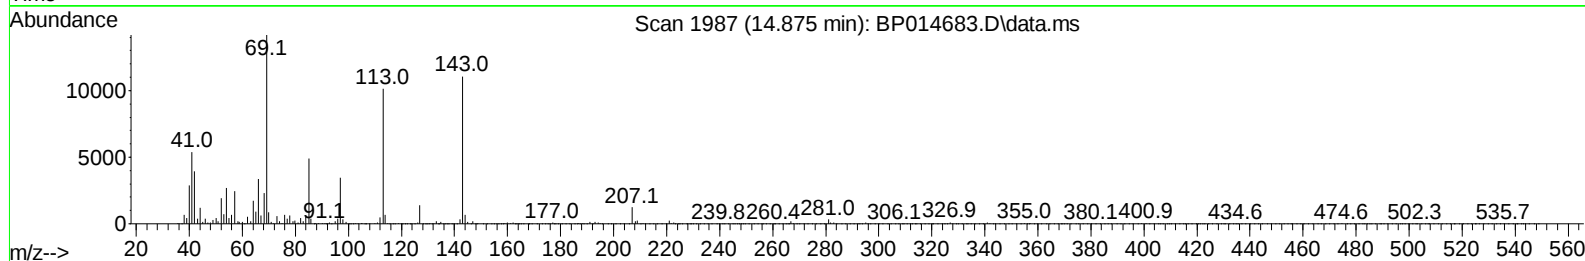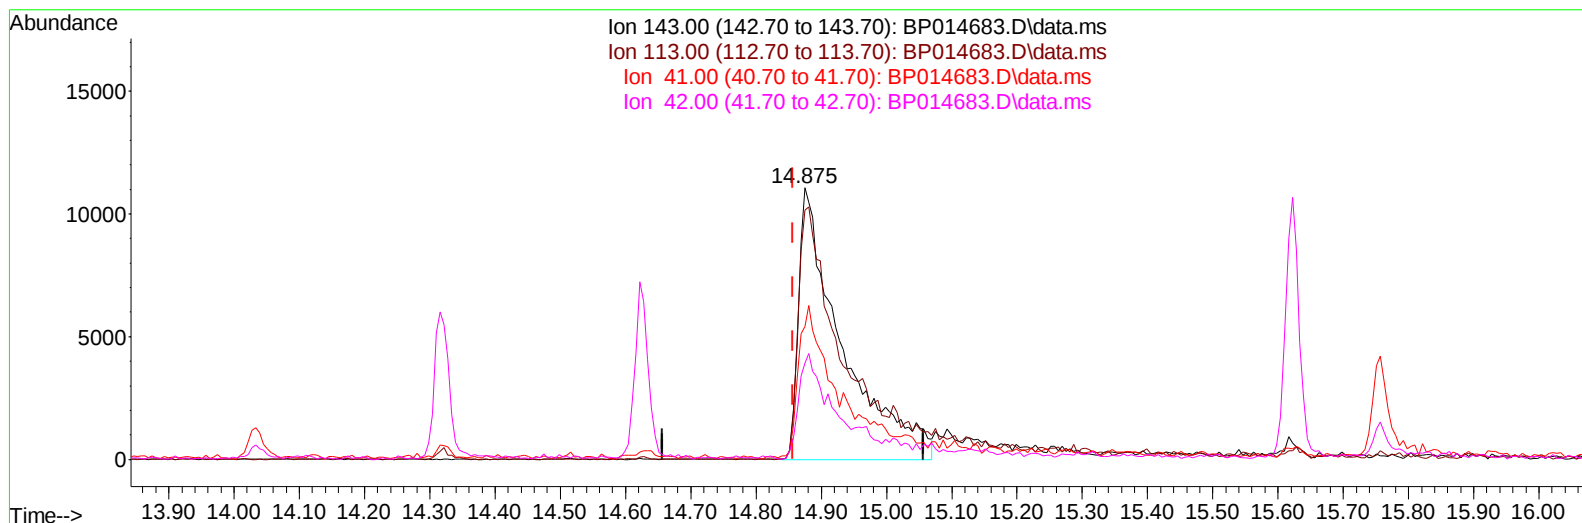

TIC: BP014683.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.875min (+ 0.018) 18.06 ng/ul m

response 50689

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	91.84
41.00	44.20	48.85
42.00	31.50	35.61

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014683.D
 Acq On : 12 Apr 2023 20:41
 Operator : CG/JU
 Sample : PB152055BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK055

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/13/2023
 Supervised By :Jagrut Upadhyay 04/13/2023

Quant Time: Apr 13 00:52:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 11 01:21:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.969	152	92890	20.000	ng/ul	0.00
20) Naphthalene-d8	10.793	136	388205	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.628	164	229141	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.386	188	482724	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	459700	20.000	ng/ul	0.00
88) Perylene-d12	23.980	264	543288	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.358	96	14607	6.098	ng/uL	0.00
4) Pyridine-d5	3.793	84	141901	23.117	ng/ul	0.00
7) Phenol-d5	7.140	99	216878	25.316	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.299	67	158521	28.840	ng/ul	0.00
11) 2-Chlorophenol-d4	7.505	132	170721	27.572	ng/ul	0.00
15) 4-Methylphenol-d8	8.693	113	175814	25.443	ng/ul	0.00
21) Nitrobenzene-d5	9.152	128	78804	25.146	ng/ul	0.00
24) 2-Nitrophenol-d4	9.875	143	87971	24.514	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.422	165	133912	20.490	ng/ul	0.00
31) 4-Chloroaniline-d4	10.946	131	184823	21.470	ng/ul	0.00
46) Dimethylphthalate-d6	14.034	166	476639	25.654	ng/ul	0.00
49) Acenaphthylene-d8	14.322	160	527877	25.606	ng/ul	0.00
54) 4-Nitrophenol-d4	14.875	143	50689m	18.059	ng/ul	0.02
60) Fluorene-d10	15.622	176	407103	26.275	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	65901	18.553	ng/ul	0.00
73) Anthracene-d10	17.486	188	626169	26.803	ng/ul	0.00
81) Pyrene-d10	19.722	212	746452	24.174	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.816	264	781268	27.067	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014683.D
Acq On : 12 Apr 2023 20:41
Operator : CG/JU
Sample : PB152055BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK055

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/13/2023
Supervised By :Jagrut Upadhyay 04/13/2023

Quant Time: Apr 13 00:52:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 11 01:21:43 2023
Response via : Initial Calibration

