




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014687.D
Acq On : 12 Apr 2023 23:32
Operator : CG/JU
Sample : 02250-11
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDY1

Manual IntegrationsAPPROVED

Quant Time: Apr 13 02:05:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 13 02:01:50 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/13/2023
Supervised By :Jagrut Upadhyay 04/13/2023

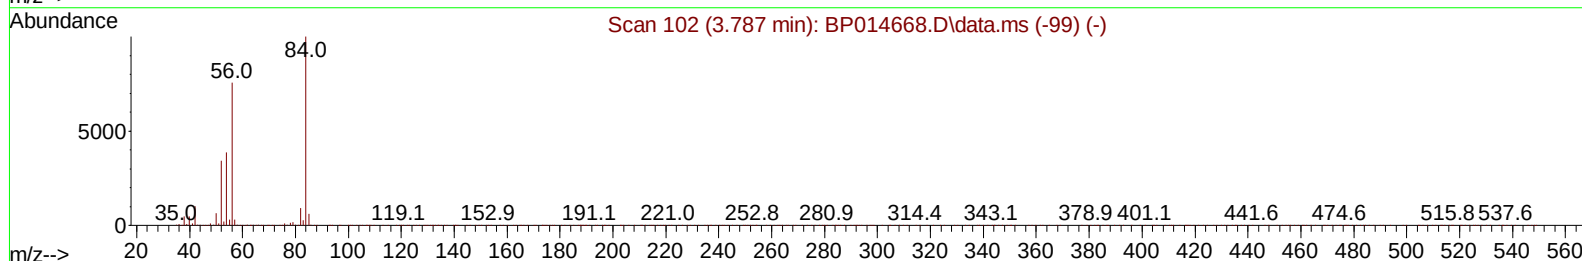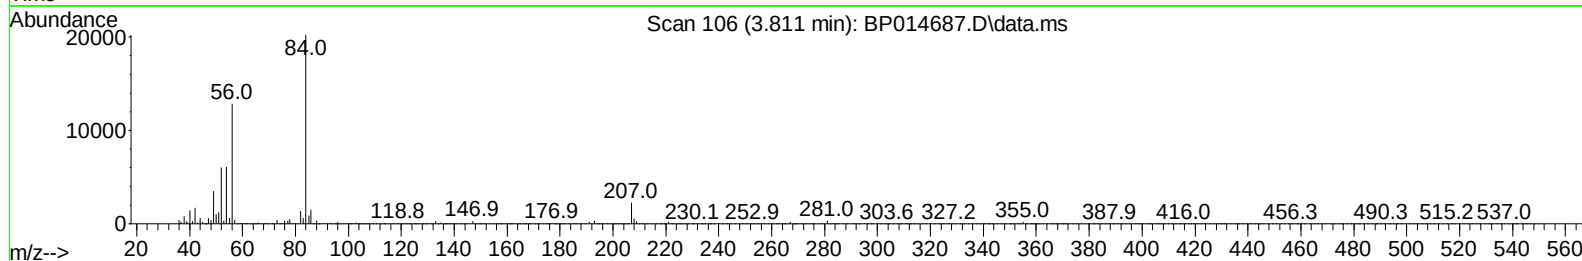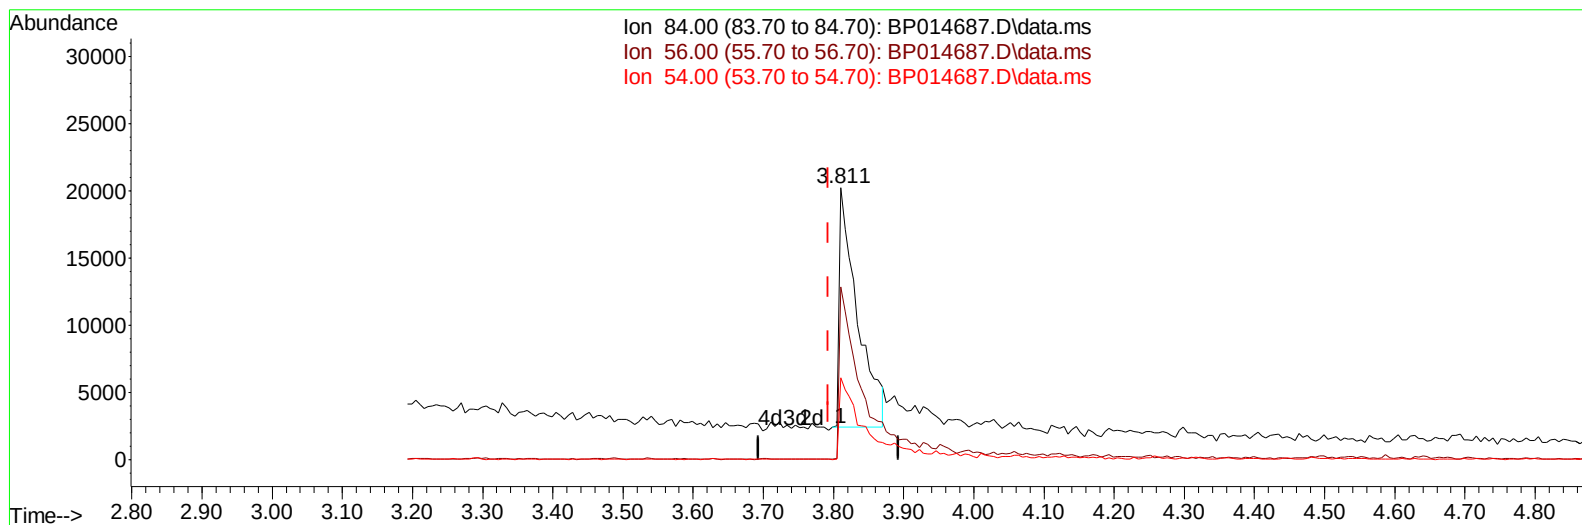

TIC: BP014687.D\data.ms

(4) Pyridine-d5 (S)

3.811min (+ 0.018) 5.27 ng/u1

response 31906

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.70	63.56
54.00	32.60	30.05
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014687.D
Acq On : 12 Apr 2023 23:32
Operator : CG/JU
Sample : 02250-11
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDY1

Manual IntegrationsAPPROVED

Quant Time: Apr 13 02:05:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 13 02:01:50 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/13/2023
Supervised By :Jagrut Upadhyay 04/13/2023

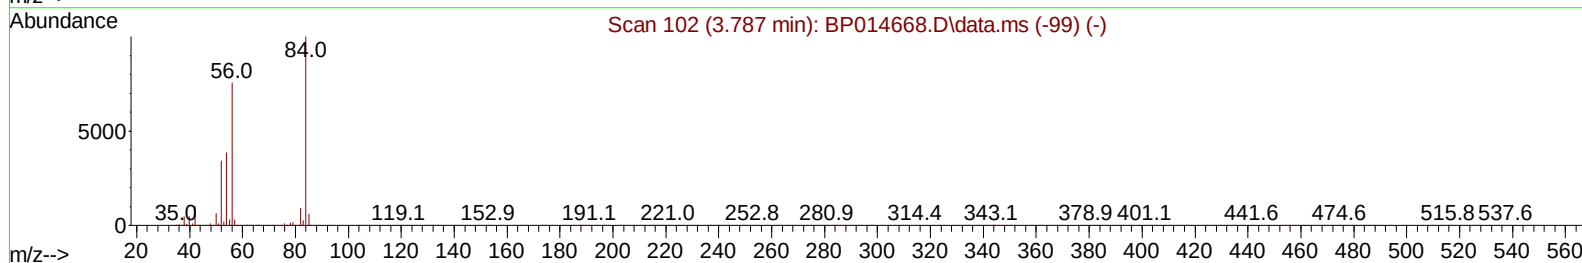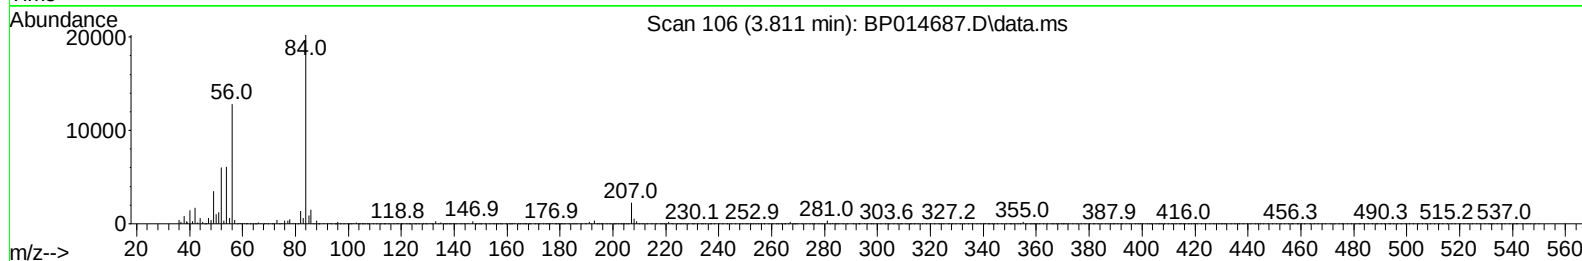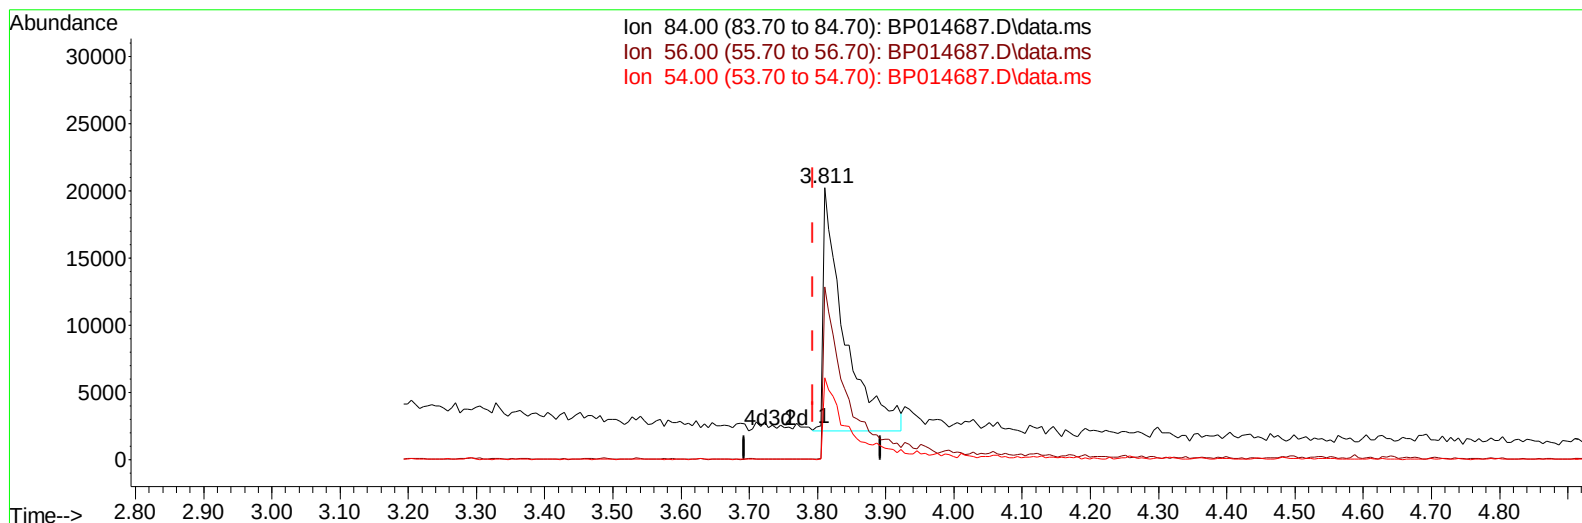

TIC: BP014687.D\data.ms

(4) Pyridine-d5 (S)

3.811min (+ 0.018) 6.46 ng/ul m

response 39098

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.70	63.56
54.00	32.60	30.05
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014687.D
Acq On : 12 Apr 2023 23:32
Operator : CG/JU
Sample : 02250-11
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDY1

Manual IntegrationsAPPROVED

Quant Time: Apr 13 02:05:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 13 02:01:50 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/13/2023
Supervised By :Jagrut Upadhyay 04/13/2023

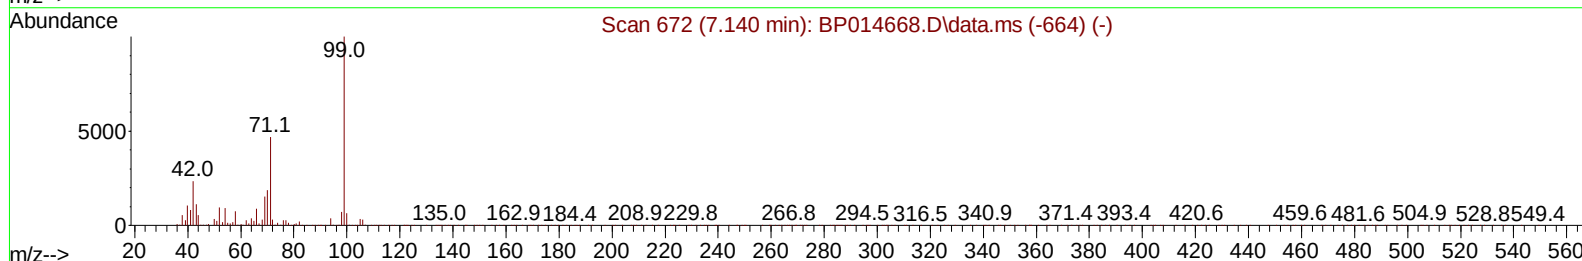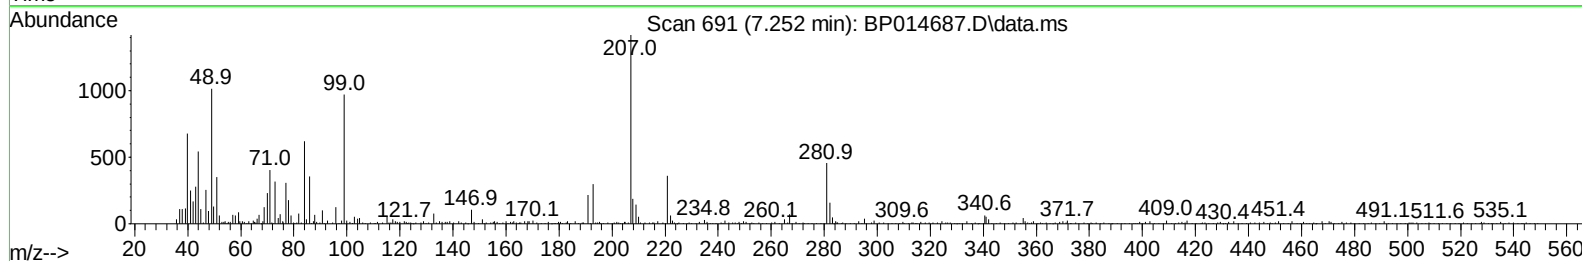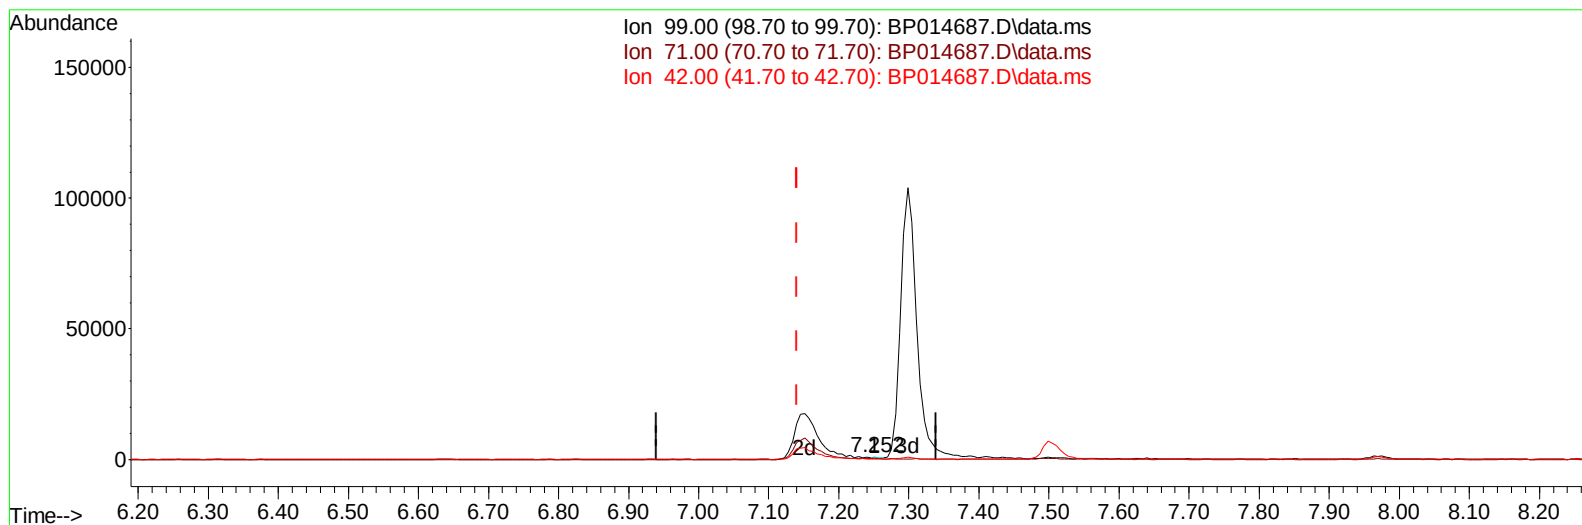

TIC: BP014687.D\data.ms

(7) Phenol-d5 (S)

7.252min (+ 0.112) 0.02 ng/u1

response 155

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	40.30	41.75
42.00	18.90	17.42
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014687.D
Acq On : 12 Apr 2023 23:32
Operator : CG/JU
Sample : 02250-11
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDY1

Manual IntegrationsAPPROVED

Quant Time: Apr 13 02:05:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 13 02:01:50 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/13/2023
Supervised By :Jagrut Upadhyay 04/13/2023

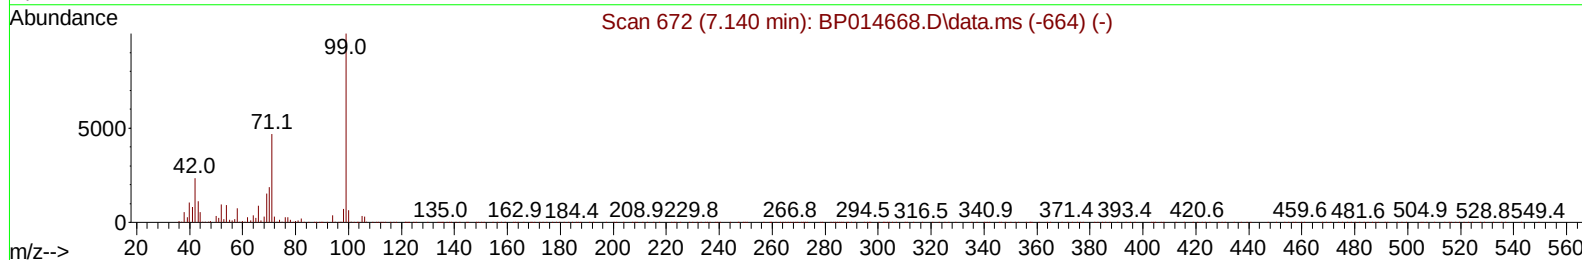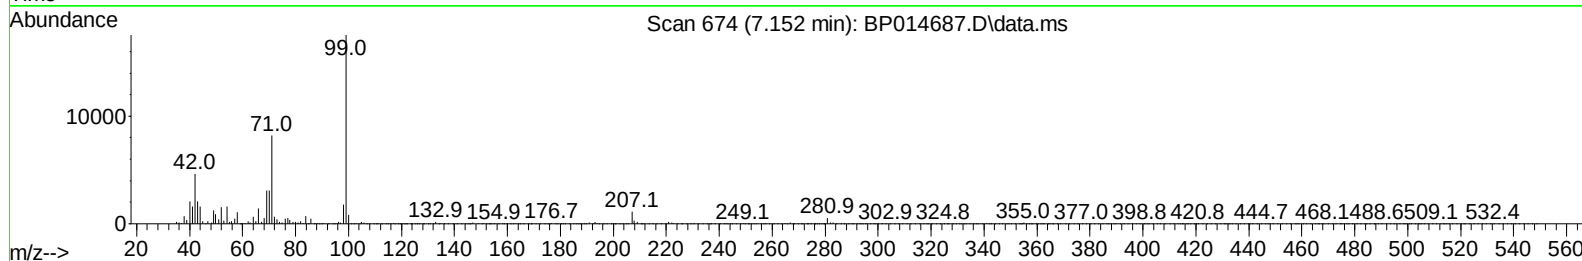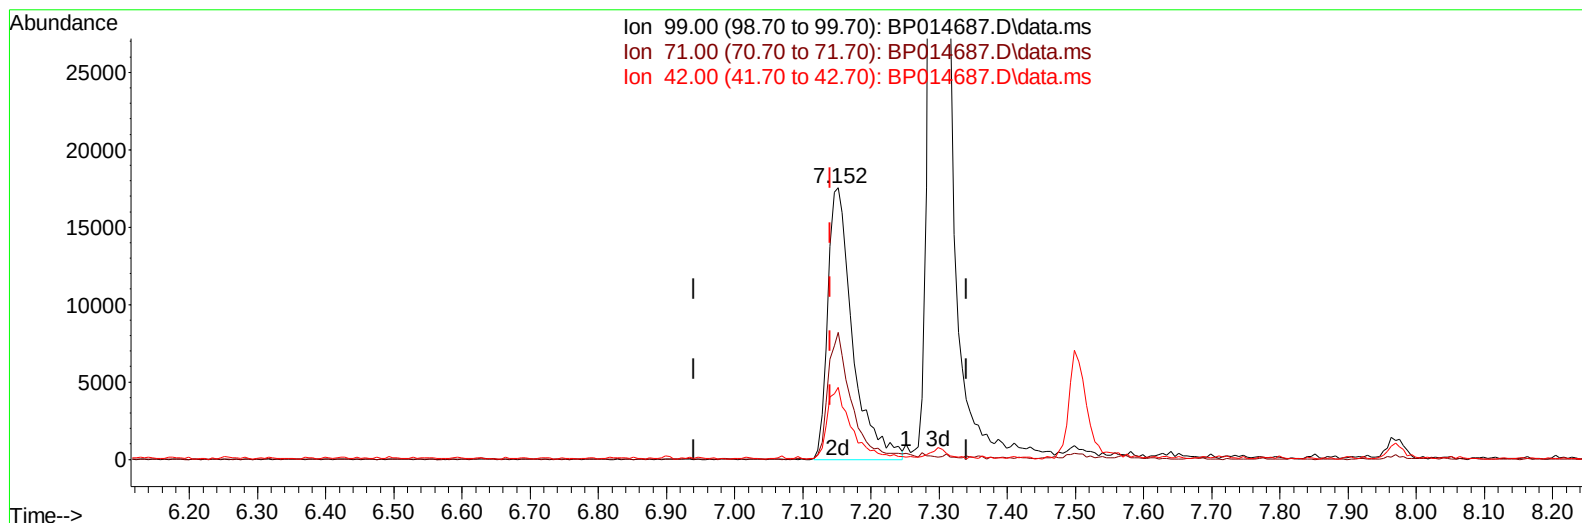

TIC: BP014687.D\data.ms

(7) Phenol-d5 (S)

7.152min (+ 0.012) 5.24 ng/ul m

response 44263

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	40.30	46.71
42.00	18.90	26.43#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014687.D
Acq On : 12 Apr 2023 23:32
Operator : CG/JU
Sample : 02250-11
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDY1

Manual IntegrationsAPPROVED

Quant Time: Apr 13 02:05:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 13 02:01:50 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/13/2023
Supervised By :Jagrut Upadhyay 04/13/2023

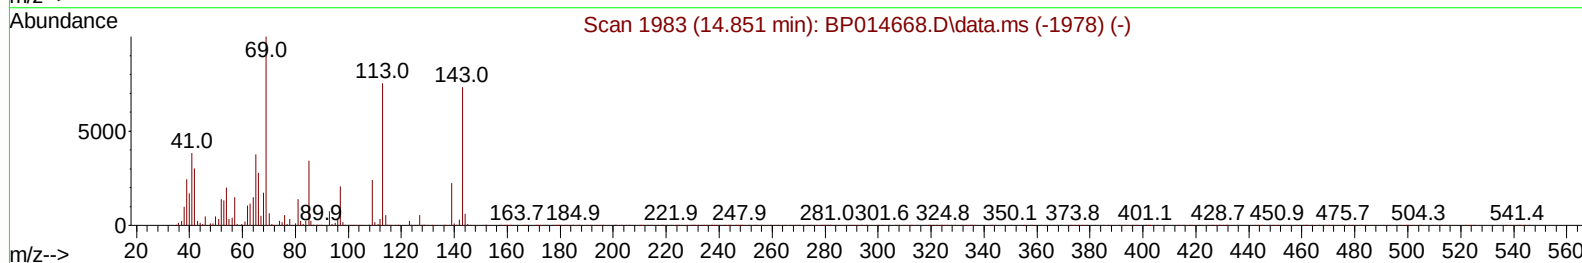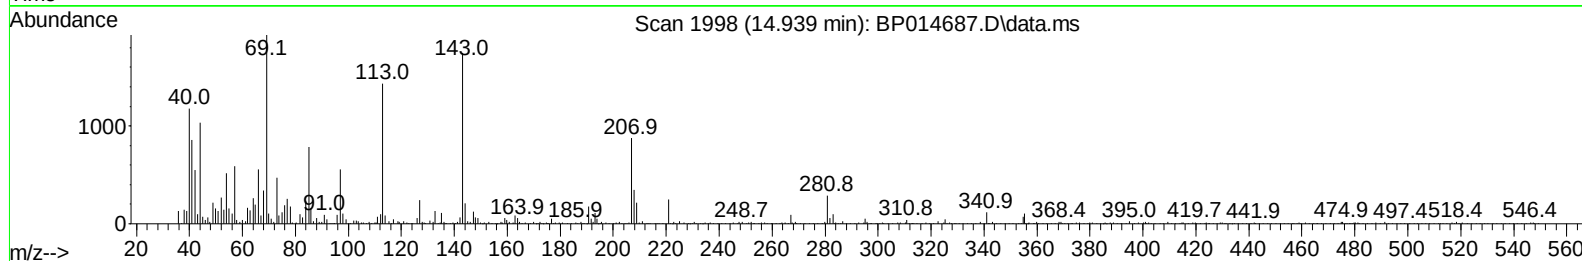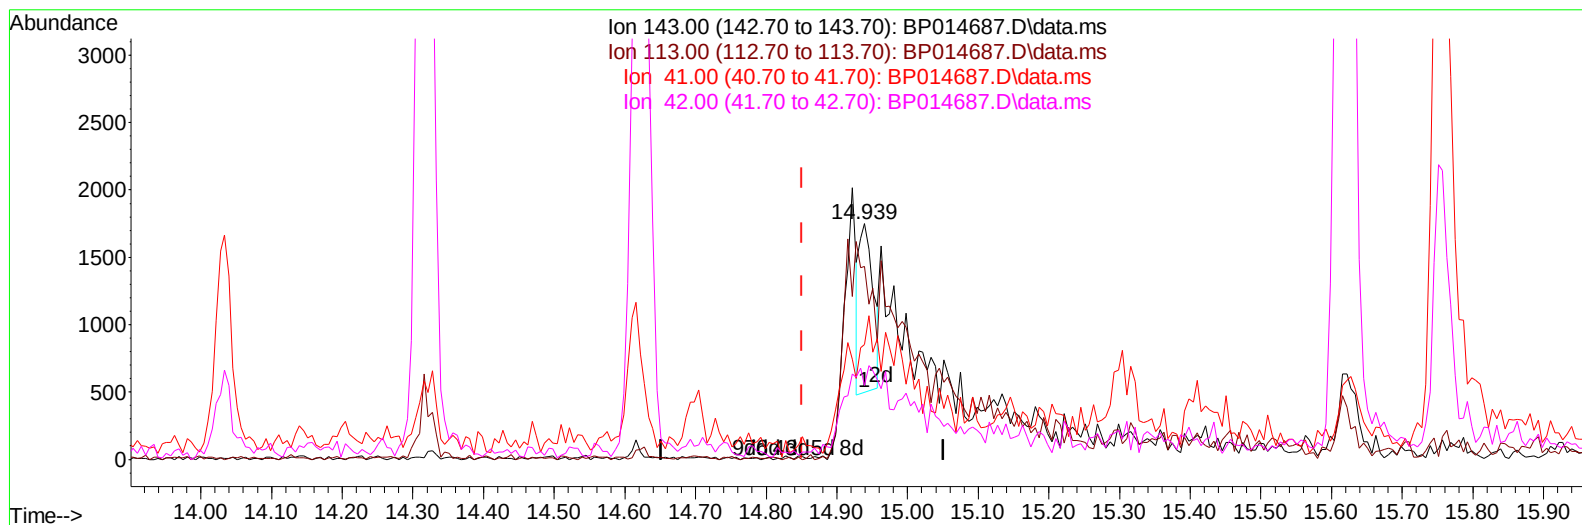

TIC: BP014687.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.939min (+ 0.088) 0.64 ng/ul

response 1696

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	81.83
41.00	44.20	48.86
42.00	31.50	31.49




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014687.D
Acq On : 12 Apr 2023 23:32
Operator : CG/JU
Sample : 02250-11
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDY1

Manual IntegrationsAPPROVED

Quant Time: Apr 13 02:05:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 13 02:01:50 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/13/2023
Supervised By :Jagrut Upadhyay 04/13/2023

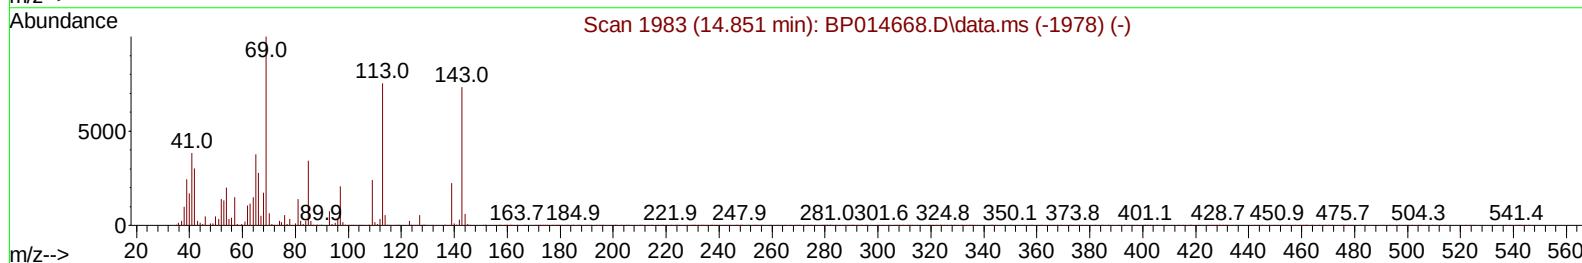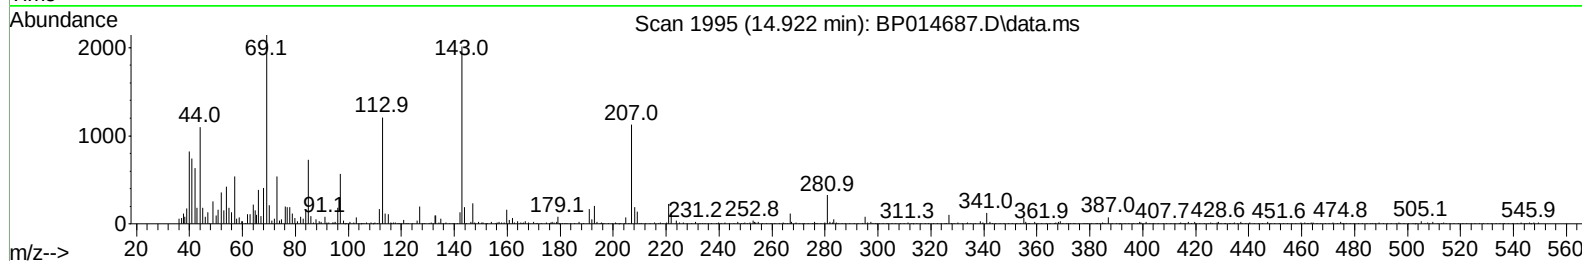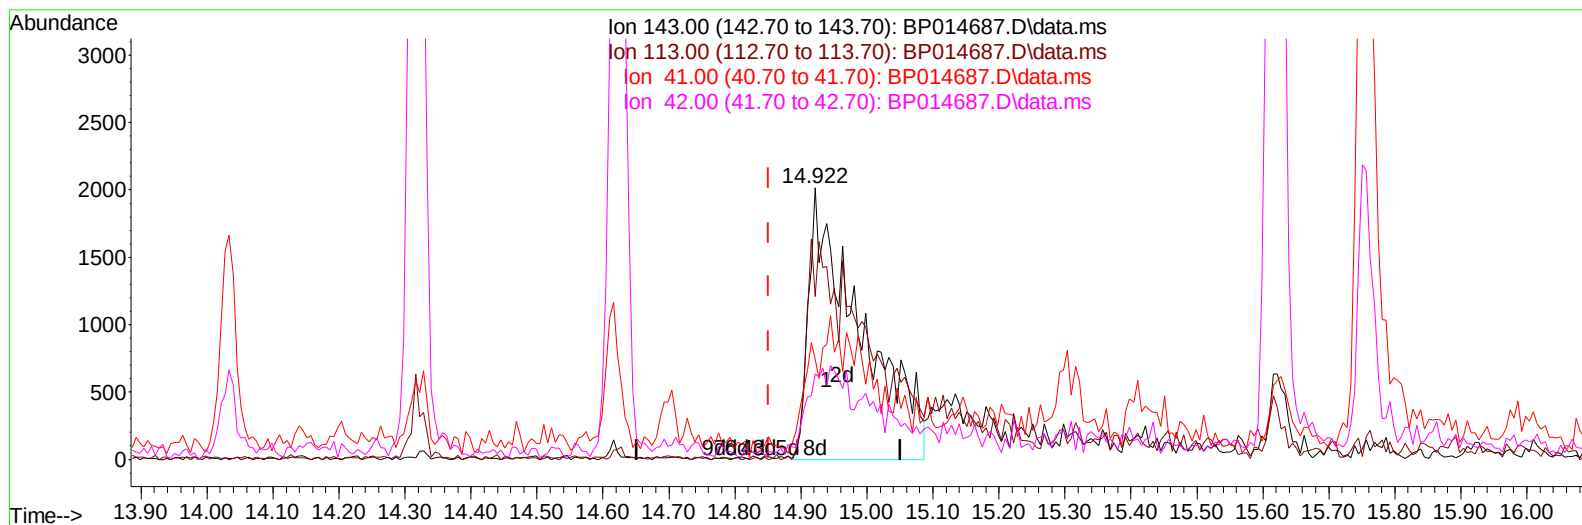

TIC: BP014687.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.922min (+ 0.071) 4.10 ng/ul m

response 10898

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	59.95#
41.00	44.20	36.82
42.00	31.50	31.41

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014687.D
 Acq On : 12 Apr 2023 23:32
 Operator : CG/JU
 Sample : 02250-11
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHDY1

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/13/2023
 Supervised By :Jagrut Upadhyay 04/13/2023

Quant Time: Apr 13 02:05:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 13 02:01:50 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.969	152	91648	20.000	ng/ul	0.00
20) Naphthalene-d8	10.787	136	358033	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.622	164	216978	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.386	188	507965	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	515519	20.000	ng/ul	0.00
88) Perylene-d12	23.974	264	610867	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.358	96	12017	5.085	ng/uL	0.00
4) Pyridine-d5	3.811	84	39098m	6.456	ng/ul	0.02
7) Phenol-d5	7.152	99	44263m	5.237	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.299	67	157723	29.084	ng/ul	0.00
11) 2-Chlorophenol-d4	7.504	132	130508	21.363	ng/ul	0.00
15) 4-Methylphenol-d8	8.693	113	84467	12.389	ng/ul	0.00
21) Nitrobenzene-d5	9.151	128	78914	27.303	ng/ul	0.00
24) 2-Nitrophenol-d4	9.875	143	86872	26.248	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.422	165	137563	22.823	ng/ul	0.00
31) 4-Chloroaniline-d4	10.945	131	175219	22.069	ng/ul	0.00
46) Dimethylphthalate-d6	14.034	166	554604	31.524	ng/ul	0.00
49) Acenaphthylene-d8	14.322	160	578664	29.643	ng/ul	0.00
54) 4-Nitrophenol-d4	14.922	143	10898m	4.100	ng/ul	0.07
60) Fluorene-d10	15.622	176	475581	32.416	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	91915	24.591	ng/ul	0.00
73) Anthracene-d10	17.486	188	845925	34.411	ng/ul	0.00
81) Pyrene-d10	19.721	212	1063485	30.712	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.815	264	1145688	35.301	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014687.D
Acq On : 12 Apr 2023 23:32
Operator : CG/JU
Sample : 02250-11
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDY1

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/13/2023
Supervised By :Jagrut Upadhyay 04/13/2023

Quant Time: Apr 13 02:05:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 13 02:01:50 2023
Response via : Initial Calibration

