




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014690.D
 Acq On : 13 Apr 2023 01:15
 Operator : CG/JU
 Sample : 02250-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHDY5

Manual IntegrationsAPPROVED

Quant Time: Apr 13 02:06:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 13 02:01:50 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/13/2023
 Supervised By :Jagrut Upadhyay 04/13/2023

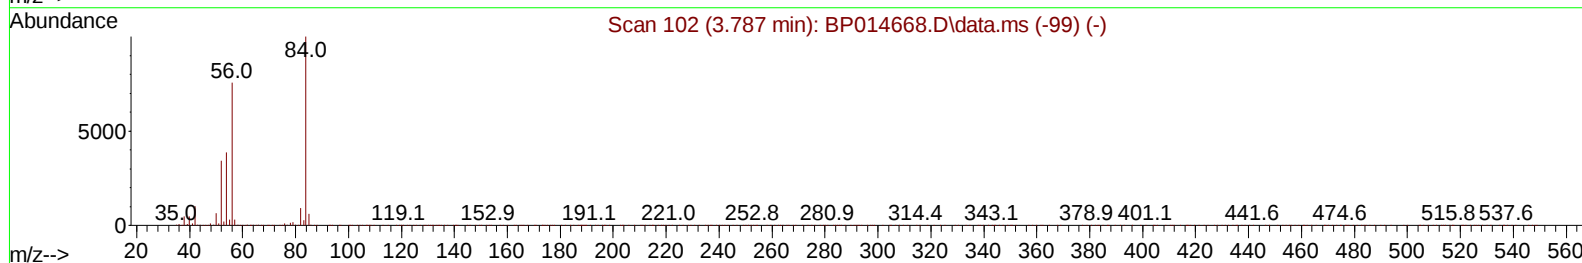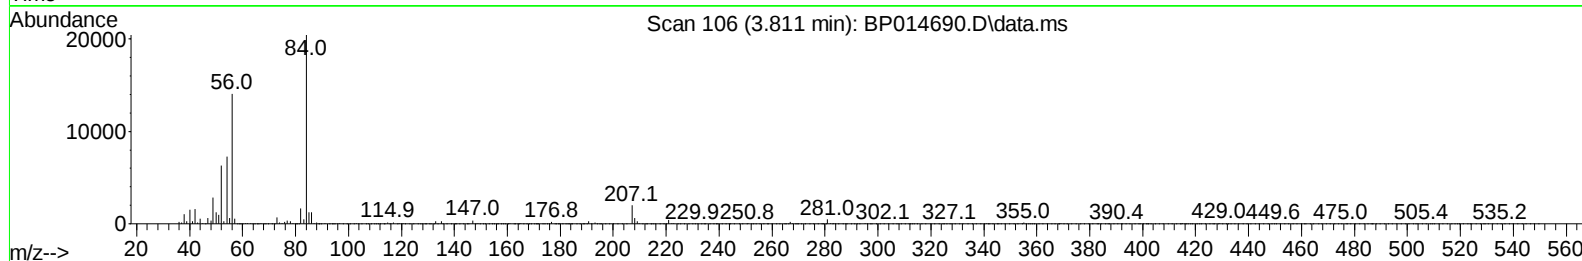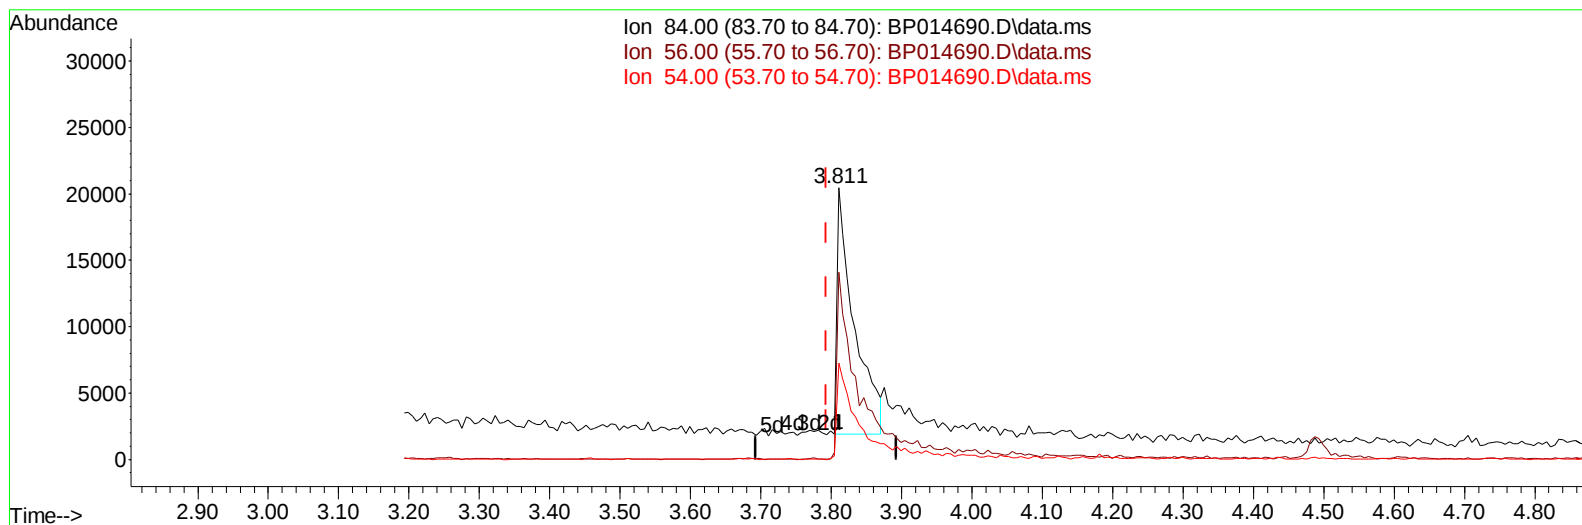

TIC: BP014690.D\data.ms

(4) Pyridine-d5 (S)

3.811min (+ 0.018) 4.87 ng/u1

response 31160

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.70	68.94
54.00	32.60	35.51
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014690.D
 Acq On : 13 Apr 2023 01:15
 Operator : CG/JU
 Sample : 02250-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHDY5

Manual IntegrationsAPPROVED

Quant Time: Apr 13 02:06:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 13 02:01:50 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/13/2023
 Supervised By :Jagrut Upadhyay 04/13/2023

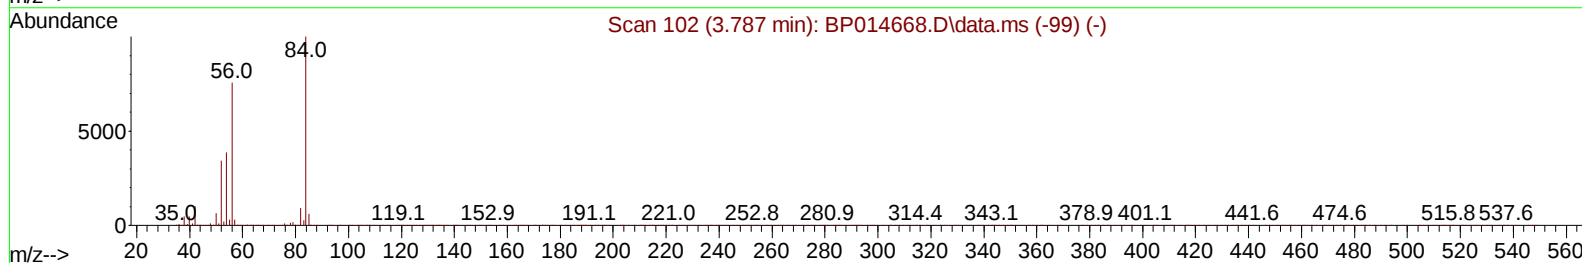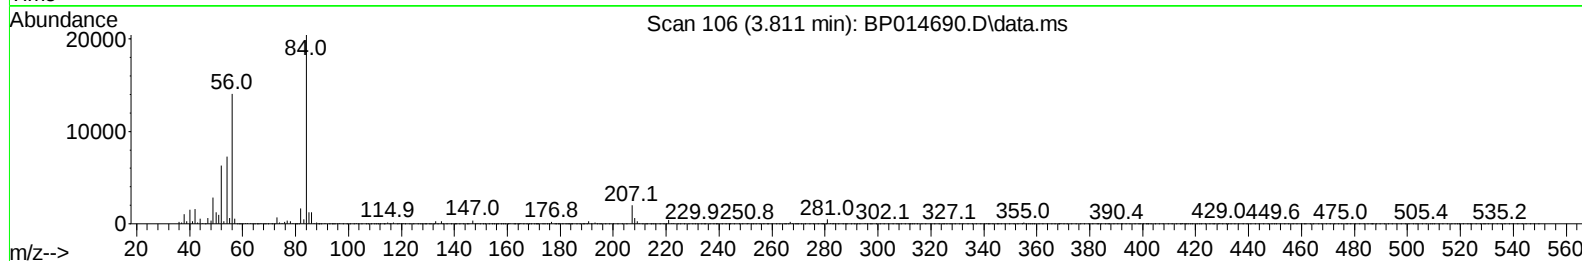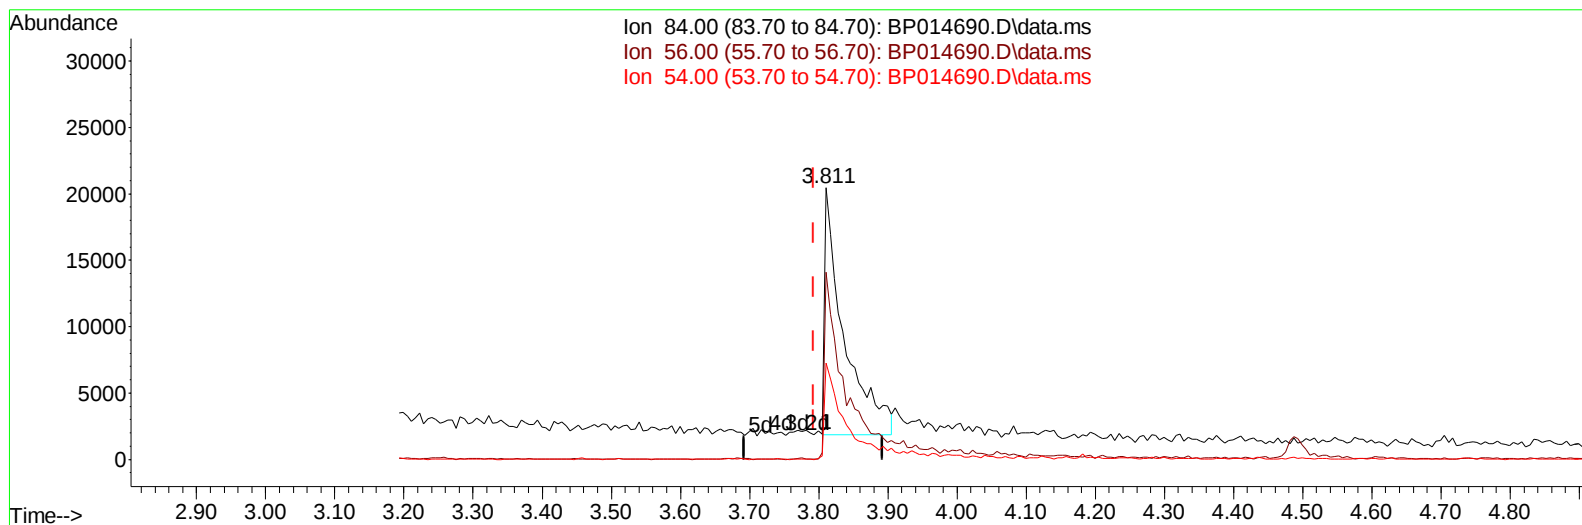

TIC: BP014690.D\data.ms

(4) Pyridine-d5 (S)

3.811min (+ 0.018) 5.67 ng/ul m

response 36270

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.70	68.94
54.00	32.60	35.51
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014690.D
Acq On : 13 Apr 2023 01:15
Operator : CG/JU
Sample : 02250-15
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDY5

Manual IntegrationsAPPROVED

Quant Time: Apr 13 02:06:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 13 02:01:50 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/13/2023
Supervised By :Jagrut Upadhyay 04/13/2023

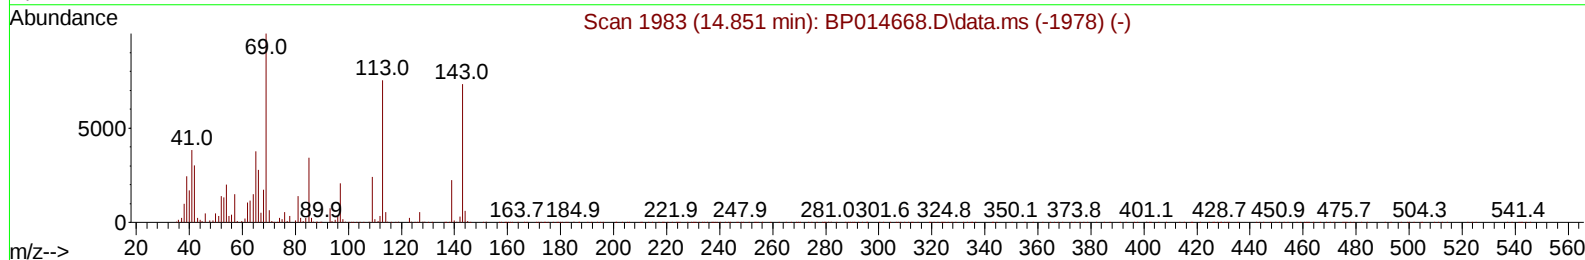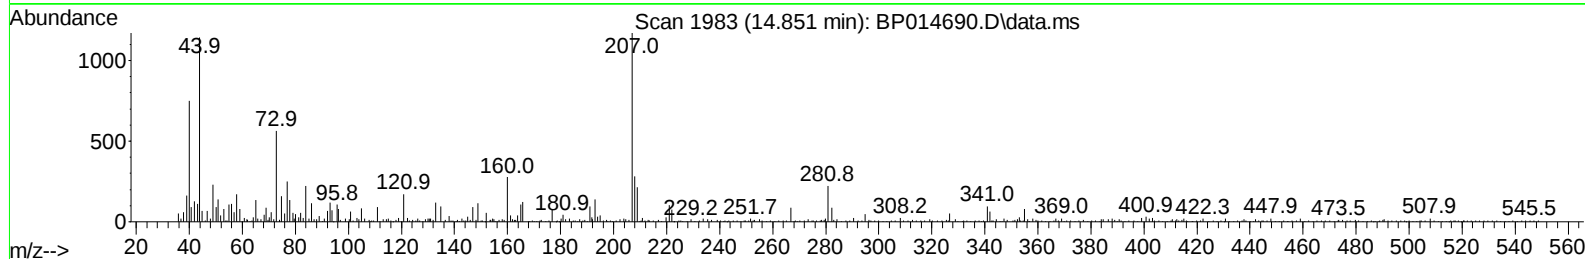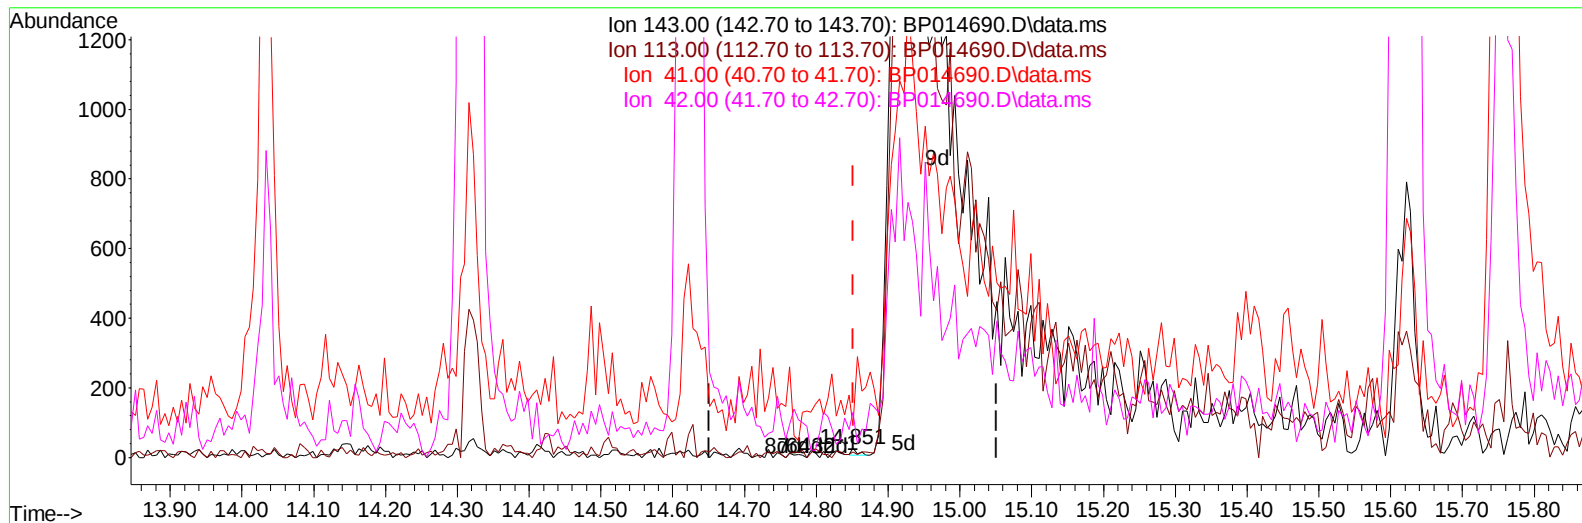

TIC: BP014690.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.851min (+ 0.000) 0.00 ng/u1

response 11

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	57.69#
41.00	44.20	350.00#
42.00	31.50	496.15#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014690.D
Acq On : 13 Apr 2023 01:15
Operator : CG/JU
Sample : 02250-15
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDY5

Manual IntegrationsAPPROVED

Quant Time: Apr 13 02:06:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 13 02:01:50 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/13/2023
Supervised By :Jagrut Upadhyay 04/13/2023

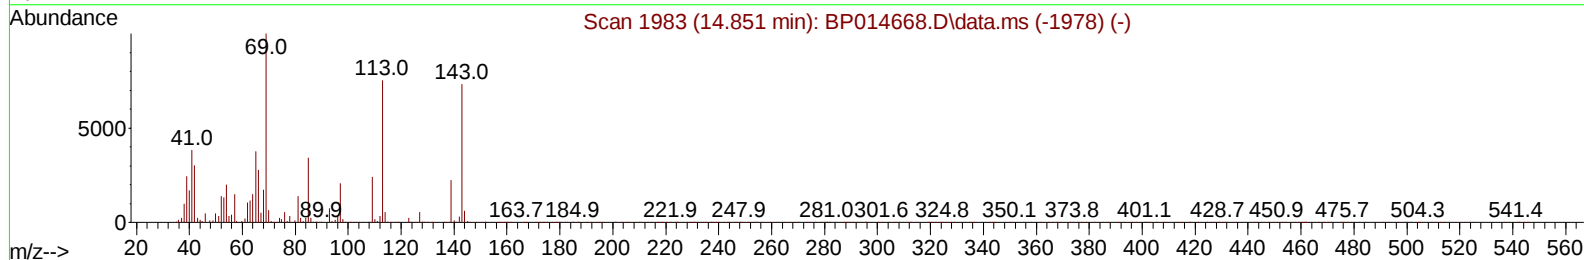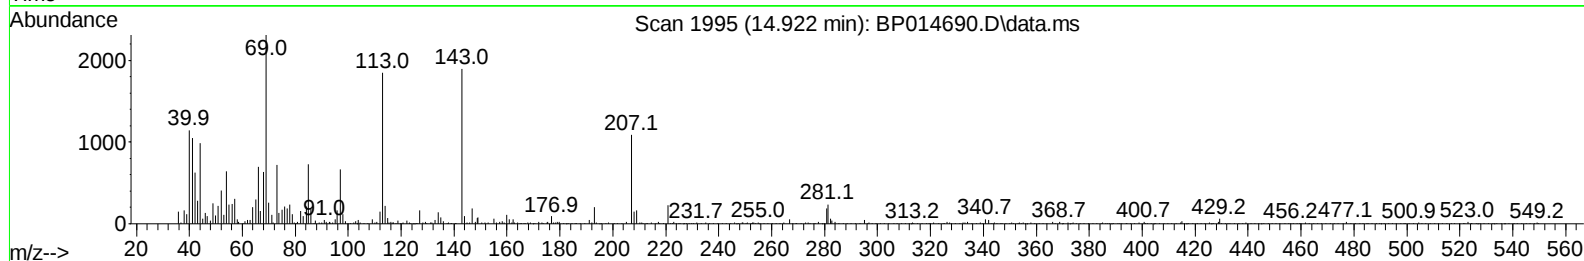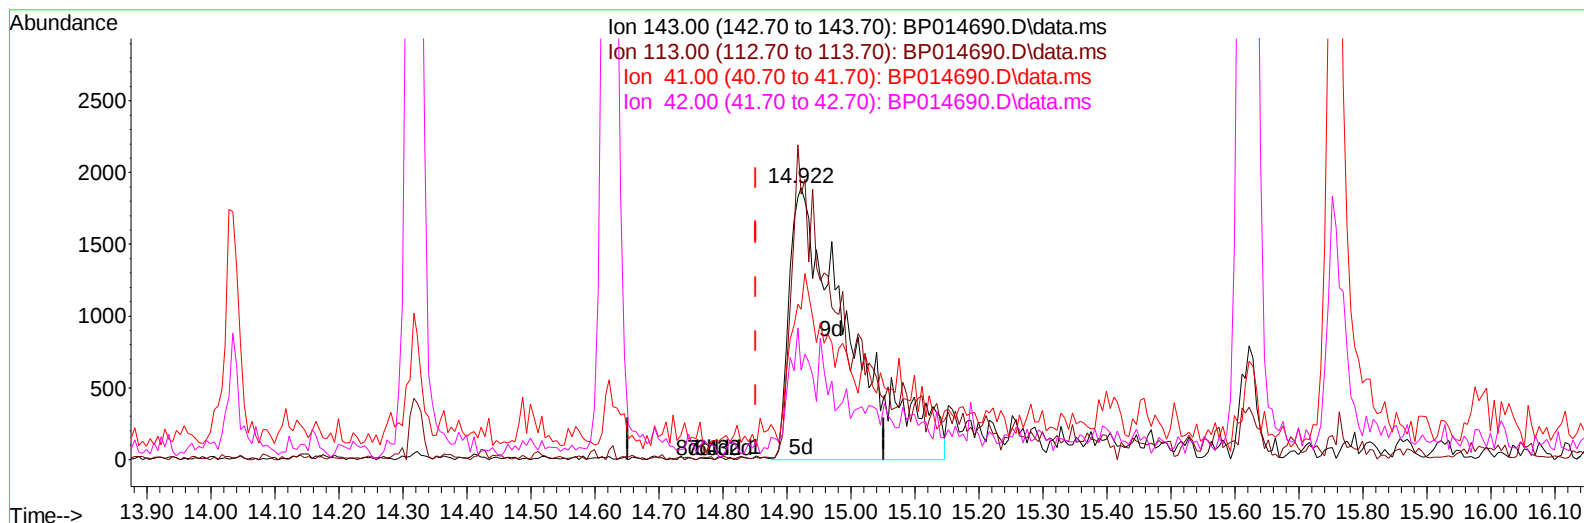

TIC: BP014690.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.922min (+ 0.071) 4.22 ng/ul m

response 12503

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	97.83
41.00	44.20	55.26#
42.00	31.50	32.91

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014690.D
 Acq On : 13 Apr 2023 01:15
 Operator : CG/JU
 Sample : 02250-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHDY5

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/13/2023
 Supervised By :Jagrut Upadhyay 04/13/2023

Quant Time: Apr 13 02:06:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 13 02:01:50 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.969	152	96757	20.000	ng/ul	0.00
20) Naphthalene-d8	10.793	136	405500	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.622	164	241901	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.387	188	480746	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	449168	20.000	ng/ul	0.00
88) Perylene-d12	23.974	264	533662	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.358	96	12378	4.961	ng/uL	0.00
4) Pyridine-d5	3.811	84	36270m	5.673	ng/ul	0.02
7) Phenol-d5	7.146	99	50665	5.678	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.299	67	180855	31.589	ng/ul	0.00
11) 2-Chlorophenol-d4	7.505	132	149900	23.242	ng/ul	0.00
15) 4-Methylphenol-d8	8.693	113	96952	13.469	ng/ul	0.00
21) Nitrobenzene-d5	9.152	128	94897	28.989	ng/ul	0.00
24) 2-Nitrophenol-d4	9.875	143	106273	28.351	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.422	165	168193	24.638	ng/ul	0.00
31) 4-Chloroaniline-d4	10.946	131	159592	17.748	ng/ul	0.00
46) Dimethylphthalate-d6	14.034	166	623408	31.784	ng/ul	0.00
49) Acenaphthylene-d8	14.316	160	690005	31.705	ng/ul	0.00
54) 4-Nitrophenol-d4	14.922	143	12503m	4.220	ng/ul	0.07
60) Fluorene-d10	15.622	176	519241	31.745	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	83417	23.581	ng/ul	0.00
73) Anthracene-d10	17.486	188	805795	34.634	ng/ul	0.00
81) Pyrene-d10	19.722	212	936104	31.027	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.816	264	999706	35.259	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014690.D
Acq On : 13 Apr 2023 01:15
Operator : CG/JU
Sample : 02250-15
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDY5

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/13/2023
Supervised By :Jagrut Upadhyay 04/13/2023

Quant Time: Apr 13 02:06:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 13 02:01:50 2023
Response via : Initial Calibration

