




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014691.D
Acq On : 13 Apr 2023 01:49
Operator : CG/JU
Sample : 02250-16
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDY6

Manual IntegrationsAPPROVED

Quant Time: Apr 13 02:34:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 13 02:01:50 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/13/2023
Supervised By :Jagrut Upadhyay 04/13/2023

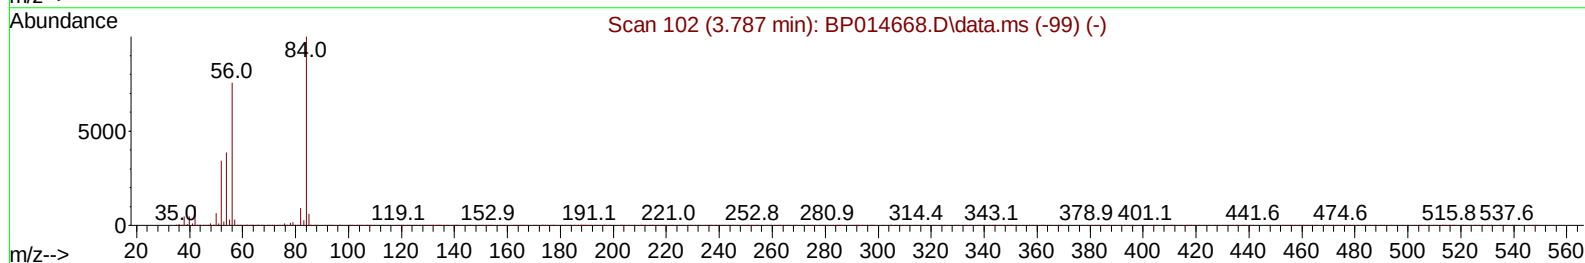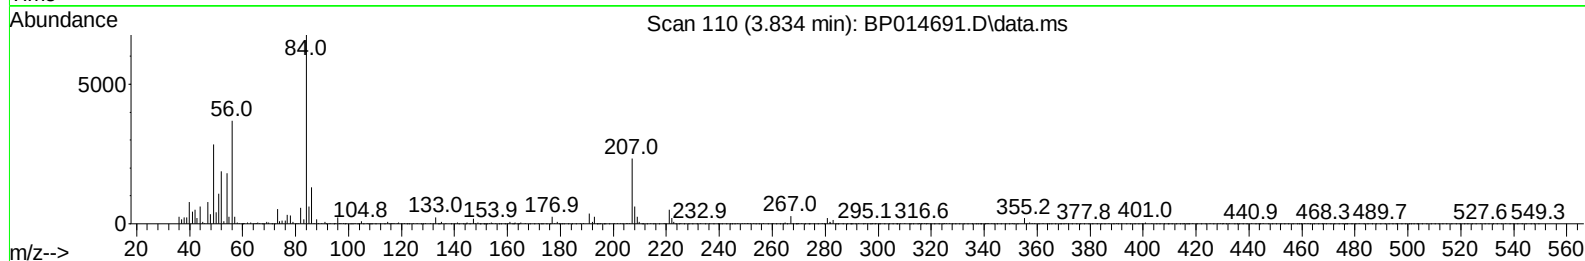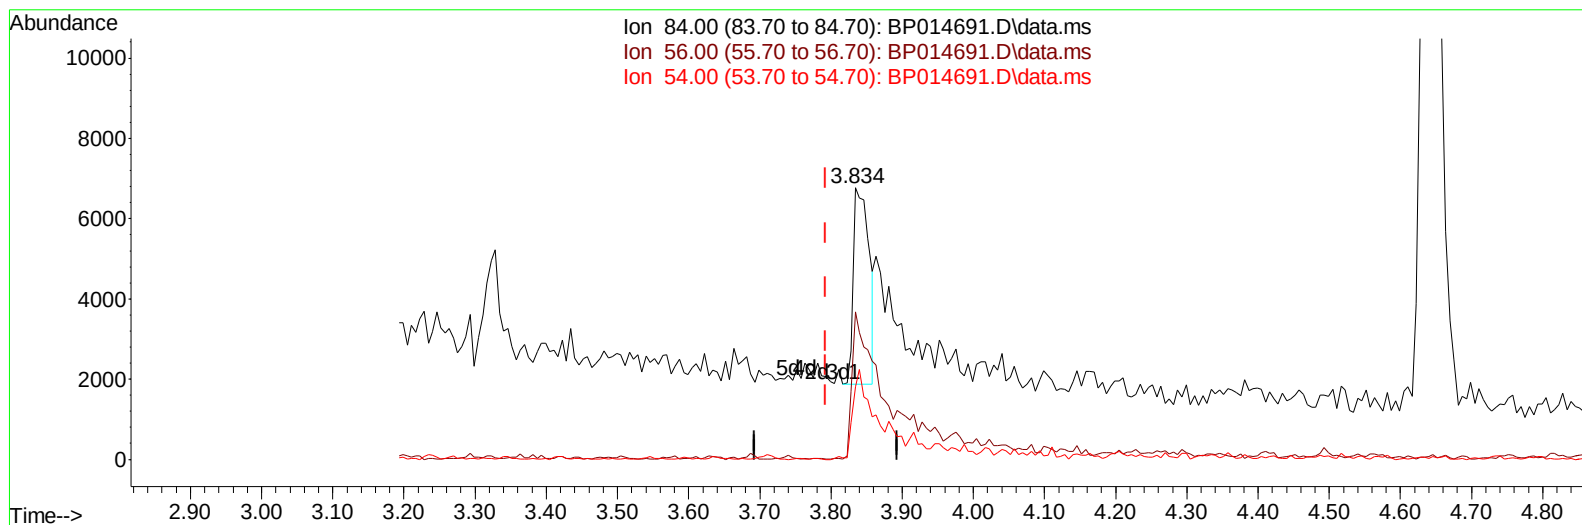

TIC: BP014691.D\data.ms

(4) Pyridine-d5 (S)

3.834min (+ 0.041) 1.20 ng/u1

response 7559

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.70	54.46
54.00	32.60	26.86
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014691.D
Acq On : 13 Apr 2023 01:49
Operator : CG/JU
Sample : 02250-16
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDY6

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/13/2023
Supervised By :Jagrut Upadhyay 04/13/2023

Quant Time: Apr 13 02:34:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 13 02:01:50 2023
Response via : Initial Calibration

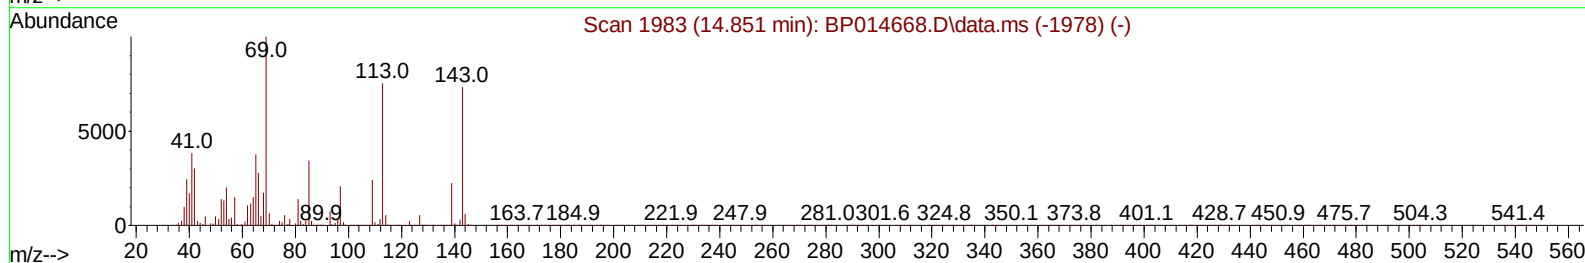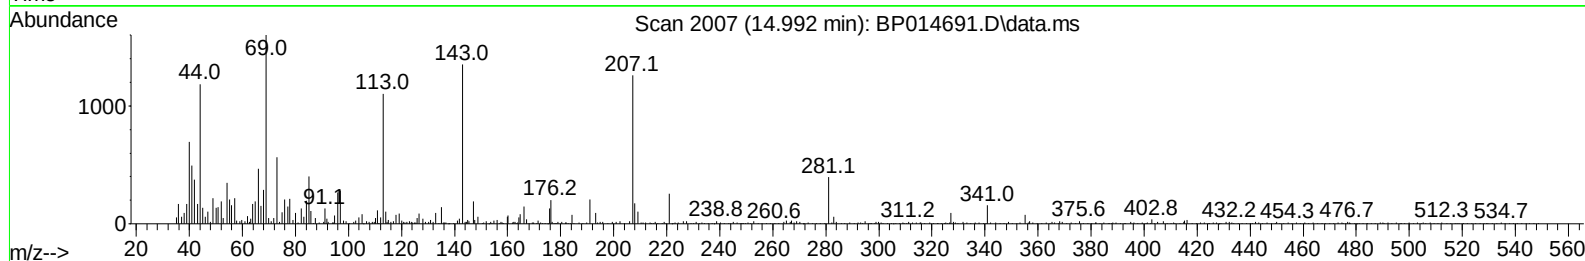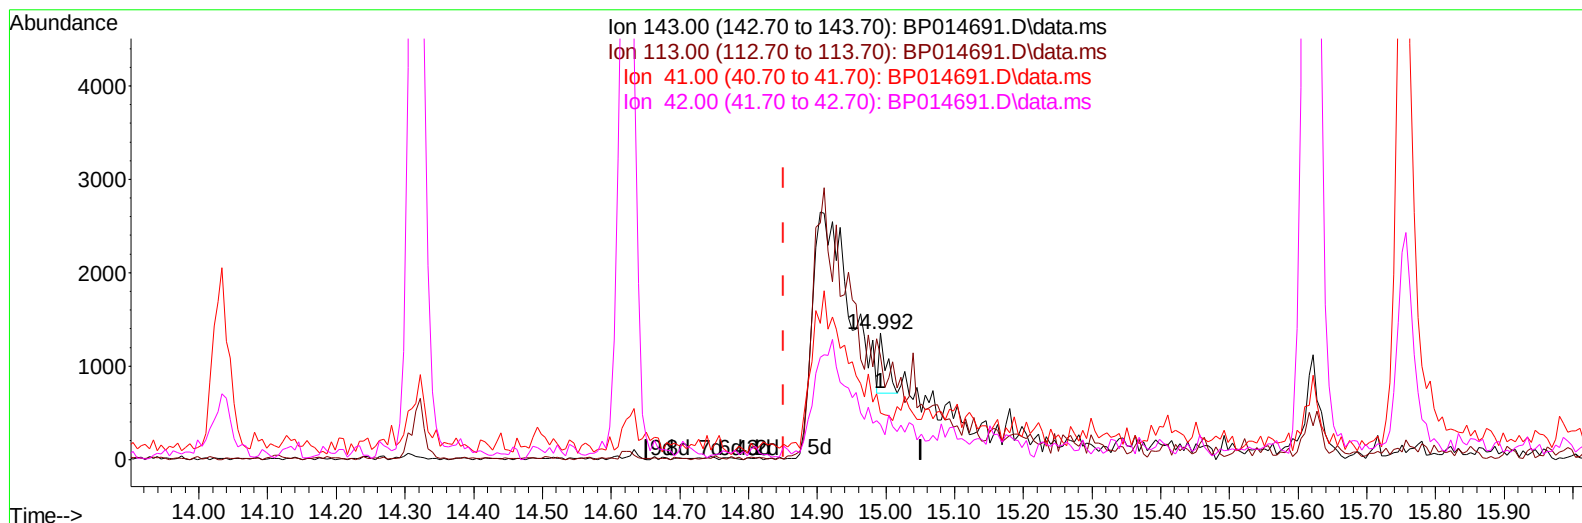

TIC: BP014691.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.992min (+ 0.141) 0.17 ng/ul

response 481

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	81.79
41.00	44.20	36.79
42.00	31.50	27.76




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014691.D
Acq On : 13 Apr 2023 01:49
Operator : CG/JU
Sample : 02250-16
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDY6

Manual IntegrationsAPPROVED

Quant Time: Apr 13 02:34:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 13 02:01:50 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/13/2023
Supervised By :Jagrut Upadhyay 04/13/2023

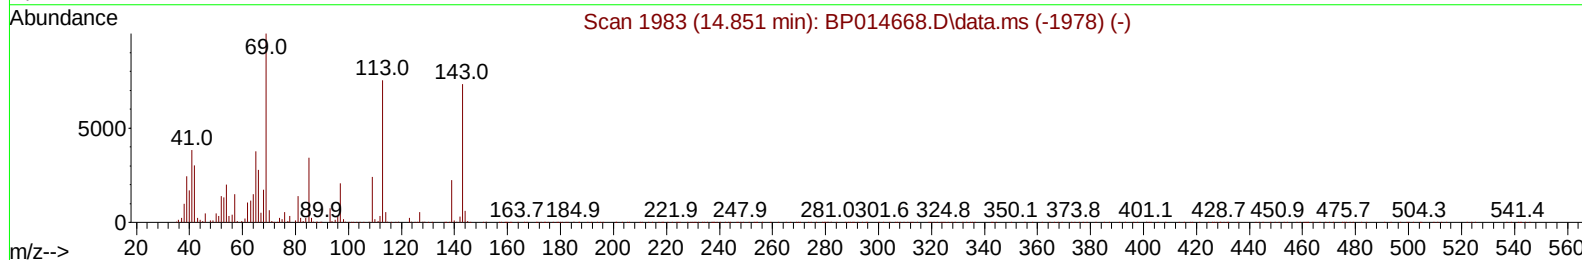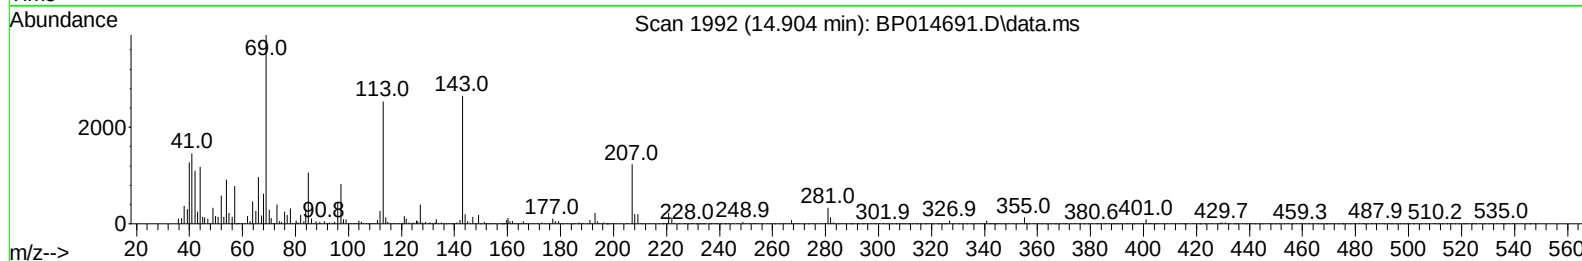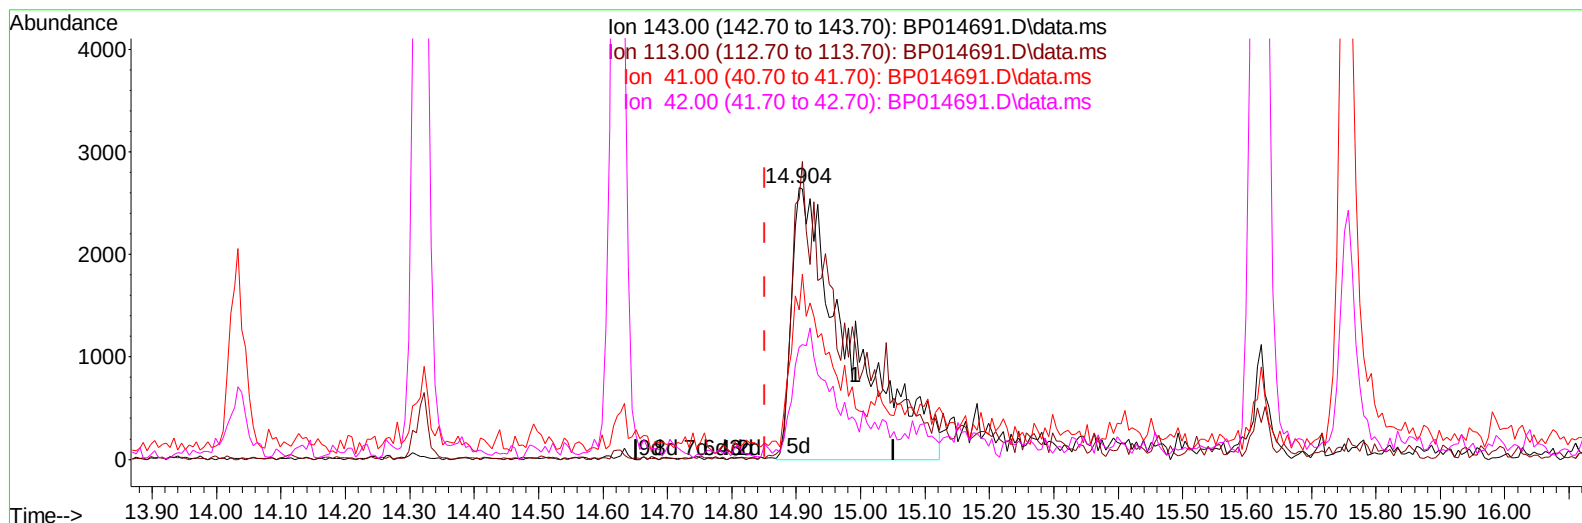

TIC: BP014691.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.904min (+ 0.053) 5.81 ng/ul m

response 16664

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	95.73
41.00	44.20	55.16#
42.00	31.50	41.41#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014691.D
 Acq On : 13 Apr 2023 01:49
 Operator : CG/JU
 Sample : 02250-16
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHDY6

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/13/2023
 Supervised By :Jagrut Upadhyay 04/13/2023

Quant Time: Apr 13 02:34:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 13 02:01:50 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.969	152	95216	20.000	ng/ul	0.00
20) Naphthalene-d8	10.787	136	391362	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.622	164	234140	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.386	188	451898	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	418319	20.000	ng/ul	0.00
88) Perylene-d12	23.974	264	514884	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.358	96	13906	5.664	ng/uL	0.00
4) Pyridine-d5	3.834	84	14711m	2.338	ng/ul	0.04
7) Phenol-d5	7.146	99	65690	7.481	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.299	67	193427	34.331	ng/ul	0.00
11) 2-Chlorophenol-d4	7.499	132	163856	25.817	ng/ul	0.00
15) 4-Methylphenol-d8	8.693	113	114451	16.158	ng/ul	0.00
21) Nitrobenzene-d5	9.146	128	101975	32.277	ng/ul	0.00
24) 2-Nitrophenol-d4	9.875	143	111806	30.905	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.416	165	171865	26.085	ng/ul	0.00
31) 4-Chloroaniline-d4	10.946	131	123999	14.288	ng/ul	0.00
46) Dimethylphthalate-d6	14.034	166	668071	35.190	ng/ul	0.00
49) Acenaphthylene-d8	14.316	160	712233	33.811	ng/ul	0.00
54) 4-Nitrophenol-d4	14.904	143	16664m	5.810	ng/ul	0.05
60) Fluorene-d10	15.622	176	566036	35.753	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	98541	29.635	ng/ul	0.00
73) Anthracene-d10	17.486	188	884944	40.464	ng/ul	0.00
81) Pyrene-d10	19.722	212	972665	34.616	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.815	264	1105766	40.422	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014691.D
Acq On : 13 Apr 2023 01:49
Operator : CG/JU
Sample : 02250-16
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDY6

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/13/2023
Supervised By :Jagrut Upadhyay 04/13/2023

Quant Time: Apr 13 02:34:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 13 02:01:50 2023
Response via : Initial Calibration

