

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014669.D
 Acq On : 12 Apr 2023 11:57
 Operator : CG/JU
 Sample : PB152041BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK041

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014669.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.357	26	29	38	rVB	30286	41199	2.33%	0.206%
2	3.793	101	103	121	rBV	218571	375772	21.23%	1.882%
3	4.110	155	157	162	rVB4	6316	7530	0.43%	0.038%
4	4.563	232	234	238	rBV5	1520	1939	0.11%	0.010%
5	4.669	250	252	254	rBV3	2029	2001	0.11%	0.010%
6	6.851	621	623	626	rVB4	1696	2154	0.12%	0.011%
7	7.140	666	672	688	rBV	303046	594215	33.58%	2.977%
8	7.298	692	699	711	rVV	277352	450402	25.45%	2.256%
9	7.504	727	734	746	rBV	357786	609487	34.44%	3.053%
10	7.610	749	752	753	rVB3	1775	1784	0.10%	0.009%
11	7.969	805	813	824	rBV	336520	561843	31.75%	2.814%
12	8.398	884	886	892	rBV6	1116	2137	0.12%	0.011%
13	8.692	929	936	954	rBV	362410	724996	40.97%	3.632%
14	9.022	990	992	995	rBV4	1557	1844	0.10%	0.009%
15	9.151	1007	1014	1026	rBV	330789	592335	33.47%	2.967%
16	9.875	1129	1137	1156	rBV	270990	512538	28.96%	2.567%
17	10.422	1223	1230	1249	rBV	282433	661414	37.38%	3.313%
18	10.792	1284	1293	1306	rBV	470389	802206	45.33%	4.018%
19	10.945	1311	1319	1343	rBV	232642	596961	33.73%	2.990%
20	11.122	1347	1349	1353	rVB5	1910	2623	0.15%	0.013%
21	11.422	1395	1400	1401	rBV5	1423	2232	0.13%	0.011%
22	11.475	1405	1409	1411	rBV4	1436	2172	0.12%	0.011%
23	12.416	1565	1569	1572	rVB5	3168	5575	0.32%	0.028%
24	13.433	1739	1742	1746	rBV5	1558	1841	0.10%	0.009%
25	13.498	1750	1753	1754	rBV3	1874	2091	0.12%	0.010%
26	13.510	1754	1755	1758	rVB3	2452	1883	0.11%	0.009%
27	13.604	1769	1771	1777	rBV7	1212	1994	0.11%	0.010%
28	13.786	1797	1802	1805	rBV7	1396	1790	0.10%	0.009%
29	14.033	1838	1844	1859	rBV	635423	955132	53.97%	4.784%
30	14.322	1886	1893	1908	rBV	714332	1093858	61.81%	5.479%
31	14.627	1938	1945	1953	rBV	640704	964671	54.51%	4.832%
32	14.886	1981	1989	2010	rBV2	59152	272373	15.39%	1.364%
33	15.469	2085	2088	2091	rVB5	2596	3667	0.21%	0.018%
34	15.504	2091	2094	2095	rBV3	2171	2138	0.12%	0.011%
35	15.622	2107	2114	2128	rBV	853763	1312116	74.15%	6.573%
36	15.757	2132	2137	2153	rBV	203479	381238	21.54%	1.910%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014669.D
 Acq On : 12 Apr 2023 11:57
 Operator : CG/JU
 Sample : PB152041BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK041

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	16.369	2238	2241	2244	rBV5	1860	2483	0.14%	0.012%
38	16.410	2247	2248	2253	rVB5	2412	3005	0.17%	0.015%
39	17.063	2355	2359	2362	rBV5	2576	3980	0.22%	0.020%
40	17.174	2375	2378	2379	rVV3	1977	2036	0.12%	0.010%
41	17.186	2379	2380	2387	rVB7	2909	4097	0.23%	0.021%
42	17.386	2408	2414	2422	rBV	727921	1054564	59.59%	5.282%
43	17.492	2425	2432	2449	rVV	890414	1356743	76.67%	6.796%
44	19.304	2737	2740	2745	rVB7	13541	16863	0.95%	0.084%
45	19.368	2749	2751	2754	rVV3	7489	8685	0.49%	0.044%
46	19.721	2805	2811	2825	rBV	1100271	1588926	89.79%	7.959%
47	21.480	3105	3110	3124	rBV	757471	1349268	76.25%	6.759%
48	23.815	3500	3507	3518	rVB2	870582	1769646	100.00%	8.864%
49	23.986	3529	3536	3548	rVB2	568185	1252912	70.80%	6.276%




Sum of corrected areas: 19963359

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014669.D
Acq On : 12 Apr 2023 11:57
Operator : CG/JU
Sample : PB152041BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK041

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

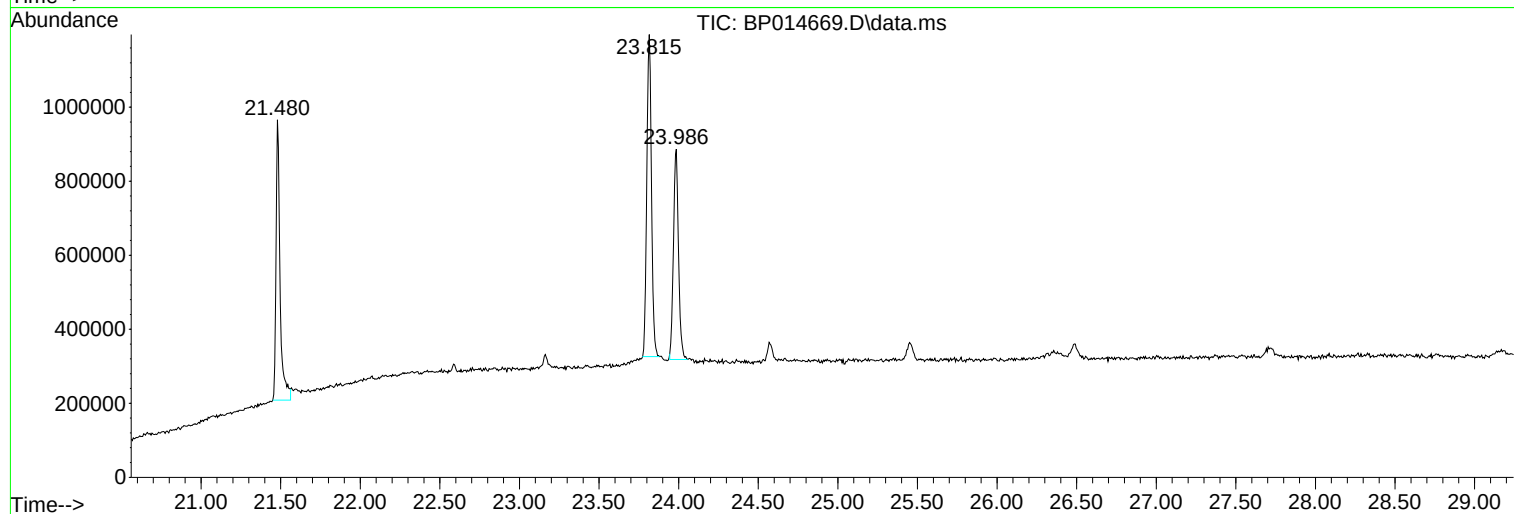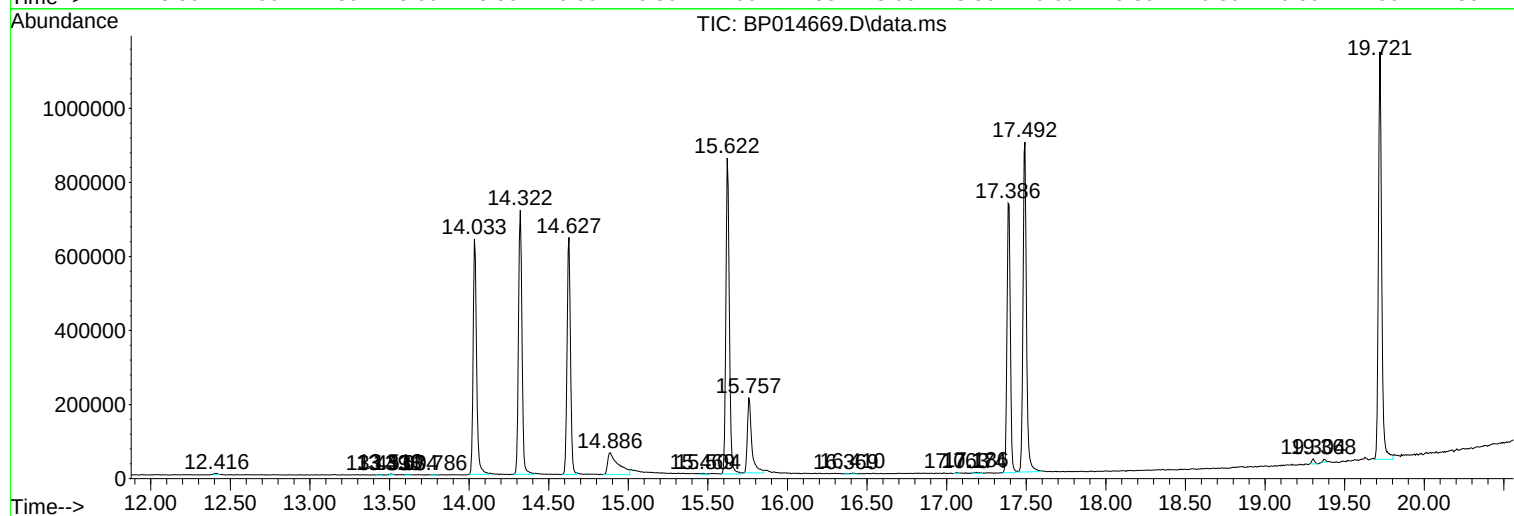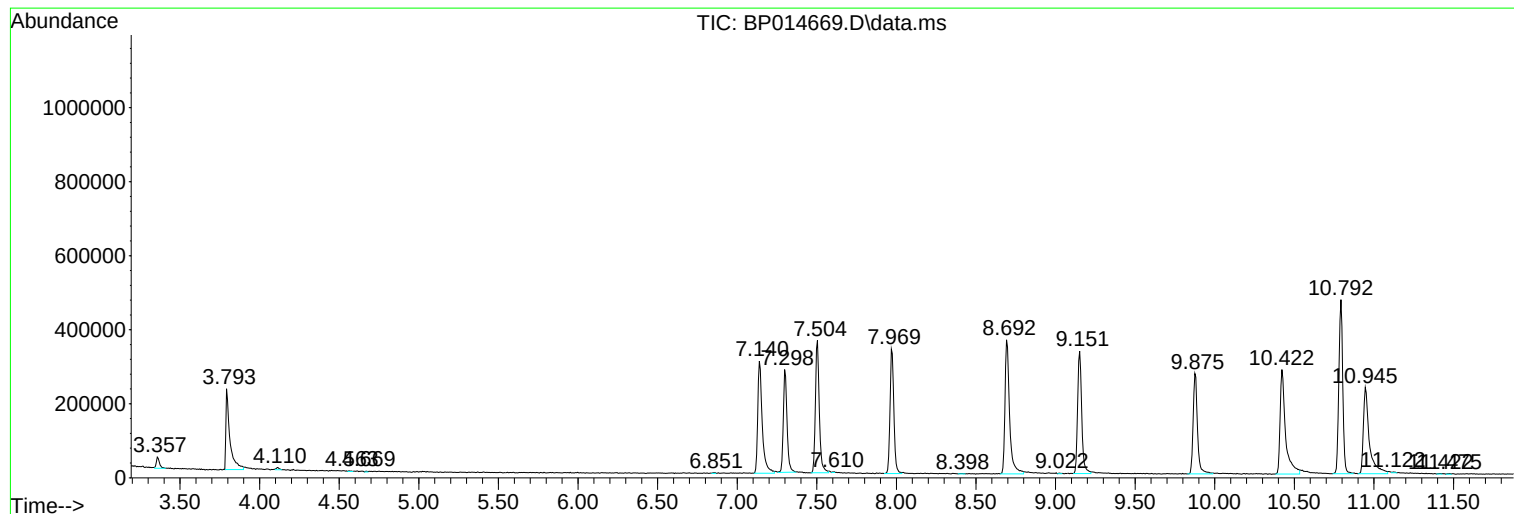

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014669.D
Acq On : 12 Apr 2023 11:57
Operator : CG/JU
Sample : PB152041BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK041

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014669.D
Acq On : 12 Apr 2023 11:57
Operator : CG/JU
Sample : PB152041BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK041

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------