

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
 Data File : BP014670.D
 Acq On : 12 Apr 2023 12:32
 Operator : CG/JU
 Sample : PB152042BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK042

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014670.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	26	29	42	rVB	32528	48202	2.33%	0.188%
2	3.793	101	103	122	rBV	302316	528944	25.53%	2.062%
3	4.111	154	157	165	rVB4	8974	13108	0.63%	0.051%
4	4.652	246	249	250	rBV3	2281	2870	0.14%	0.011%
5	7.140	663	672	693	rBV	439463	825741	39.86%	3.219%
6	7.305	693	700	714	rVB	362536	607790	29.34%	2.369%
7	7.505	727	734	750	rBV	472785	818867	39.53%	3.192%
8	7.975	806	814	826	rBV	428084	723204	34.91%	2.819%
9	8.693	929	936	953	rBV	547737	1014368	48.96%	3.954%
10	8.946	977	979	983	rVB4	2243	2260	0.11%	0.009%
11	9.152	1006	1014	1032	rBV	493623	850979	41.08%	3.317%
12	9.875	1129	1137	1158	rBV	396043	725984	35.04%	2.830%
13	10.422	1223	1230	1255	rBV	427194	946568	45.69%	3.690%
14	10.793	1286	1293	1305	rBV	626010	1046783	50.53%	4.081%
15	10.946	1310	1319	1347	rBV	353403	834321	40.27%	3.252%
16	11.369	1389	1391	1395	rBV5	1487	2465	0.12%	0.010%
17	11.999	1495	1498	1501	rBV5	1424	2372	0.11%	0.009%
18	12.405	1562	1567	1573	rBV8	5570	13711	0.66%	0.053%
19	12.634	1602	1606	1609	rVB5	1737	2937	0.14%	0.011%
20	13.510	1750	1755	1757	rBV6	4461	5252	0.25%	0.020%
21	14.034	1837	1844	1860	rBV	831370	1302213	62.86%	5.076%
22	14.322	1886	1893	1906	rBV	1006715	1492689	72.05%	5.819%
23	14.628	1937	1945	1958	rBV	827481	1265856	61.10%	4.935%
24	14.875	1978	1987	2011	rBV2	92091	396198	19.12%	1.544%
25	15.622	2107	2114	2130	rBV	1180980	1755733	84.75%	6.844%
26	15.757	2131	2137	2153	rVV	306893	523462	25.27%	2.041%
27	15.863	2153	2155	2161	rVB7	8365	13992	0.68%	0.055%
28	17.181	2374	2379	2380	rBV5	2787	3633	0.18%	0.014%
29	17.387	2408	2414	2424	rVV	922957	1365380	65.90%	5.323%
30	17.492	2425	2432	2452	rVB	1169478	1788676	86.34%	6.973%
31	17.681	2462	2464	2466	rBV3	2255	2105	0.10%	0.008%
32	17.745	2473	2475	2479	rVB5	2758	2171	0.10%	0.008%
33	18.557	2611	2613	2617	rVB5	2533	2657	0.13%	0.010%
34	18.981	2683	2685	2686	rBV2	4604	2611	0.13%	0.010%
35	19.304	2736	2740	2745	rBV4	15837	25102	1.21%	0.098%
36	19.375	2749	2752	2754	rBV3	10401	11177	0.54%	0.044%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014670.D
Acq On : 12 Apr 2023 12:32
Operator : CG/JU
Sample : PB152042BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK042

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Title : SVOA CALIBRATION

37	19.722	2805	2811	2828	rBV	1284896	1829027	88.28%	7.130%
38	21.480	3105	3110	3124	rBV	860237	1344123	64.88%	5.240%
39	23.816	3501	3507	3521	rVB2	1008974	2071742	100.00%	8.076%
40	23.980	3529	3535	3547	rVB2	651107	1437114	69.37%	5.602%




Sum of corrected areas: 25652387

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014670.D
Acq On : 12 Apr 2023 12:32
Operator : CG/JU
Sample : PB152042BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK042

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

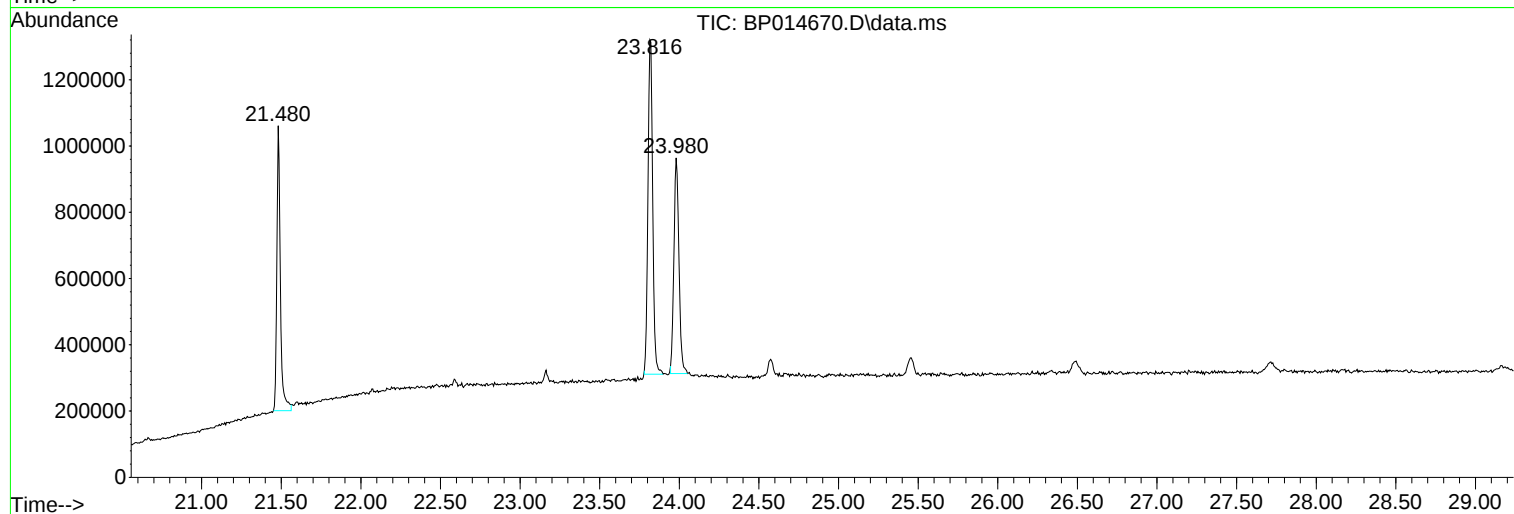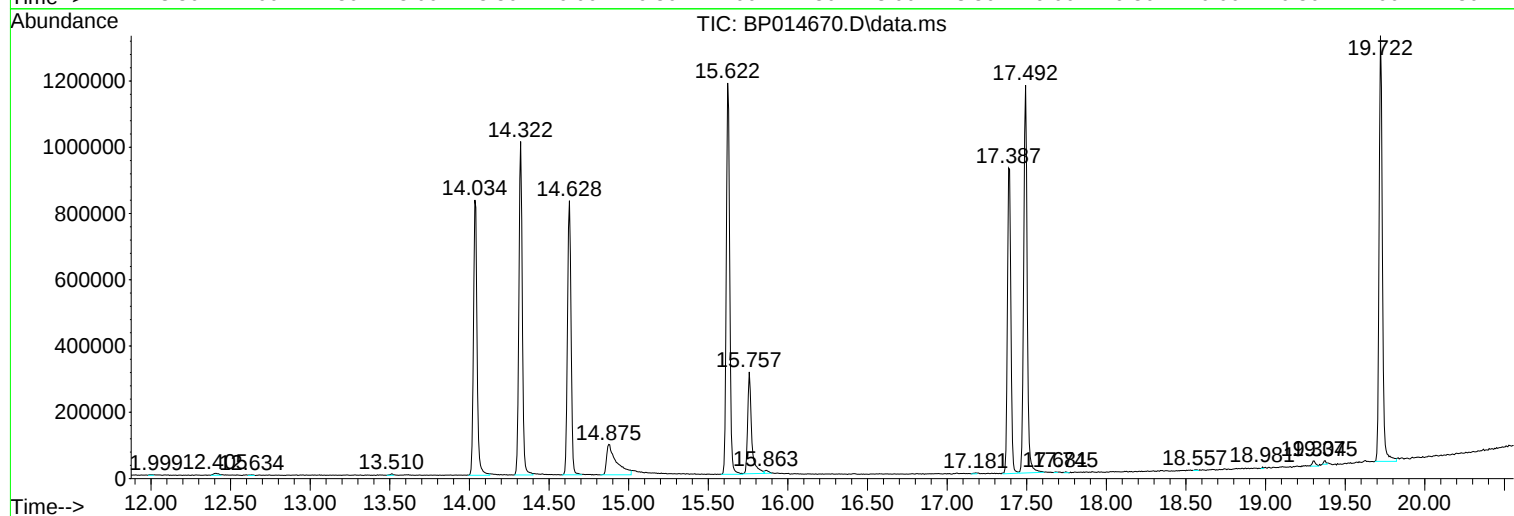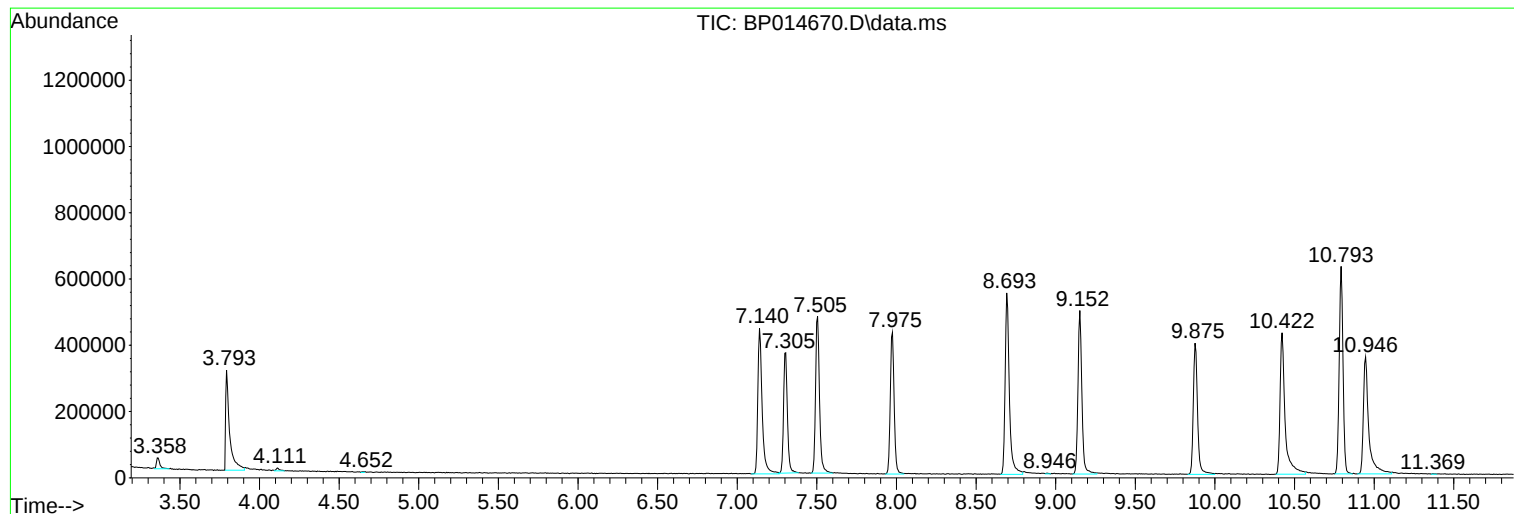

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014670.D
Acq On : 12 Apr 2023 12:32
Operator : CG/JU
Sample : PB152042BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK042

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041223\
Data File : BP014670.D
Acq On : 12 Apr 2023 12:32
Operator : CG/JU
Sample : PB152042BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK042

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc